



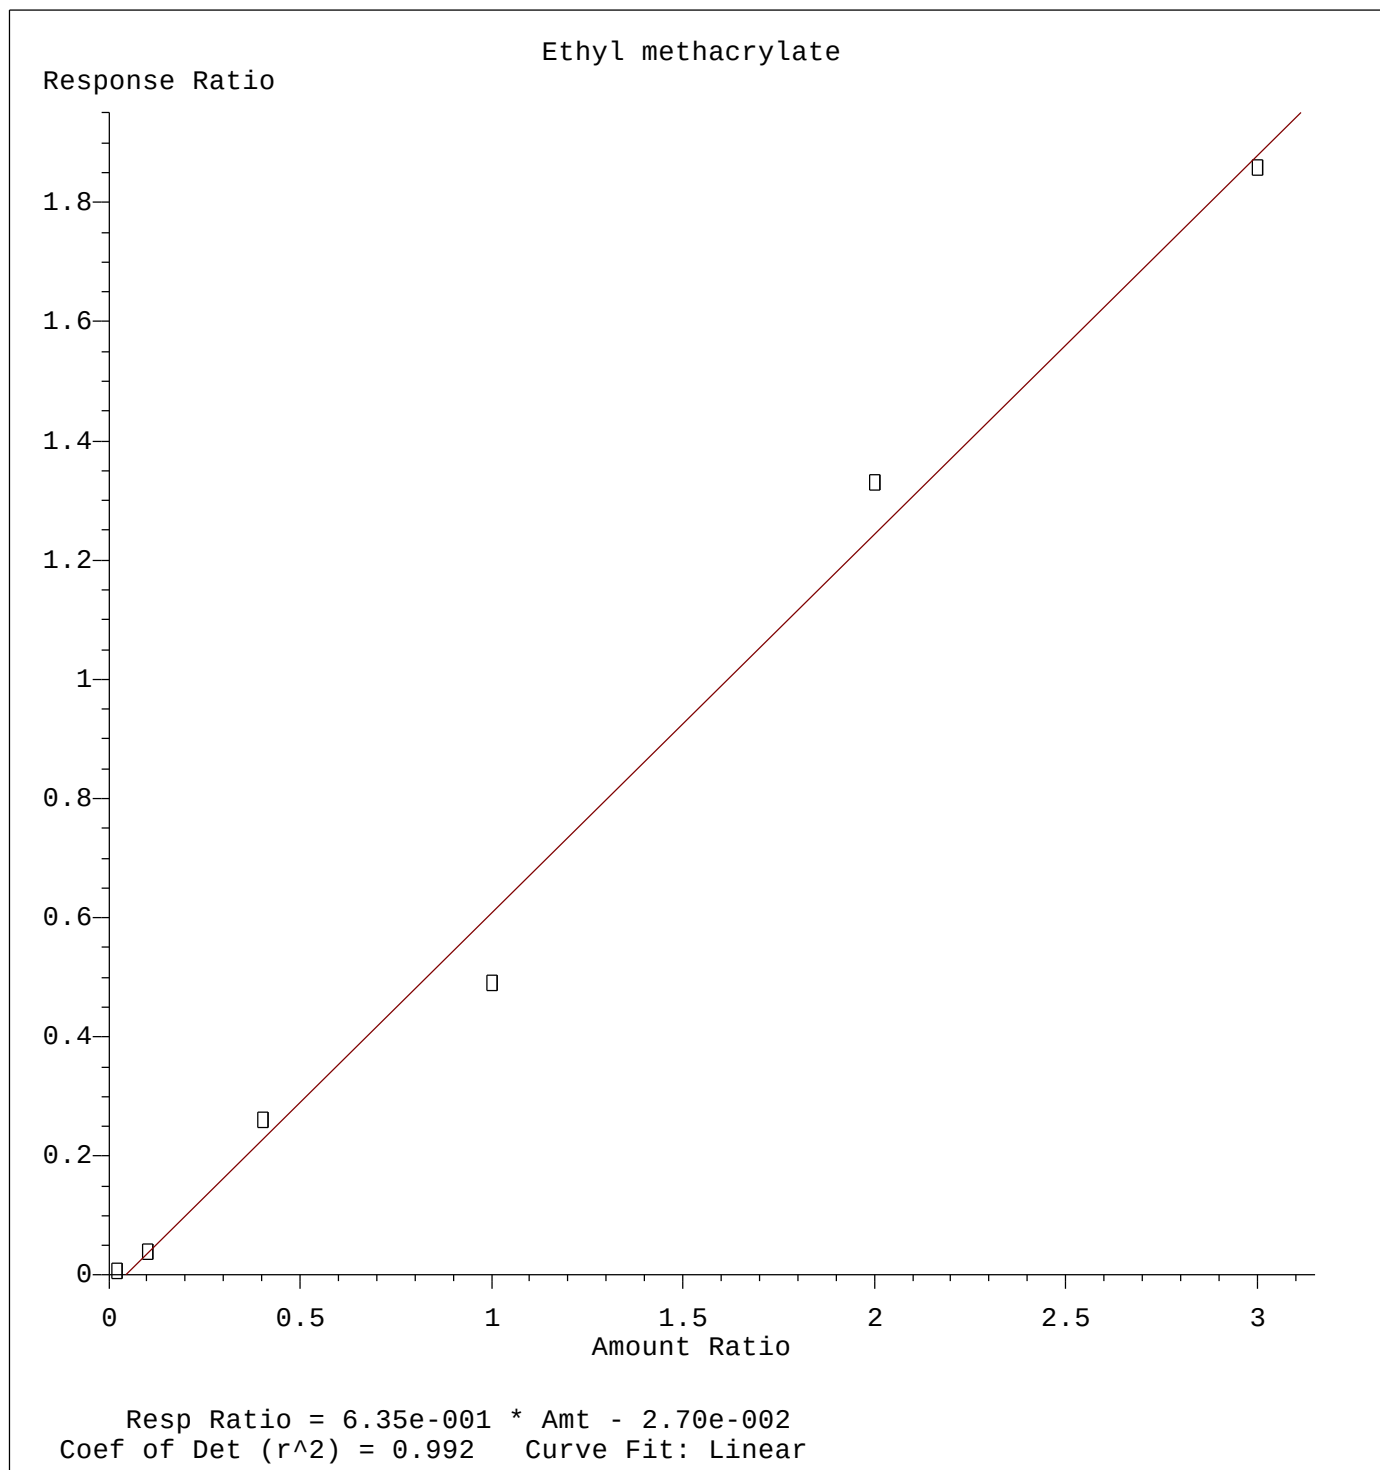

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N120919W.M
Calibration Table Last Updated: Tue Dec 10 01:09:52 2019


2-Hexanone

Response Ratio

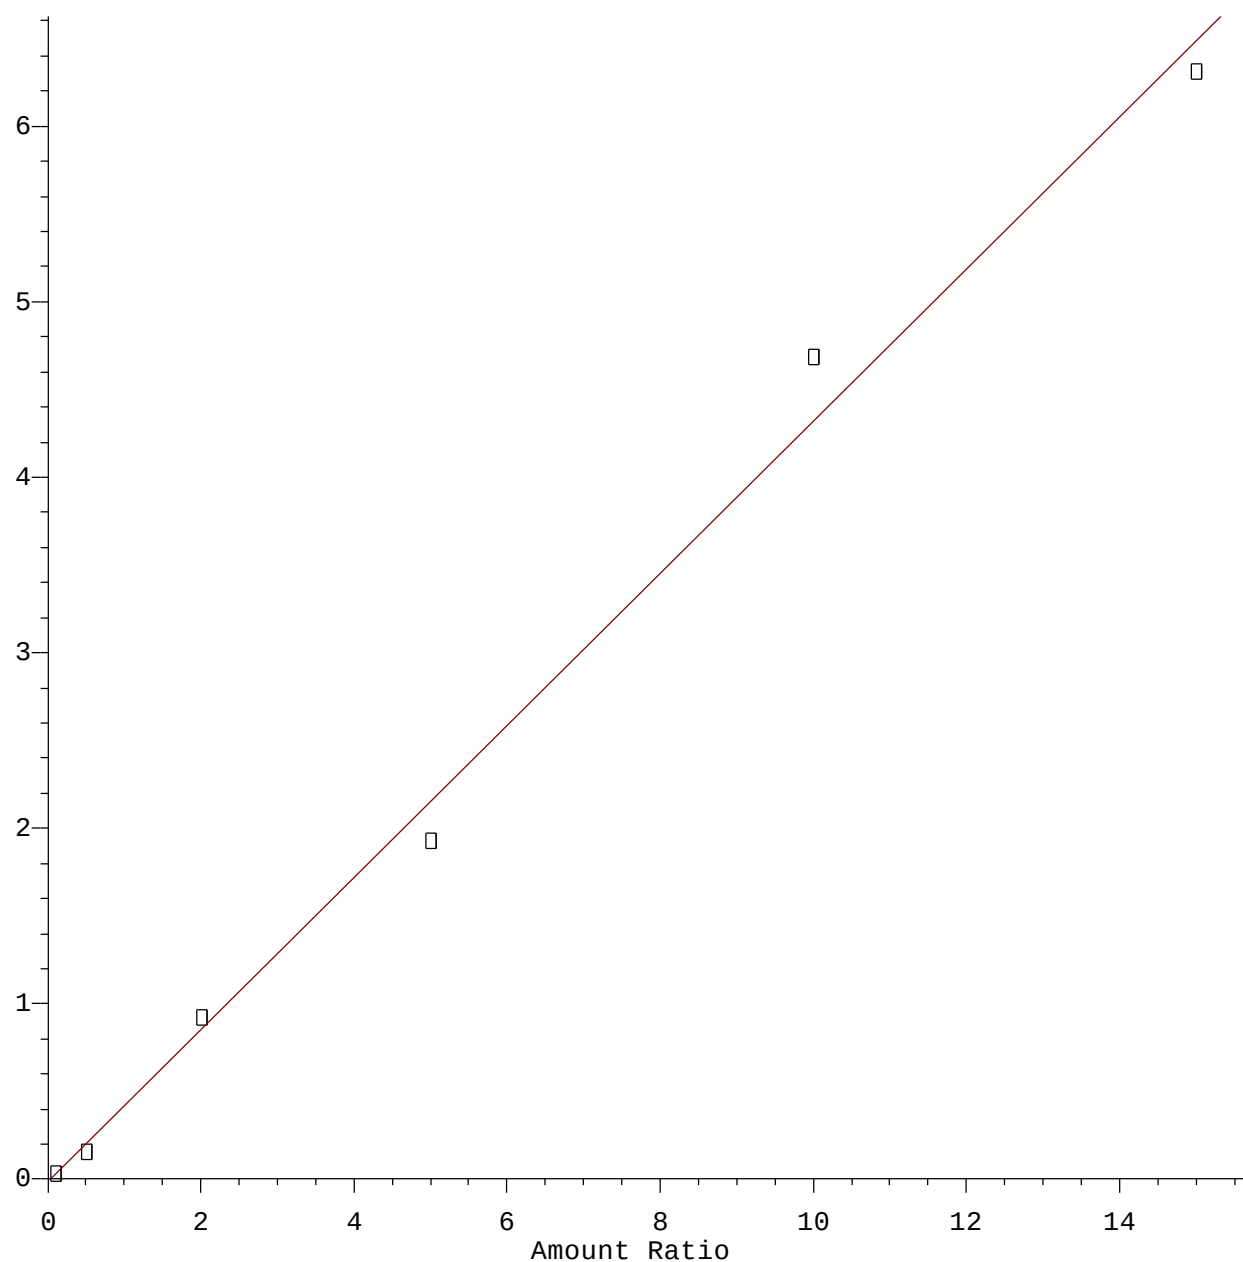

Resp Ratio = $4.34 \times 10^{-1} \times \text{Amt} - 1.92 \times 10^{-2}$
Coef of Det (r^2) = 0.993 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N120919W.M
Calibration Table Last Updated: Tue Dec 10 01:09:52 2019

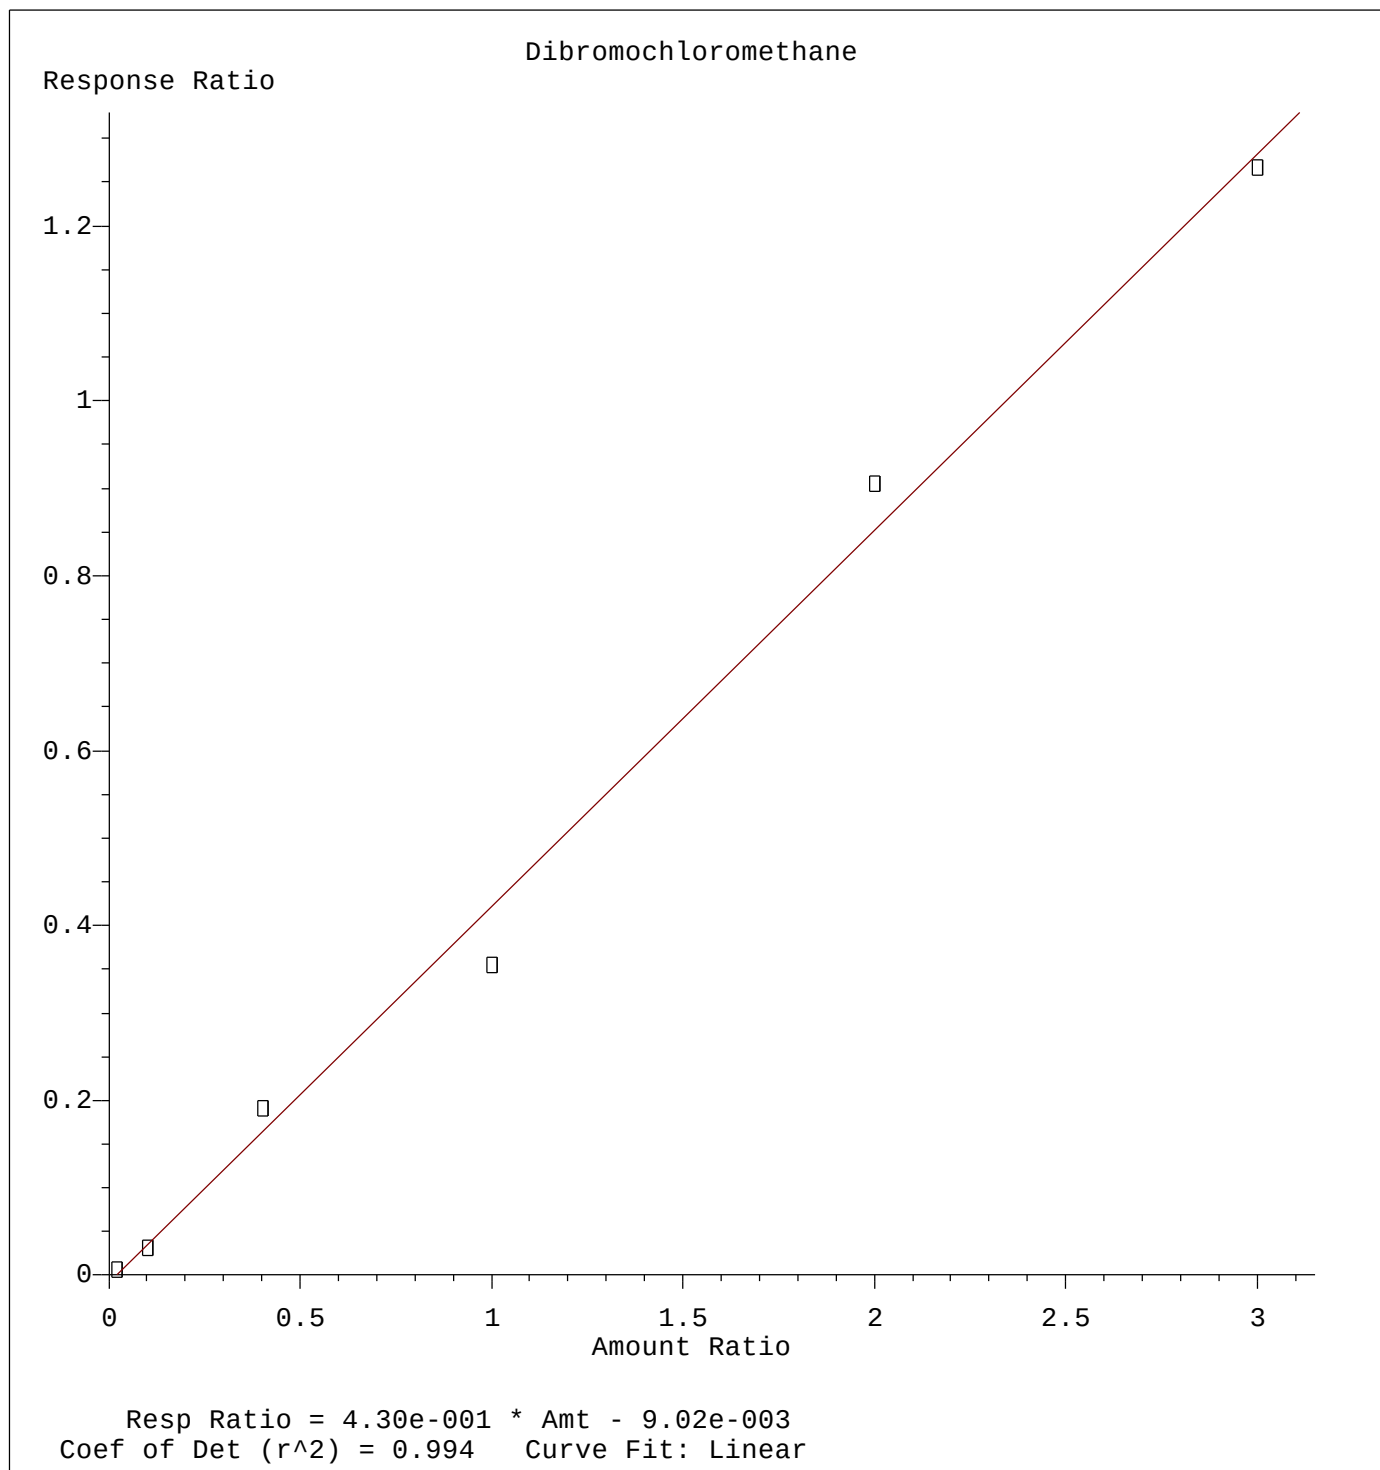

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N120919W.M
Calibration Table Last Updated: Tue Dec 10 01:09:52 2019

1,2-Dibromo-3-Chloropropane

Response Ratio

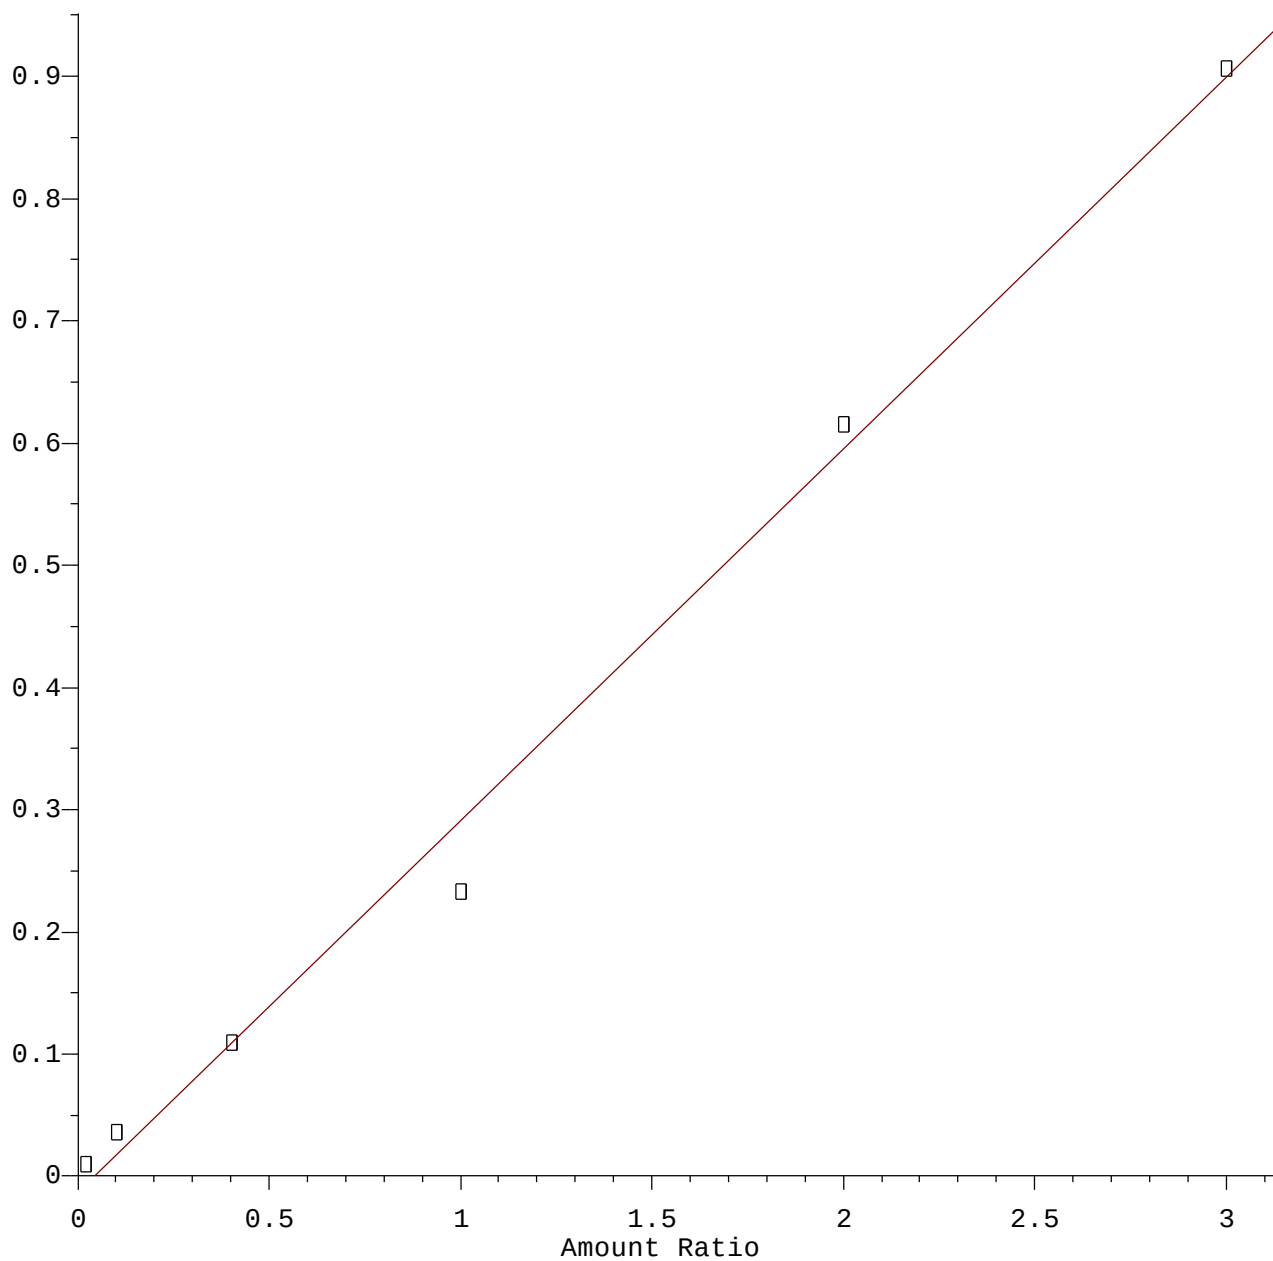


Resp Ratio = $3.04 \times 10^{-1} \times \text{Amt} - 1.27 \times 10^{-2}$
Coef of Det (r^2) = 0.993 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N120919W.M
Calibration Table Last Updated: Tue Dec 10 01:09:52 2019


1,2,3-Trichlorobenzene

Response Ratio

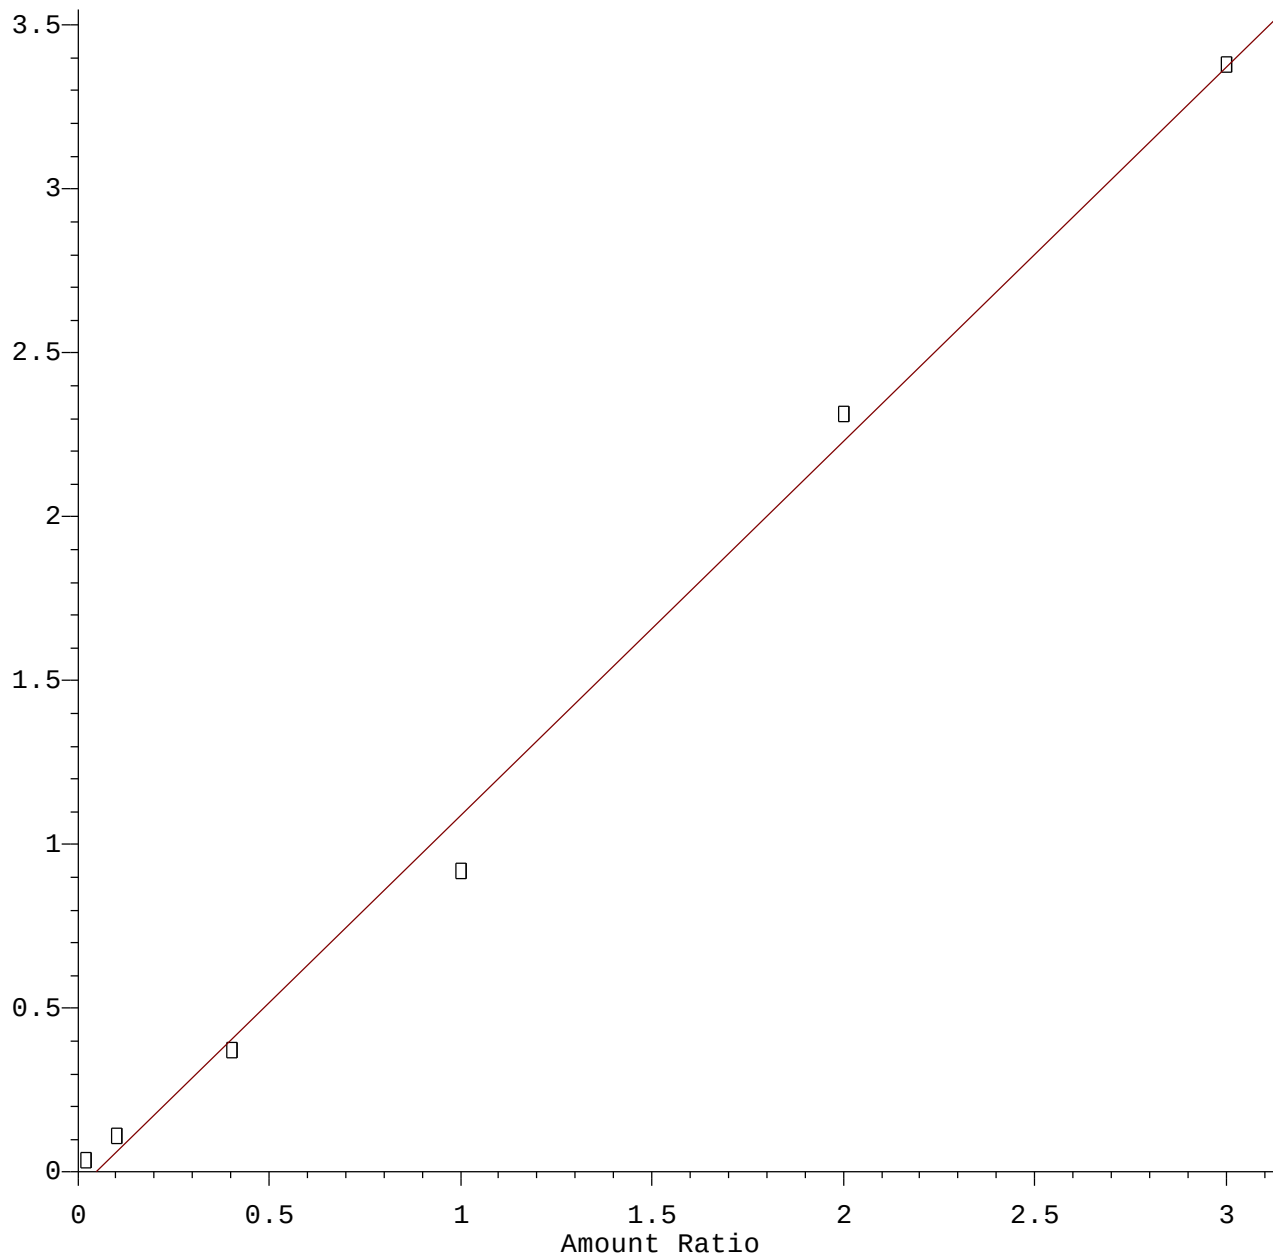

Resp Ratio = 1.14×10^0 * Amt - 5.51×10^{-2}
Coef of Det (r^2) = 0.995 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N120919W.M
Calibration Table Last Updated: Tue Dec 10 01:09:52 2019

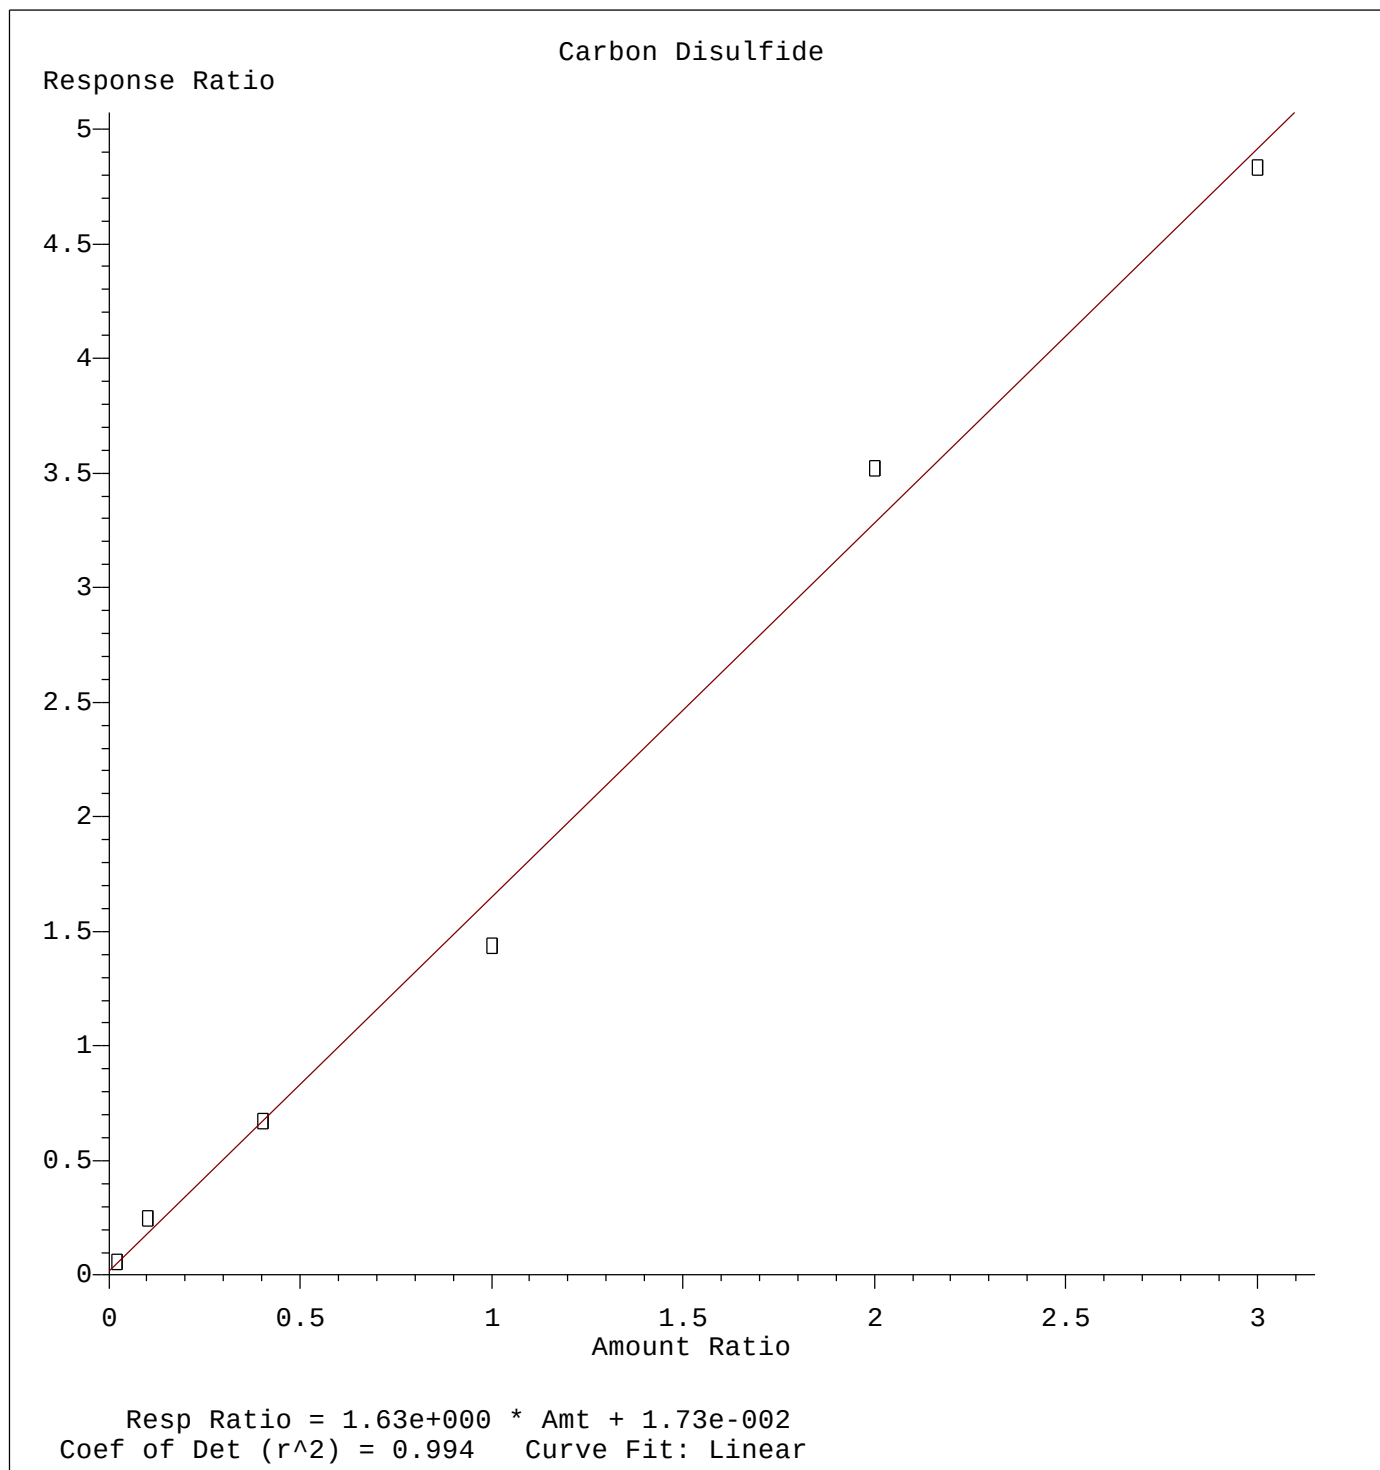

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N120919W.M
Calibration Table Last Updated: Tue Dec 10 01:09:52 2019

Methylene Chloride

Response Ratio

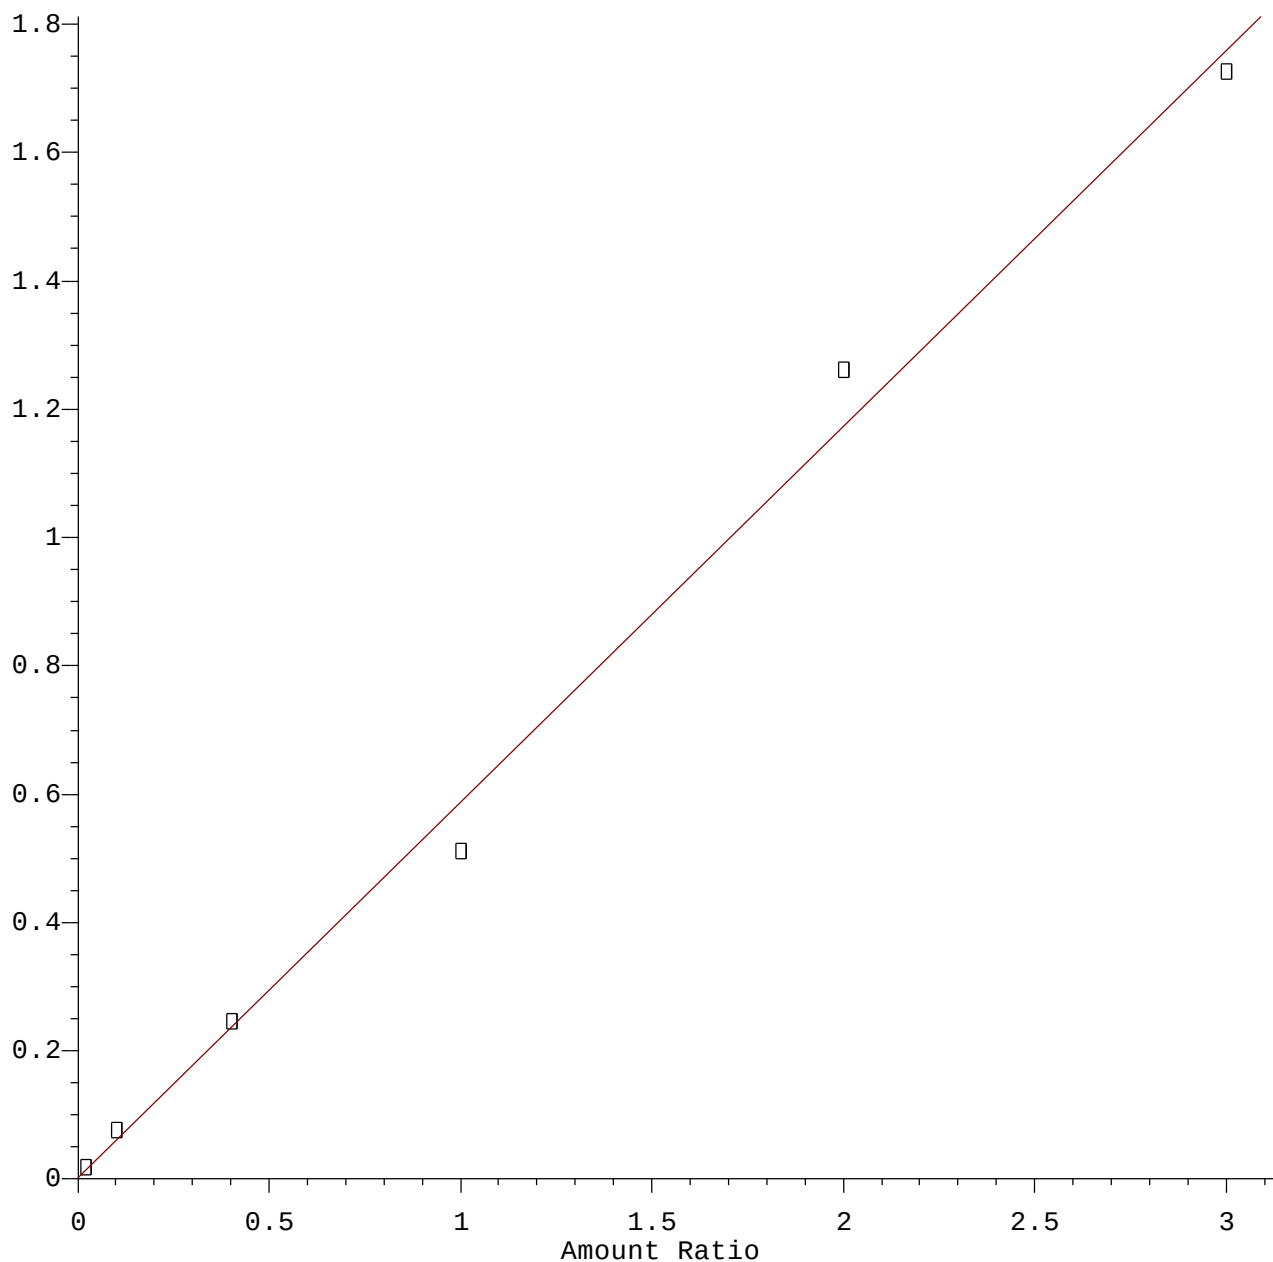


Resp Ratio = $5.85 \times 10^{-1} \times \text{Amt} + 3.22 \times 10^{-3}$
Coef of Det (r^2) = 0.994 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N120919W.M
Calibration Table Last Updated: Tue Dec 10 01:09:52 2019


Bromochloromethane

Response Ratio

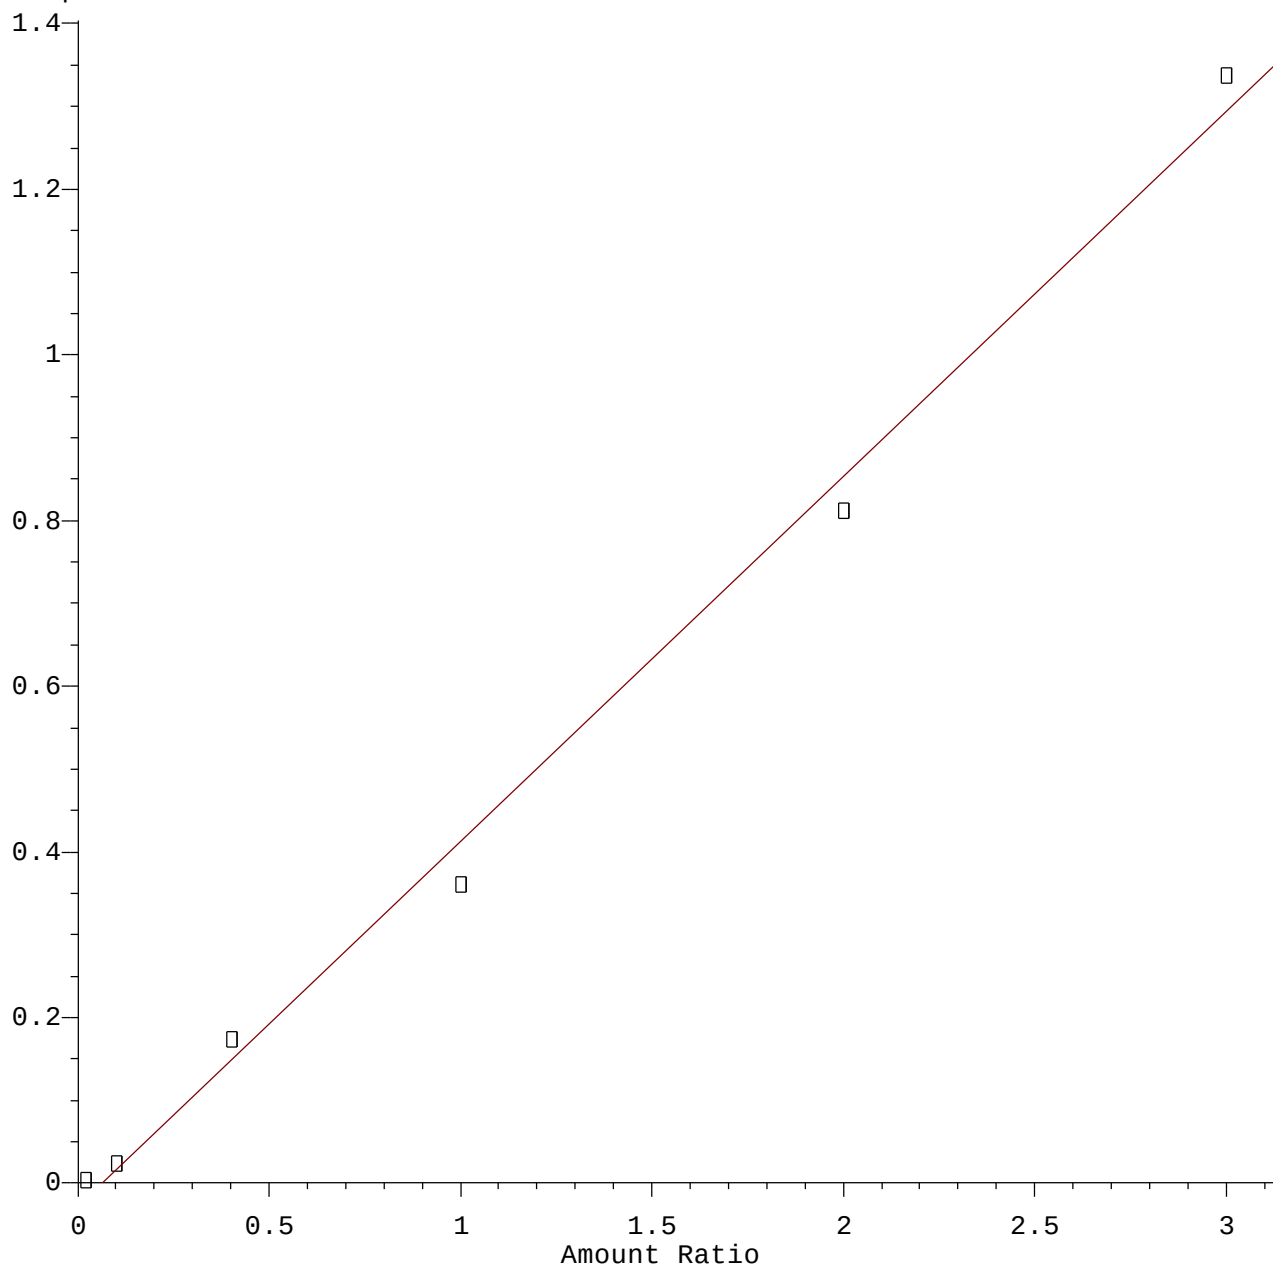

Resp Ratio = $4.40 \times 10^{-1} \times \text{Amt} - 2.74 \times 10^{-2}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N120919W.M
Calibration Table Last Updated: Tue Dec 10 01:09:52 2019

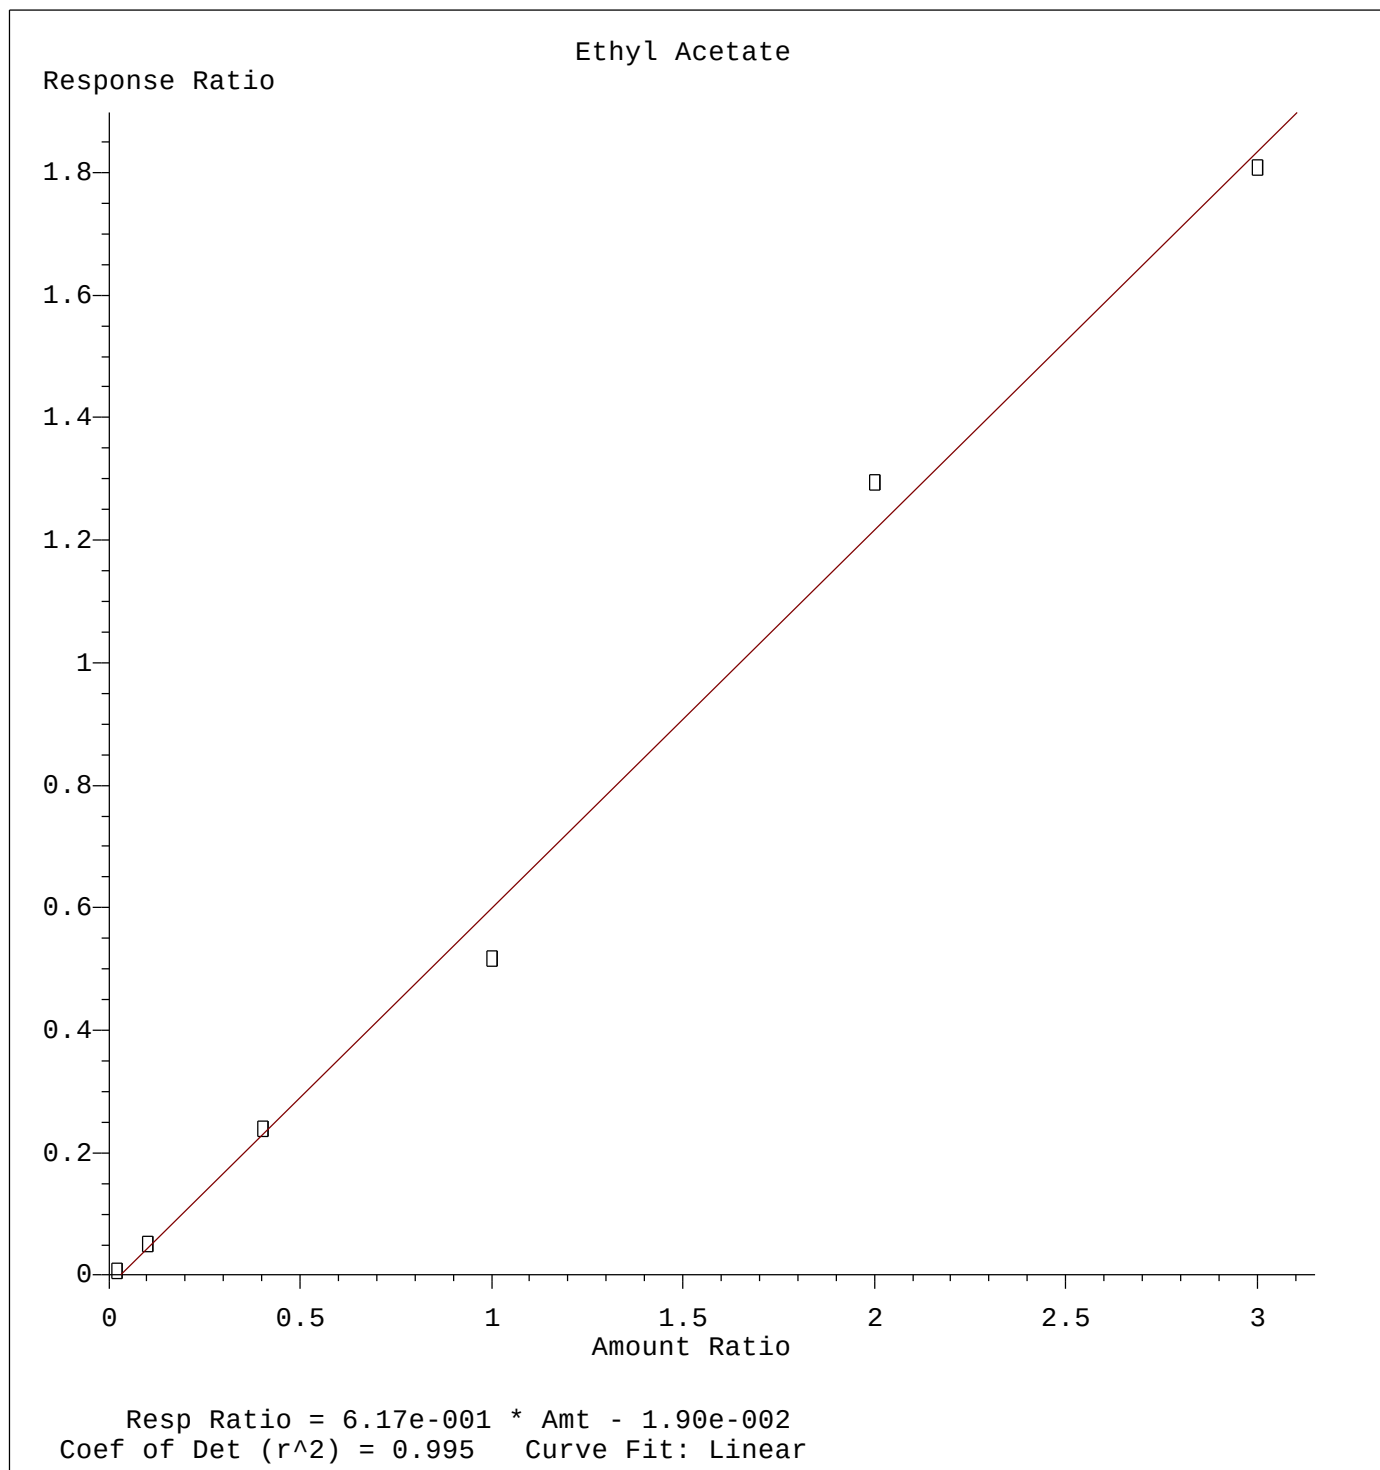

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N120919W.M
Calibration Table Last Updated: Tue Dec 10 01:09:52 2019

4-Methyl-2-Pentanone

Response Ratio

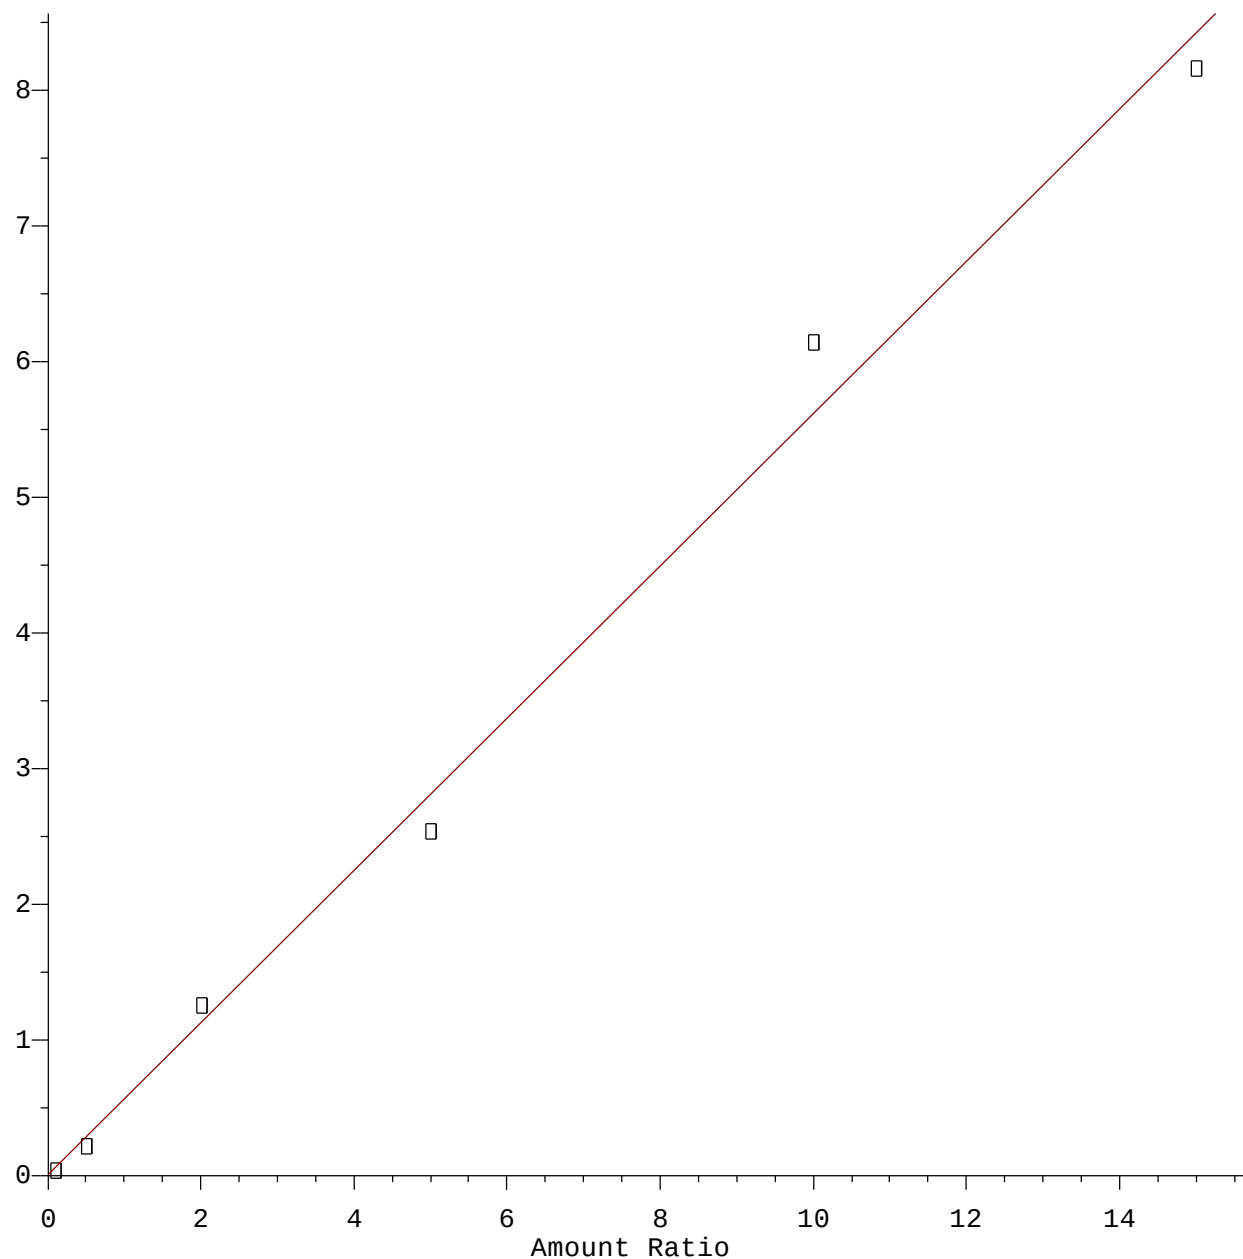

Resp Ratio = $5.61 \times 10^{-1} \times \text{Amt} + 9.12 \times 10^{-3}$
Coef of Det (r^2) = 0.992 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N120919W.M
Calibration Table Last Updated: Tue Dec 10 01:09:52 2019