


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN120919\
Data File : VN059524.D
Acq On : 9 Dec 2019 13:37
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N120919W.M
Title : SW846 8260
Last Update : Tue Dec 10 01:09:52 2019

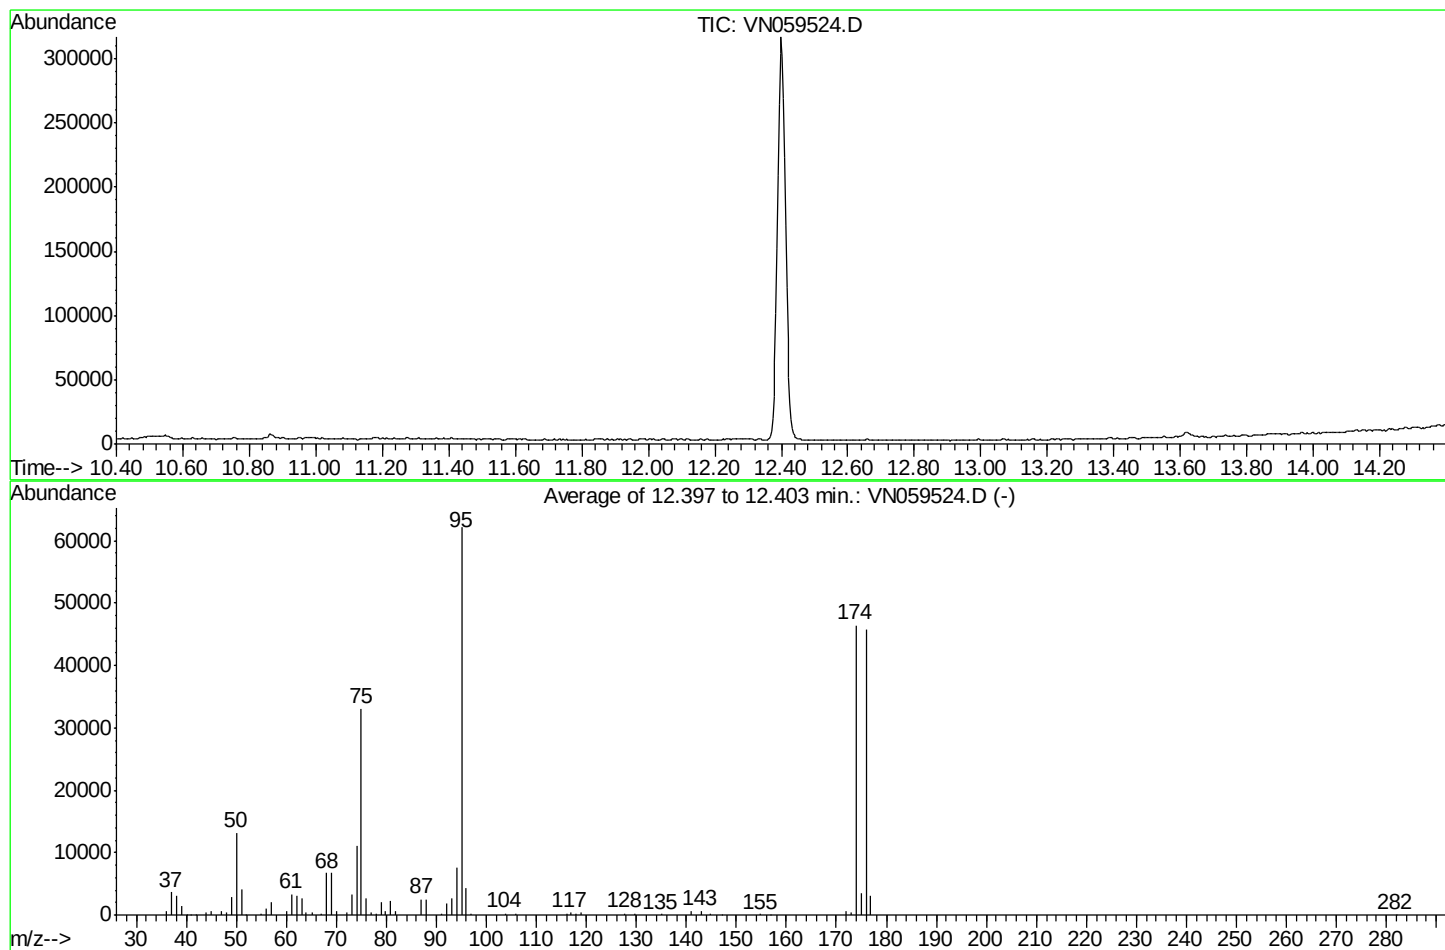

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	13196	PASS
75	95	30	60	53.3	33109	PASS
95	95	100	100	100.0	62170	PASS
96	95	5	9	6.9	4274	PASS
173	174	0.00	2	1.1	493	PASS
174	95	50	100	74.6	46405	PASS
175	174	5	9	7.7	3593	PASS
176	174	95	101	98.7	45816	PASS
177	176	5	9	6.7	3068	PASS