

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120921\
 Data File : VN069942.D
 Acq On : 10 Dec 2021 5:03
 Operator : JC/MD
 Sample : PB141262ZHE#08
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB141262ZHE#08

Quant Time: Dec 10 08:15:09 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
 Quant Title : SW846 8260
 QLast Update : Fri Dec 03 08:46:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.088	168	1077203	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	2104972	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.744	117	2436224	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.675	152	973537	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	879651	52.889	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 105.780%	
35) Dibromofluoromethane	8.024	113	643407	48.798	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 97.600%	
50) Toluene-d8	10.443	98	2818349	53.234	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 106.460%	
62) 4-Bromofluorobenzene	12.731	95	1144607	59.677	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 119.360%	
Target Compounds						
					Qvalue	
3) Chloromethane	2.309	50	3349	0.213	ug/l	90
11) Tert butyl alcohol	5.315	59	11237	3.574	ug/l #	71
13) Acrolein	4.049	56	943	0.352	ug/l #	48
16) Acetone	4.296	43	72900	7.286	ug/l	96
18) Methyl Acetate	4.859	43	56635	1.875	ug/l #	87
20) Methylene Chloride	5.098	84	40354	3.034	ug/l	85
25) 2-Butanone	7.348	43	16697	1.228	ug/l #	87
29) Tetrahydrofuran	7.691	42	2175	0.263	ug/l #	49
31) Cyclohexane	8.086	56	29260	1.264	ug/l #	28
36) 1,1-Dichloropropene	8.088	75	92962	4.639	ug/l #	49
38) Carbon Tetrachloride	8.091	117	111655	5.682	ug/l #	16
43) Isopropyl Acetate	8.566	43	183366	4.155	ug/l #	78
45) 1,2-Dichloropropane	9.622	63	8324	0.506	ug/l #	44
48) Methyl methacrylate	9.545	41	31527	1.531	ug/l #	8
51) 4-Methyl-2-Pentanone	10.333	43	17951	0.627	ug/l	95
53) t-1,3-Dichloropropene	10.717	75	52	2.796	ug/l #	43
54) cis-1,3-Dichloropropene	10.242	75	171518	8.385	ug/l #	72
56) Ethyl methacrylate	10.703	69	571	2.298	ug/l #	24
57) 1,3-Dichloropropane	11.089	76	104788	3.944	ug/l #	43
59) 2-Hexanone	11.089	43	1912933	88.319	ug/l #	47
60) Dibromochloromethane	11.489	129	1064	2.439	ug/l #	11
71) Bromoform	12.715	173	1339	2.816	ug/l #	29
74) N-amyl acetate	12.197	43	74469	1.944	ug/l #	53
76) 1,2,3-Trichloropropane	12.731	75	647125	23.179	ug/l #	1
80) 1,3,5-Trimethylbenzene	13.061	105	17977	0.258	ug/l	100
81) trans-1,4-Dichloro-2-b...	12.731	75	647125	73.761	ug/l #	5
93) 1,2,4-Trichlorobenzene	15.271	180	283	2.895	ug/l #	35
95) Naphthalene	15.499	128	1581	4.016	ug/l #	82
96) 1,2,3-Trichlorobenzene	15.702	180	359	2.458	ug/l #	12


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120921\
Data File : VN069942.D
Acq On : 10 Dec 2021 5:03
Operator : JC/MD
Sample : PB141262ZHE#08
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB141262ZHE#08

Quant Time: Dec 10 08:15:09 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
Quant Title : SW846 8260
QLast Update : Fri Dec 03 08:46:47 2021
Response via : Initial Calibration




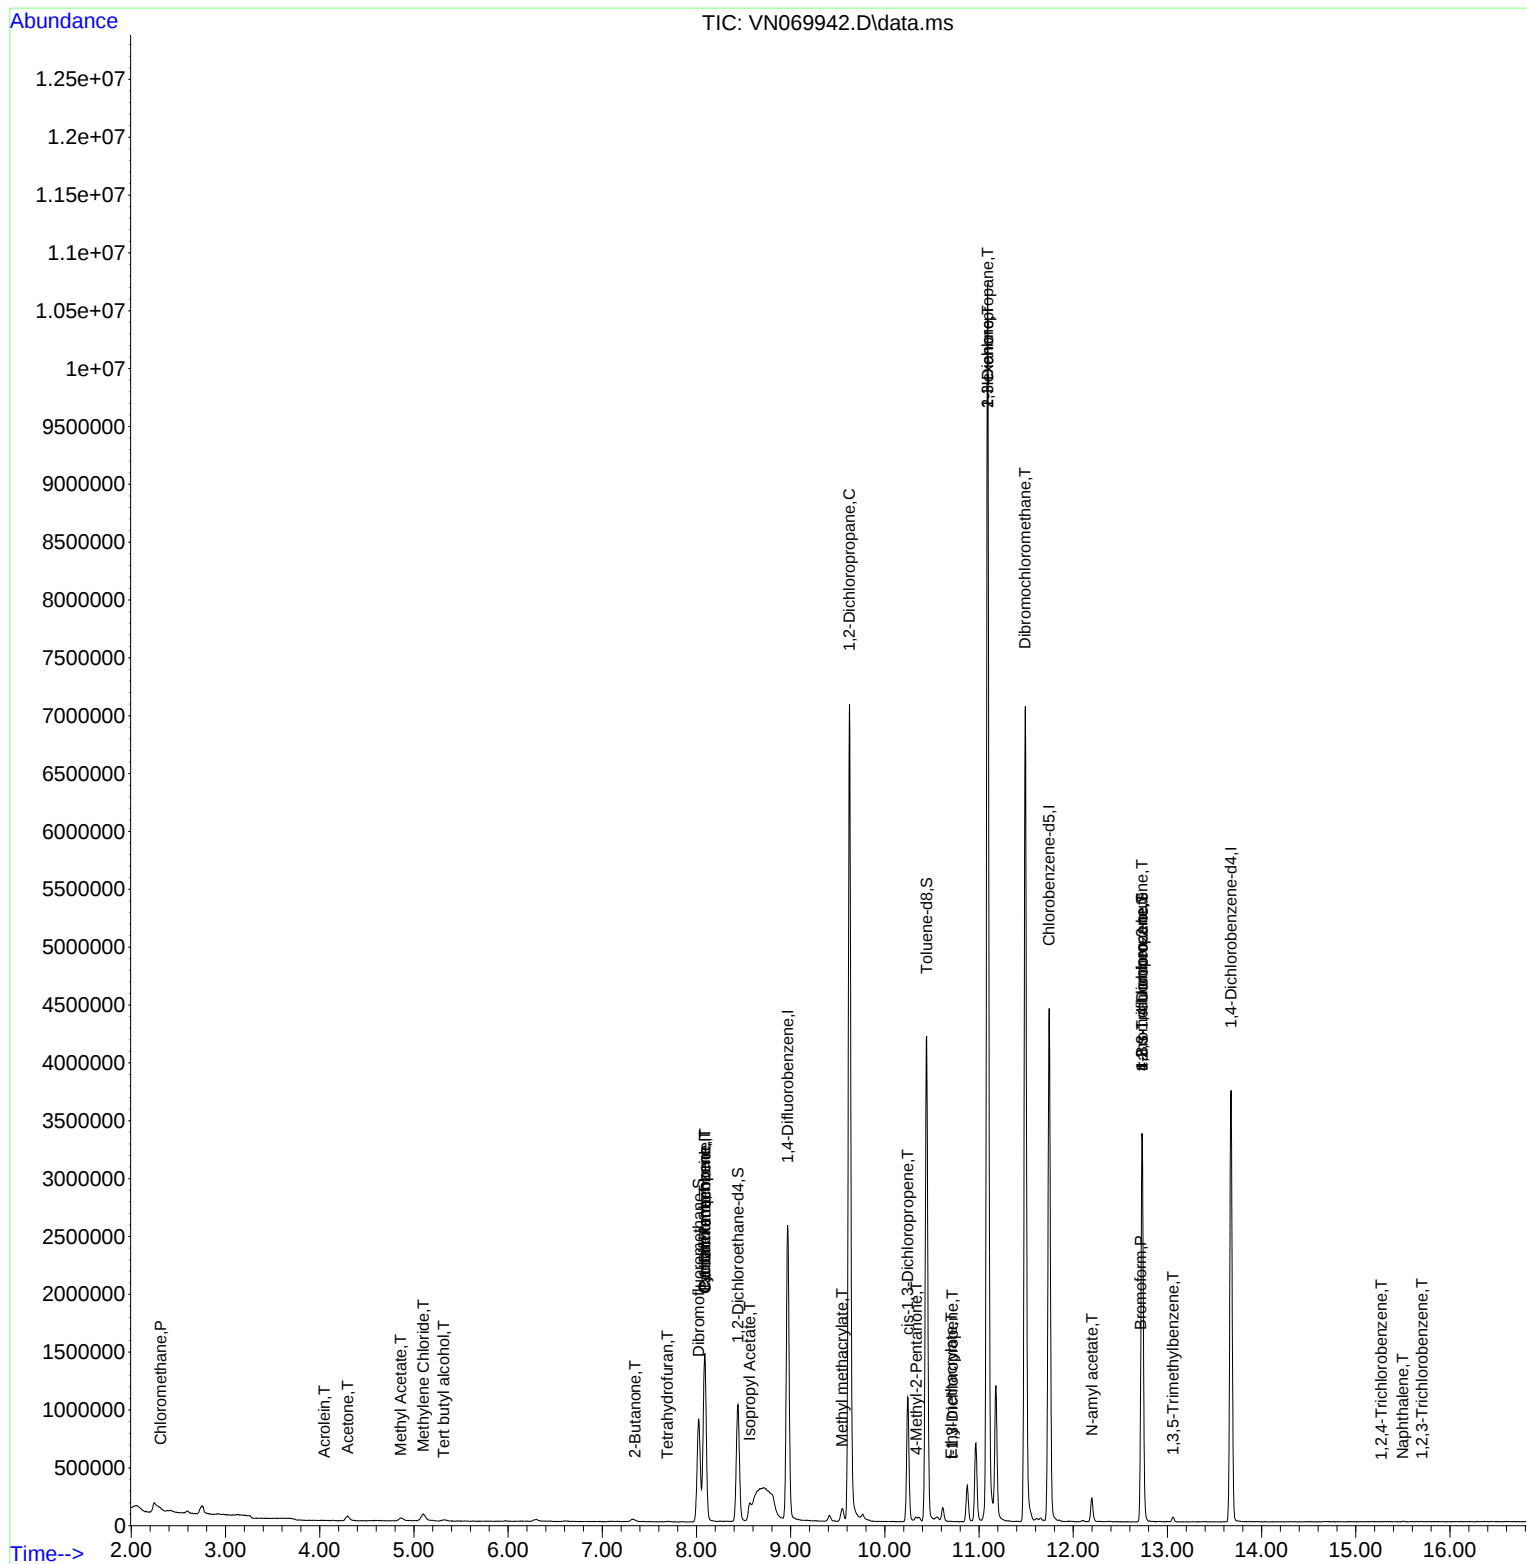


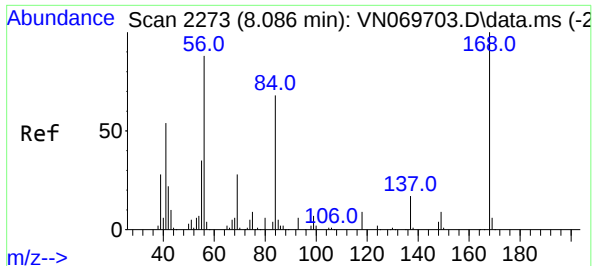

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 21
Delta R.T. 0.002 min
Lab File: VN069942.D
Acq: 10 Dec 2021 5:03




Instrument :
MSVOA_N
ClientSampleId :
PB141262ZHE#08


Tgt Ion:168 Resp: 1077203
Ion Ratio Lower Upper
168 100
99 61.8 41.3 61.9

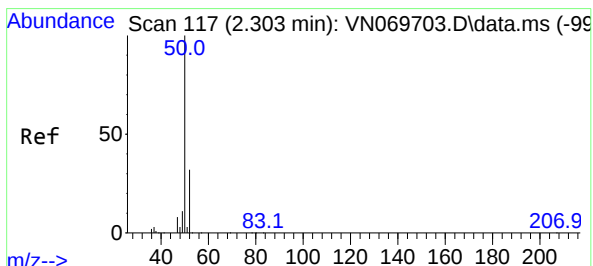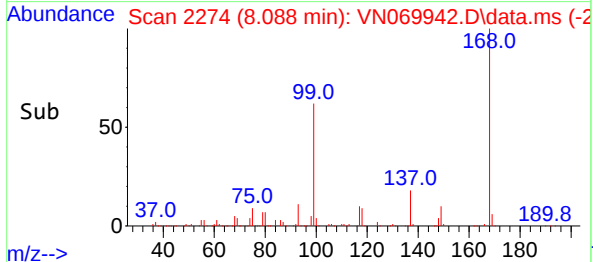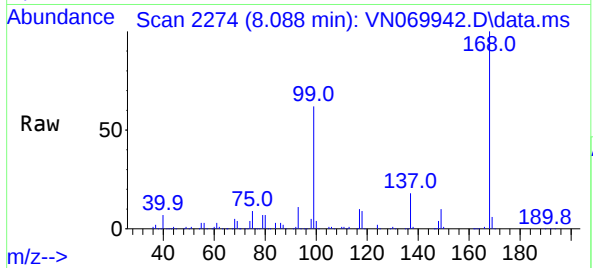

#3
Chloromethane
Concen: 0.213 ug/l
RT: 2.309 min Scan# 119
Delta R.T. 0.006 min
Lab File: VN069942.D
Acq: 10 Dec 2021 5:03

Tgt Ion: 50 Resp: 3349
Ion Ratio Lower Upper
50 100
52 26.0 25.4 38.0


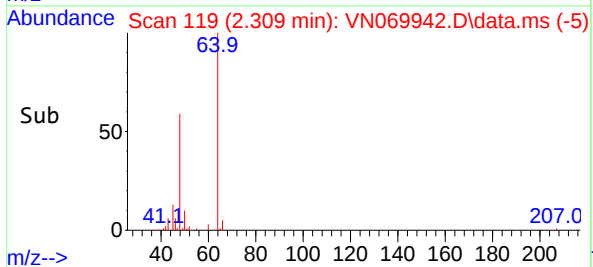

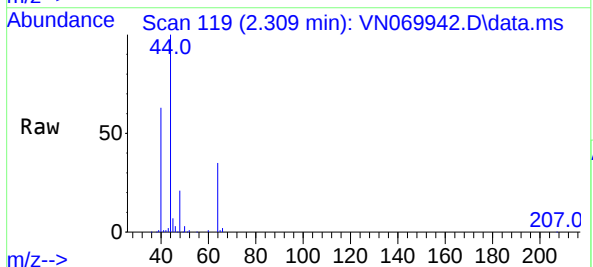


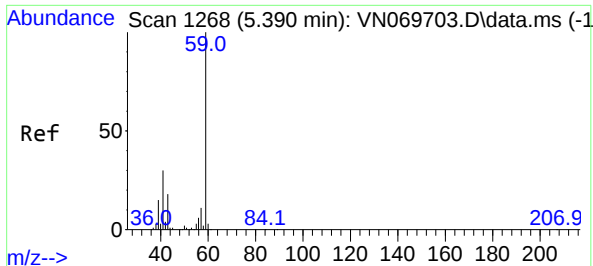

#11
Tert butyl alcohol
Concen: 3.574 ug/l
RT: 5.315 min Scan# 11
Delta R.T. -0.075 min
Lab File: VN069942.D
Acq: 10 Dec 2021 5:03




Instrument :
MSVOA_N
ClientSampleId :
PB141262ZHE#08


Tgt Ion: 59 Resp: 11237
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1#

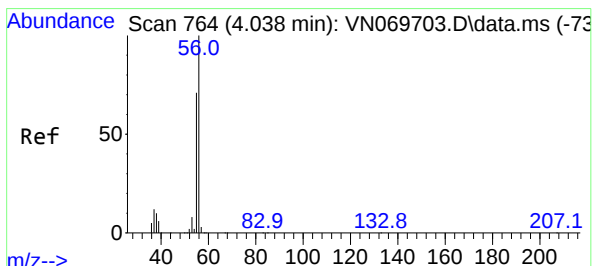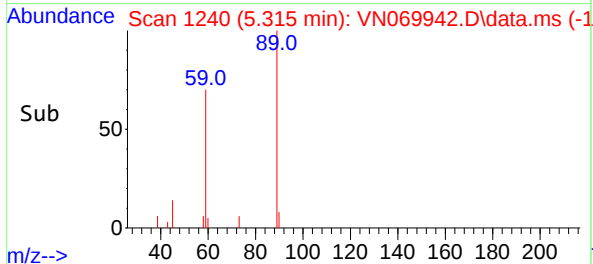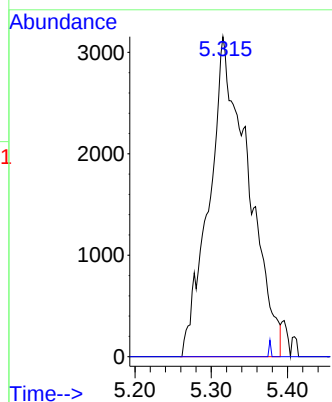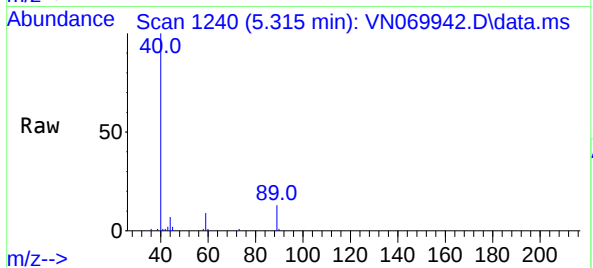

#13
Acrolein
Concen: 0.352 ug/l
RT: 4.049 min Scan# 768
Delta R.T. 0.011 min
Lab File: VN069942.D
Acq: 10 Dec 2021 5:03

Tgt Ion: 56 Resp: 943
Ion Ratio Lower Upper
56 100
55 28.1 56.6 85.0#


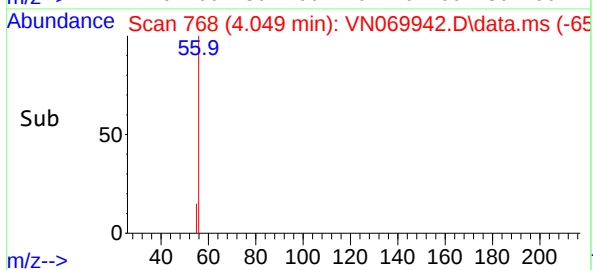
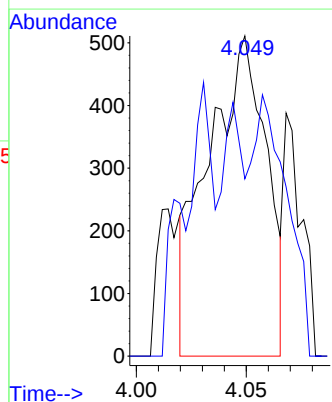
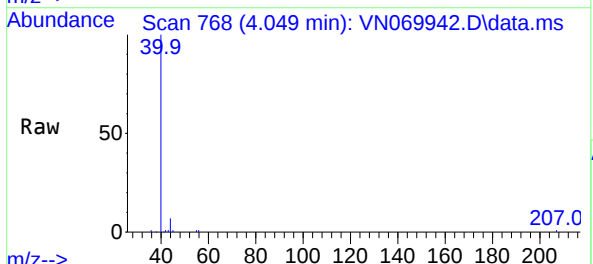




#16
Acetone
Concen: 7.286 ug/l
RT: 4.296 min Scan# 80
Delta R.T. 0.006 min
Lab File: VN069942.D
Acq: 10 Dec 2021 5:03




Instrument :
MSVOA_N
ClientSampleId :
PB141262ZHE#08


Tgt Ion: 43 Resp: 72900
Ion Ratio Lower Upper
43 100
58 26.6 23.1 34.7

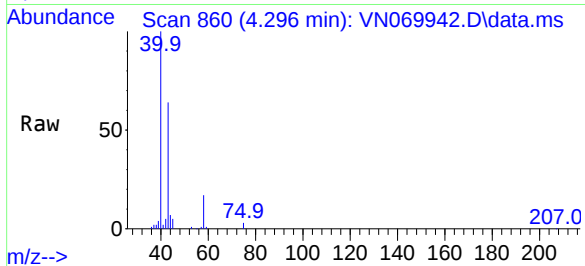

#18
Methyl Acetate
Concen: 1.875 ug/l
RT: 4.859 min Scan# 1070
Delta R.T. 0.003 min
Lab File: VN069942.D
Acq: 10 Dec 2021 5:03


Tgt Ion: 43 Resp: 56635
Ion Ratio Lower Upper
43 100
74 17.7 19.4 29.2#

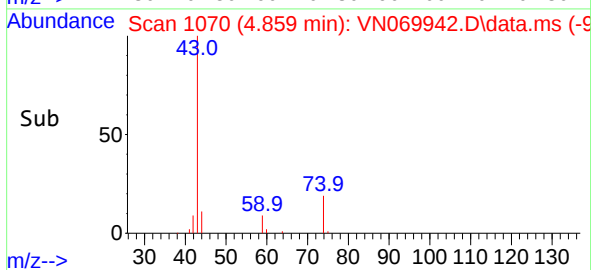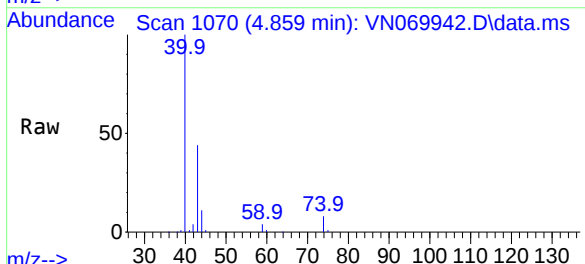



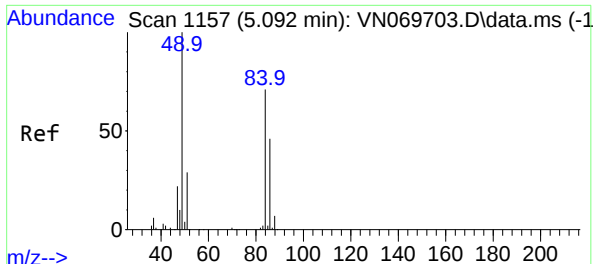


#20
Methylene Chloride
Concen: 3.034 ug/l
RT: 5.098 min Scan# 1157
Delta R.T. 0.006 min
Lab File: VN069942.D
Acq: 10 Dec 2021 5:03

Instrument :
MSVOA_N
ClientSampleId :
PB141262ZHE#08



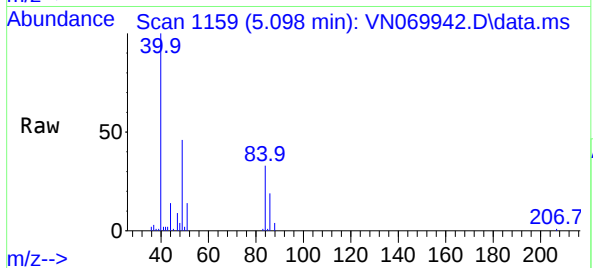



Tgt Ion:	84	Resp:	40354
Ion	Ratio	Lower	Upper
84	100		
49	138.1	93.5	140.3
51	42.3	29.4	44.2
86	57.2	53.0	79.4

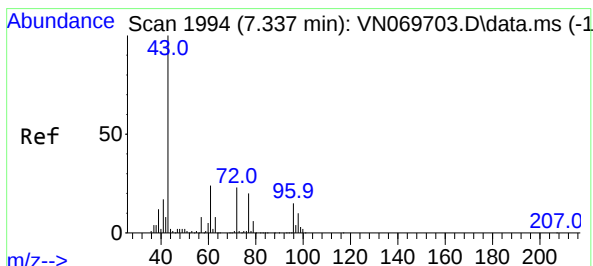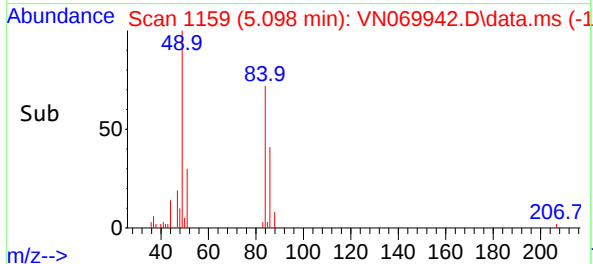

#25
2-Butanone
Concen: 1.228 ug/l
RT: 7.348 min Scan# 1998
Delta R.T. 0.011 min
Lab File: VN069942.D
Acq: 10 Dec 2021 5:03

Tgt Ion:	43	Resp:	16697
Ion	Ratio	Lower	Upper
43	100		
72	20.6	21.7	32.5

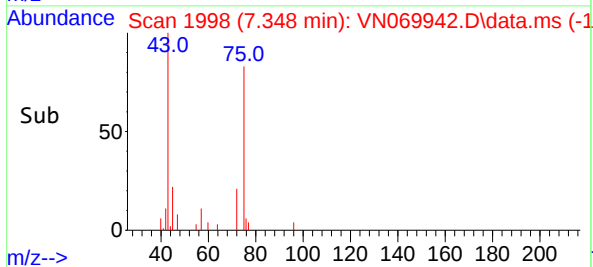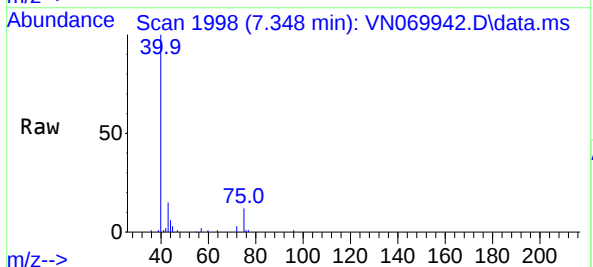



#29

Tetrahydrofuran

Concen: 0.263 ug/l

RT: 7.691 min Scan# 21

Delta R.T. 0.005 min

Lab File: VN069942.D

Acq: 10 Dec 2021 5:03

Instrument :

MSVOA_N

ClientSampleId :

PB141262ZHE#08





Tgt Ion: 42 Resp: 2175

Ion Ratio Lower Upper

42 100

72 0.0 36.3 54.5#

71 23.2 34.7 52.1#

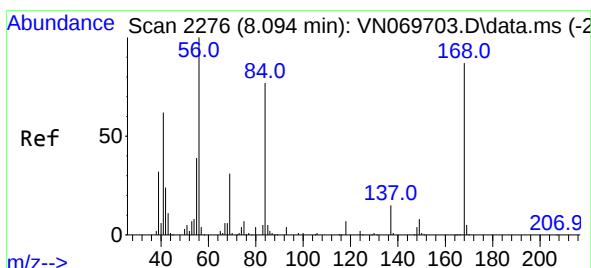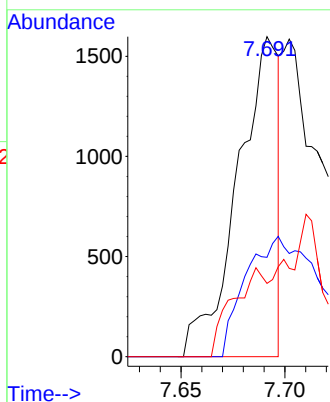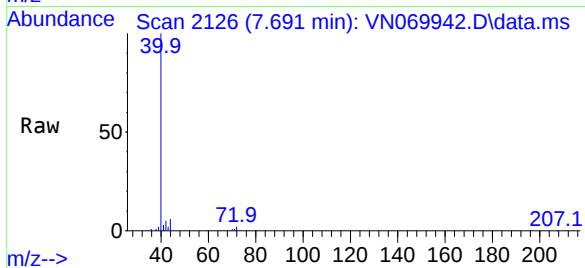

#31

Cyclohexane

Concen: 1.264 ug/l

RT: 8.086 min Scan# 2273

Delta R.T. -0.008 min

Lab File: VN069942.D

Acq: 10 Dec 2021 5:03




Tgt Ion: 56 Resp: 29260


Ion Ratio Lower Upper

56 100

69 156.0 27.1 40.7#

84 110.2 73.4 110.0#

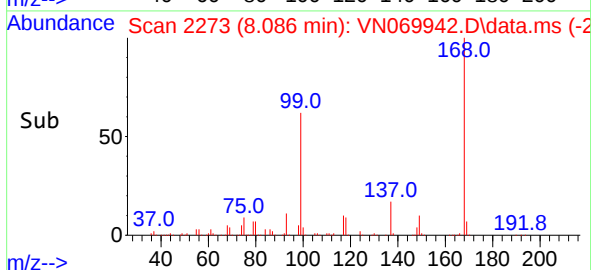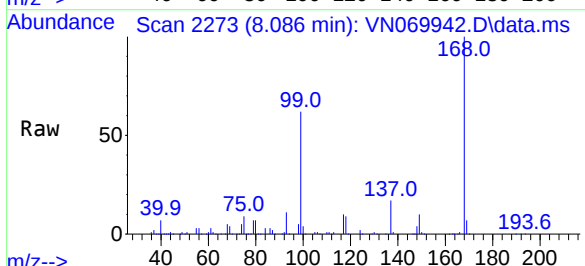



#33

1,2-Dichloroethane-d4

Concen: 52.889 ug/l

RT: 8.440 min Scan# 24

Delta R.T. 0.003 min

Lab File: VN069942.D

Acq: 10 Dec 2021 5:03

Instrument :

MSVOA_N

ClientSampleId :





PB141262ZHE#08

Tgt Ion: 65 Resp: 879651

Ion Ratio Lower Upper

65 100

67 50.4 0.0 103.0

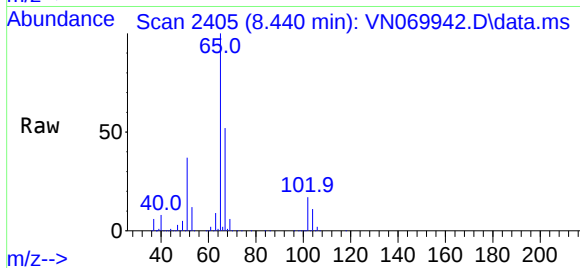

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.968 min Scan# 2602

Delta R.T. 0.000 min

Lab File: VN069942.D

Acq: 10 Dec 2021 5:03




Tgt Ion: 114 Resp: 2104972


Ion Ratio Lower Upper

114 100

63 23.6 0.0 37.8

88 16.2 0.0 27.4


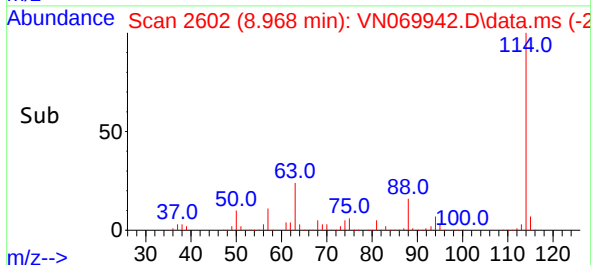
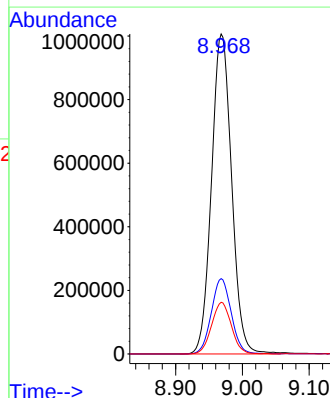
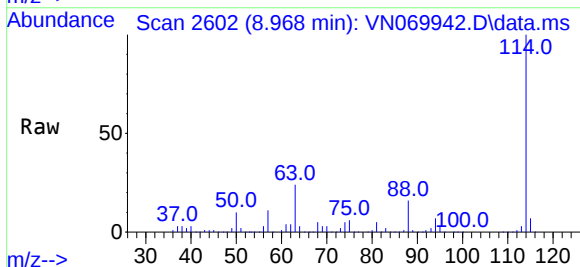


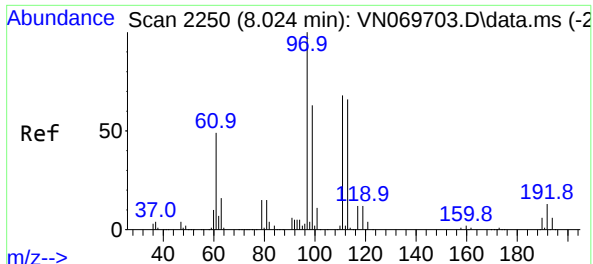

#35
Dibromofluoromethane
Concen: 48.798 ug/l
RT: 8.024 min Scan# 211
Delta R.T. 0.000 min
Lab File: VN069942.D
Acq: 10 Dec 2021 5:03




Instrument :
MSVOA_N
ClientSampleId :
PB141262ZHE#08


Tgt Ion:113 Resp: 643407
Ion Ratio Lower Upper
113 100
111 103.3 82.2 123.2
192 18.5 16.9 25.3

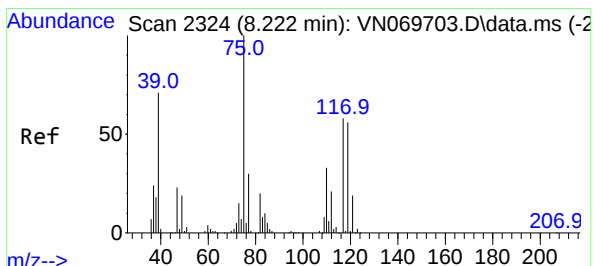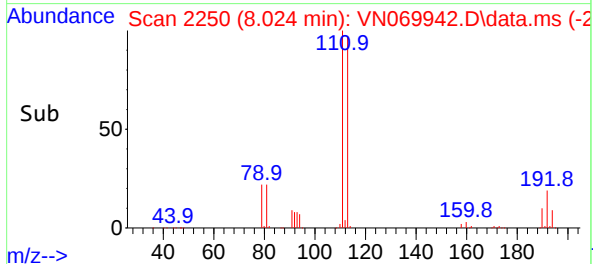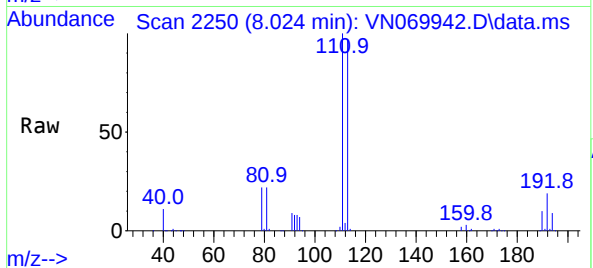

#36
1,1-Dichloropropene
Concen: 4.639 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.134 min
Lab File: VN069942.D
Acq: 10 Dec 2021 5:03

Tgt Ion: 75 Resp: 92962
Ion Ratio Lower Upper
75 100
110 9.1 18.4 55.2#
77 0.1 24.4 36.6#


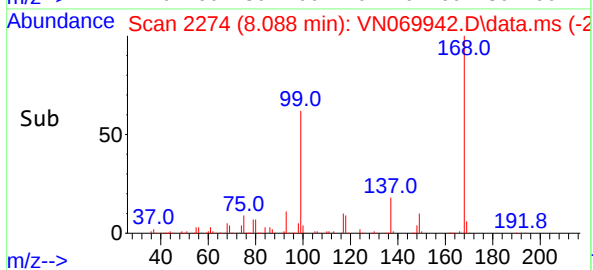

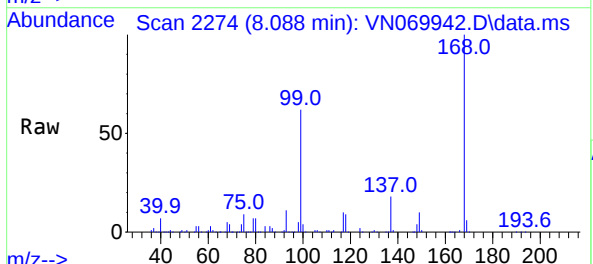




#38
Carbon Tetrachloride
Concen: 5.682 ug/l
RT: 8.091 min Scan# 211
Delta R.T. -0.115 min
Lab File: VN069942.D
Acq: 10 Dec 2021 5:03




Instrument :
MSVOA_N
ClientSampleId :
PB141262ZHE#08


Tgt Ion:117 Resp: 111655
Ion Ratio Lower Upper
117 100
119 4.4 76.1 114.1#
121 0.0 24.2 36.2#

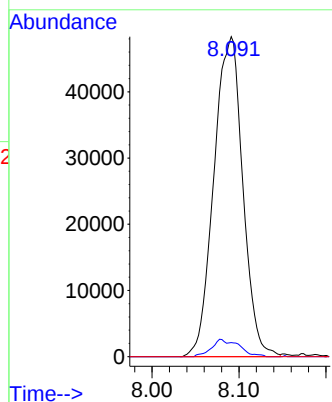

#43
Isopropyl Acetate
Concen: 4.155 ug/l
RT: 8.566 min Scan# 2452
Delta R.T. 0.003 min
Lab File: VN069942.D
Acq: 10 Dec 2021 5:03

Tgt Ion: 43 Resp: 183366
Ion Ratio Lower Upper
43 100
61 12.2 20.4 30.6#
87 7.8 11.2 16.8#


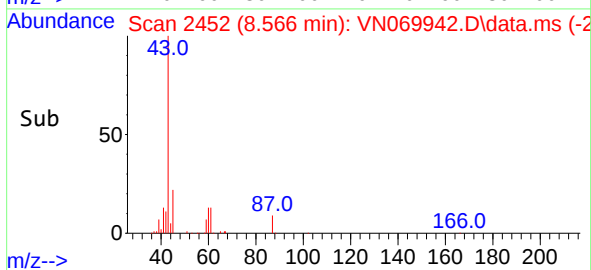




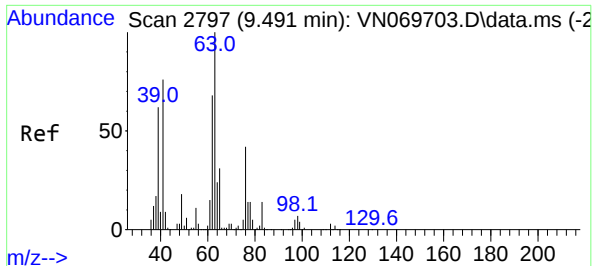

#45
1,2-Dichloropropane
Concen: 0.506 ug/l
RT: 9.622 min Scan# 21
Delta R.T. 0.132 min
Lab File: VN069942.D
Acq: 10 Dec 2021 5:03




Instrument :
MSVOA_N
ClientSampleId :
PB141262ZHE#08


Tgt Ion: 63 Resp: 8324
Ion Ratio Lower Upper
63 100
65 0.0 24.7 37.1#

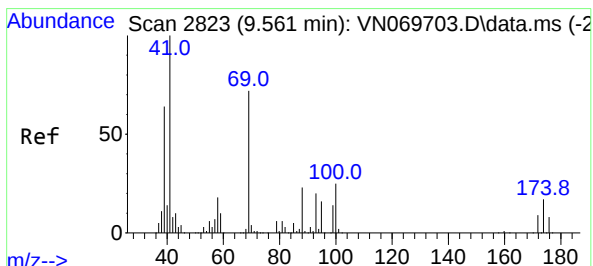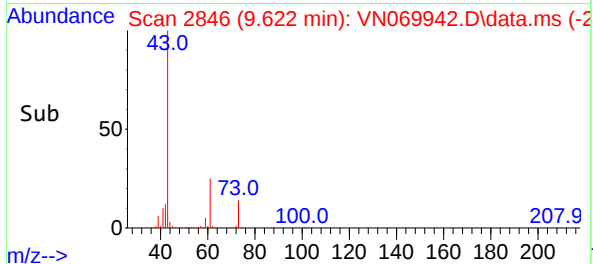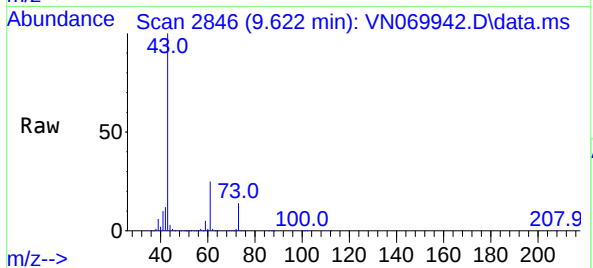

#48
Methyl methacrylate
Concen: 1.531 ug/l
RT: 9.545 min Scan# 2817
Delta R.T. -0.016 min
Lab File: VN069942.D
Acq: 10 Dec 2021 5:03

Tgt Ion: 41 Resp: 31527
Ion Ratio Lower Upper
41 100
69 0.0 72.4 108.6#
39 0.0 58.4 87.6#


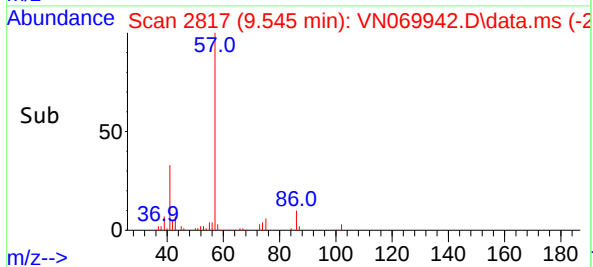

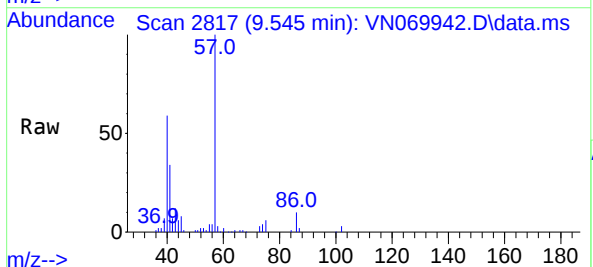


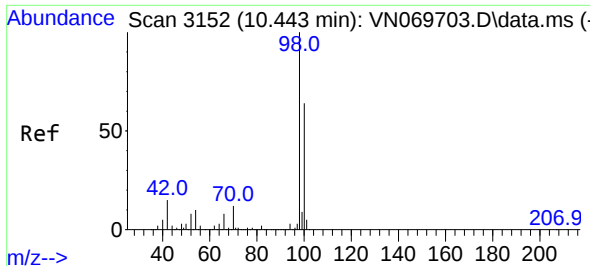

#50
Toluene-d8
Concen: 53.234 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. 0.000 min
Lab File: VN069942.D
Acq: 10 Dec 2021 5:03




Instrument :
MSVOA_N
ClientSampleId :
PB141262ZHE#08


Tgt Ion: 98 Resp: 2818349
Ion Ratio Lower Upper
98 100
100 63.6 50.4 75.6

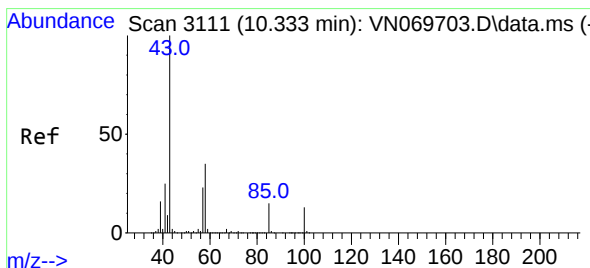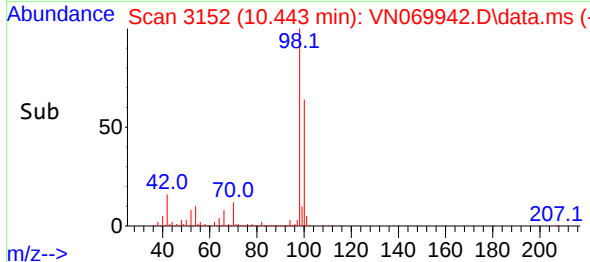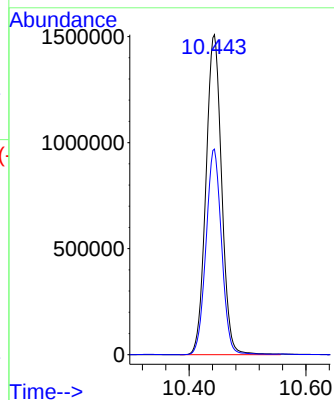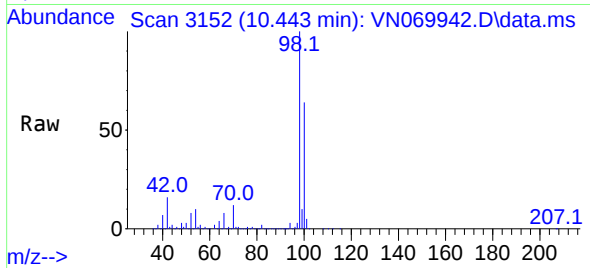

#51
4-Methyl-2-Pentanone
Concen: 0.627 ug/l
RT: 10.333 min Scan# 3111
Delta R.T. 0.000 min
Lab File: VN069942.D
Acq: 10 Dec 2021 5:03

Tgt Ion: 43 Resp: 17951
Ion Ratio Lower Upper
43 100
58 41.3 30.4 45.6


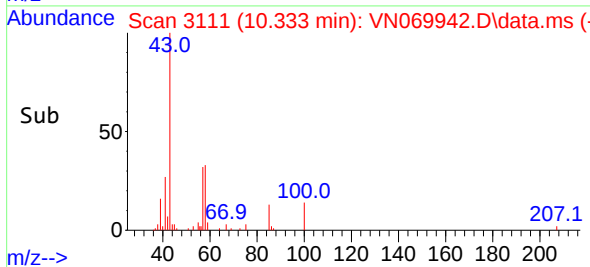
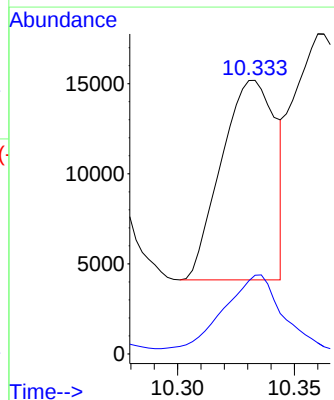
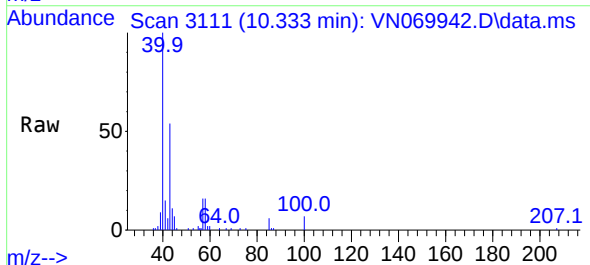




#53
t-1,3-Dichloropropene
Concen: 2.796 ug/l
RT: 10.717 min Scan# 31
Delta R.T. -0.002 min
Lab File: VN069942.D
Acq: 10 Dec 2021 5:03




Instrument :
MSVOA_N
ClientSampleId :
PB141262ZHE#08


Tgt Ion: 75 Resp: 52
Ion Ratio Lower Upper
75 100
77 0.0 25.6 38.4#

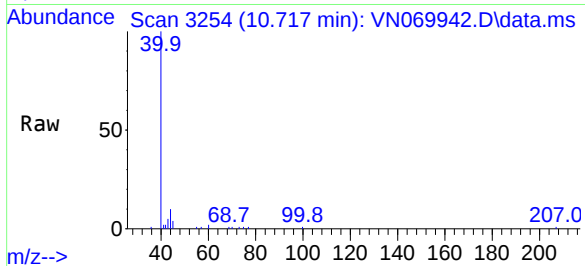

#54
cis-1,3-Dichloropropene
Concen: 8.385 ug/l
RT: 10.242 min Scan# 3077
Delta R.T. 0.051 min
Lab File: VN069942.D
Acq: 10 Dec 2021 5:03

Tgt Ion: 75 Resp: 171518
Ion Ratio Lower Upper
75 100
77 0.5 26.4 39.6#
39 46.0 42.5 63.7


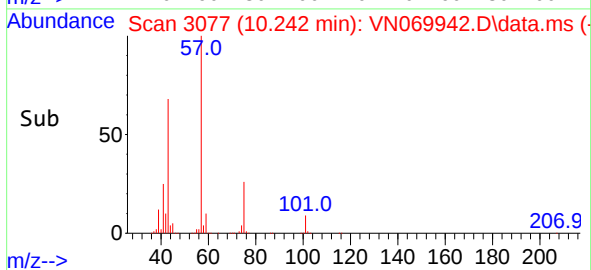

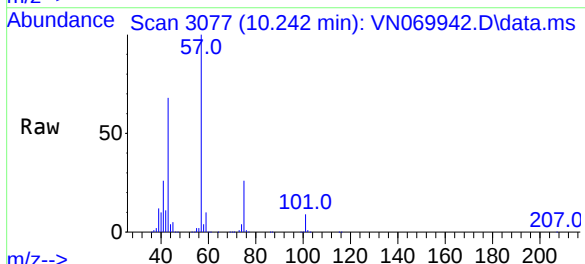




#56
Ethyl methacrylate
Concen: 2.298 ug/l
RT: 10.703 min Scan# 31
Delta R.T. -0.059 min
Lab File: VN069942.D
Acq: 10 Dec 2021 5:03




Instrument :
MSVOA_N
ClientSampleId :
PB141262ZHE#08


Tgt Ion: 69 Resp: 571
Ion Ratio Lower Upper
69 100
41 0.0 51.4 77.0#
39 0.0 34.6 52.0#



#57
1,3-Dichloropropane
Concen: 3.944 ug/l
RT: 11.089 min Scan# 3393
Delta R.T. 0.043 min
Lab File: VN069942.D
Acq: 10 Dec 2021 5:03

Tgt Ion: 76 Resp: 104788
Ion Ratio Lower Upper
76 100
78 0.3 25.7 38.5#


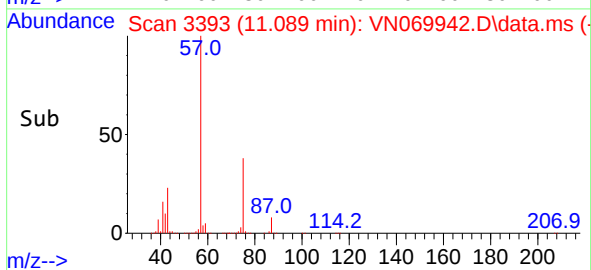






#59
2-Hexanone
Concen: 88.319 ug/l
RT: 11.089 min Scan# 31
Delta R.T. 0.002 min
Lab File: VN069942.D
Acq: 10 Dec 2021 5:03




Instrument :
MSVOA_N
ClientSampleId :
PB141262ZHE#08


Tgt Ion: 43 Resp: 1912933
Ion Ratio Lower Upper
43 100
58 16.3 26.9 80.7#

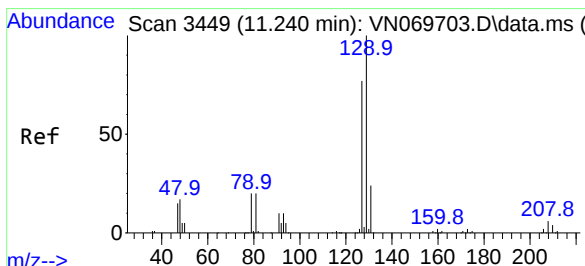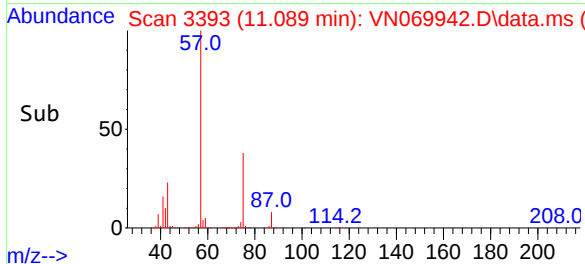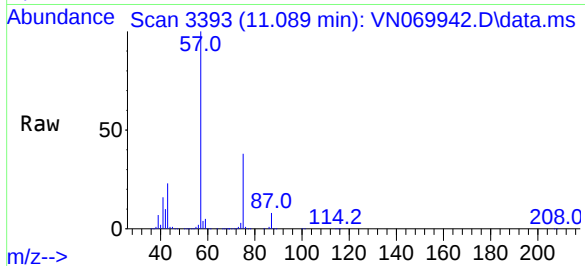

#60
Dibromochloromethane
Concen: 2.439 ug/l
RT: 11.489 min Scan# 3542
Delta R.T. 0.249 min
Lab File: VN069942.D
Acq: 10 Dec 2021 5:03

Tgt Ion:129 Resp: 1064
Ion Ratio Lower Upper
129 100
127 0.0 38.6 116.0#


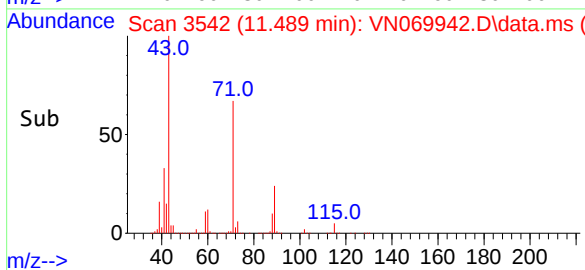

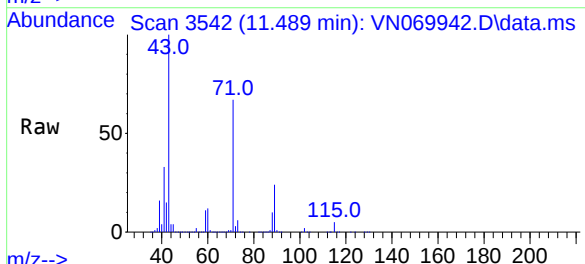




#62
4-Bromofluorobenzene
Concen: 59.677 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. -0.000 min
Lab File: VN069942.D
Acq: 10 Dec 2021 5:03




Instrument :
MSVOA_N
ClientSampleId :
PB141262ZHE#08


Tgt Ion: 95 Resp: 1144607
Ion Ratio Lower Upper
95 100
174 76.4 0.0 187.2
176 73.3 0.0 181.4

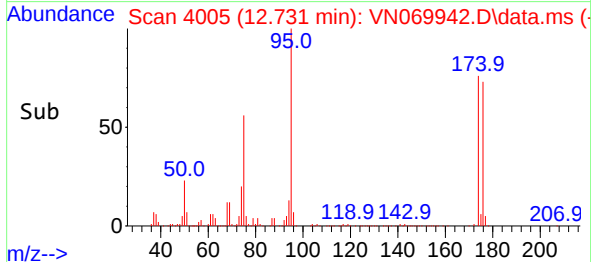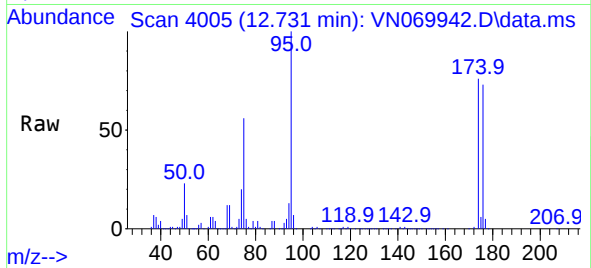

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.744 min Scan# 3637
Delta R.T. -0.002 min
Lab File: VN069942.D
Acq: 10 Dec 2021 5:03

Tgt Ion: 117 Resp: 2436224
Ion Ratio Lower Upper
117 100
82 58.2 42.4 63.6
119 32.0 25.4 38.2


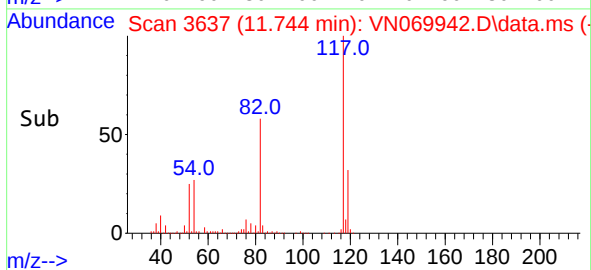




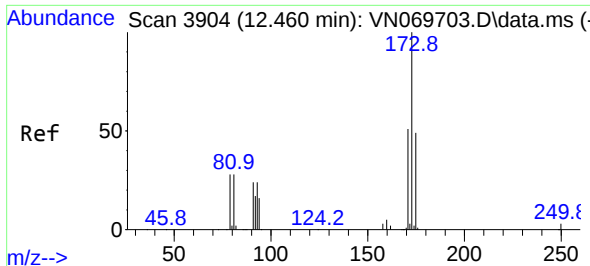

#71
Bromoform
Concen: 2.816 ug/l
RT: 12.715 min Scan# 3904
Delta R.T. 0.255 min
Lab File: VN069942.D
Acq: 10 Dec 2021 5:03




Instrument :
MSVOA_N
ClientSampleId :
PB141262ZHE#08


Tgt Ion:173 Resp: 1339
Ion Ratio Lower Upper
173 100
175 0.0 24.2 72.6#
254 0.0 0.0 0.0

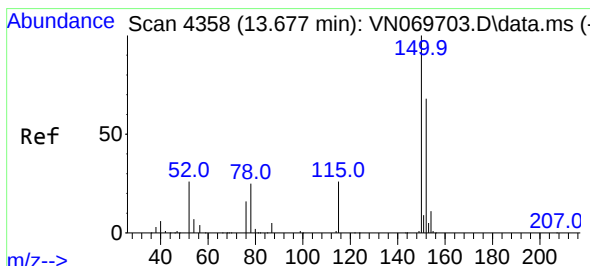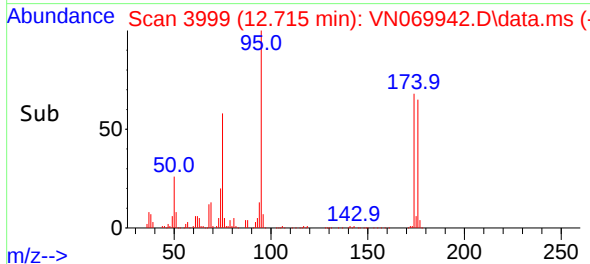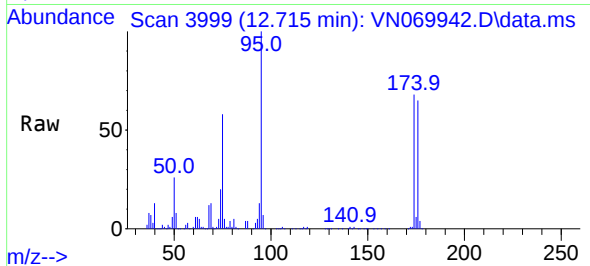

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.675 min Scan# 4357
Delta R.T. -0.003 min
Lab File: VN069942.D
Acq: 10 Dec 2021 5:03

Tgt Ion:152 Resp: 973537
Ion Ratio Lower Upper
152 100
115 60.4 27.5 82.5
150 156.2 0.0 344.4


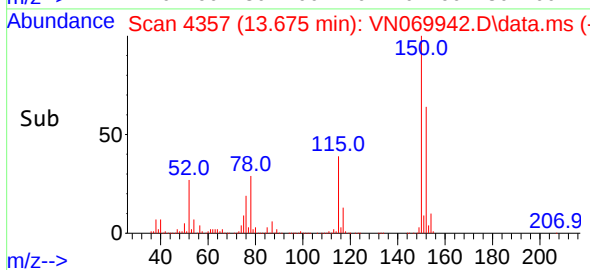

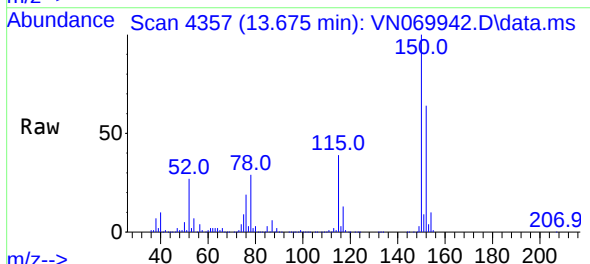




#74
N-amy1 acetate
Concen: 1.944 ug/l
RT: 12.197 min Scan# 31
Delta R.T. -0.190 min
Lab File: VN069942.D
Acq: 10 Dec 2021 5:03




Instrument :
MSVOA_N
ClientSampleId :
PB141262ZHE#08


Tgt Ion: 43	Resp: 74469
Ion Ratio	Lower Upper
43 100	
70 2.5	33.4 50.0#
55 4.9	19.3 28.9#
61 8.6	18.5 27.7#

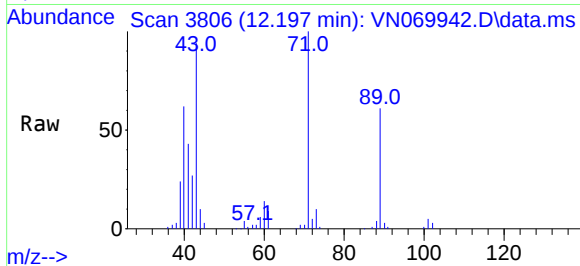

#76
1,2,3-Trichloropropane
Concen: 23.179 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. -0.150 min
Lab File: VN069942.D
Acq: 10 Dec 2021 5:03

Tgt Ion: 75	Resp: 647125
Ion Ratio	Lower Upper
75 100	
77 1.0	82.6 247.8#


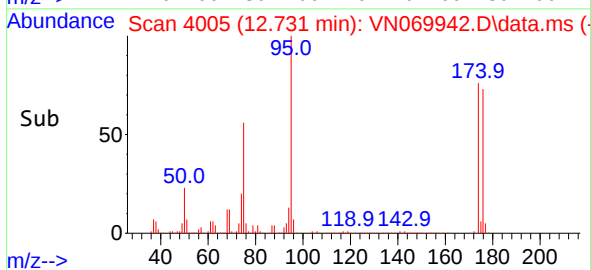

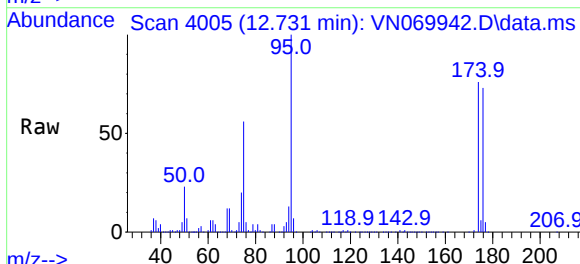




#80
1,3,5-Trimethylbenzene
Concen: 0.258 ug/l
RT: 13.061 min Scan# 4128
Delta R.T. 0.000 min
Lab File: VN069942.D
Acq: 10 Dec 2021 5:03




Instrument :
MSVOA_N
ClientSampleId :
PB141262ZHE#08


Tgt Ion:105 Resp: 17977
Ion Ratio Lower Upper
105 100
120 49.3 24.6 73.6

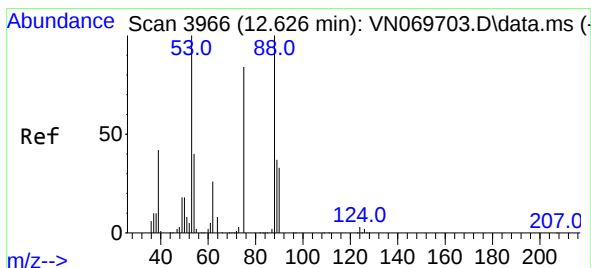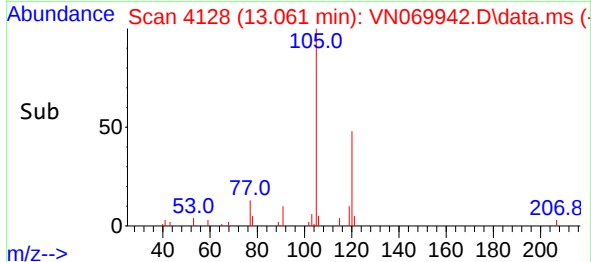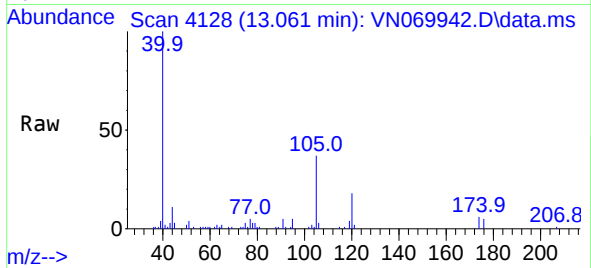

#81
trans-1,4-Dichloro-2-butene
Concen: 73.761 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. 0.105 min
Lab File: VN069942.D
Acq: 10 Dec 2021 5:03

Tgt Ion: 75 Resp: 647125
Ion Ratio Lower Upper
75 100
53 0.1 90.5 135.7#
89 0.0 38.2 57.4#


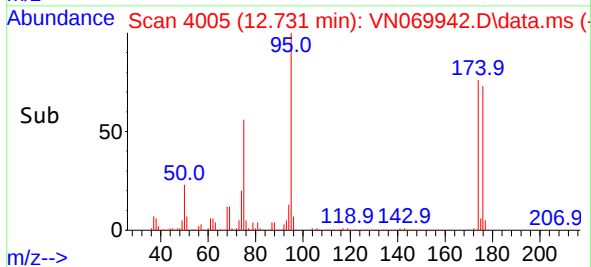

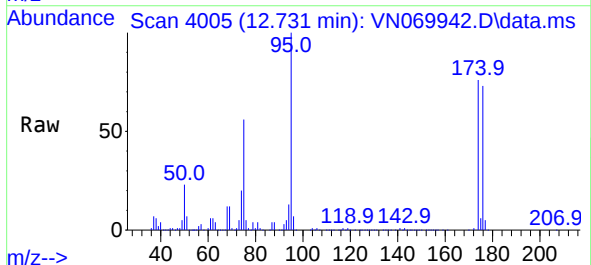




#93
1,2,4-Trichlorobenzene
Concen: 2.895 ug/l
RT: 15.271 min Scan# 49
Delta R.T. 0.006 min
Lab File: VN069942.D
Acq: 10 Dec 2021 5:03




Instrument :
MSVOA_N
ClientSampleId :
PB141262ZHE#08


Tgt Ion:180 Resp: 283
Ion Ratio Lower Upper
180 100
182 29.7 48.3 144.9#
145 0.0 14.5 43.5#

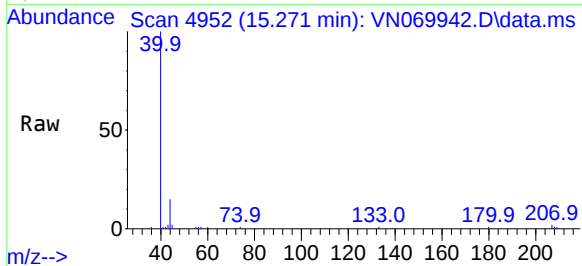

#95
Naphthalene
Concen: 4.016 ug/l
RT: 15.499 min Scan# 5037
Delta R.T. -0.008 min
Lab File: VN069942.D
Acq: 10 Dec 2021 5:03


Tgt Ion:128 Resp: 1581
Ion Ratio Lower Upper
128 100
127 19.9 10.5 15.7#
129 3.4 8.7 13.1#

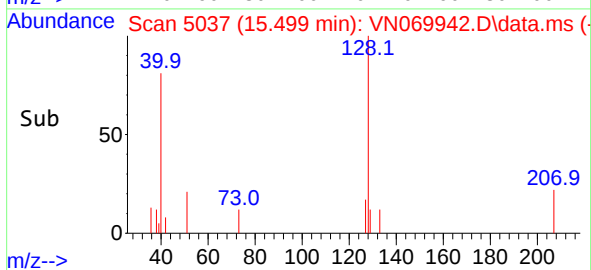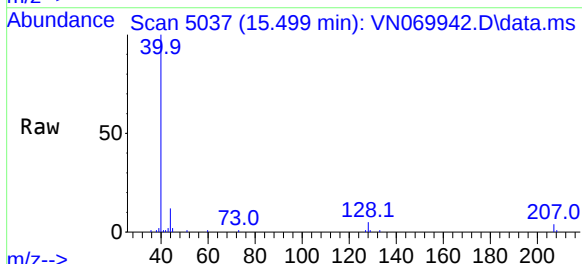



#96
 1,2,3-Trichlorobenzene
 Concen: 2.458 ug/l
 RT: 15.702 min Scan# 51
 Delta R.T. 0.000 min
 Lab File: VN069942.D
 Acq: 10 Dec 2021 5:03

Instrument :
 MSVOA_N
 ClientSampleId :
 PB141262ZHE#08

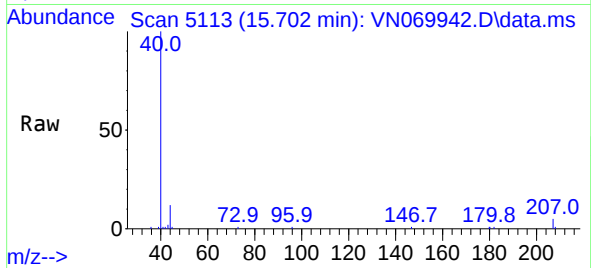

Tgt Ion	Ratio	Lower	Upper
180	100		
182	0.0	47.4	142.2#
145	0.0	15.0	45.1#

