
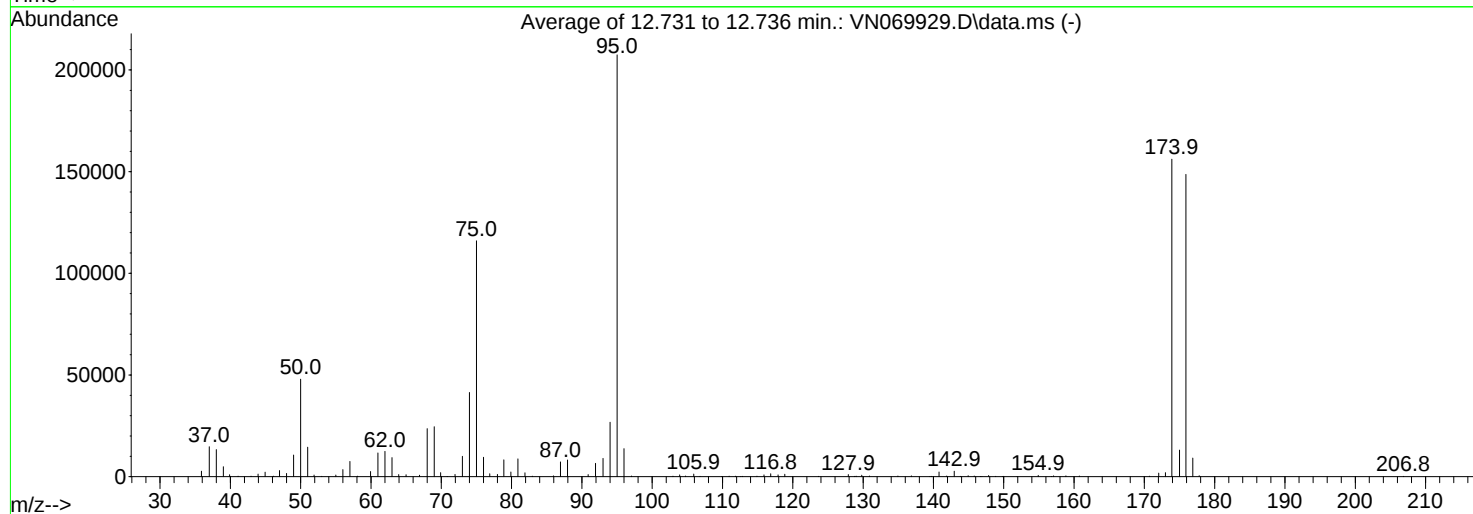


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120921\
Data File : VN069929.D
Acq On : 9 Dec 2021 23:08
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
Title : SW846 8260
Last Update : Fri Dec 03 08:46:47 2021

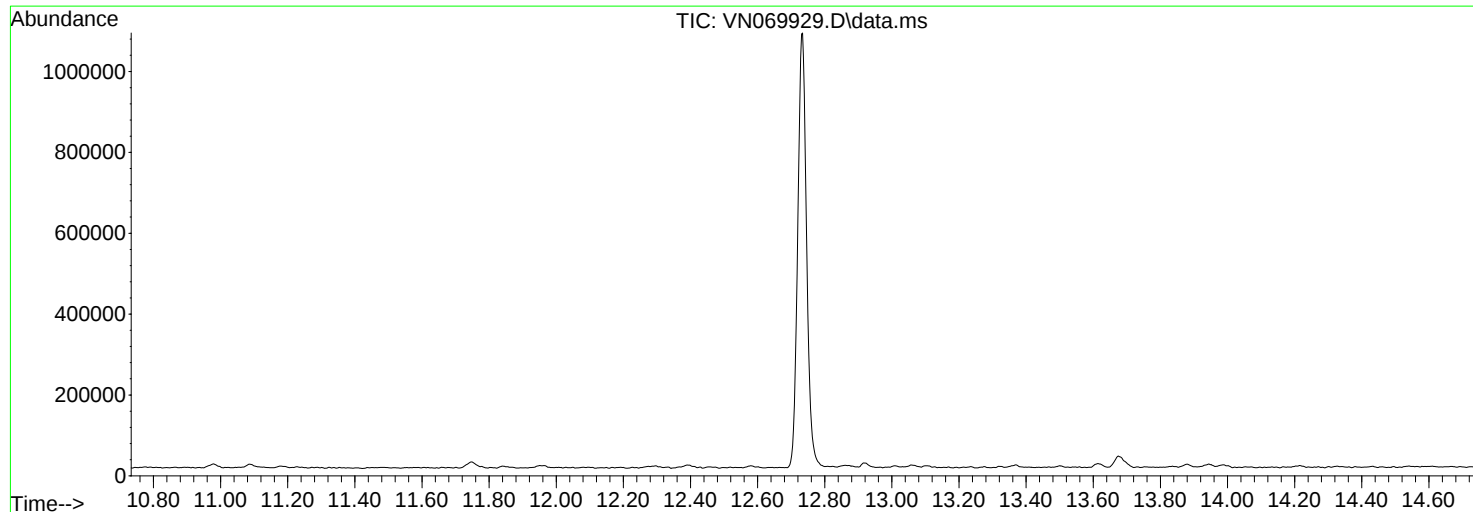

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3987

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.1	47957	PASS
75	95	30	60	55.9	115971	PASS
95	95	100	100	100.0	207445	PASS
96	95	5	9	6.6	13739	PASS
173	174	0.00	2	1.3	1960	PASS
174	95	50	100	75.3	156160	PASS
175	174	5	9	8.4	13106	PASS
176	174	95	101	95.2	148693	PASS
177	176	5	9	6.1	9113	PASS