
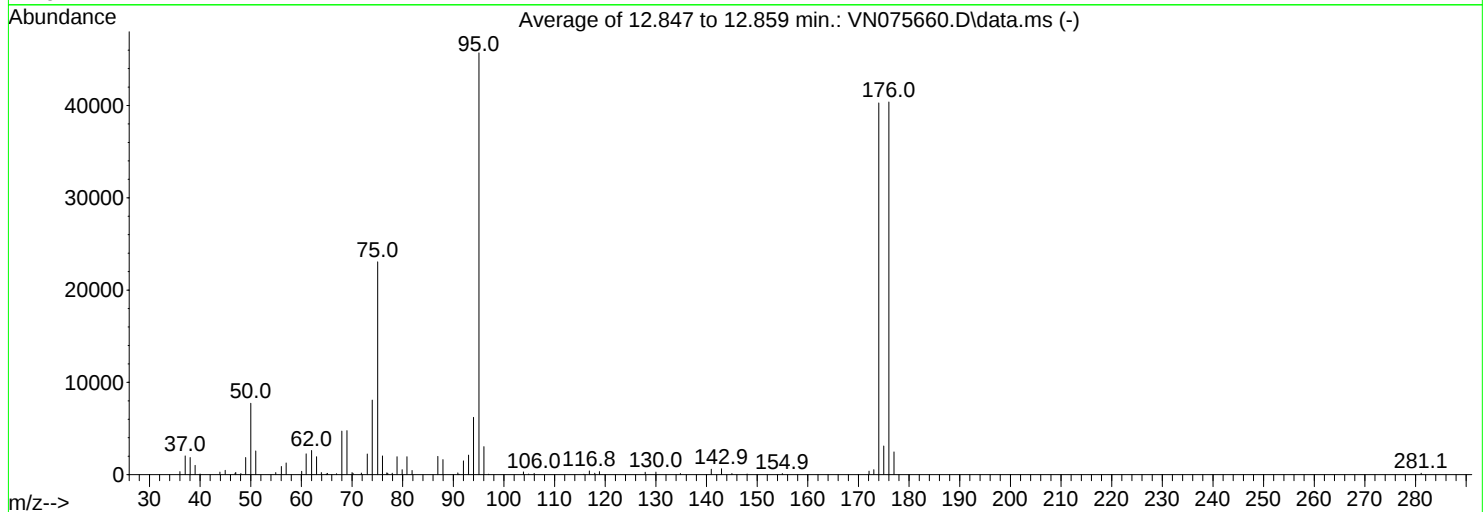


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120922\
Data File : VN075660.D
Acq On : 09 Dec 2022 09:06
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120922W.M
Title : SW846 8260
Last Update : Mon Dec 12 07:54:35 2022

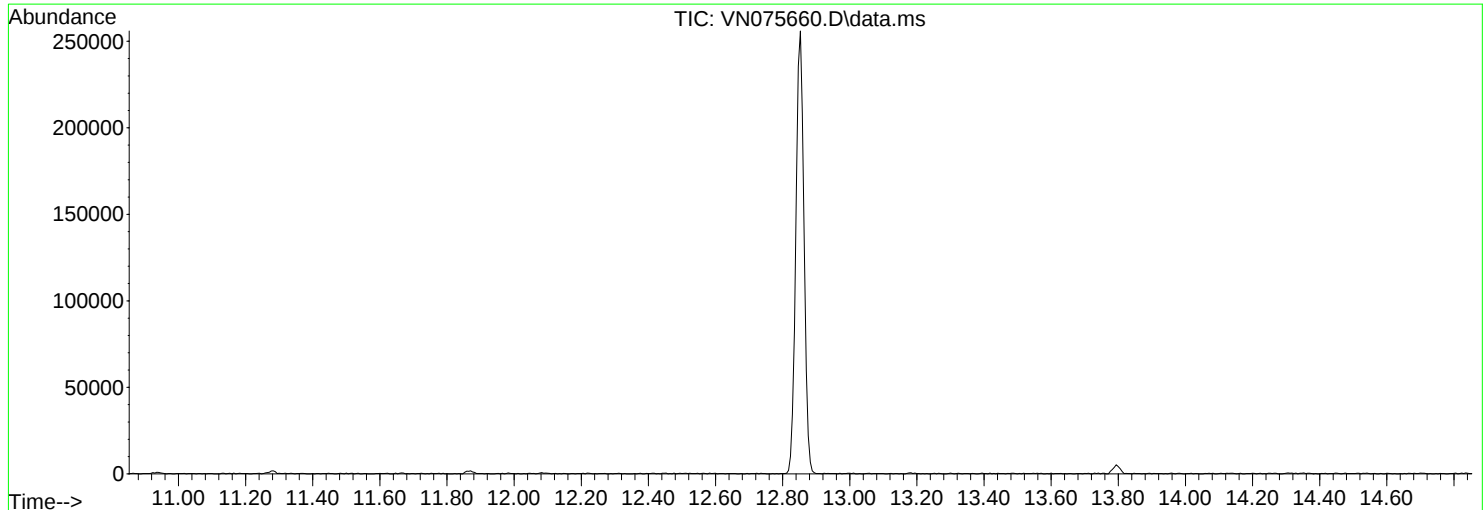

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	7734	PASS
75	95	30	60	50.5	23061	PASS
95	95	100	100	100.0	45707	PASS
96	95	5	9	6.6	3037	PASS
173	174	0.00	2	1.3	537	PASS
174	95	50	100	88.1	40285	PASS
175	174	5	9	7.7	3101	PASS
176	174	95	101	100.2	40381	PASS
177	176	5	9	6.1	2454	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	330	50.00	7734	65.00	73	76.00	203
37.05	2024	51.00	2566	65.15	147	76.85	188
38.05	1848	54.95	221	66.95	111	77.05	16
39.00	1001	56.05	879	68.00	4722	77.95	14
40.00	67	57.00	1264	69.00	4769	78.90	1945
43.90	272	60.05	370	70.00	228	79.90	539
44.95	468	60.95	2260	70.20	141	80.85	1948
46.90	158	62.00	2617	71.85	166	81.85	447
47.05	242	63.00	1940	73.00	2235	86.95	1980
48.05	120	63.95	234	74.00	8081	87.95	1636
49.00	1865	64.90	56	75.05	23061	90.90	188

Average of 12.847 to 12.859 min.: VN075660.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
91.10	50	116.85	403	172.10	377		
92.00	1500	117.95	151	173.05	537		
93.00	2120	118.85	331	174.00	40285		
94.00	6204	127.90	266	175.00	3101		
95.05	45707	130.00	280	176.00	40381		
96.05	3037	134.85	123	177.00	2454		
97.00	53	140.95	583	281.10	149		
103.85	296	142.95	649				
104.90	65	145.00	127				
105.95	143	148.00	65				
115.80	61	154.95	114				

Instrument :

MSVOA_N

ClientSampleId :

BFB