


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120922\
Data File : VN075679.D
Acq On : 09 Dec 2022 23:26
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120922W.M
Title : SW846 8260
Last Update : Mon Dec 12 07:54:35 2022

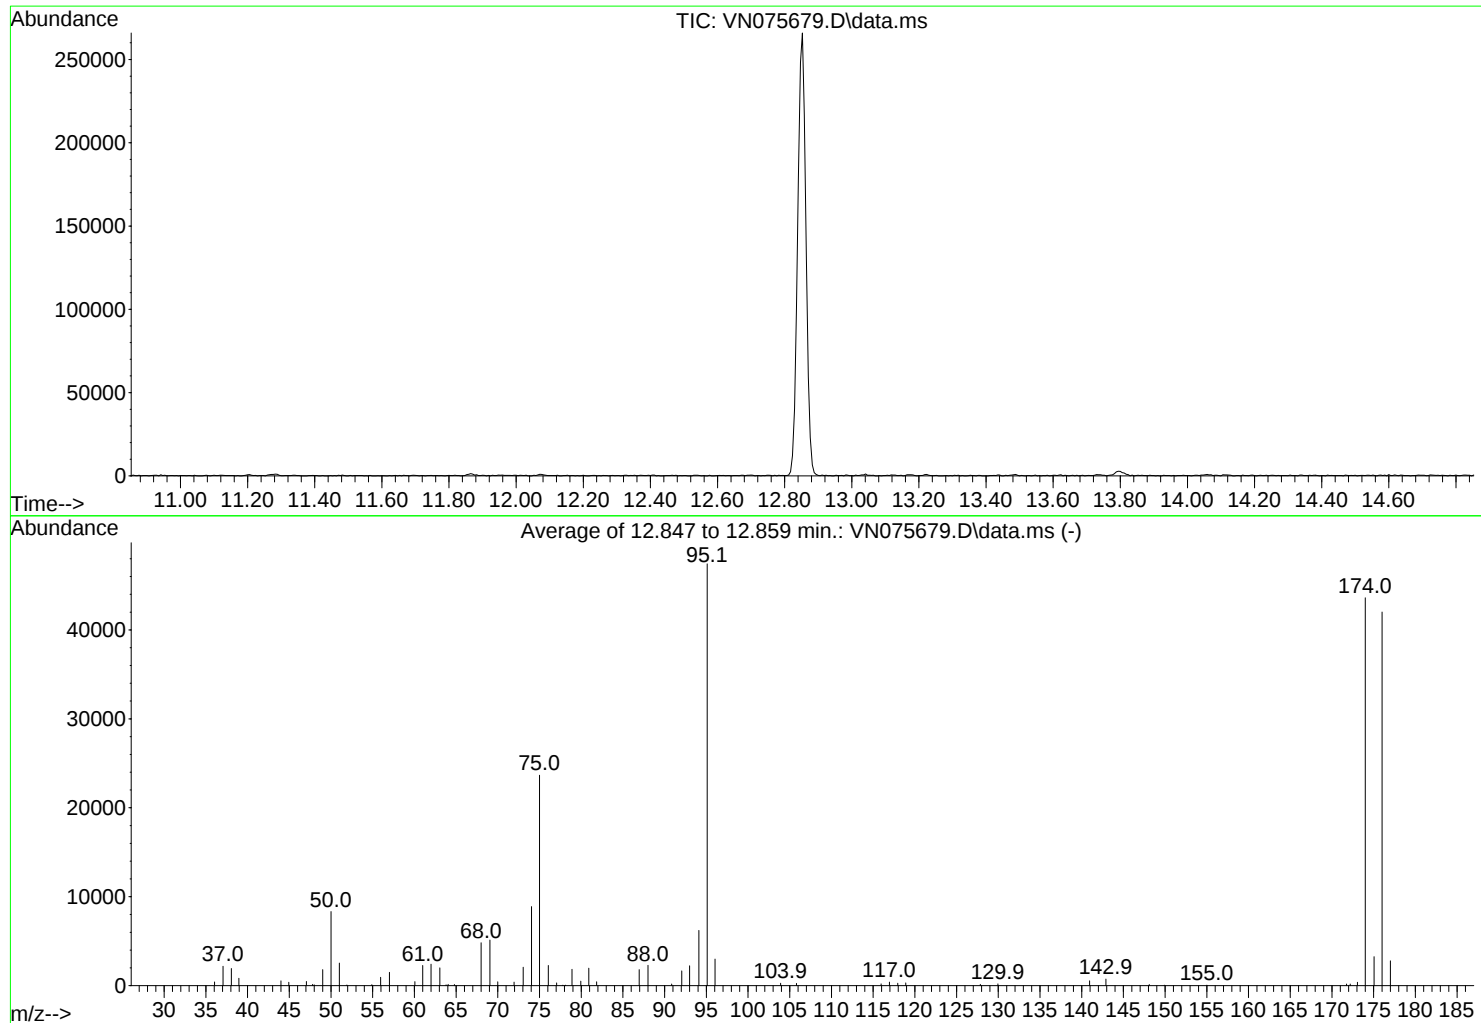

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	8333	PASS
75	95	30	60	49.9	23659	PASS
95	95	100	100	100.0	47429	PASS
96	95	5	9	6.3	2993	PASS
173	174	0.00	2	0.9	380	PASS
174	95	50	100	92.0	43616	PASS
175	174	5	9	7.5	3262	PASS
176	174	95	101	96.3	42008	PASS
177	176	5	9	6.7	2798	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	409	51.00	2531	64.80	125	78.10	51
37.05	2187	51.90	67	68.00	4816	78.90	184
38.05	1921	54.90	110	69.05	5135	79.95	50
38.95	830	55.95	929	70.00	436	80.90	196
44.00	534	57.00	1488	71.95	390	81.85	432
44.95	385	60.05	449	73.05	2076	86.95	1803
47.05	476	61.00	2267	74.05	8880	88.00	2281
47.80	144	62.00	2413	75.00	23659	90.85	189
48.00	98	63.05	2003	76.05	2261	92.05	1661
49.00	1794	63.80	85	77.05	305	93.00	2240
50.00	8333	64.05	149	77.80	59	94.10	6213

Average of 12.847 to 12.859 min.: VN075679.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
95.10	47429	142.90	736				
96.05	2993	148.10	118				
103.90	267	149.90	58				
105.80	256	155.00	61				
115.95	203	171.75	182				
116.95	390	172.20	183				
117.95	277	173.05	380				
118.90	303	174.00	43616				
127.85	146	175.05	3262				
129.95	192	176.00	42008				
140.95	546	177.00	2798				