
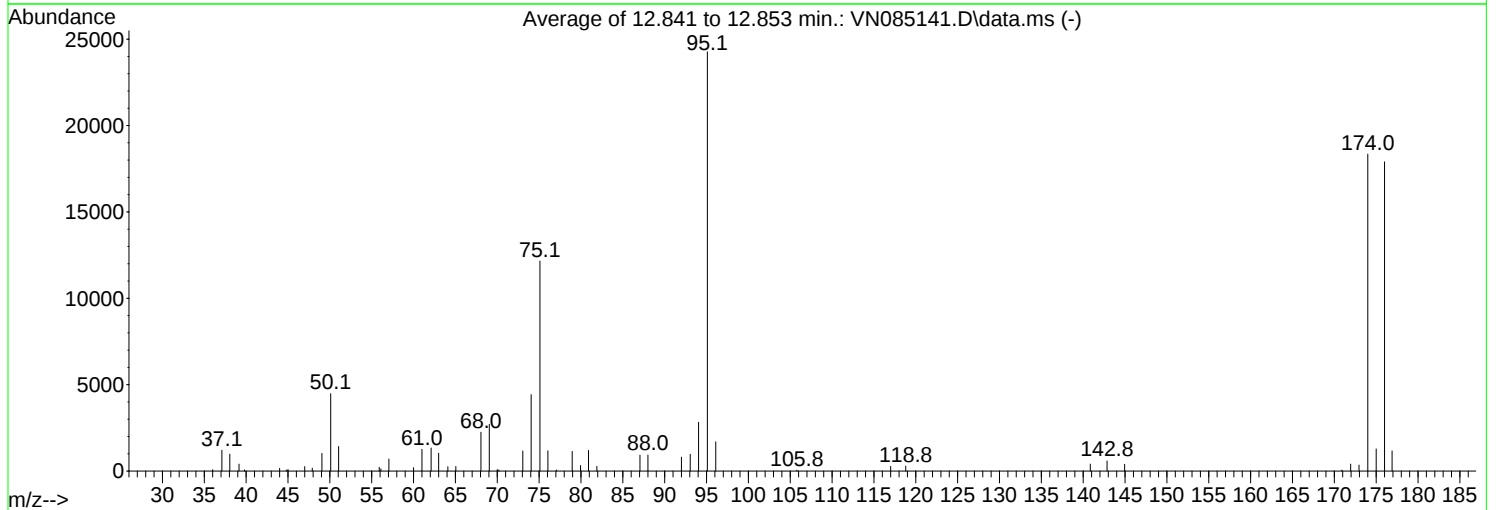


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120924\
Data File : VN085141.D
Acq On : 09 Dec 2024 09:58
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112224W.M
Title : SW846 8260
Last Update : Sat Nov 23 02:54:10 2024

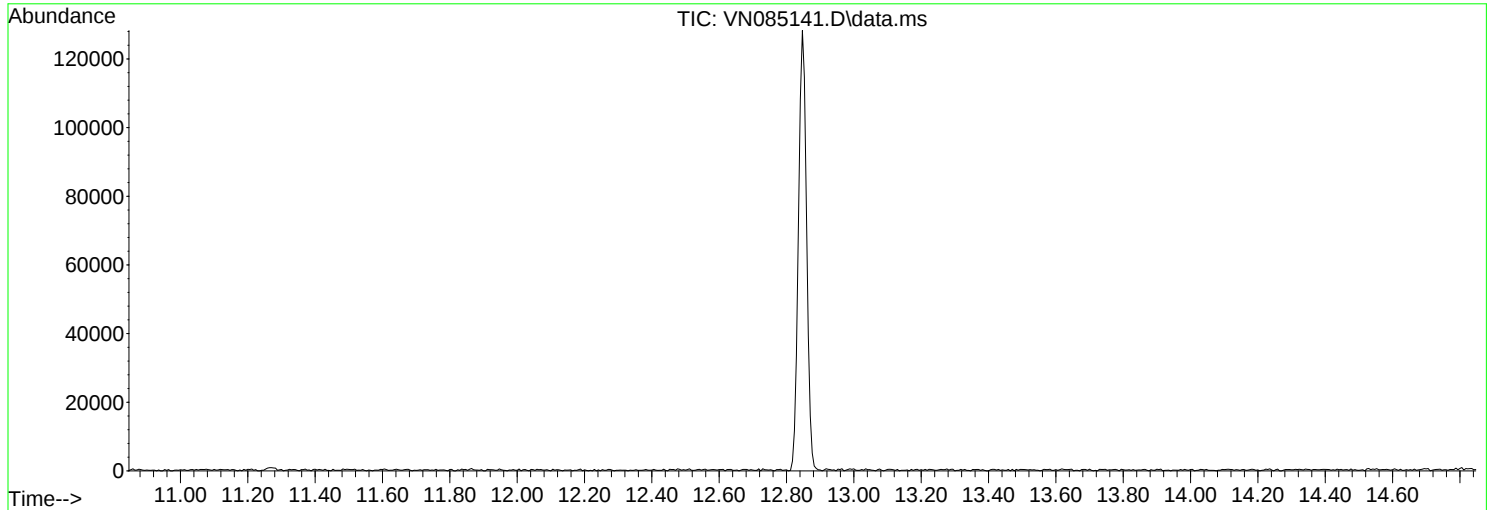

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	4480	PASS
75	95	30	60	50.1	12157	PASS
95	95	100	100	100.0	24272	PASS
96	95	5	9	7.0	1696	PASS
173	174	0.00	2	1.9	347	PASS
174	95	50	100	75.6	18349	PASS
175	174	5	9	7.0	1283	PASS
176	174	95	101	97.6	17900	PASS
177	176	5	9	6.5	1169	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	79	50.10	4480	68.05	2251	80.90	1193
37.10	1210	51.05	1422	69.05	2710	81.90	274
38.05	981	55.90	223	70.00	90	87.05	923
39.15	405	56.10	132	70.20	67	88.00	930
39.80	70	57.05	697	73.05	1163	92.00	809
44.00	159	60.00	197	74.05	4427	93.05	972
44.80	59	61.00	1260	75.10	12157	94.05	2827
45.00	94	62.10	1336	76.05	1175	95.10	24272
47.00	261	63.00	1033	77.10	61	96.10	1696
47.90	170	64.10	253	78.95	1138	105.80	56
49.05	1026	65.05	266	79.95	322	117.00	271

Average of 12.841 to 12.853 min.: VN085141.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
118.80	286						
140.85	407						
142.85	585						
144.95	392						
170.90	59						
171.95	404						
172.95	347						
174.00	18349						
175.00	1283						
176.00	17900						
176.90	1169						

Instrument :

MSVOA_N

ClientSampleId :

BFB