


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN121018\
 Data File : VN052740.D
 Acq On : 10 Dec 2018 8:40
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112718W.M
 Title : SW846 8260
 Last Update : Mon Dec 03 03:24:02 2018

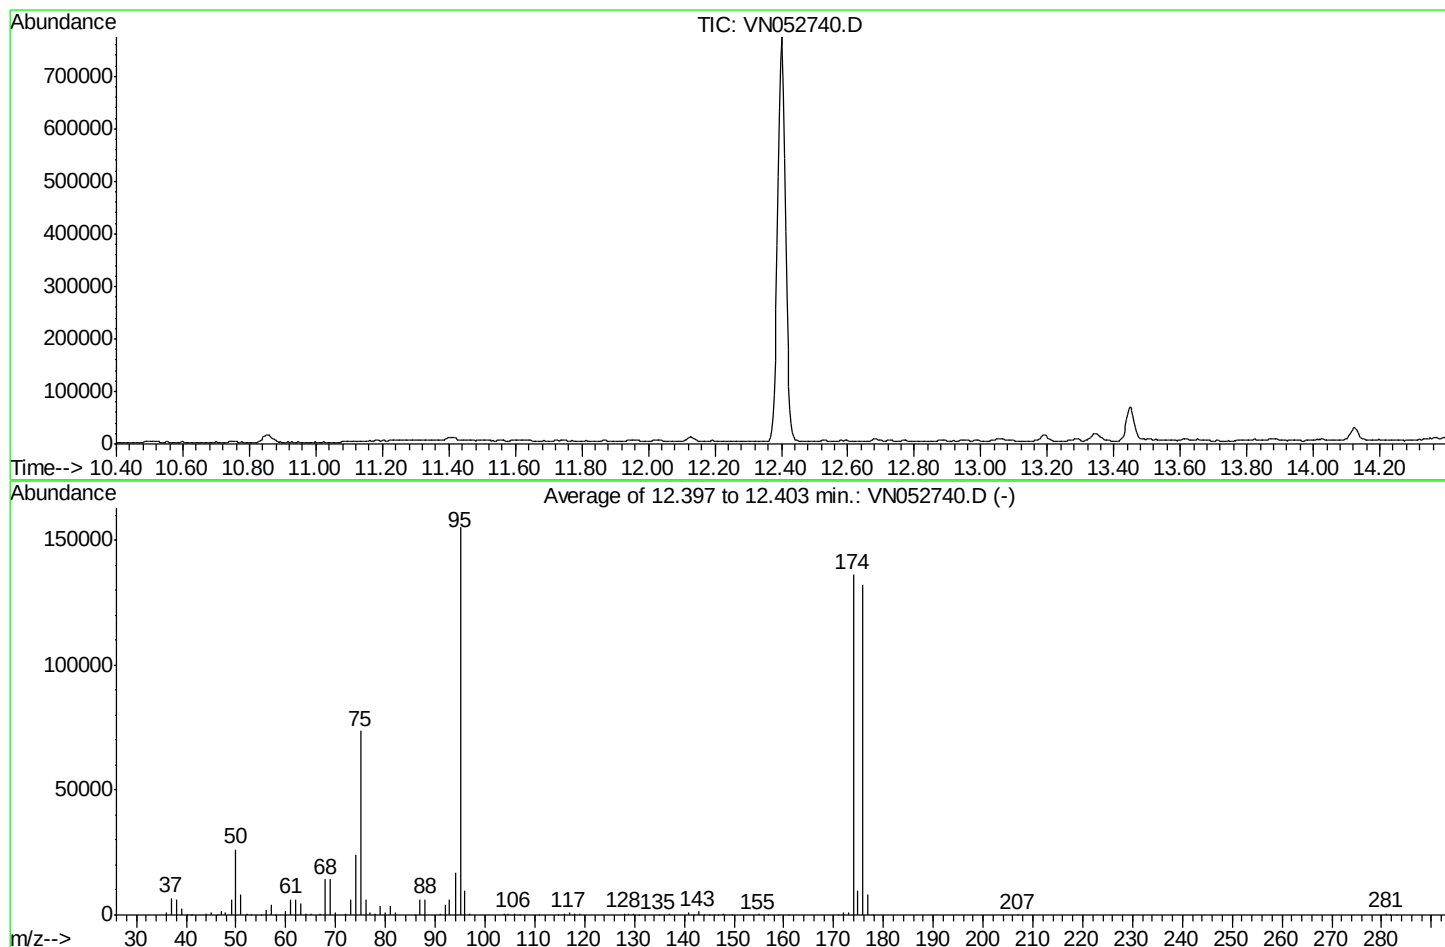

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3289

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	26272	PASS
75	95	30	60	47.5	73720	PASS
95	95	100	100	100.0	155050	PASS
96	95	5	9	6.1	9517	PASS
173	174	0.00	2	0.9	1231	PASS
174	95	50	100	87.8	136181	PASS
175	174	5	9	7.2	9755	PASS
176	174	95	101	96.9	132013	PASS
177	176	5	9	6.4	8401	PASS