


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN121018\
Data File : VN052766.D
Acq On : 10 Dec 2018 21:24
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 28 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112718W.M
Title : SW846 8260
Last Update : Mon Dec 03 03:24:02 2018

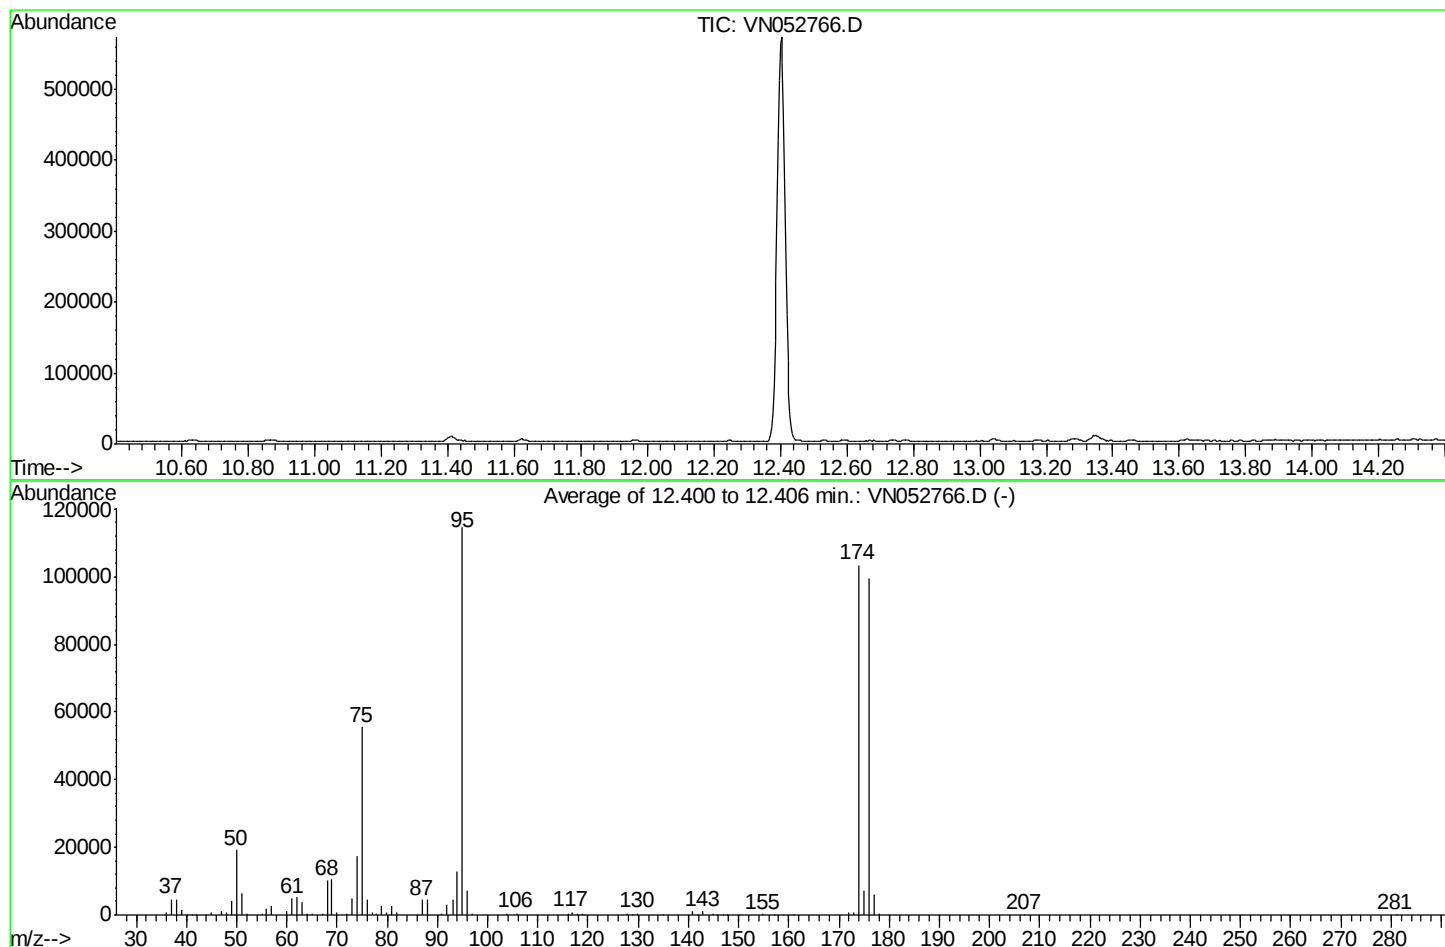

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	19141	PASS
75	95	30	60	48.4	55474	PASS
95	95	100	100	100.0	114600	PASS
96	95	5	9	6.4	7390	PASS
173	174	0.00	2	0.8	858	PASS
174	95	50	100	90.2	103381	PASS
175	174	5	9	7.0	7248	PASS
176	174	95	101	96.3	99568	PASS
177	176	5	9	6.2	6168	PASS