


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN121019\
 Data File : VN059536.D
 Acq On : 10 Dec 2019 10:06
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N120919W.M
 Title : SW846 8260
 Last Update : Tue Dec 10 01:09:52 2019

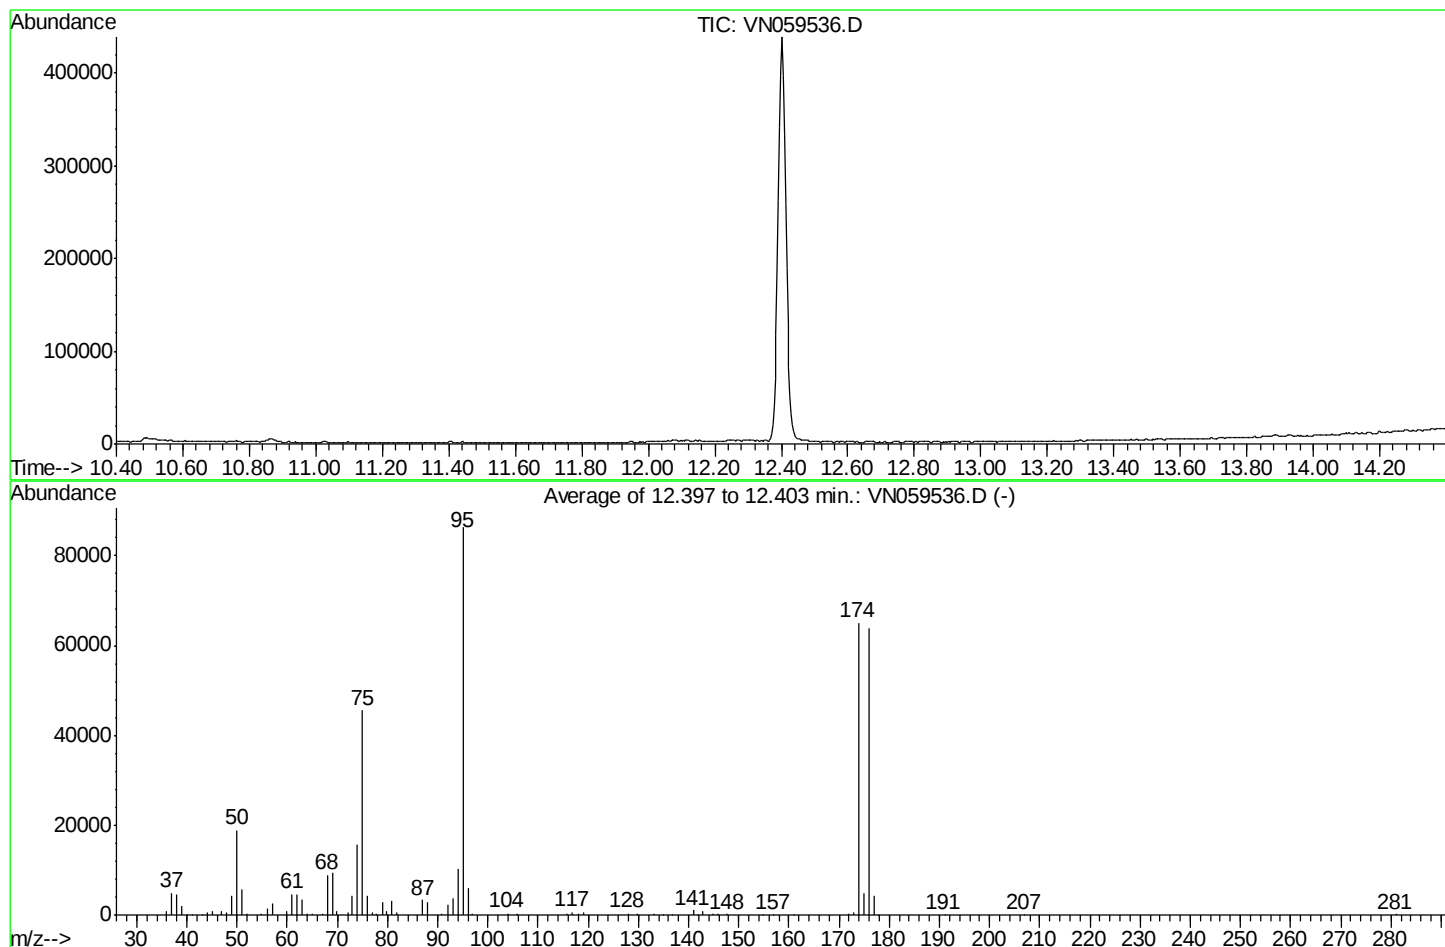

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	18858	PASS
75	95	30	60	52.8	45557	PASS
95	95	100	100	100.0	86312	PASS
96	95	5	9	7.1	6106	PASS
173	174	0.00	2	0.9	584	PASS
174	95	50	100	75.4	65064	PASS
175	174	5	9	7.3	4749	PASS
176	174	95	101	98.1	63826	PASS
177	176	5	9	6.6	4214	PASS