



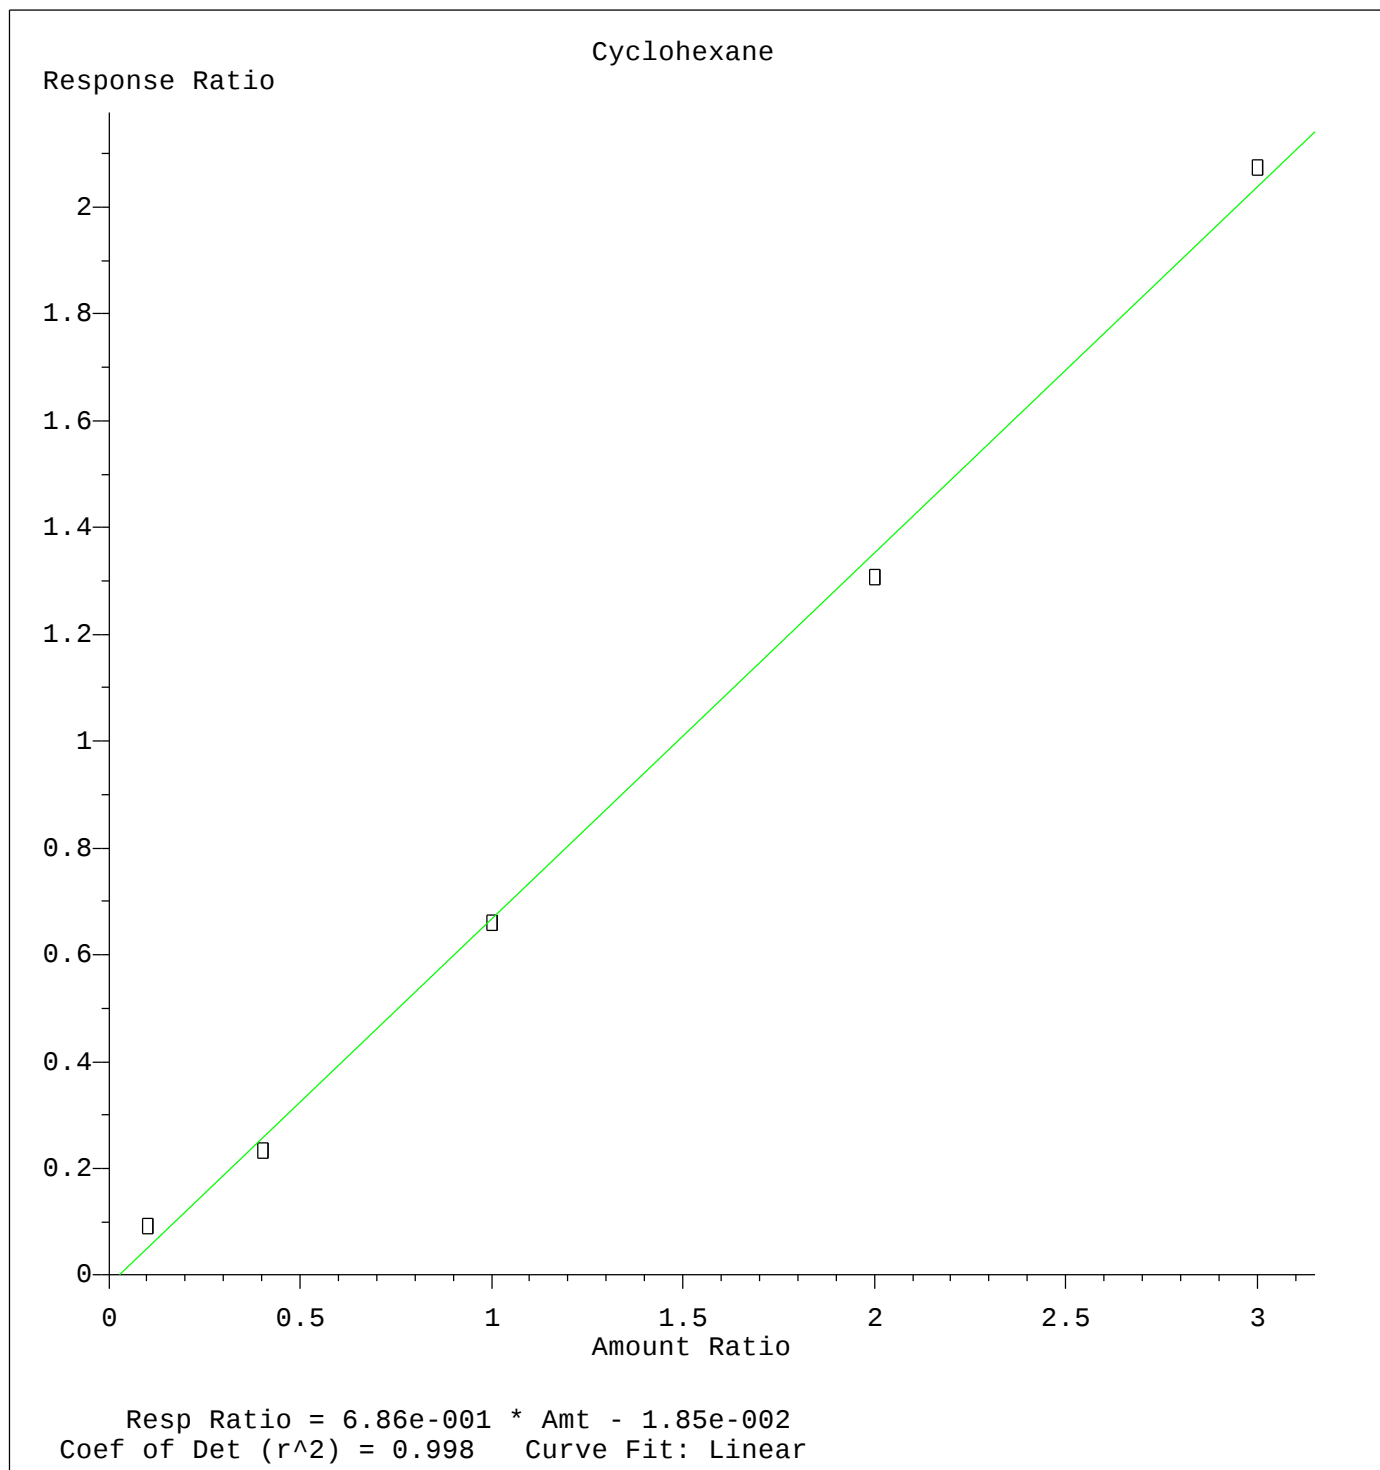

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121020W.M
Calibration Table Last Updated: Fri Dec 11 07:09:49 2020


1,2,4-Trichlorobenzene

Response Ratio

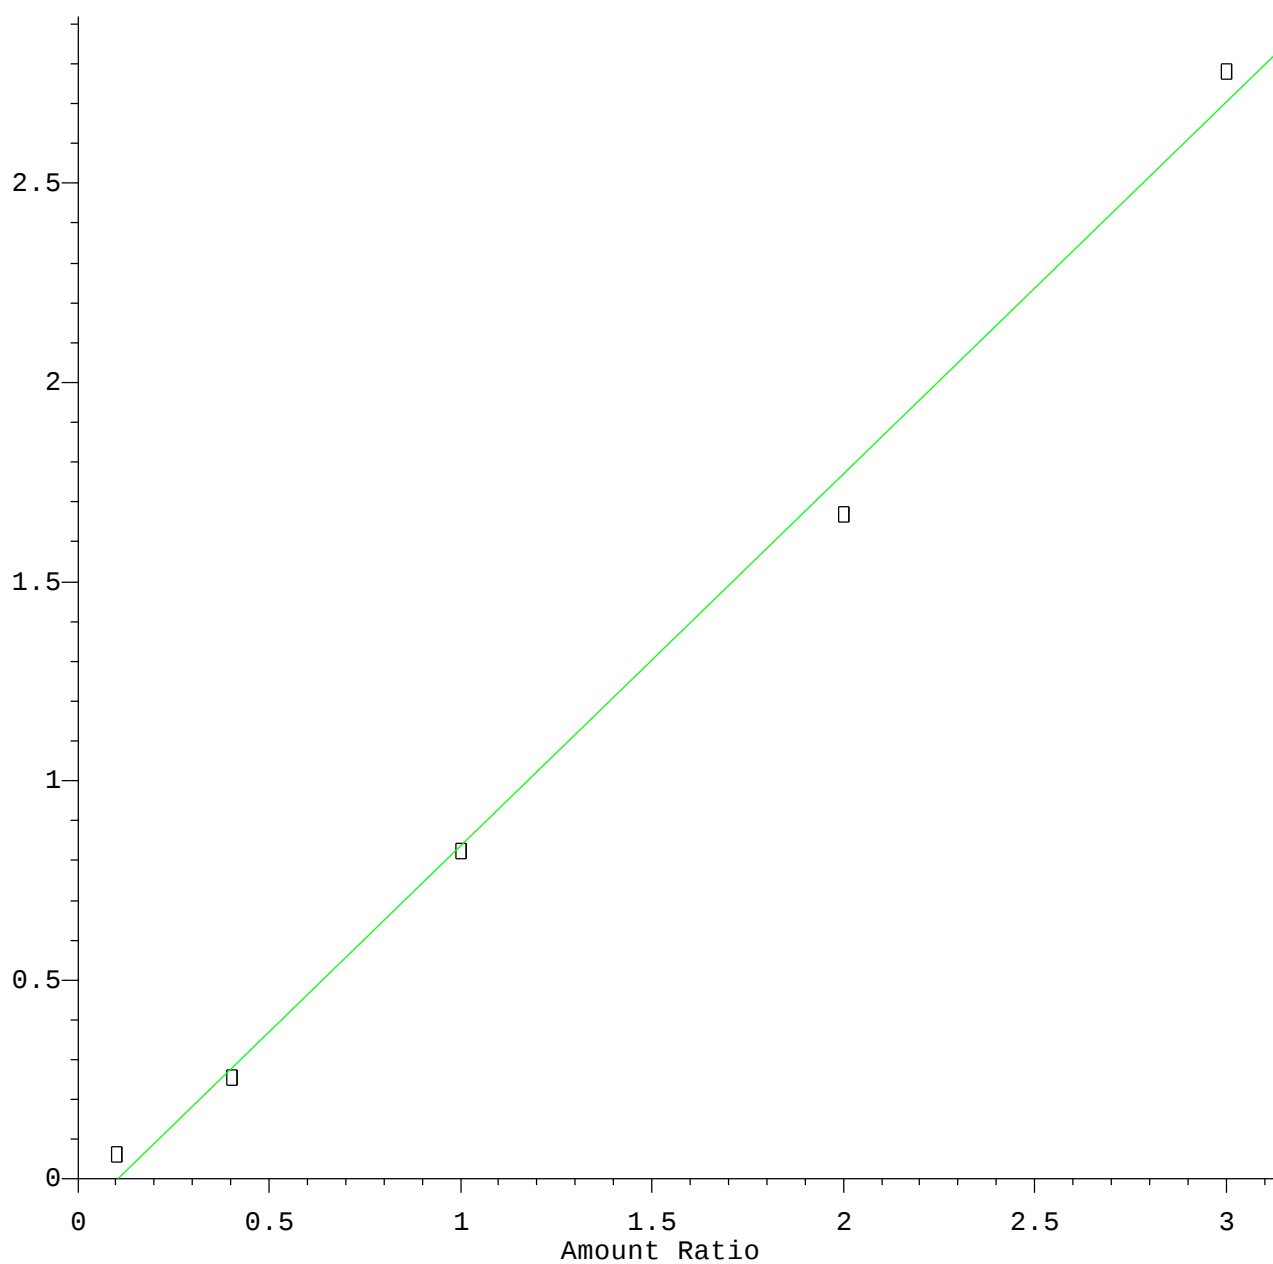

Resp Ratio = $9.34 \times 10^{-1} \times \text{Amt} - 9.81 \times 10^{-2}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121020W.M
Calibration Table Last Updated: Fri Dec 11 07:09:49 2020

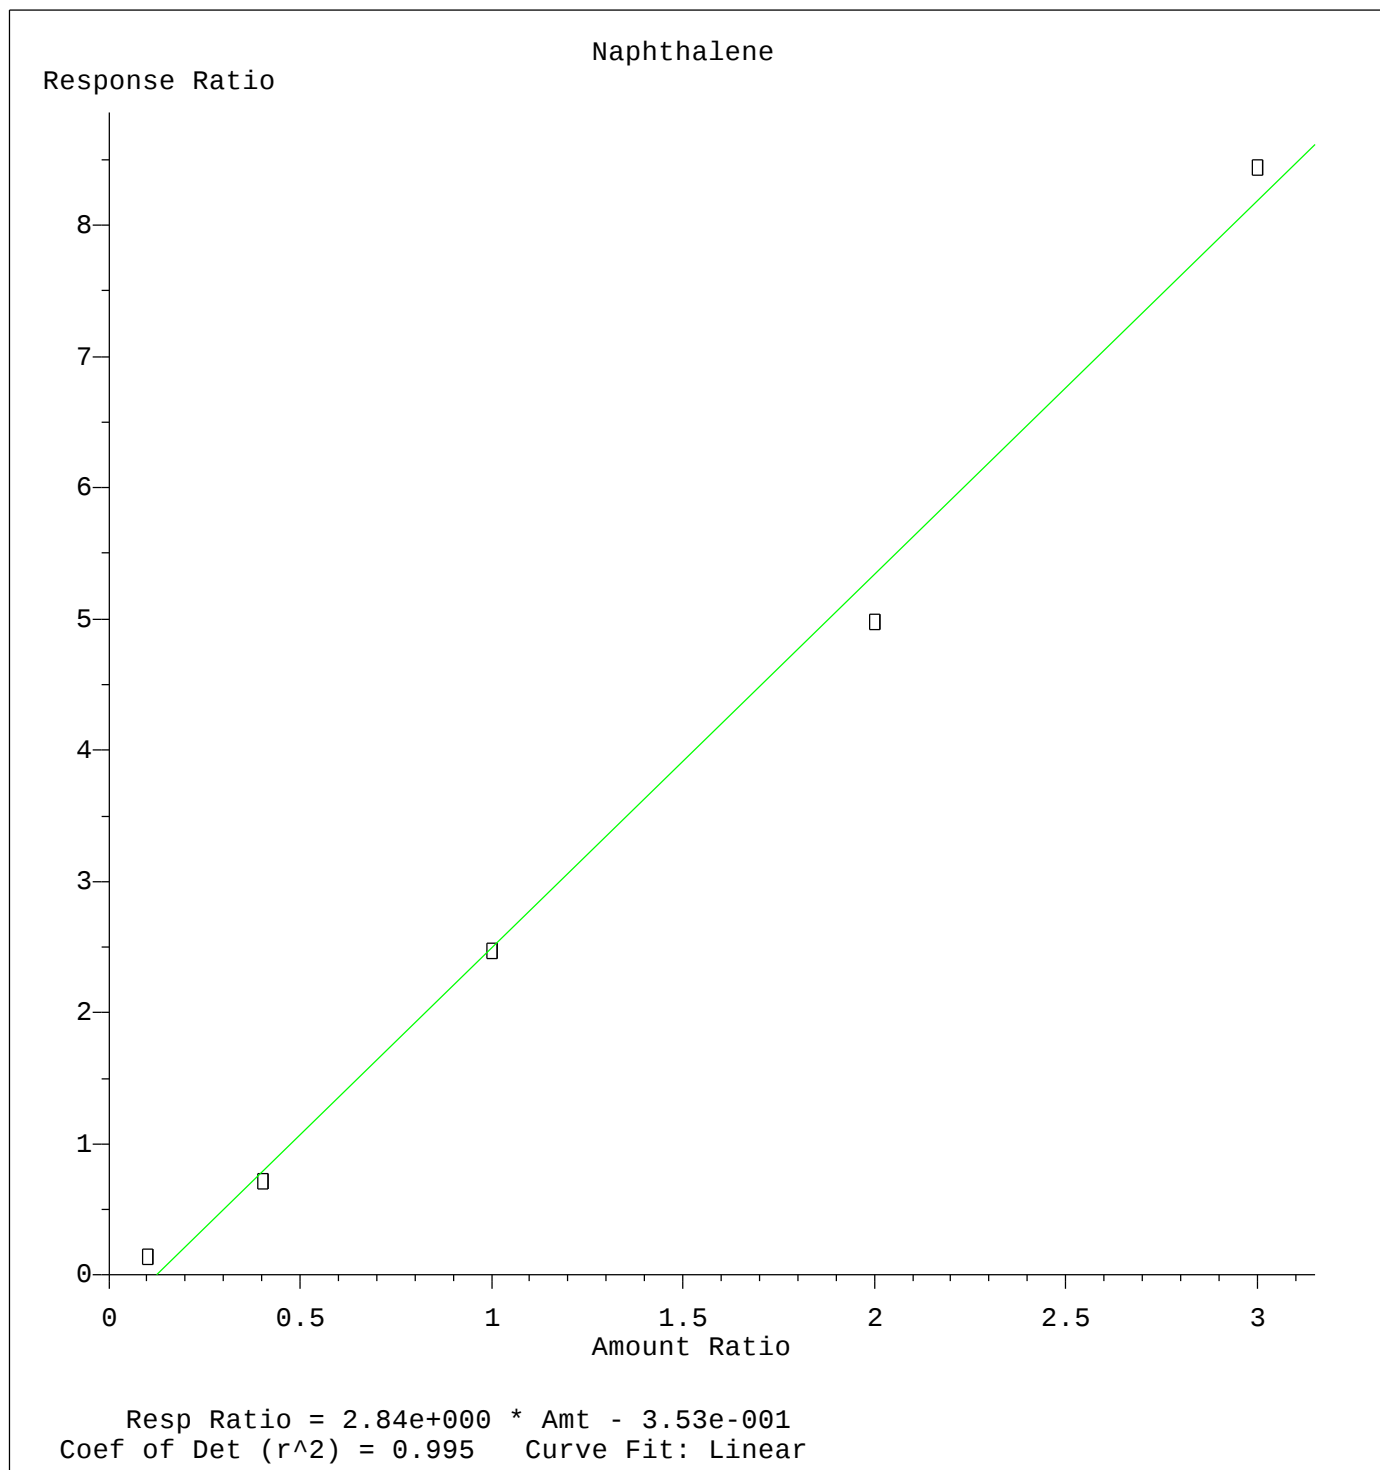

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121020W.M
Calibration Table Last Updated: Fri Dec 11 07:09:49 2020

1,2,3-Trichlorobenzene

Response Ratio

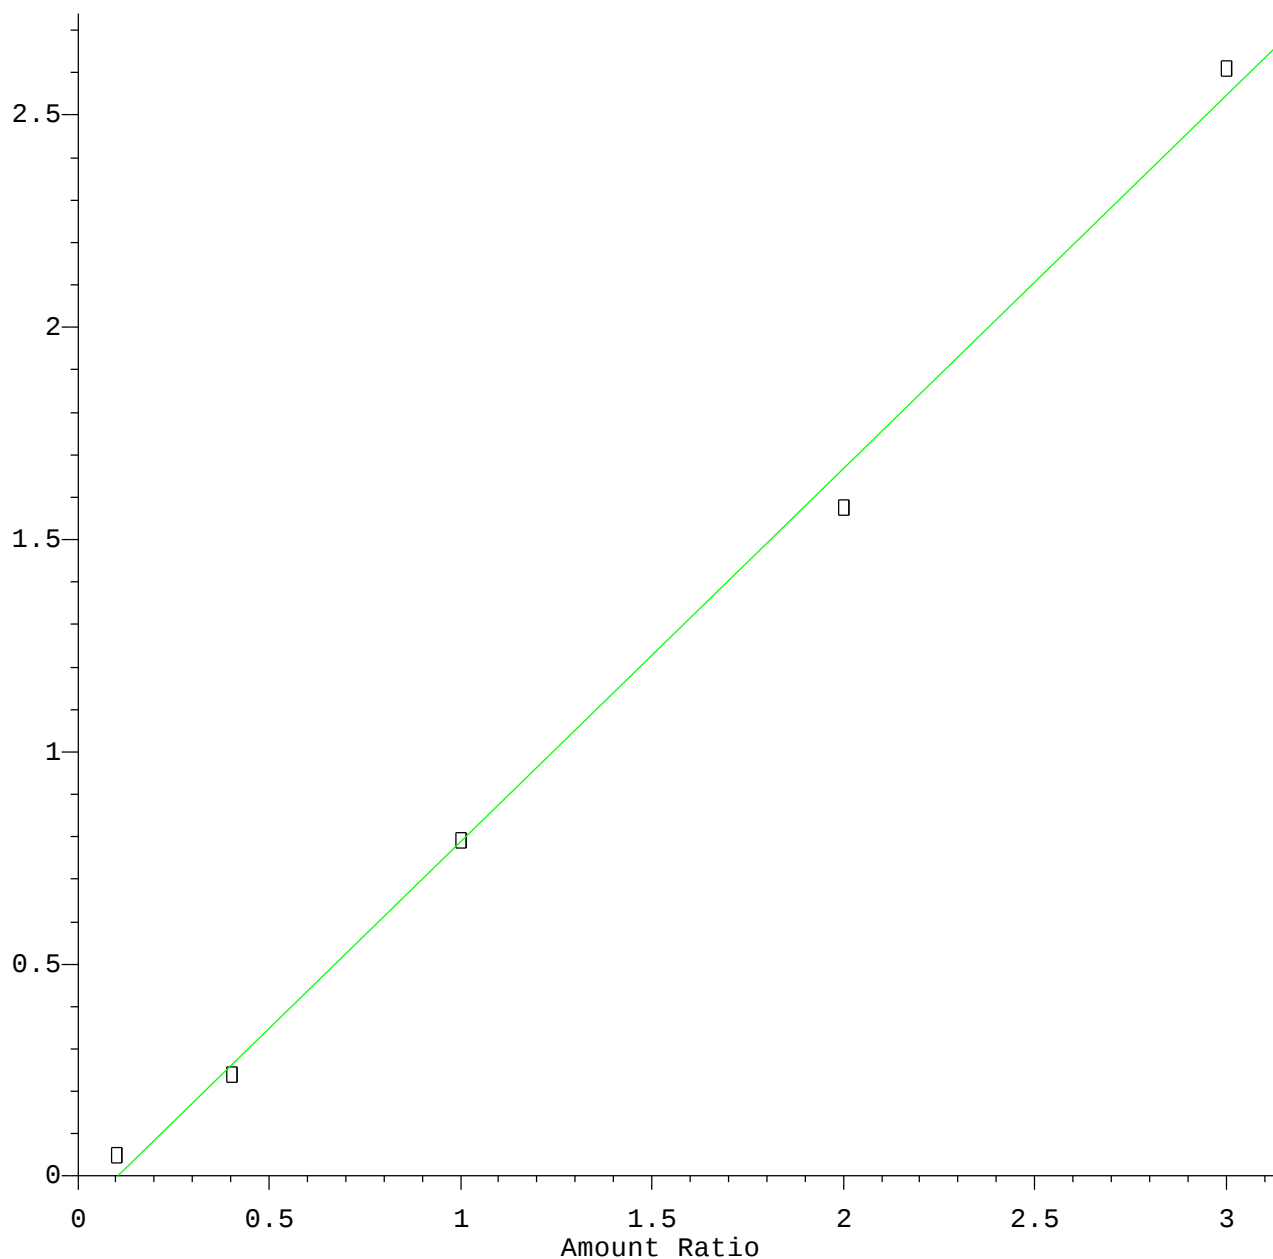


Resp Ratio = $8.78 \times 10^{-1} \times \text{Amt} - 8.97 \times 10^{-2}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121020W.M
Calibration Table Last Updated: Fri Dec 11 07:09:49 2020


Dichlorodifluoromethane

Response Ratio

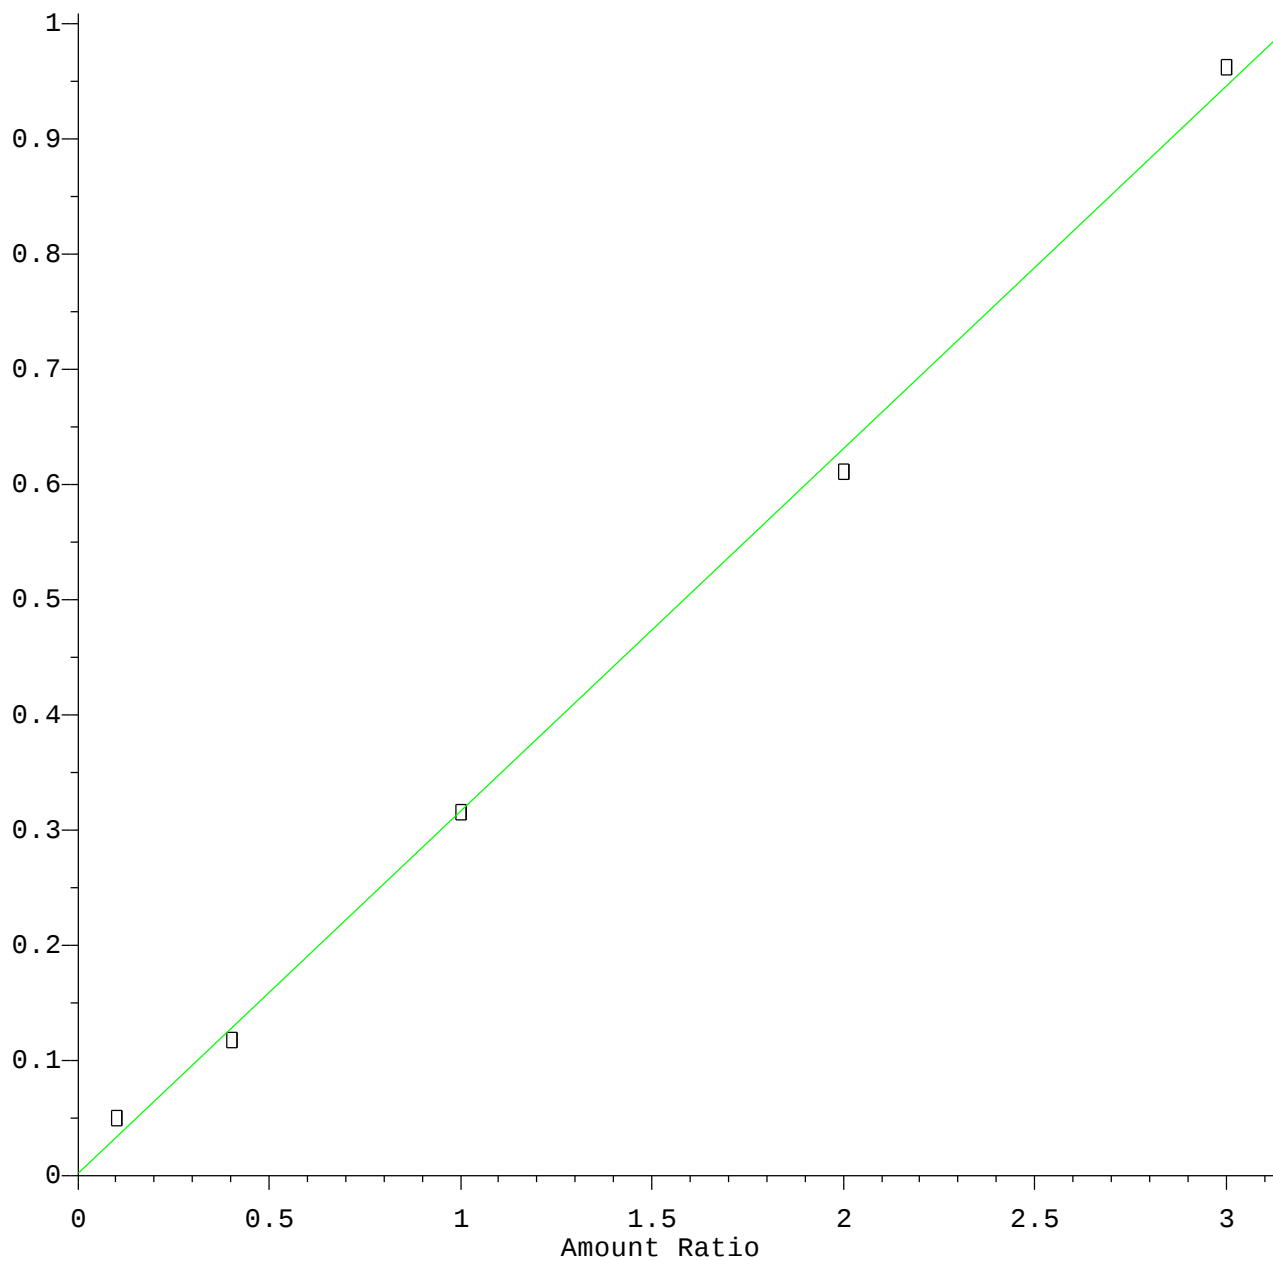


Resp Ratio = $3.15 \times 10^{-1} \times \text{Amt} + 1.83 \times 10^{-3}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121020W.M
Calibration Table Last Updated: Fri Dec 11 07:09:49 2020

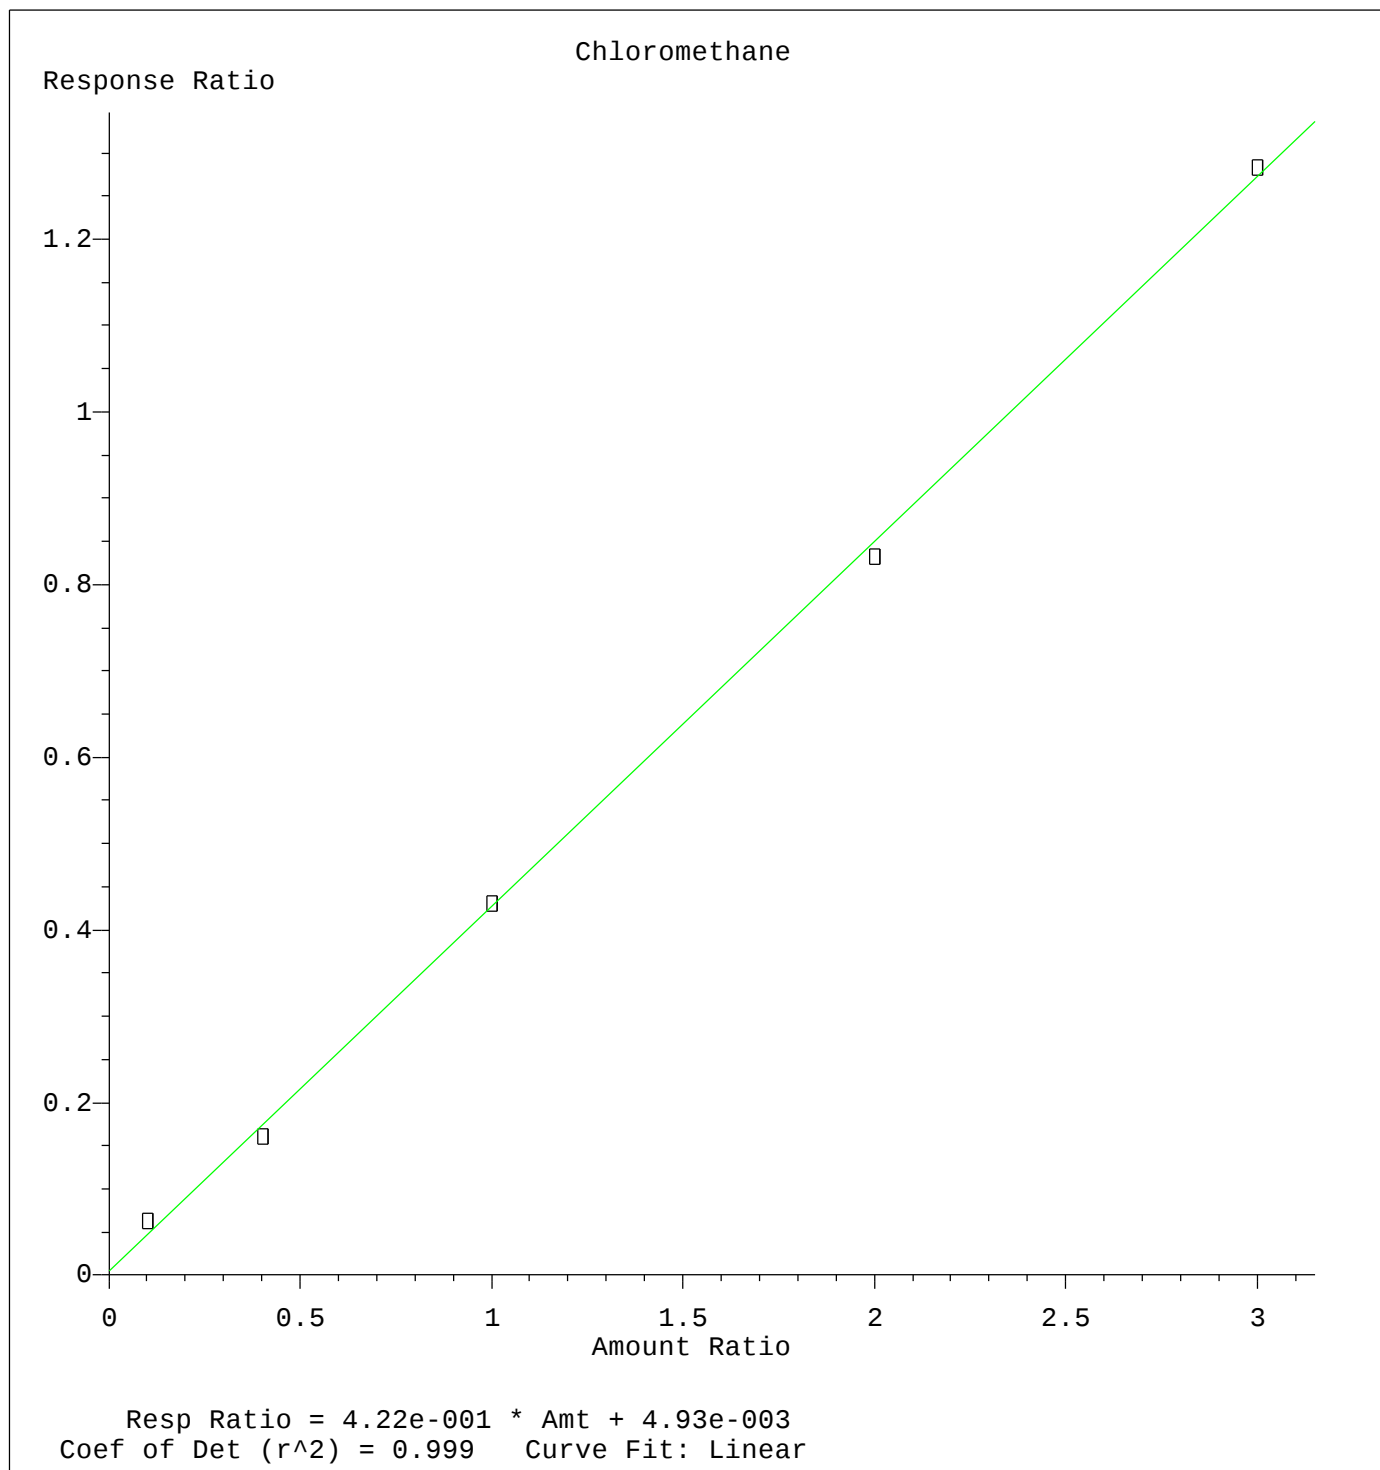


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121020W.M
Calibration Table Last Updated: Fri Dec 11 07:09:49 2020

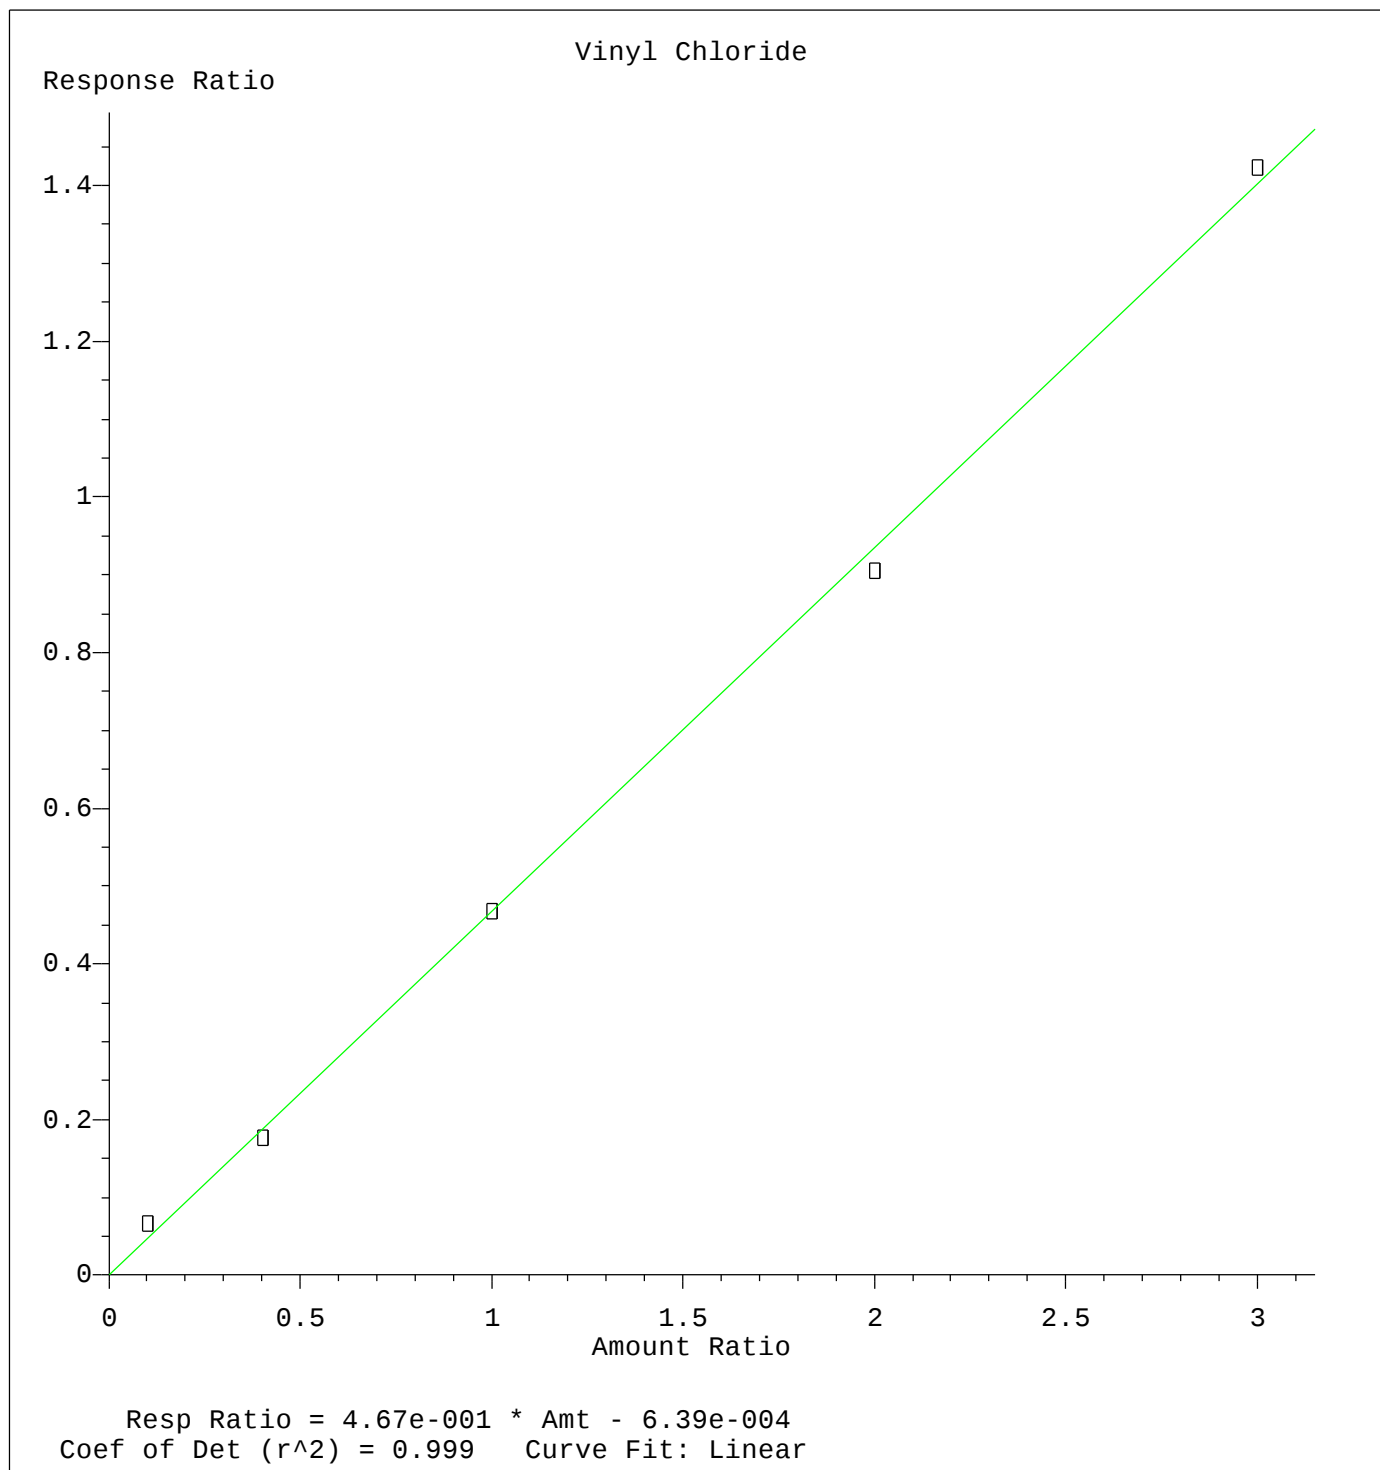


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121020W.M
Calibration Table Last Updated: Fri Dec 11 07:09:49 2020

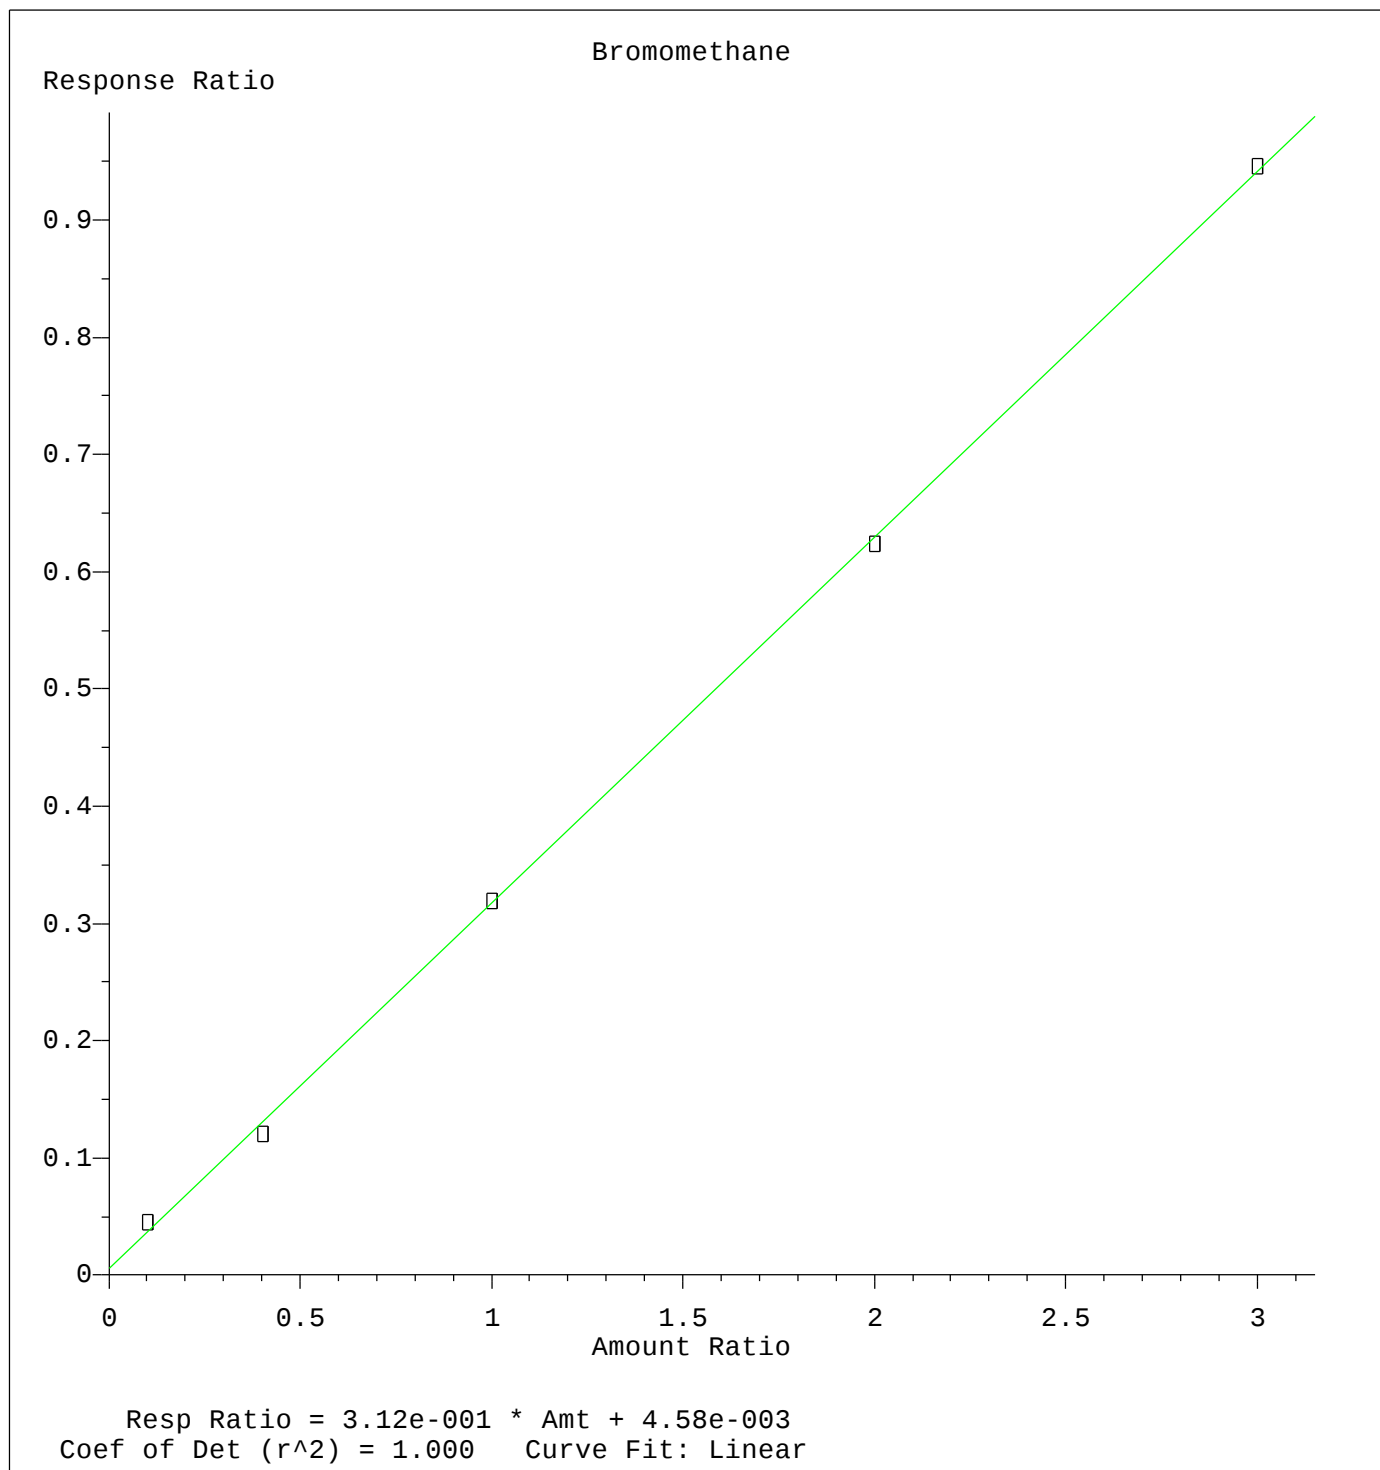

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121020W.M
Calibration Table Last Updated: Fri Dec 11 07:09:49 2020

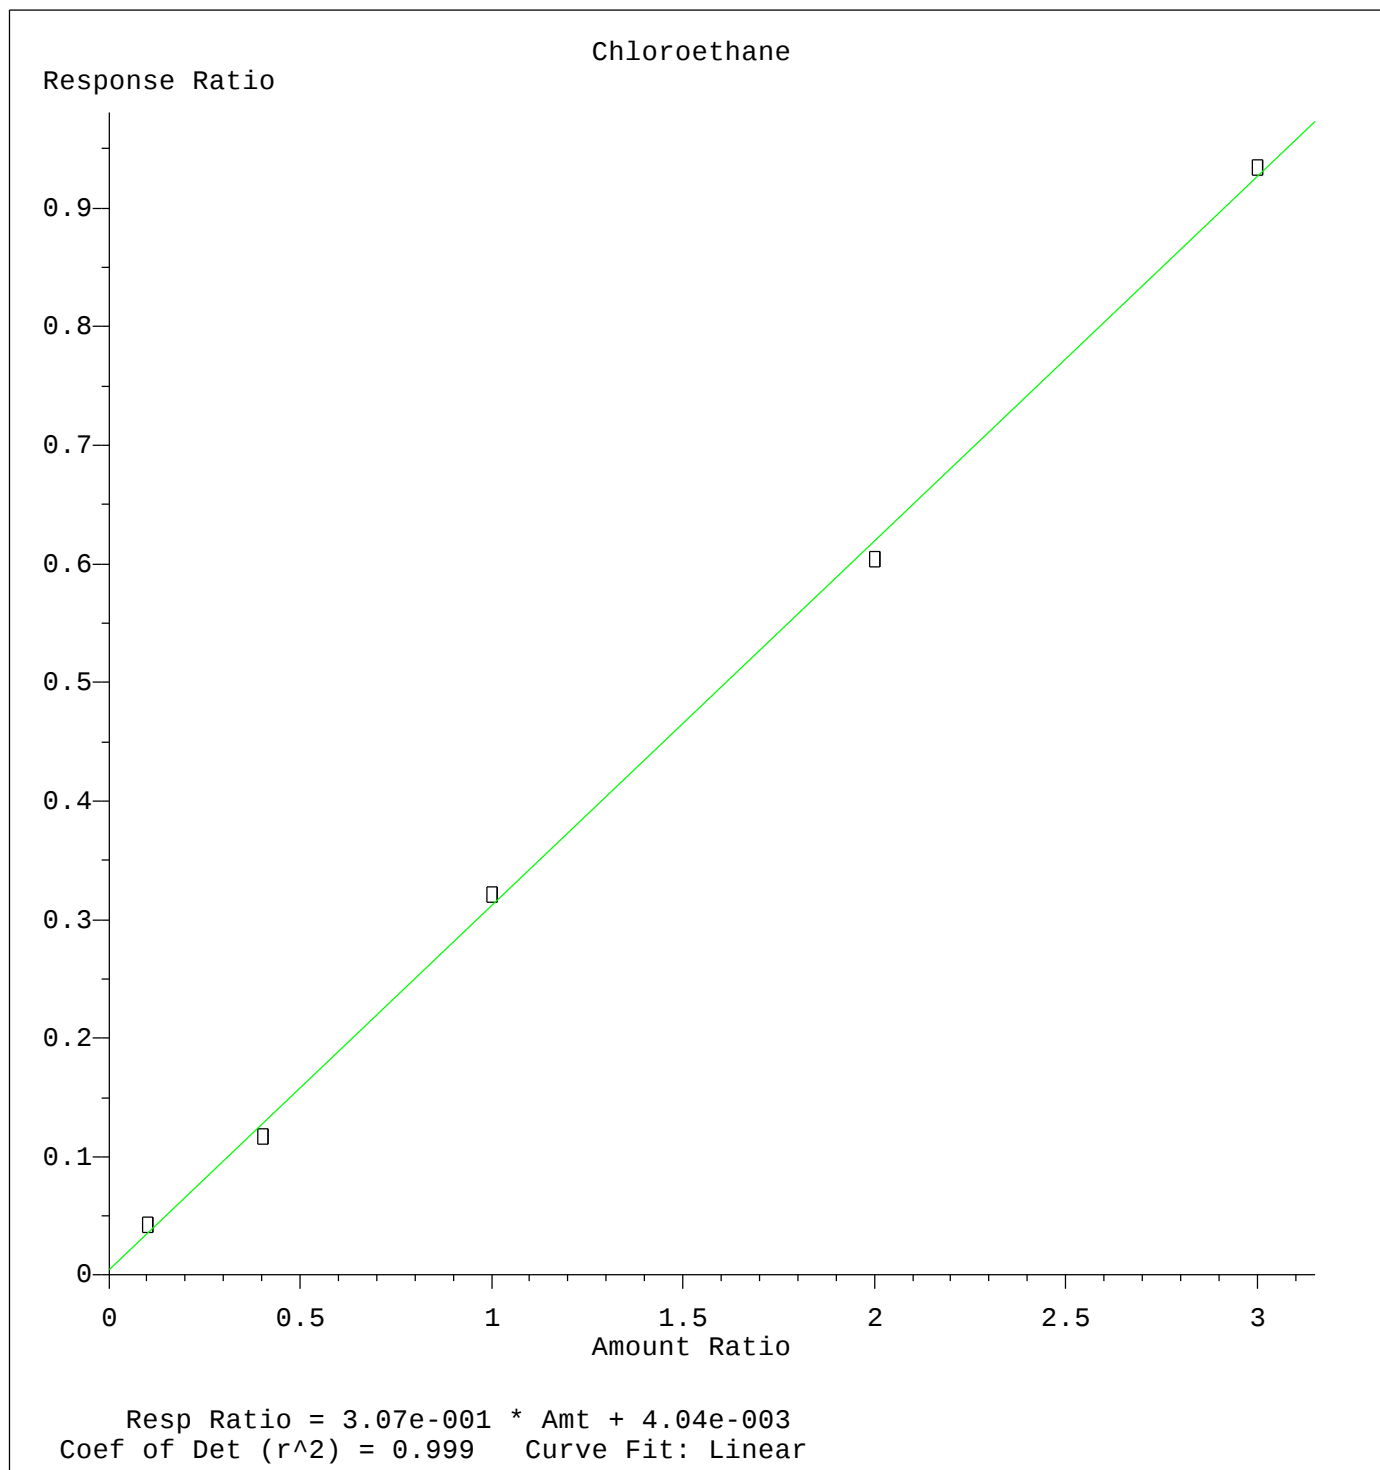

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121020W.M
Calibration Table Last Updated: Fri Dec 11 07:09:49 2020

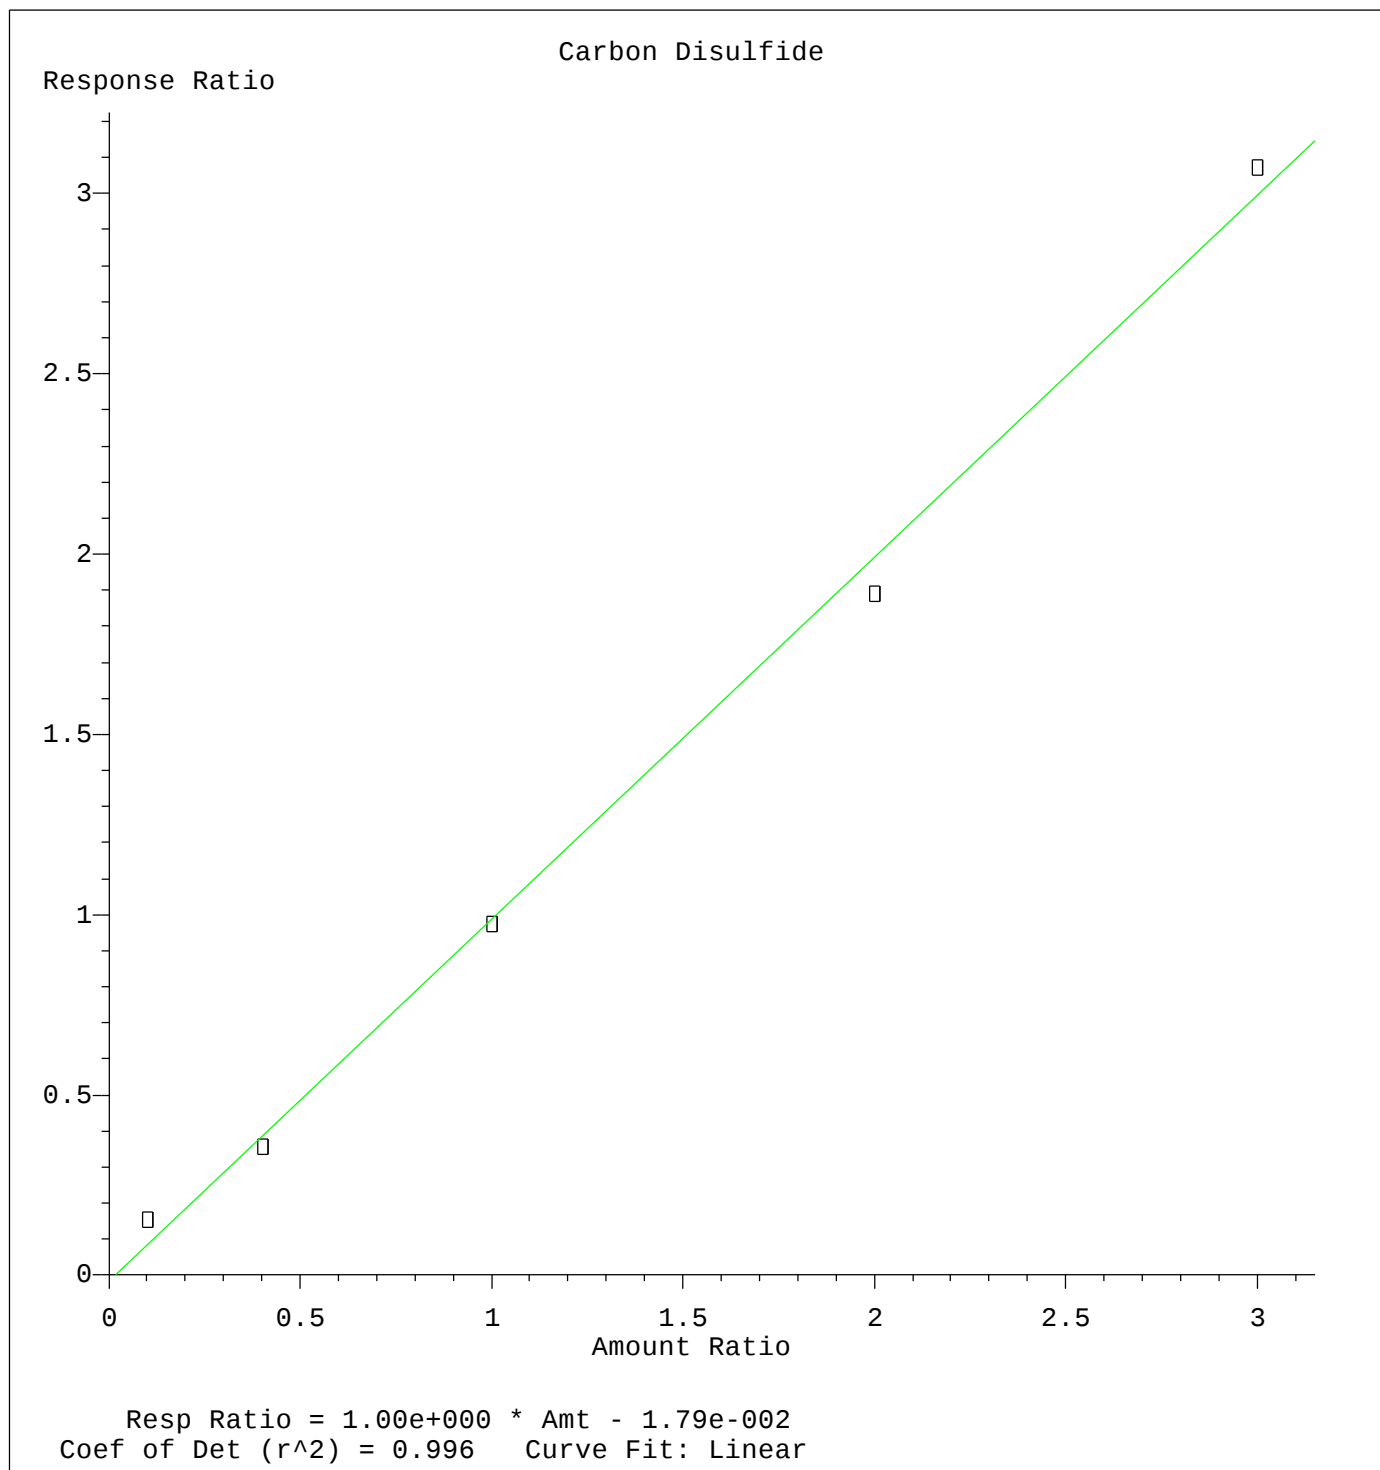

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121020W.M
Calibration Table Last Updated: Fri Dec 11 07:09:49 2020