


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN121020\
 Data File : VN065036.D
 Acq On : 10 Dec 2020 9:21
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121020W.M
 Title : SW846 8260
 Last Update : Fri Dec 11 07:09:49 2020

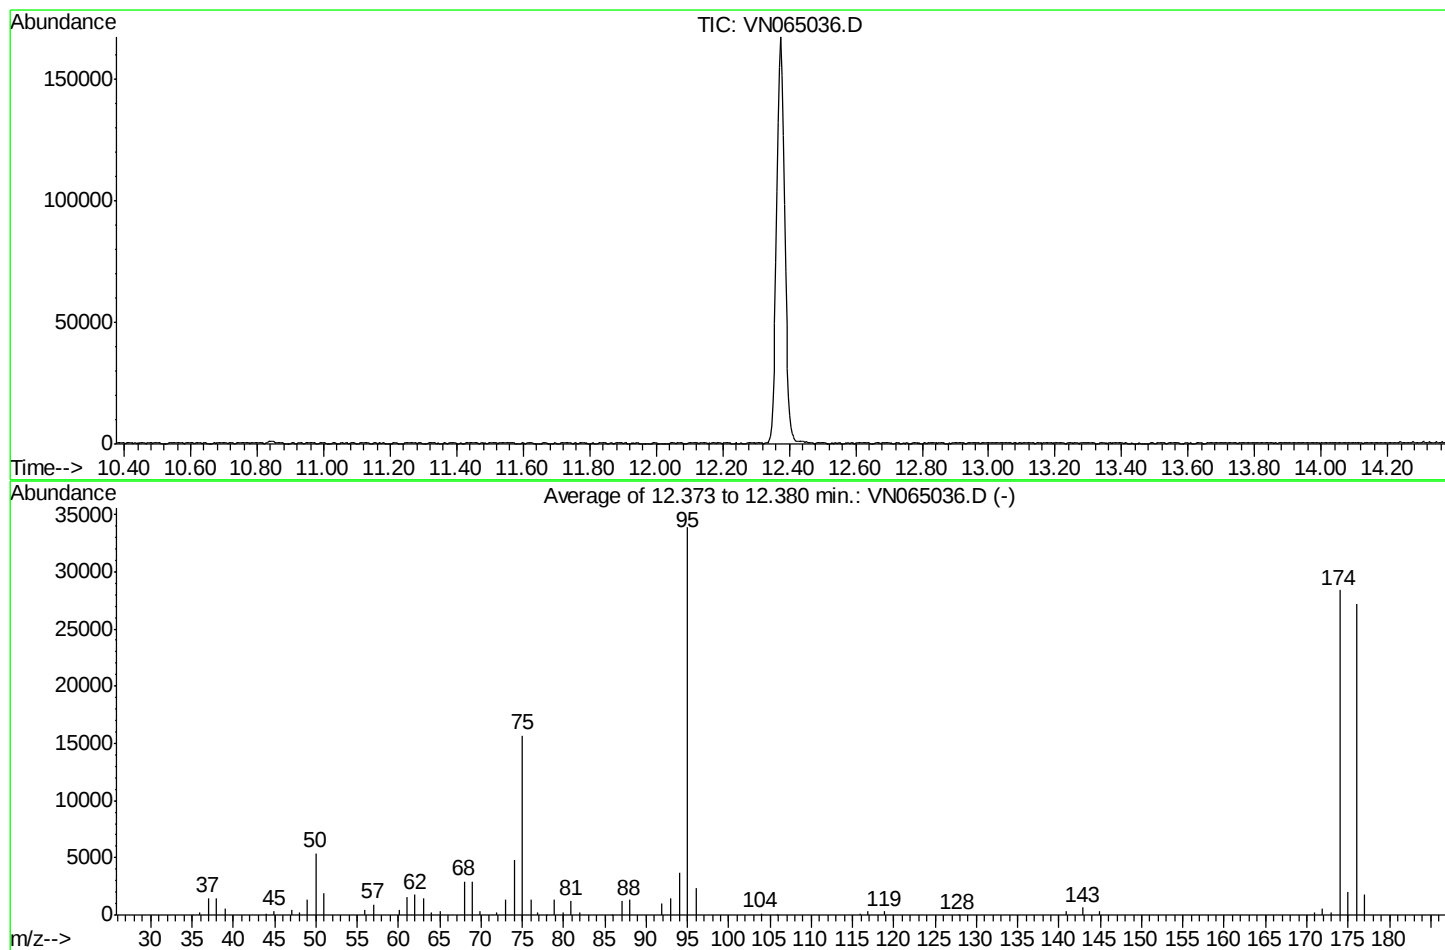

AutoFind: Scans 3307, 3308, 3309; Background Corrected with Scan 3294

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	5415	PASS
75	95	30	60	46.4	15708	PASS
95	95	100	100	100.0	33880	PASS
96	95	5	9	7.1	2408	PASS
173	174	0.00	2	0.9	256	PASS
174	95	50	100	83.8	28386	PASS
175	174	5	9	7.2	2045	PASS
176	174	95	101	95.7	27160	PASS
177	176	5	9	6.5	1778	PASS