


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN121020\
 Data File : VN065047.D
 Acq On : 10 Dec 2020 16:41
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121020W.M
 Title : SW846 8260
 Last Update : Fri Dec 11 07:09:49 2020

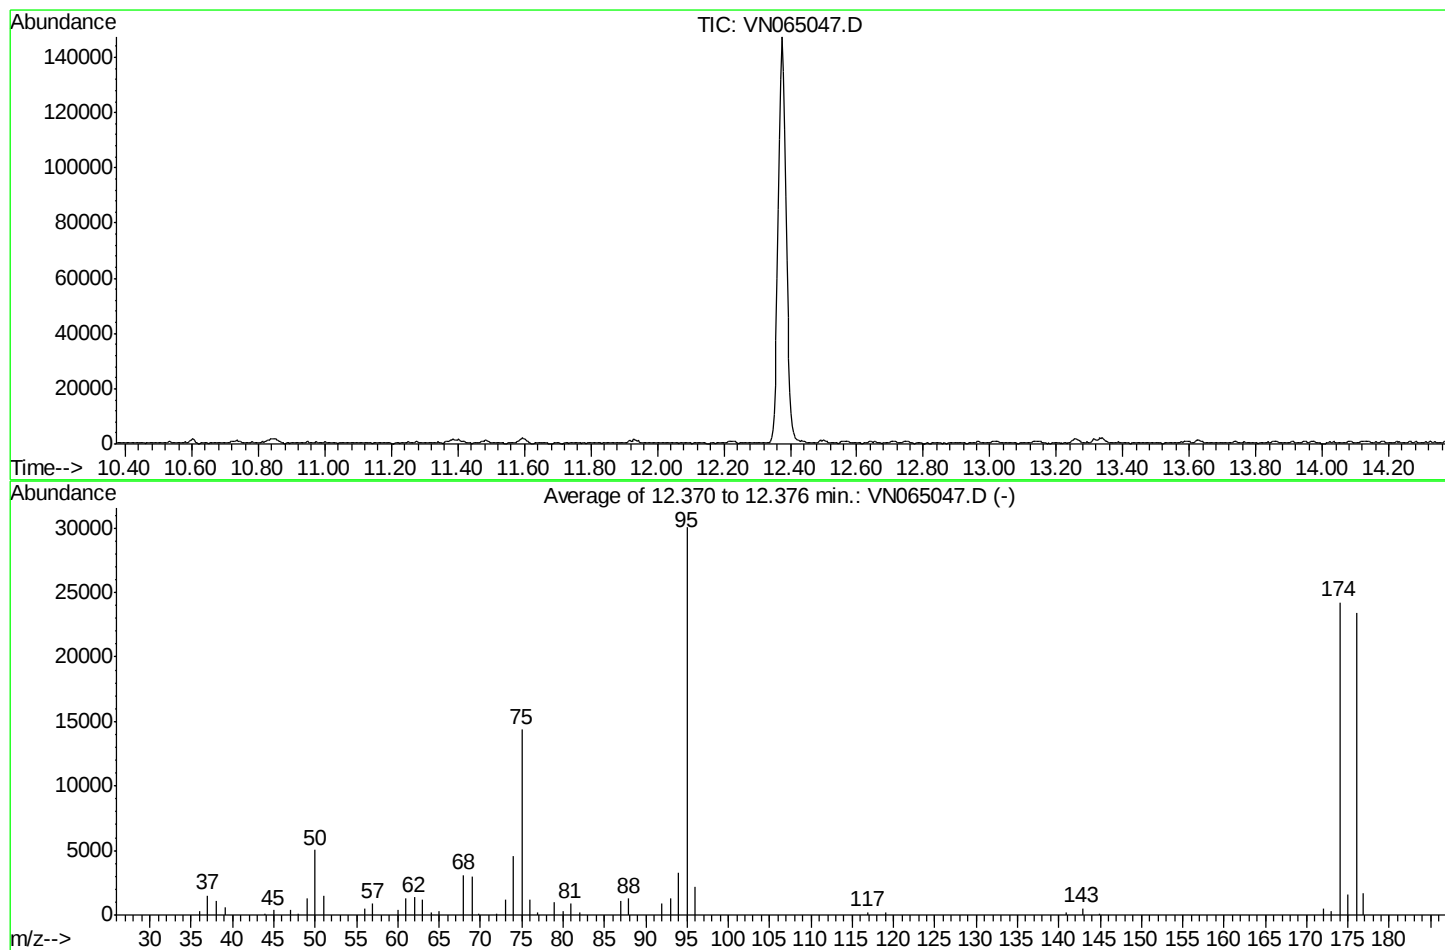

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3294

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	5025	PASS
75	95	30	60	47.8	14365	PASS
95	95	100	100	100.0	30053	PASS
96	95	5	9	7.2	2160	PASS
173	174	0.00	2	1.4	329	PASS
174	95	50	100	80.7	24248	PASS
175	174	5	9	6.6	1606	PASS
176	174	95	101	96.7	23456	PASS
177	176	5	9	7.1	1654	PASS