

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121021\
 Data File : VN069970.D
 Acq On : 10 Dec 2021 20:14
 Operator : JC/MD
 Sample : M4969-09
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 RW-1A

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
 Title : SW846 8260

Signal : TIC: VN069970.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.593	218	225	243	rVB2	54536	90355	1.02%	0.125%
2	3.140	416	429	449	rVB	170351	390388	4.41%	0.541%
3	3.513	556	568	595	rVB4	54589	135373	1.53%	0.188%
4	4.291	831	858	886	rBV2	91663	292342	3.30%	0.405%
5	4.586	950	968	992	rBV2	30504	95249	1.08%	0.132%
6	5.079	1125	1152	1153	rBV4	54556	117901	1.33%	0.163%
7	5.377	1233	1263	1308	rBV4	743449	2711235	30.62%	3.759%
8	5.621	1326	1354	1386	rVB3	473532	1660875	18.76%	2.303%
9	6.487	1646	1677	1702	rBV5	115572	460488	5.20%	0.638%
10	6.610	1708	1723	1745	rVB6	37038	105576	1.19%	0.146%
11	6.900	1811	1831	1864	rBV7	50875	170741	1.93%	0.237%
12	7.147	1904	1923	1940	rBV3	219531	628601	7.10%	0.871%
13	7.217	1941	1949	1971	rVB4	65119	174828	1.97%	0.242%
14	7.345	1978	1997	2018	rVB2	35893	99599	1.13%	0.138%
15	7.844	2173	2183	2202	rVB3	52343	126223	1.43%	0.175%
16	8.024	2227	2250	2261	rBV	920898	2274510	25.69%	3.153%
17	8.088	2261	2274	2293	rVV	1660829	3920160	44.28%	5.435%
18	8.177	2297	2307	2330	rVB7	90672	244608	2.76%	0.339%
19	8.442	2385	2406	2427	rBV3	1229268	3431300	38.76%	4.757%
20	8.536	2428	2441	2456	rBV2	521764	1155143	13.05%	1.601%
21	8.968	2582	2602	2629	rBV	2761424	5966874	67.40%	8.273%
22	9.199	2675	2688	2697	rBV3	75228	155059	1.75%	0.215%
23	9.421	2755	2771	2777	rBV6	78991	155802	1.76%	0.216%
24	9.797	2896	2911	2919	rBV6	138862	299913	3.39%	0.416%
25	9.877	2936	2941	2960	rVB6	50969	93377	1.05%	0.129%
26	9.971	2962	2976	2986	rBV4	169133	331153	3.74%	0.459%
27	10.202	3046	3062	3092	rBV2	420349	1118327	12.63%	1.550%
28	10.322	3095	3107	3121	rVB3	181073	329958	3.73%	0.457%
29	10.443	3134	3152	3168	rBV	4350813	8110193	91.61%	11.244%
30	10.550	3185	3192	3207	rVB3	100990	181437	2.05%	0.252%
31	10.859	3294	3307	3326	rVB3	100321	205048	2.32%	0.284%
32	10.945	3326	3339	3359	rVB2	113943	217328	2.45%	0.301%
33	11.089	3378	3393	3399	rBV	248342	437059	4.94%	0.606%
34	11.130	3399	3408	3430	rVB	573787	1052466	11.89%	1.459%
35	11.459	3517	3531	3542	rBV2	78873	148590	1.68%	0.206%
36	11.588	3565	3579	3618	rVB3	266985	859769	9.71%	1.192%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121021\
 Data File : VN069970.D
 Acq On : 10 Dec 2021 20:14
 Operator : JC/MD
 Sample : M4969-09
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 RW-1A

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
 Title : SW846 8260

37	11.744	3619	3637	3665	rBV	4822539	8853114	100.00%	12.274%
38	11.851	3667	3677	3699	rVV6	121264	312481	3.53%	0.433%
39	11.950	3701	3714	3740	rVB3	178610	412219	4.66%	0.572%
40	12.361	3849	3867	3877	rBV3	63394	134327	1.52%	0.186%
41	12.578	3936	3948	3962	rBV	645656	1057869	11.95%	1.467%
42	12.731	3988	4005	4033	rBV	3931853	6907753	78.03%	9.577%
43	12.849	4037	4049	4060	rVV9	51685	110541	1.25%	0.153%
44	12.921	4061	4076	4093	rVB	1194039	2050760	23.16%	2.843%
45	13.058	4120	4127	4145	rVB7	84722	157447	1.78%	0.218%
46	13.222	4174	4188	4200	rBV	135579	244522	2.76%	0.339%
47	13.356	4221	4238	4257	rVB9	62561	175324	1.98%	0.243%
48	13.498	4282	4291	4305	rVB3	52107	104534	1.18%	0.145%
49	13.675	4341	4357	4386	rBV	4323349	7612384	85.99%	10.554%
50	13.838	4407	4418	4422	rBV2	315436	447132	5.05%	0.620%
51	13.876	4423	4432	4466	rVB	1548553	2760898	31.19%	3.828%
52	14.217	4547	4559	4571	rBV	188377	313815	3.54%	0.435%
53	14.281	4572	4583	4589	rVV2	94064	154206	1.74%	0.214%
54	14.329	4589	4601	4618	rVB	645594	1090319	12.32%	1.512%
55	14.541	4669	4680	4689	rBV	103536	167838	1.90%	0.233%
56	14.812	4769	4781	4796	rVB	189563	321669	3.63%	0.446%
57	14.930	4809	4825	4839	rBV4	272630	532917	6.02%	0.739%
58	15.313	4955	4968	4983	rVB6	38944	95665	1.08%	0.133%
59	15.507	5026	5040	5056	rVB	81805	163329	1.84%	0.226%




Sum of corrected areas: 72128911

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121021\
Data File : VN069970.D
Acq On : 10 Dec 2021 20:14
Operator : JC/MD
Sample : M4969-09
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
RW-1A

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

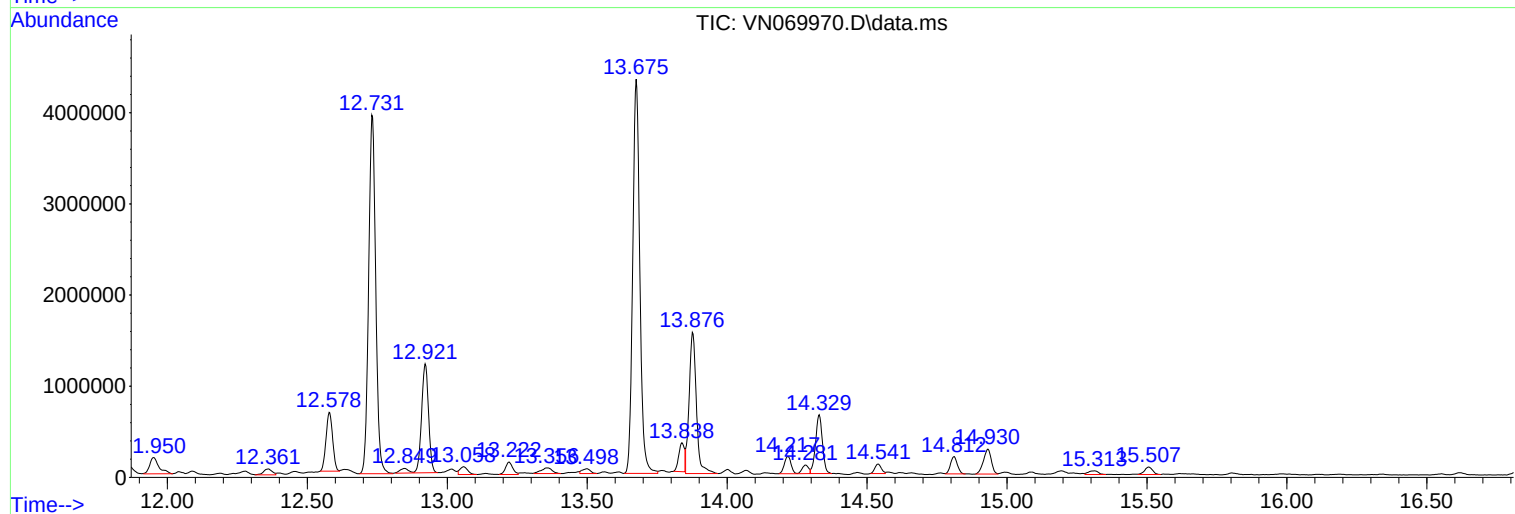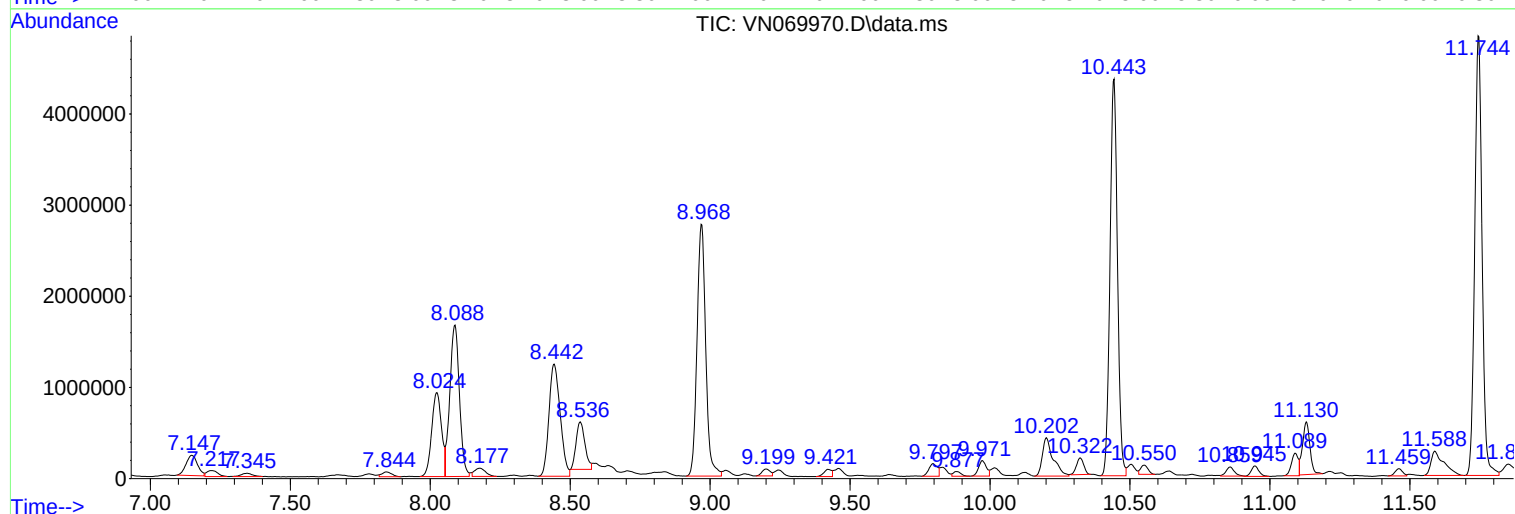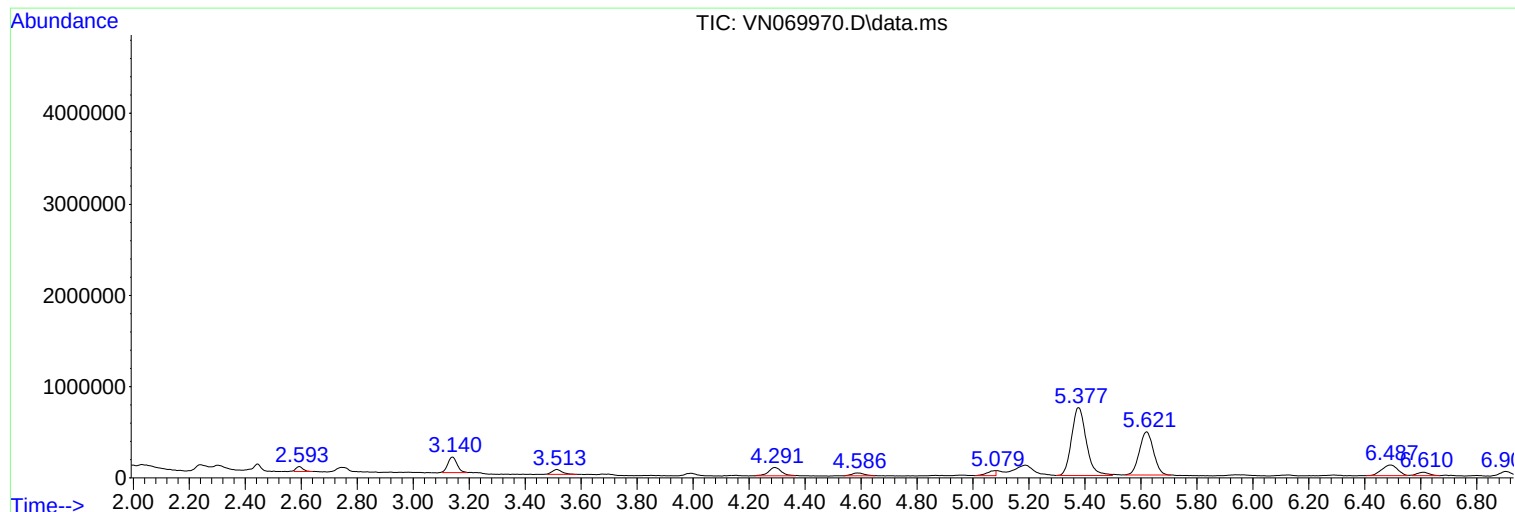

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121021\
Data File : VN069970.D
Acq On : 10 Dec 2021 20:14
Operator : JC/MD
Sample : M4969-09
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
RW-1A

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121021\
Data File : VN069970.D
Acq On : 10 Dec 2021 20:14
Operator : JC/MD
Sample : M4969-09
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
RW-1A

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------