
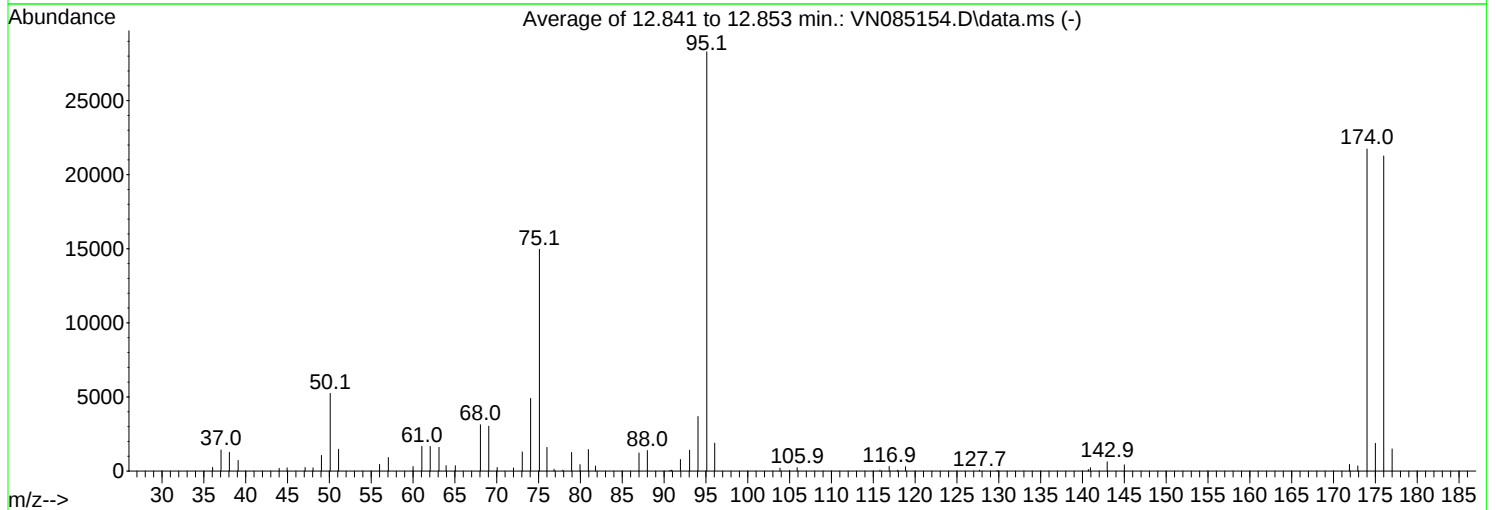


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121024\
Data File : VN085154.D
Acq On : 10 Dec 2024 08:37
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112224W.M
Title : SW846 8260
Last Update : Sat Nov 23 02:54:10 2024

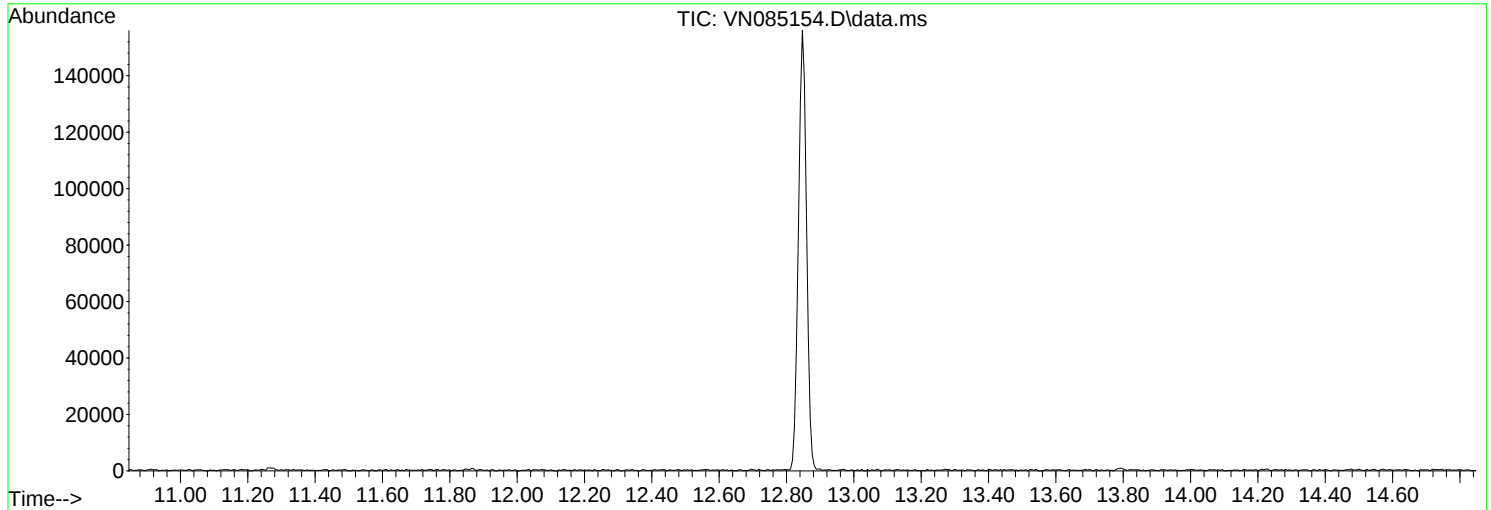

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	5248	PASS
75	95	30	60	52.9	14972	PASS
95	95	100	100	100.0	28296	PASS
96	95	5	9	6.7	1886	PASS
173	174	0.00	2	1.6	350	PASS
174	95	50	100	76.8	21733	PASS
175	174	5	9	8.6	1875	PASS
176	174	95	101	97.8	21264	PASS
177	176	5	9	7.0	1494	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	256	56.00	454	72.00	211	87.00	1221
37.05	1426	57.05	915	73.05	1291	88.00	1385
38.05	1269	60.00	309	74.05	4900	90.70	55
39.10	716	61.05	1664	75.10	14972	90.90	66
44.00	187	62.05	1661	76.00	1601	91.95	782
44.95	220	63.10	1606	76.85	127	93.05	1406
47.10	246	63.95	362	77.90	60	94.05	3684
48.05	222	65.05	365	78.95	1260	95.10	28296
49.05	1057	68.05	3126	79.95	436	96.05	1886
50.10	5248	69.05	3033	80.95	1454	103.85	197
51.10	1469	70.05	247	81.80	341	105.00	52

Average of 12.841 to 12.853 min.: VN085154.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
105.90	230	171.90	447				
115.80	63	172.90	350				
116.90	317	174.00	21733				
117.90	59	175.00	1875				
118.85	299	176.00	21264				
127.70	66	177.00	1494				
129.80	52						
140.70	111						
140.95	226						
142.95	629						
145.00	422						

Instrument :

MSVOA_N

ClientSampleId :

BFB