


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN121119\
Data File : VN059553.D
Acq On : 11 Dec 2019 9:29
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N120919W.M
Title : SW846 8260
Last Update : Tue Dec 10 01:09:52 2019

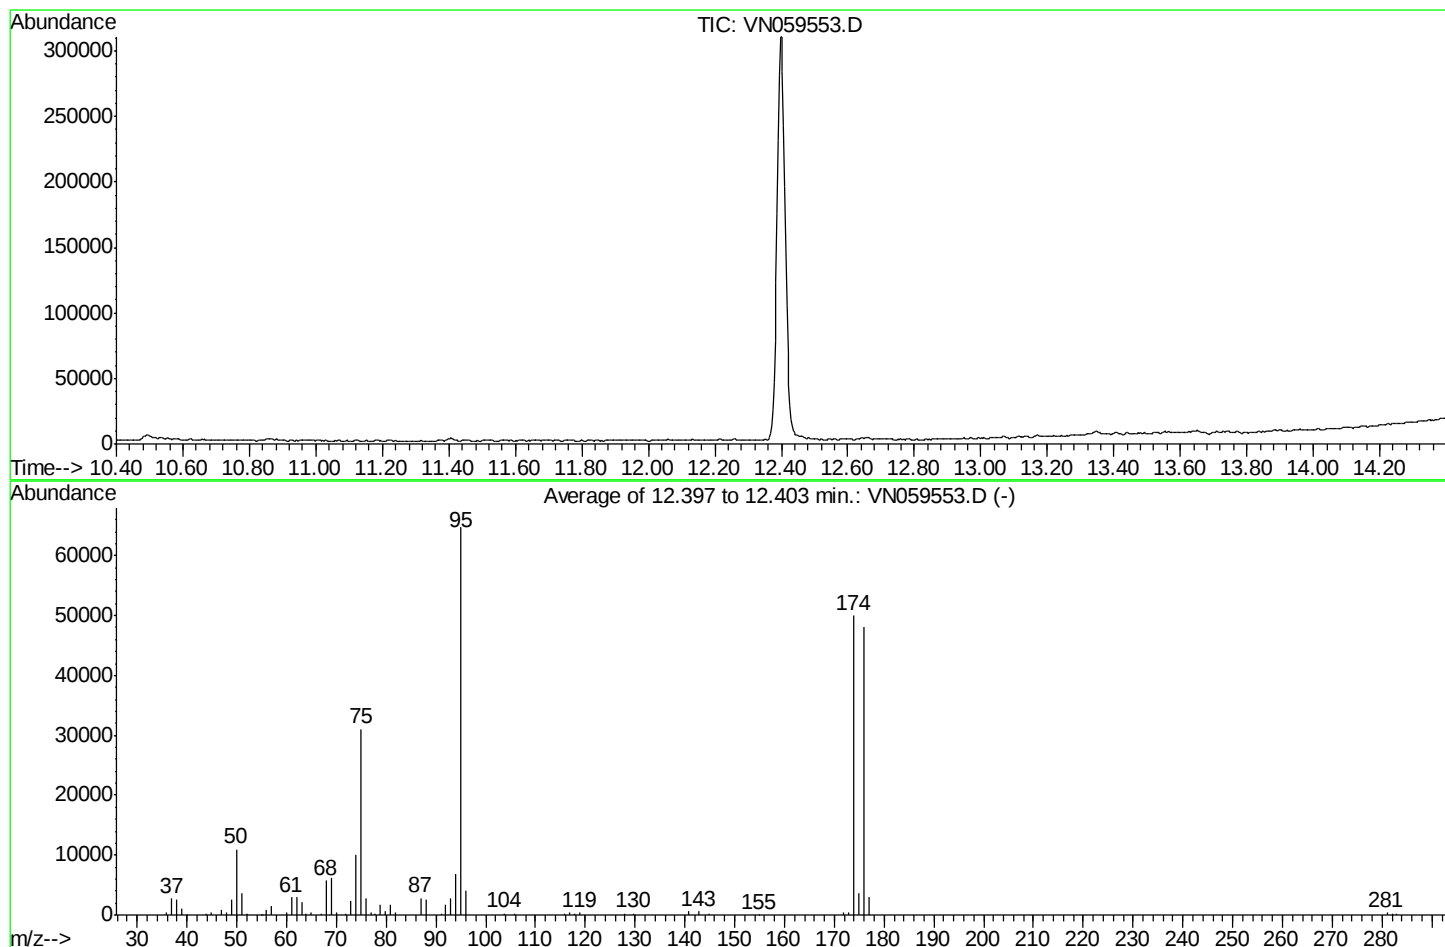

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	10942	PASS
75	95	30	60	48.0	31058	PASS
95	95	100	100	100.0	64741	PASS
96	95	5	9	6.3	4083	PASS
173	174	0.00	2	0.9	444	PASS
174	95	50	100	77.2	49970	PASS
175	174	5	9	7.4	3714	PASS
176	174	95	101	96.5	48202	PASS
177	176	5	9	6.3	3031	PASS