


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121120\
 Data File : VN065069.D
 Acq On : 11 Dec 2020 13:05
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121120W.M
 Title : SW846 8260
 Last Update : Sat Dec 12 04:18:15 2020

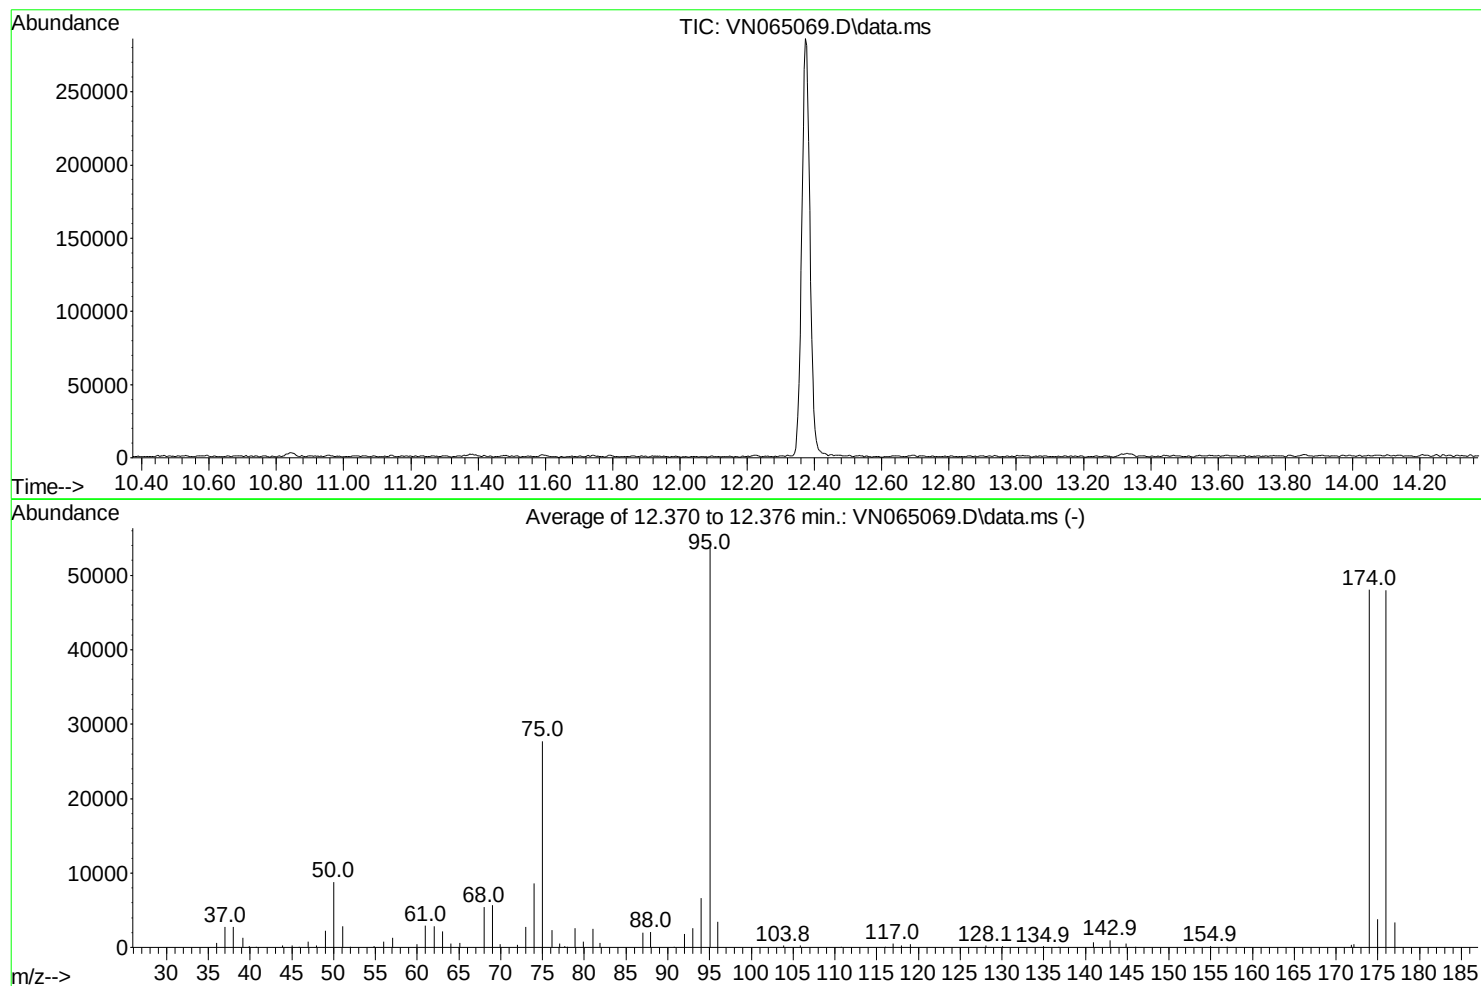

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	8815	PASS
75	95	30	60	51.7	27717	PASS
95	95	100	100	100.0	53656	PASS
96	95	5	9	6.5	3472	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	89.7	48120	PASS
175	174	5	9	7.9	3803	PASS
176	174	95	101	99.7	47960	PASS
177	176	5	9	7.0	3378	PASS