

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121121\
 Data File : VN070001.D
 Acq On : 11 Dec 2021 11:51
 Operator : JC/MD
 Sample : VN1211MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1211MBL01

Quant Time: Dec 12 16:17:14 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
 Quant Title : SW846 8260
 QLast Update : Fri Dec 03 08:46:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.086	168	1000380	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	1901998	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.747	117	2148427	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	806451	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	807501	52.279	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	104.560%
35) Dibromofluoromethane	8.024	113	595786	50.008	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	100.020%
50) Toluene-d8	10.443	98	2514846	52.571	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	105.140%
62) 4-Bromofluorobenzene	12.734	95	1011469	58.364	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	116.720%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121121\
Data File : VN070001.D
Acq On : 11 Dec 2021 11:51
Operator : JC/MD
Sample : VN1211MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1211MBL01

Quant Time: Dec 12 16:17:14 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
Quant Title : SW846 8260
QLast Update : Fri Dec 03 08:46:47 2021
Response via : Initial Calibration




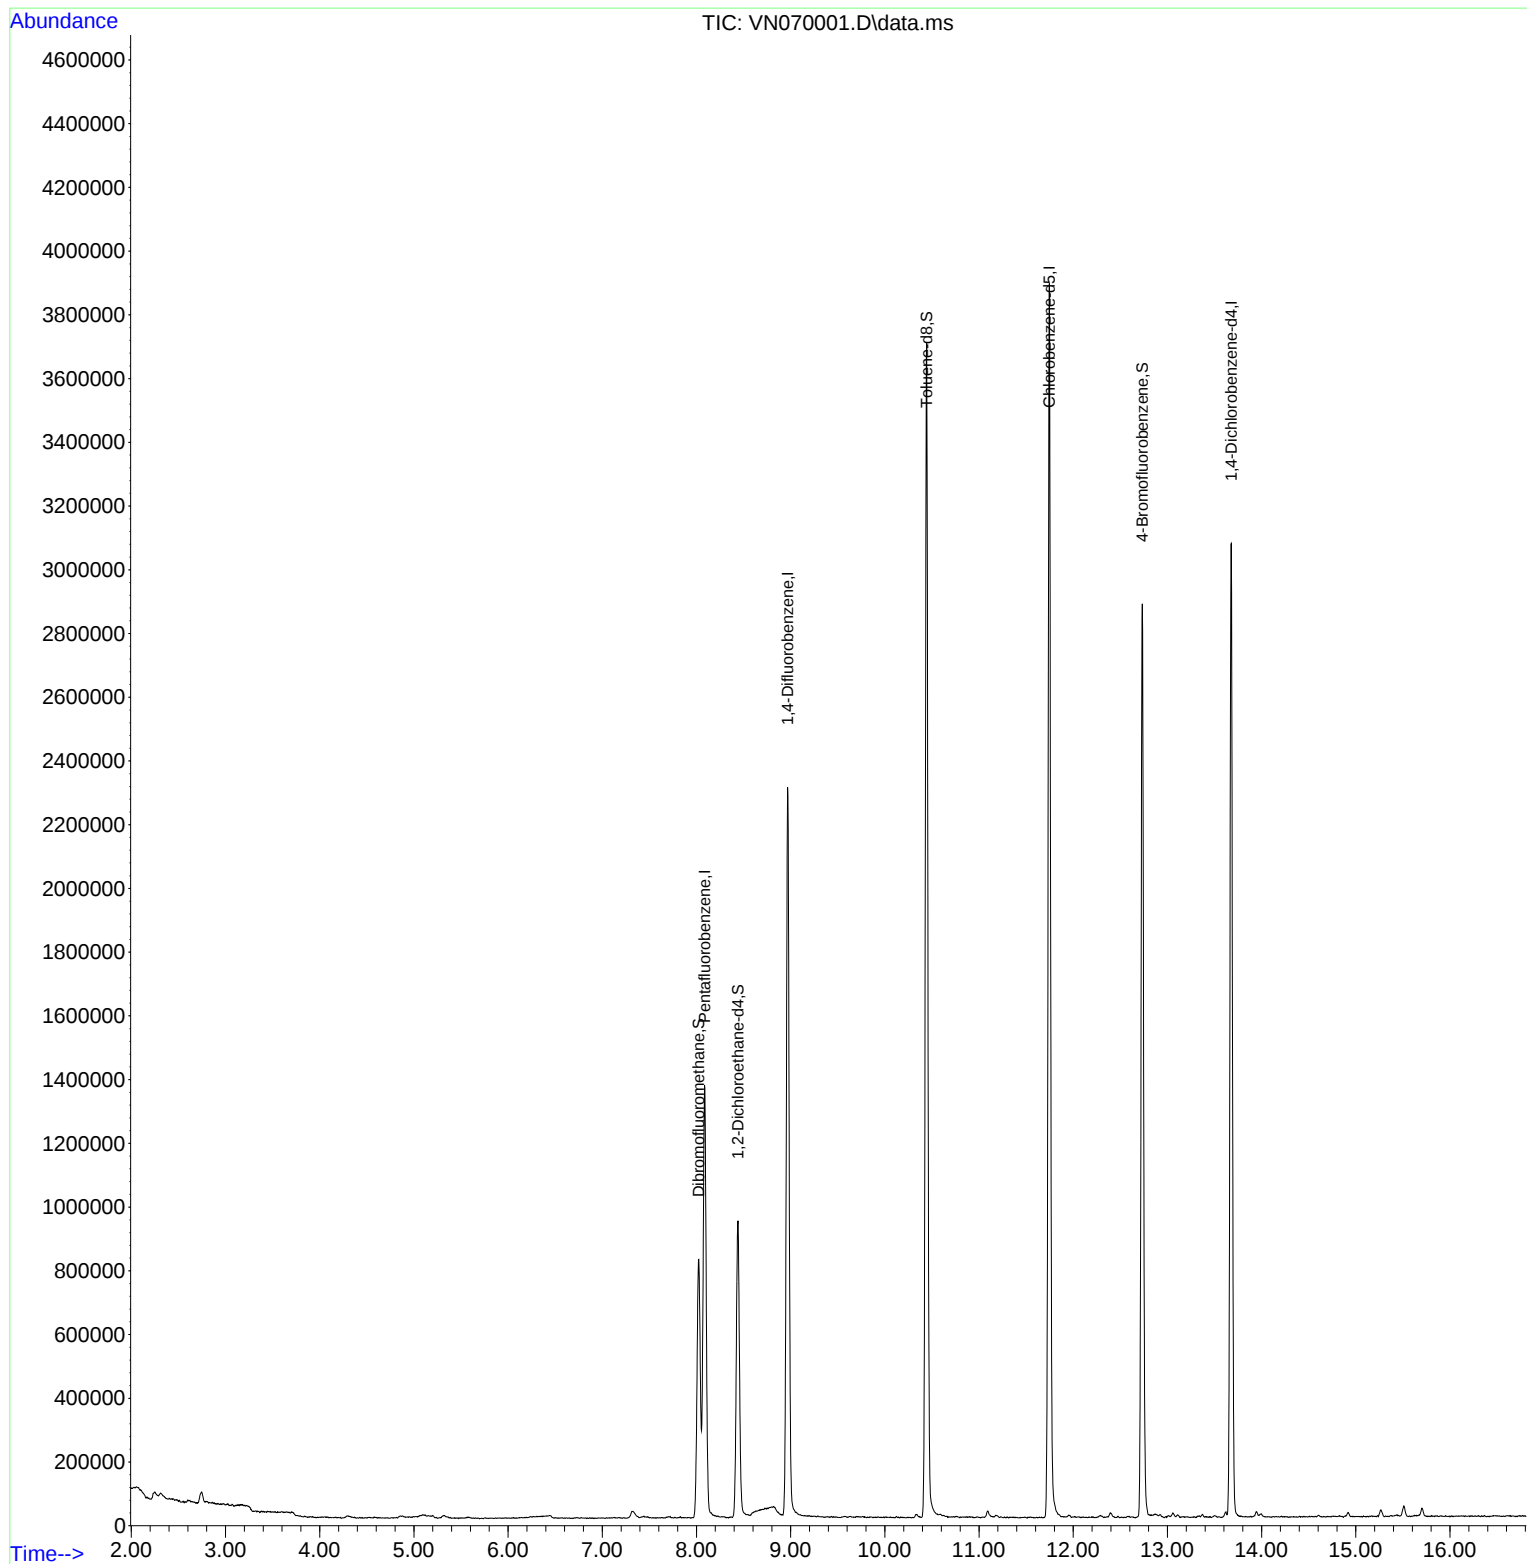


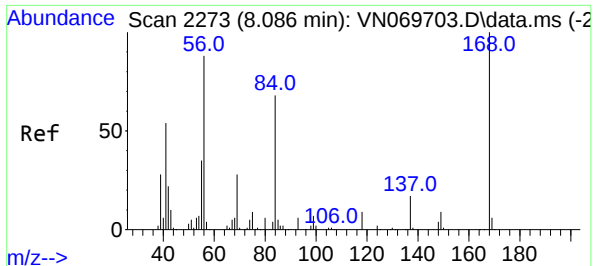

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.086 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN070001.D
Acq: 11 Dec 2021 11:51




Instrument :
MSVOA_N
ClientSampleId :
VN1211MBL01


Tgt Ion:168 Resp: 1000380
Ion Ratio Lower Upper
168 100
99 60.9 41.3 61.9

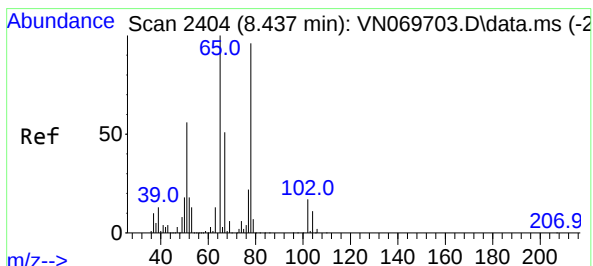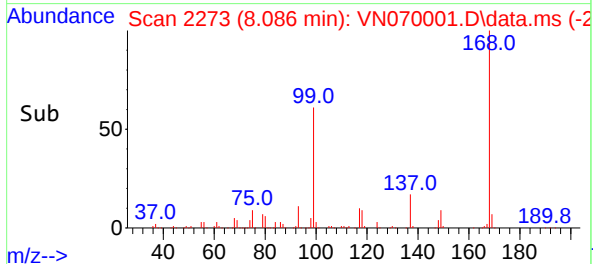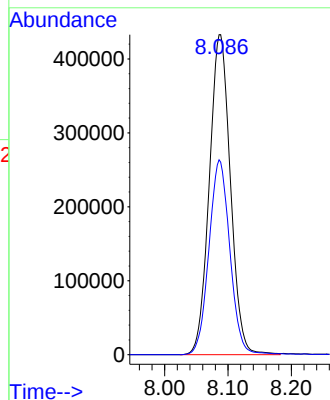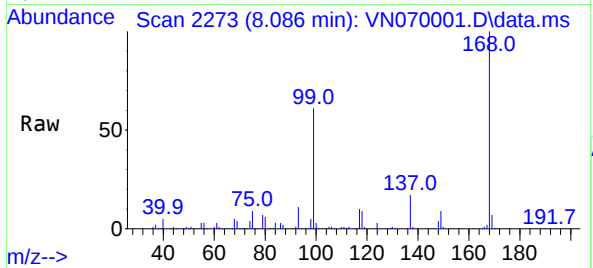

#33
1,2-Dichloroethane-d4
Concen: 52.279 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. 0.003 min
Lab File: VN070001.D
Acq: 11 Dec 2021 11:51

Tgt Ion: 65 Resp: 807501
Ion Ratio Lower Upper
65 100
67 51.1 0.0 103.0


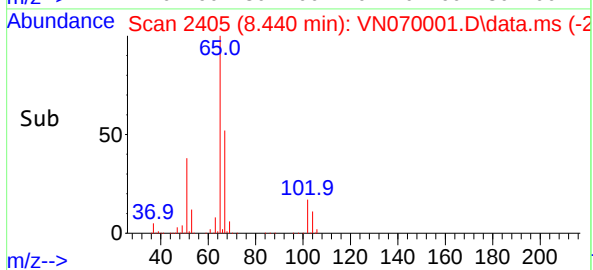
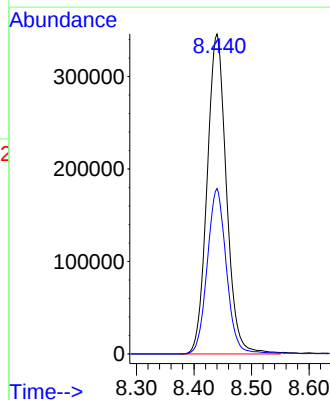
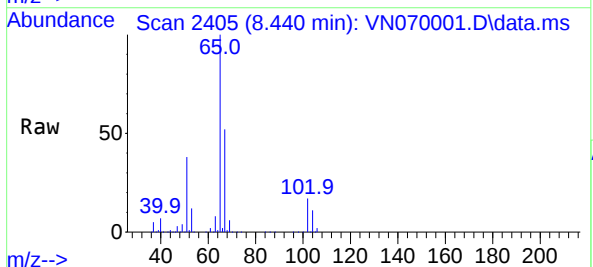


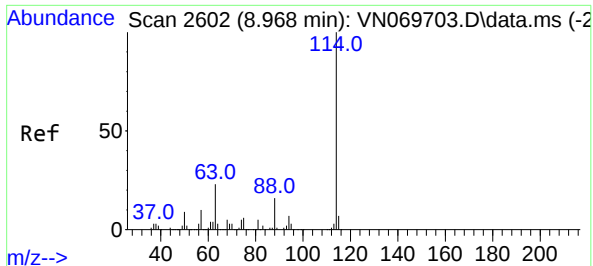

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.968 min Scan# 2602
Delta R.T. 0.000 min
Lab File: VN070001.D
Acq: 11 Dec 2021 11:51




Instrument :
MSVOA_N
ClientSampleId :
VN1211MBL01


Tgt Ion:114 Resp: 1901998
Ion Ratio Lower Upper
114 100
63 23.7 0.0 37.8
88 15.8 0.0 27.4

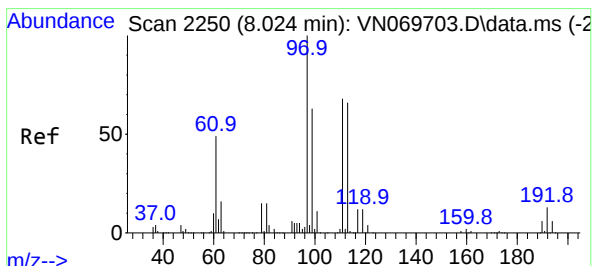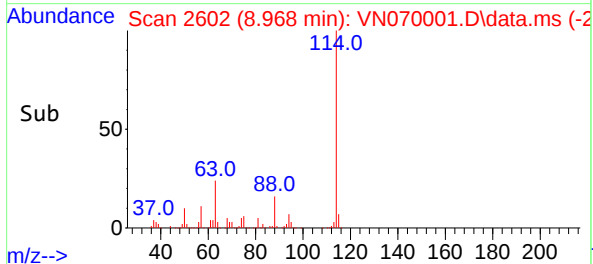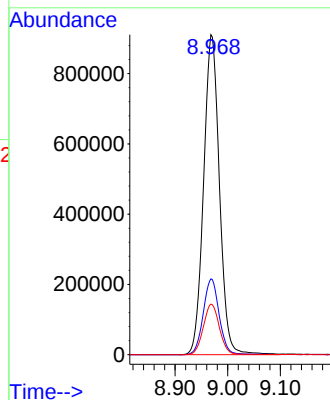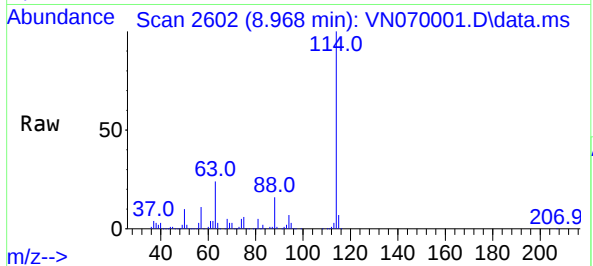

#35
Dibromofluoromethane
Concen: 50.008 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.000 min
Lab File: VN070001.D
Acq: 11 Dec 2021 11:51

Tgt Ion:113 Resp: 595786
Ion Ratio Lower Upper
113 100
111 103.6 82.2 123.2
192 18.8 16.9 25.3


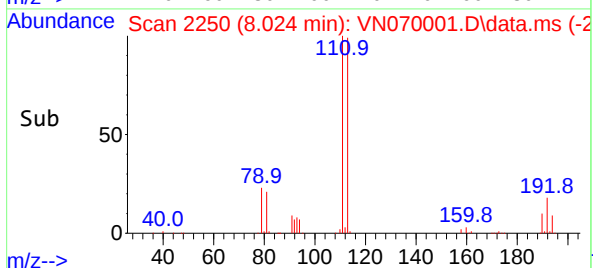
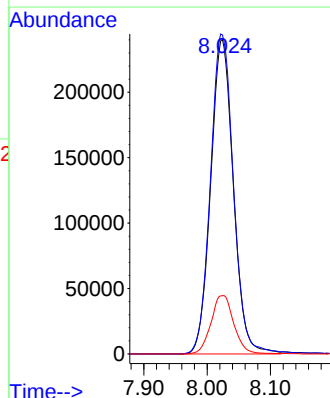
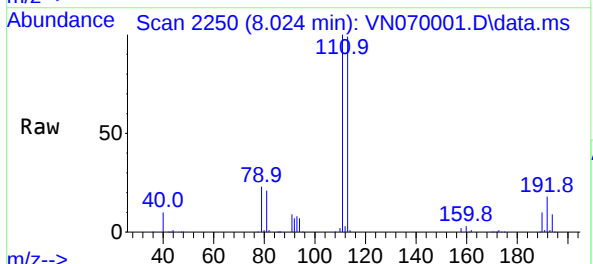


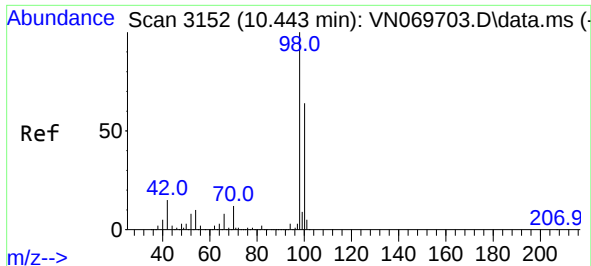

#50
Toluene-d8
Concen: 52.571 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. 0.000 min
Lab File: VN070001.D
Acq: 11 Dec 2021 11:51




Instrument :
MSVOA_N
ClientSampleId :
VN1211MBL01


Tgt Ion: 98 Resp: 2514846
Ion Ratio Lower Upper
98 100
100 63.3 50.4 75.6

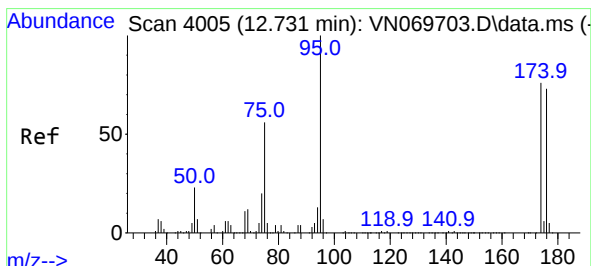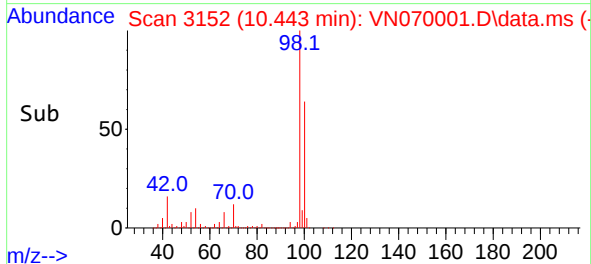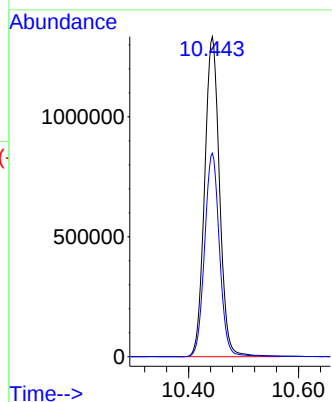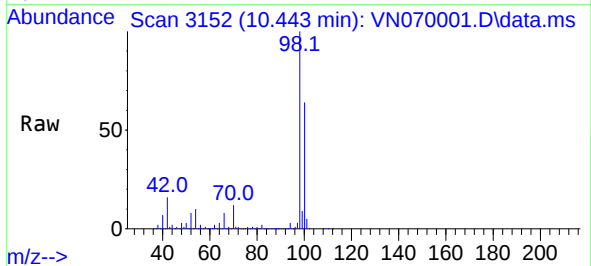

#62
4-Bromofluorobenzene
Concen: 58.364 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. 0.003 min
Lab File: VN070001.D
Acq: 11 Dec 2021 11:51


Tgt Ion: 95 Resp: 1011469
Ion Ratio Lower Upper
95 100
174 76.3 0.0 187.2
176 74.0 0.0 181.4

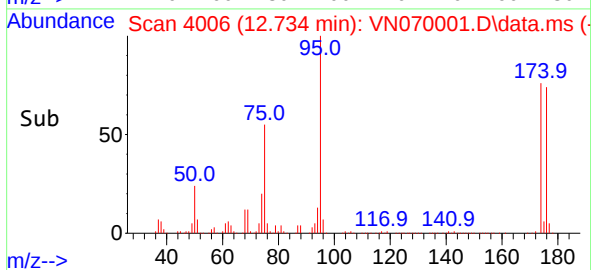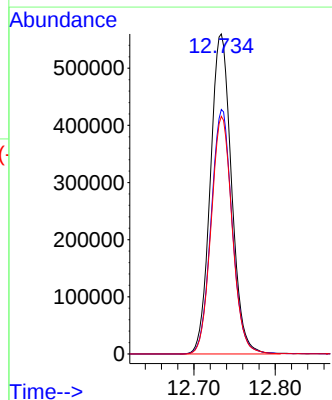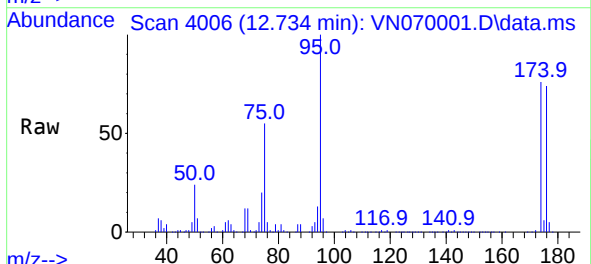

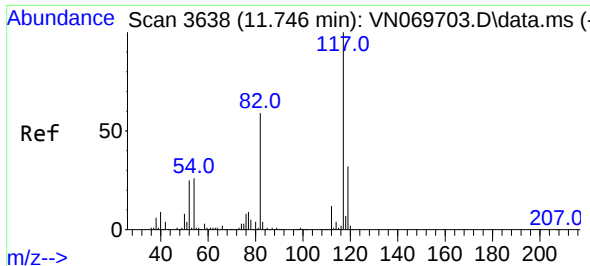




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.747 min Scan# 30
Delta R.T. 0.001 min
Lab File: VN070001.D
Acq: 11 Dec 2021 11:51

Instrument :
MSVOA_N
ClientSampleId :
VN1211MBL01

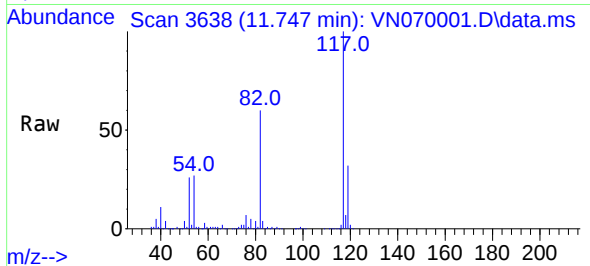

Tgt Ion:117 Resp: 2148427

Ion	Ratio	Lower	Upper
117	100		
82	59.9	42.4	63.6
119	32.1	25.4	38.2

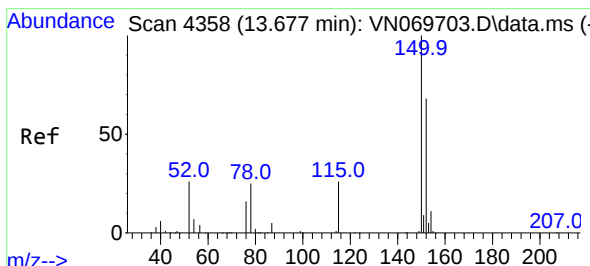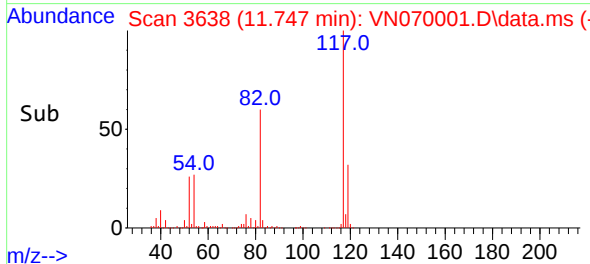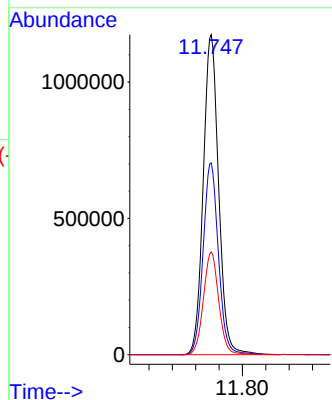

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.678 min Scan# 4358
Delta R.T. 0.000 min
Lab File: VN070001.D
Acq: 11 Dec 2021 11:51

Tgt Ion:152 Resp: 806451

Ion	Ratio	Lower	Upper
152	100		
115	62.4	27.5	82.5
150	159.0	0.0	344.4

