


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN121218\
Data File : VN052816.D
Acq On : 12 Dec 2018 8:26
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N112618W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Tue Nov 27 00:48:33 2018

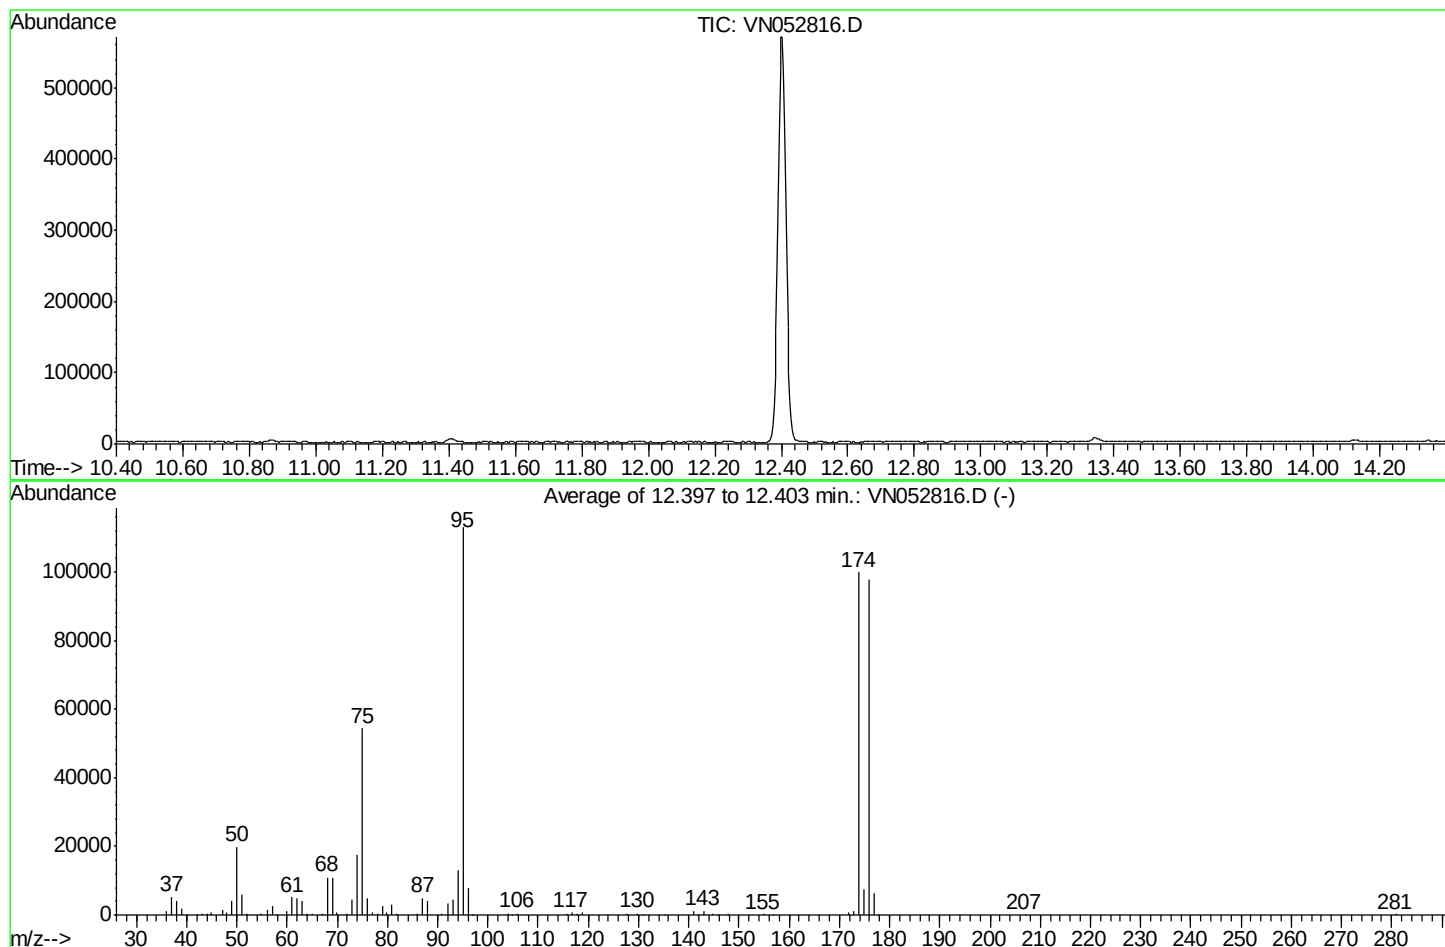

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	19968	PASS
75	95	30	60	48.2	54490	PASS
95	95	100	100	100.0	113064	PASS
96	95	5	9	7.1	7994	PASS
173	174	0.00	2	1.0	957	PASS
174	95	50	100	88.4	100002	PASS
175	174	5	9	7.4	7363	PASS
176	174	95	101	97.9	97925	PASS
177	176	5	9	6.4	6260	PASS