


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN121218\
Data File : VN052823.D
Acq On : 12 Dec 2018 13:23
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 8 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121218W.M
Title : SW846 8260
Last Update : Thu Dec 13 01:08:35 2018

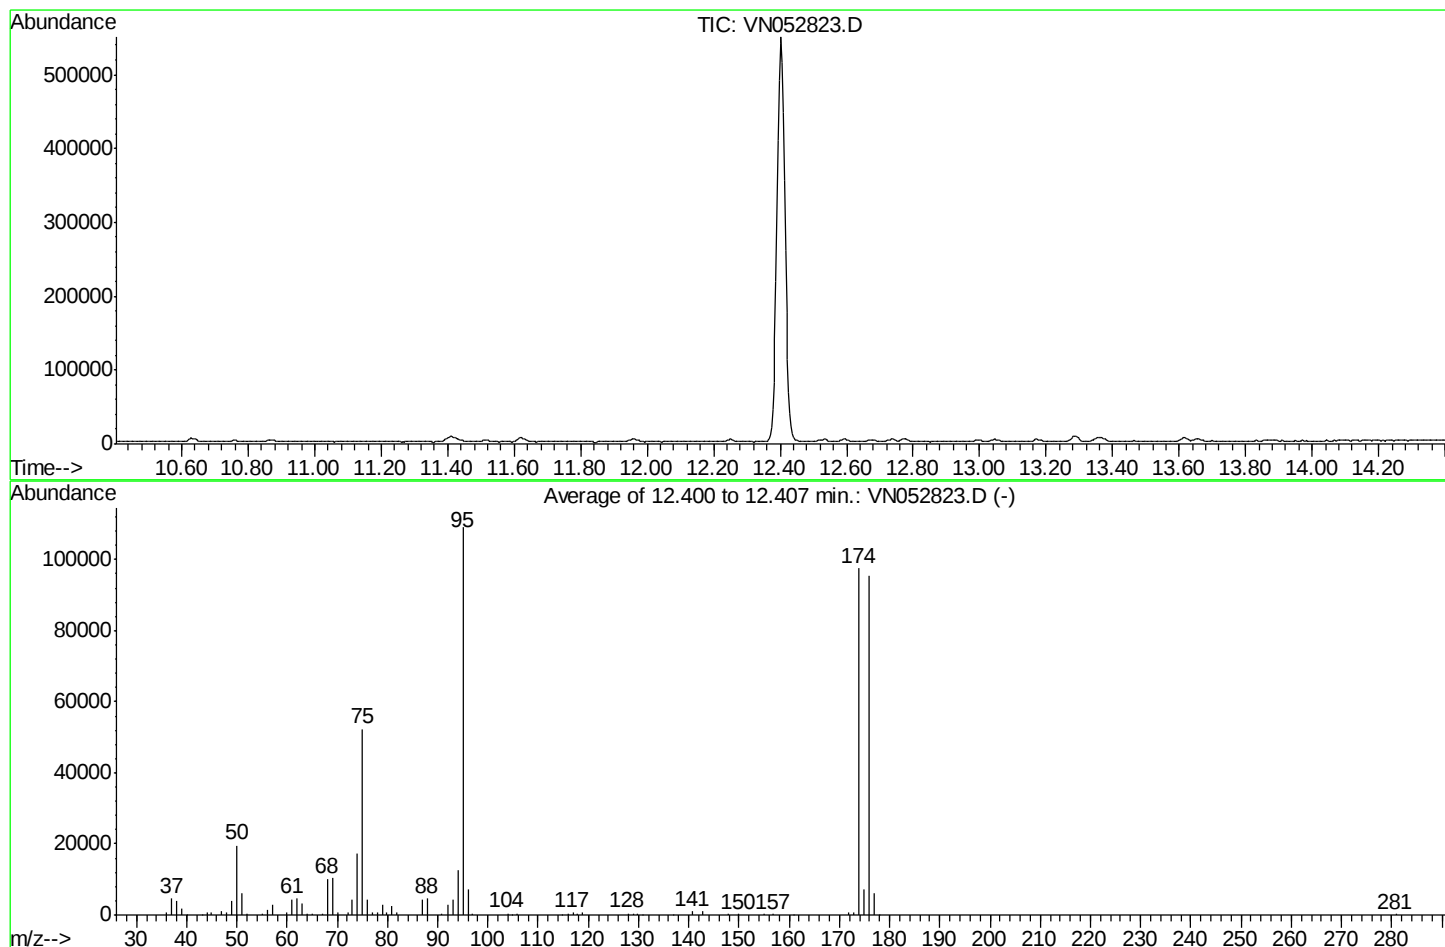

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	19589	PASS
75	95	30	60	48.0	52328	PASS
95	95	100	100	100.0	109056	PASS
96	95	5	9	6.7	7294	PASS
173	174	0.00	2	0.8	826	PASS
174	95	50	100	89.3	97440	PASS
175	174	5	9	7.4	7190	PASS
176	174	95	101	97.9	95442	PASS
177	176	5	9	6.5	6218	PASS