

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN121219\
 Data File : VN059576.D
 Acq On : 12 Dec 2019 15:53
 Operator : JC/SP
 Sample : VN1212WBSD01
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1212WBSD01

Quant Time: Dec 13 04:07:29 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N120919W.M
 Quant Title : SW846 8260
 QLast Update : Tue Dec 10 01:09:52 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0	0.00	ug/l	-7.64
34) 1,4-Difluorobenzene	0.00	114	0	0.00	ug/l	-8.57
63) Chlorobenzene-d5	0.00	117	0	0.00	ug/l	-11.40
72) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ug/l	-13.34
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	0.00	65	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
35) Dibromofluoromethane	0.00	113	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
50) Toluene-d8	0.00	98	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
62) 4-Bromofluorobenzene	12.37	95	182	0.00	ug/l	-0.03
Spiked Amount 50.000			Recovery	=	0.00%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_N\DATA\VN121219\
Data File : VN059576.D
Acq On : 12 Dec 2019 15:53
Operator : JC/SP
Sample : VN1212WBSD01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1212WBSD01

Quant Time: Dec 13 04:07:29 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N120919W.M
Quant Title : SW846 8260
QLast Update : Tue Dec 10 01:09:52 2019
Response via : Initial Calibration

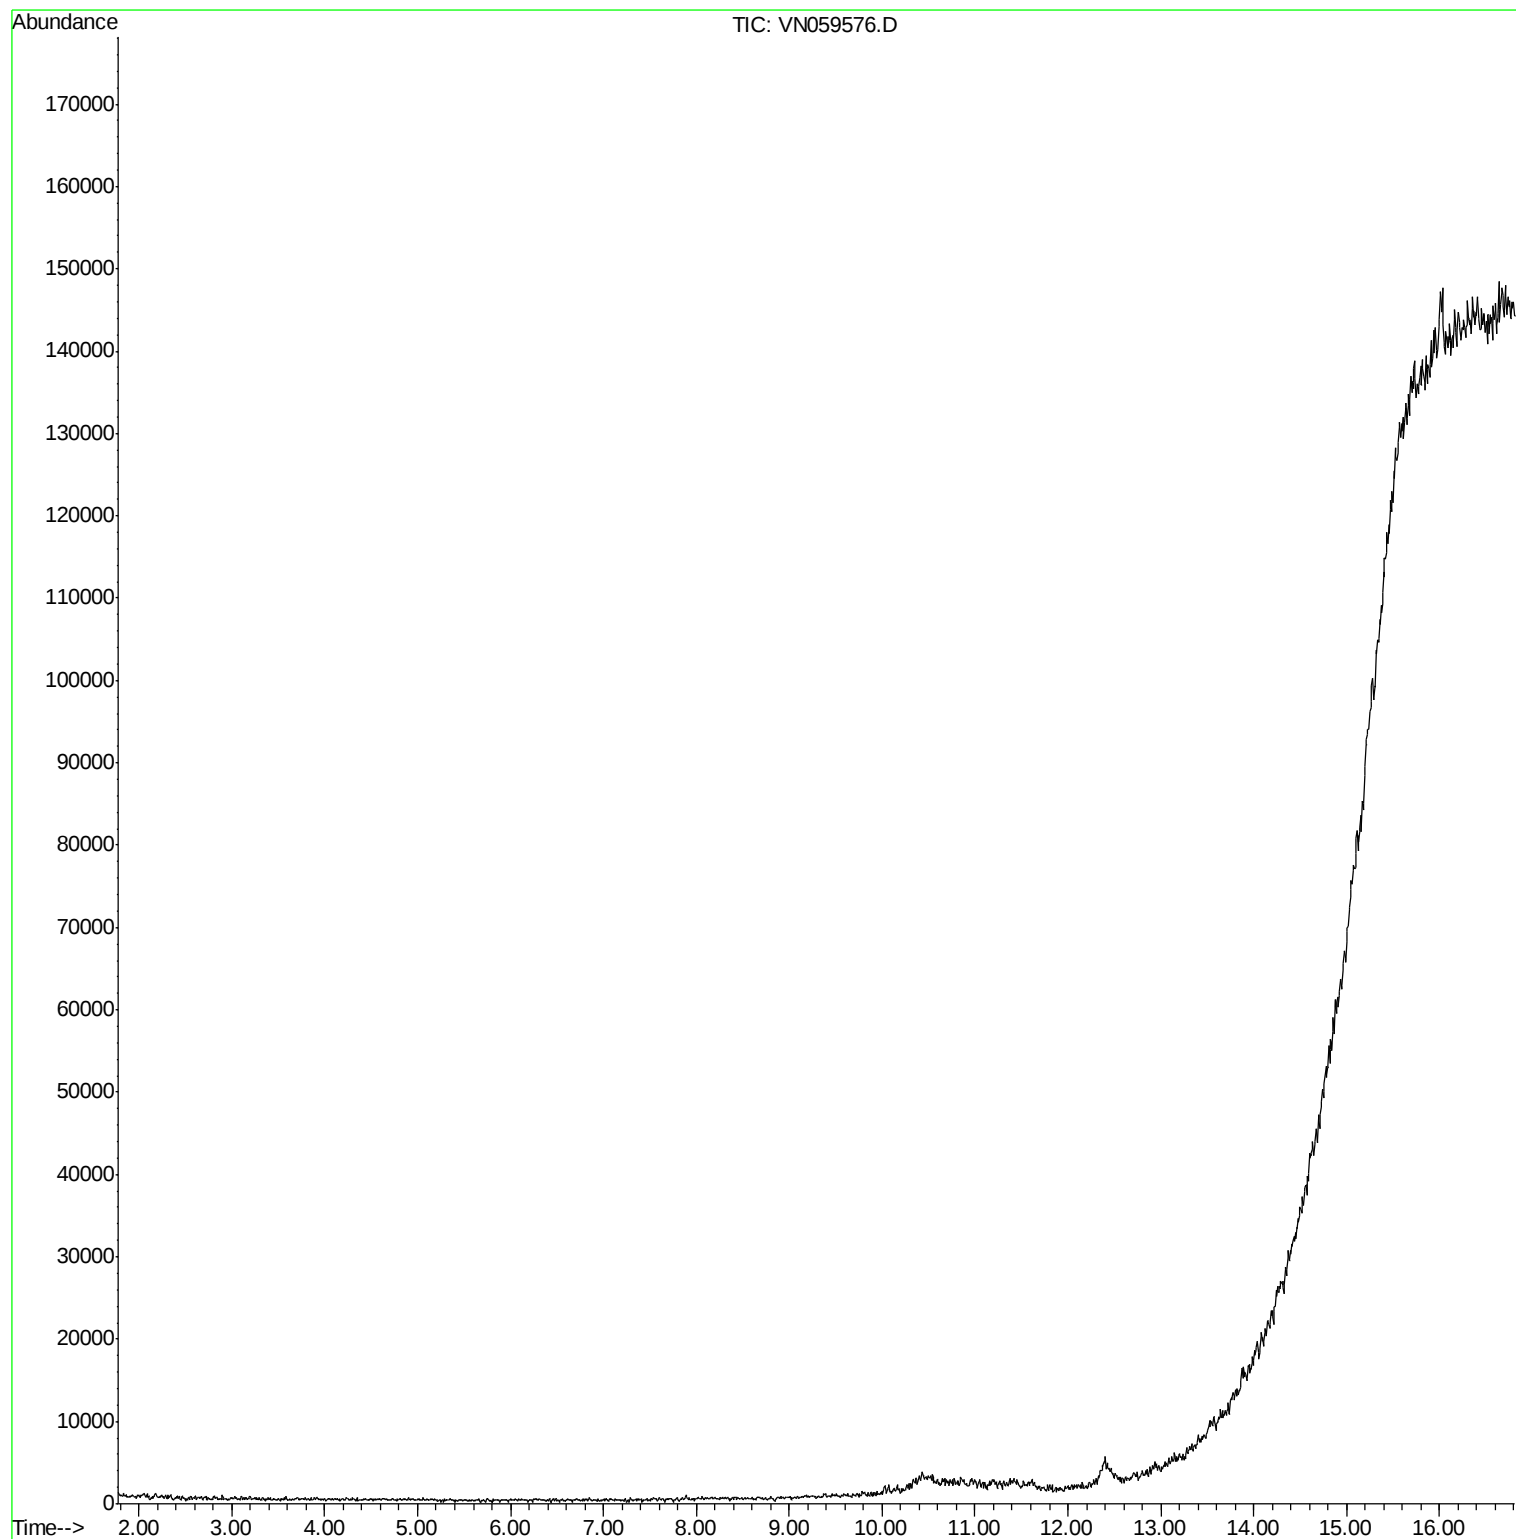

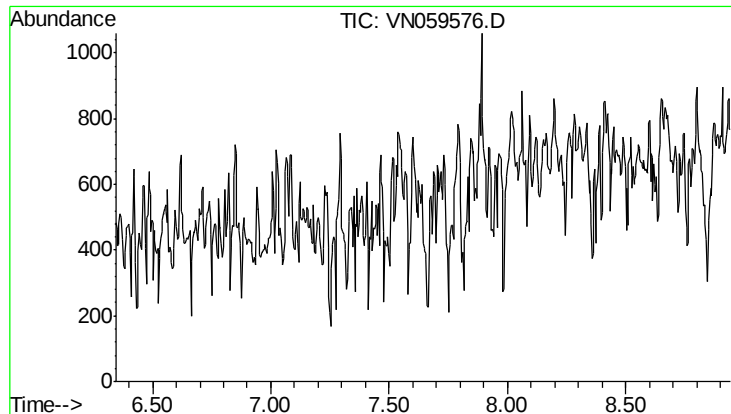

#1

Pentafluorobenzene

Concen: 0.000 ug/l

Expected RT: 7.64 min

Lab File: VN059576.D

Acq: 12 Dec 2019 15:53

Tgt Ion: 168

Sig Exp Ratio

168 100



99 58.3

Instrument :

MSVOA_N

ClientSampleId :

VN1212WBSD01

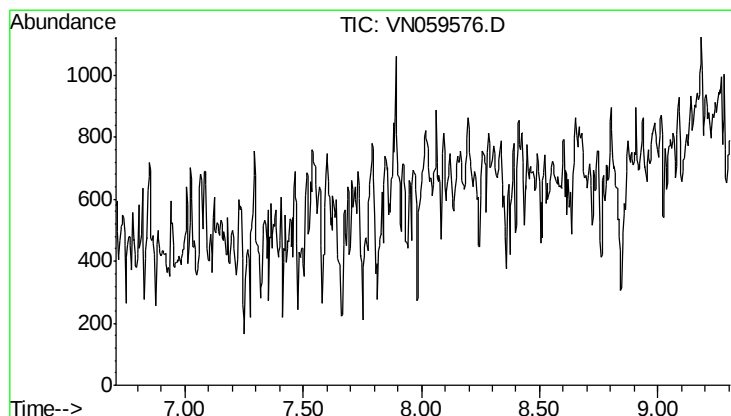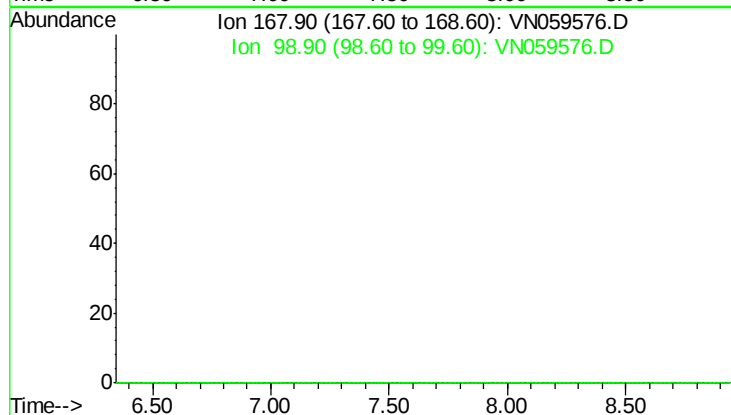

#33

1,2-Dichloroethane-d4

Concen: 0.000 ug/l

Expected RT: 8.01 min

Lab File: VN059576.D


Acq: 12 Dec 2019 15:53


Tgt Ion: 65

Sig Exp Ratio

65 100

67 51.8


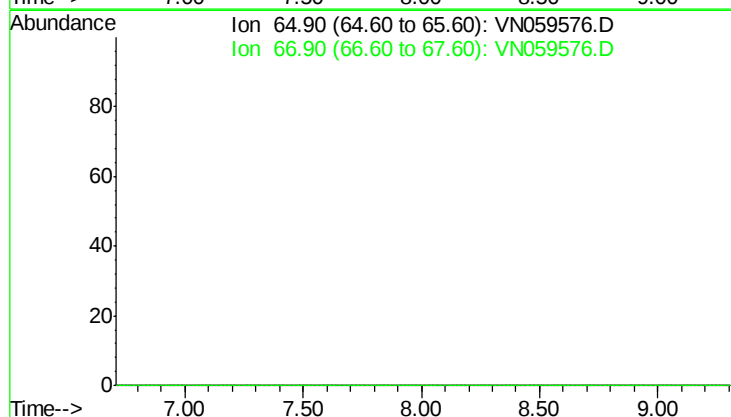


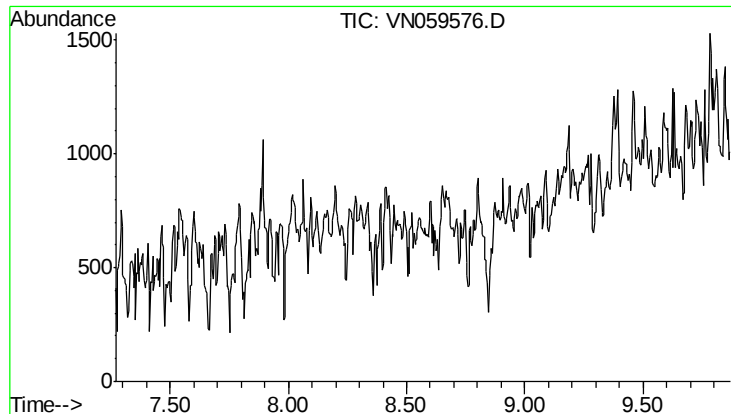

#34
 1,4-Difluorobenzene
 Concen: 0.000 ug/l
 Expected RT: 8.57 min
 Lab File: VN059576.D
 Acq: 12 Dec 2019 15:53


Instrument :
 MSVOA_N
 ClientSampleId :
 VN1212WBSD01


Tgt Ion	Exp Ratio
114	100
63	22.5
88	16.1

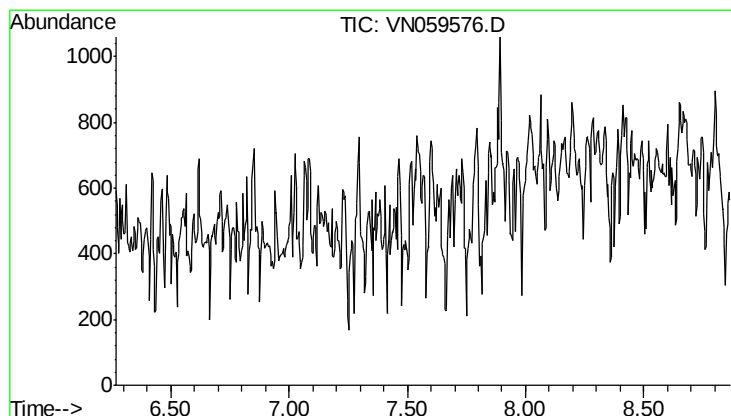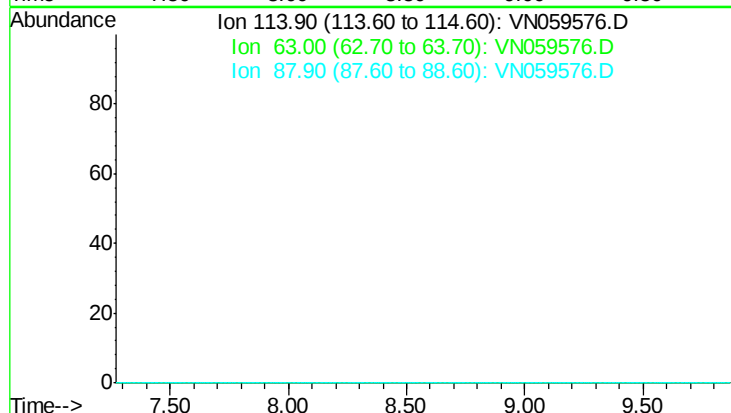

#35
 Dibromofluoromethane
 Concen: 0.000 ug/l
 Expected RT: 7.57 min
 Lab File: VN059576.D
 Acq: 12 Dec 2019 15:53

Tgt Ion	Exp Ratio
113	100
111	102.8
192	18.5

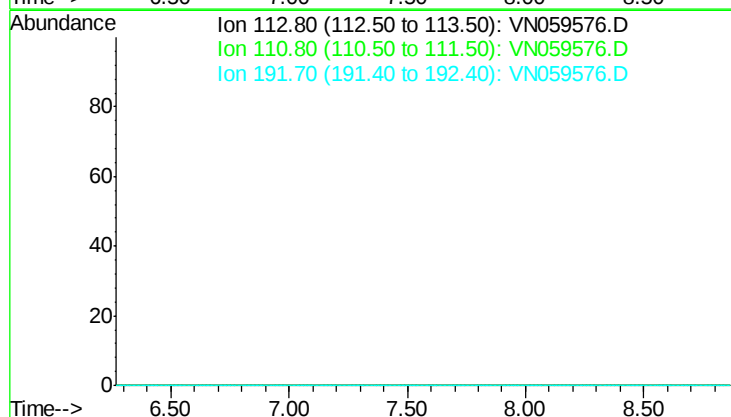


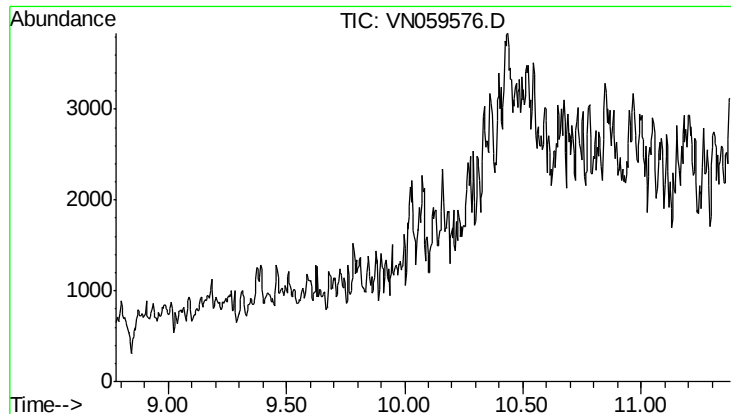


#50
Toluene-d8
Concen: 0.000 ug/l
Expected RT: 10.08 min

Lab File: VN059576.D
Acq: 12 Dec 2019 15:53




Instrument :
MSVOA_N
ClientSampleId :
VN1212WBSD01


Tgt Ion: 98
Sig Exp Ratio
98 100
100 64.8

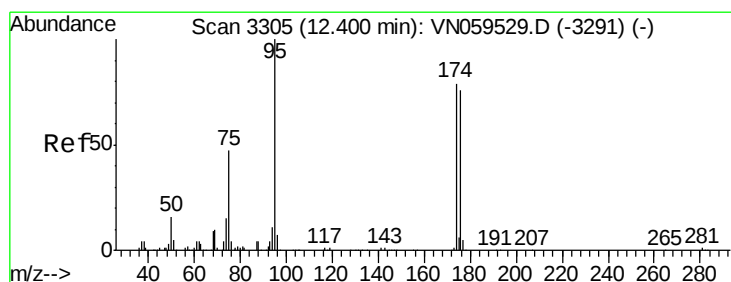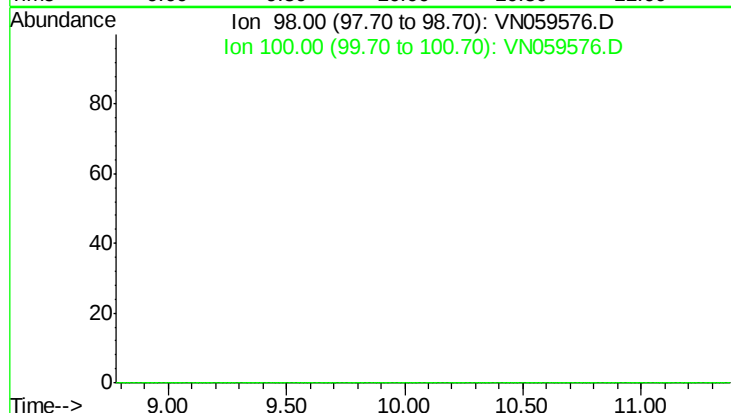

#62
4-Bromofluorobenzene
Concen: 0.000 ug/l
RT: 12.37 min Scan# 3297
Delta R.T. -0.03 min
Lab File: VN059576.D
Acq: 12 Dec 2019 15:53

Tgt Ion: 95 Resp: 182
Ion Ratio Lower Upper
95 100
174 0.0 0.0 158.0
176 0.0 0.0 155.4

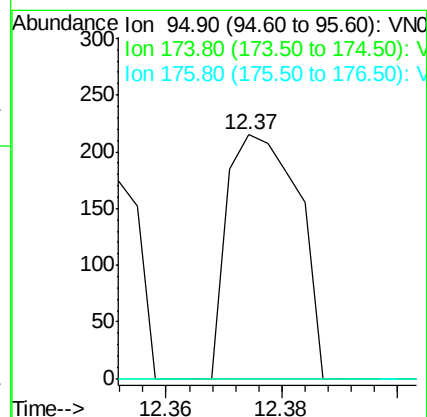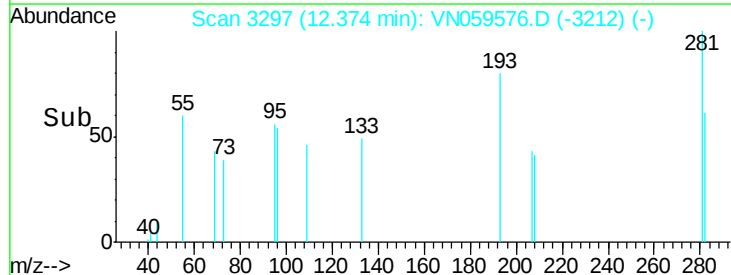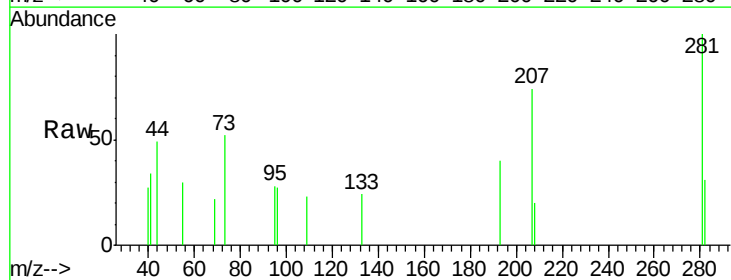


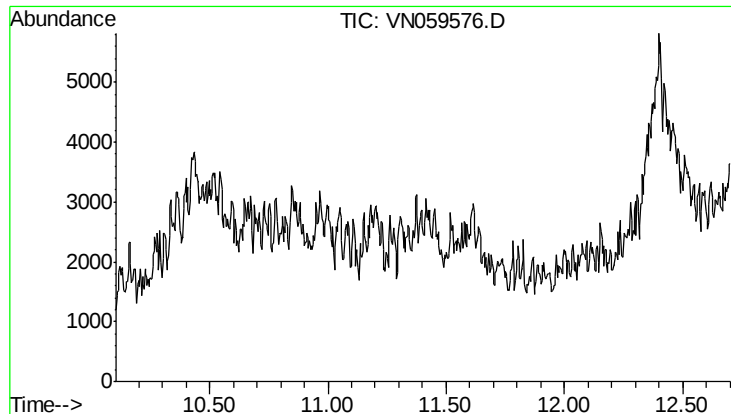


#63
 Chlorobenzene-d5
 Concen: 0.000 ug/l
 Expected RT: 11.40 min

Lab File: VN059576.D
 Acq: 12 Dec 2019 15:53

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1212WBSD01

Tgt Ion: 117
 Sig Exp Ratio
 117 100
 82 58.1
 119 31.5

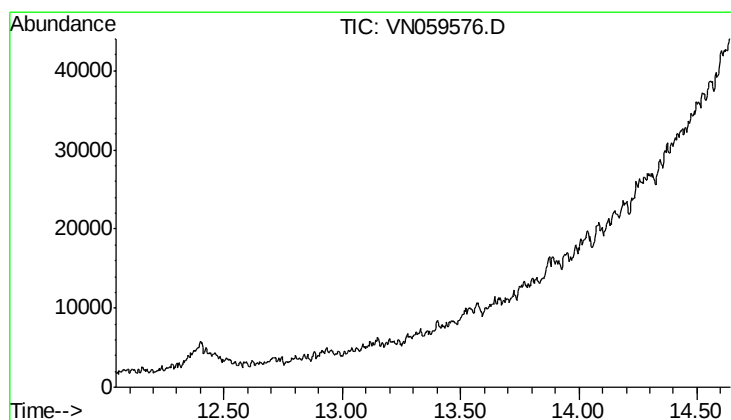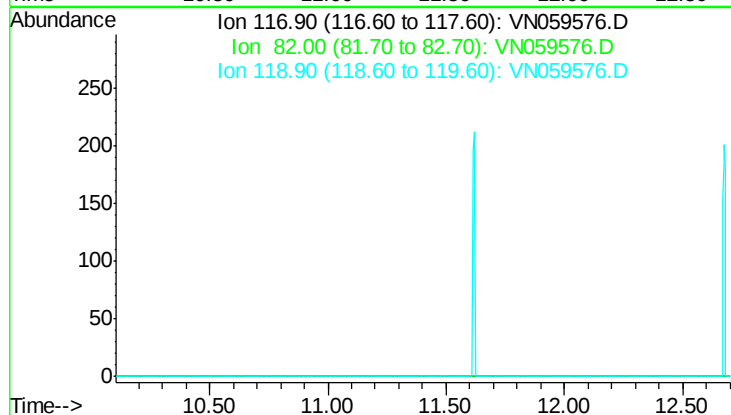

#72
 1,4-Dichlorobenzene-d4
 Concen: 0.000 ug/l
 Expected RT: 13.34 min

Lab File: VN059576.D
 Acq: 12 Dec 2019 15:53

Tgt Ion: 152
 Sig Exp Ratio
 152 100
 115 58.8
 150 171.2

