

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121222\
 Data File : VN075707.D
 Acq On : 12 Dec 2022 12:44
 Operator : JC\MD
 Sample : VN1212WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1212WBL01

Quant Time: Dec 13 01:32:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120922W.M
 Quant Title : SW846 8260
 QLast Update : Mon Dec 12 07:54:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.229	168	234510	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	364622	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	320790	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	143772	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	119576	48.057	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	96.120%
35) Dibromofluoromethane	8.177	113	109233	49.102	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	98.200%
50) Toluene-d8	10.570	98	416375	49.839	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	99.680%
62) 4-Bromofluorobenzene	12.853	95	133825	46.850	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	93.700%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121222\
Data File : VN075707.D
Acq On : 12 Dec 2022 12:44
Operator : JC\MD
Sample : VN1212WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1212WBL01

Quant Time: Dec 13 01:32:08 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120922W.M
Quant Title : SW846 8260
QLast Update : Mon Dec 12 07:54:35 2022
Response via : Initial Calibration




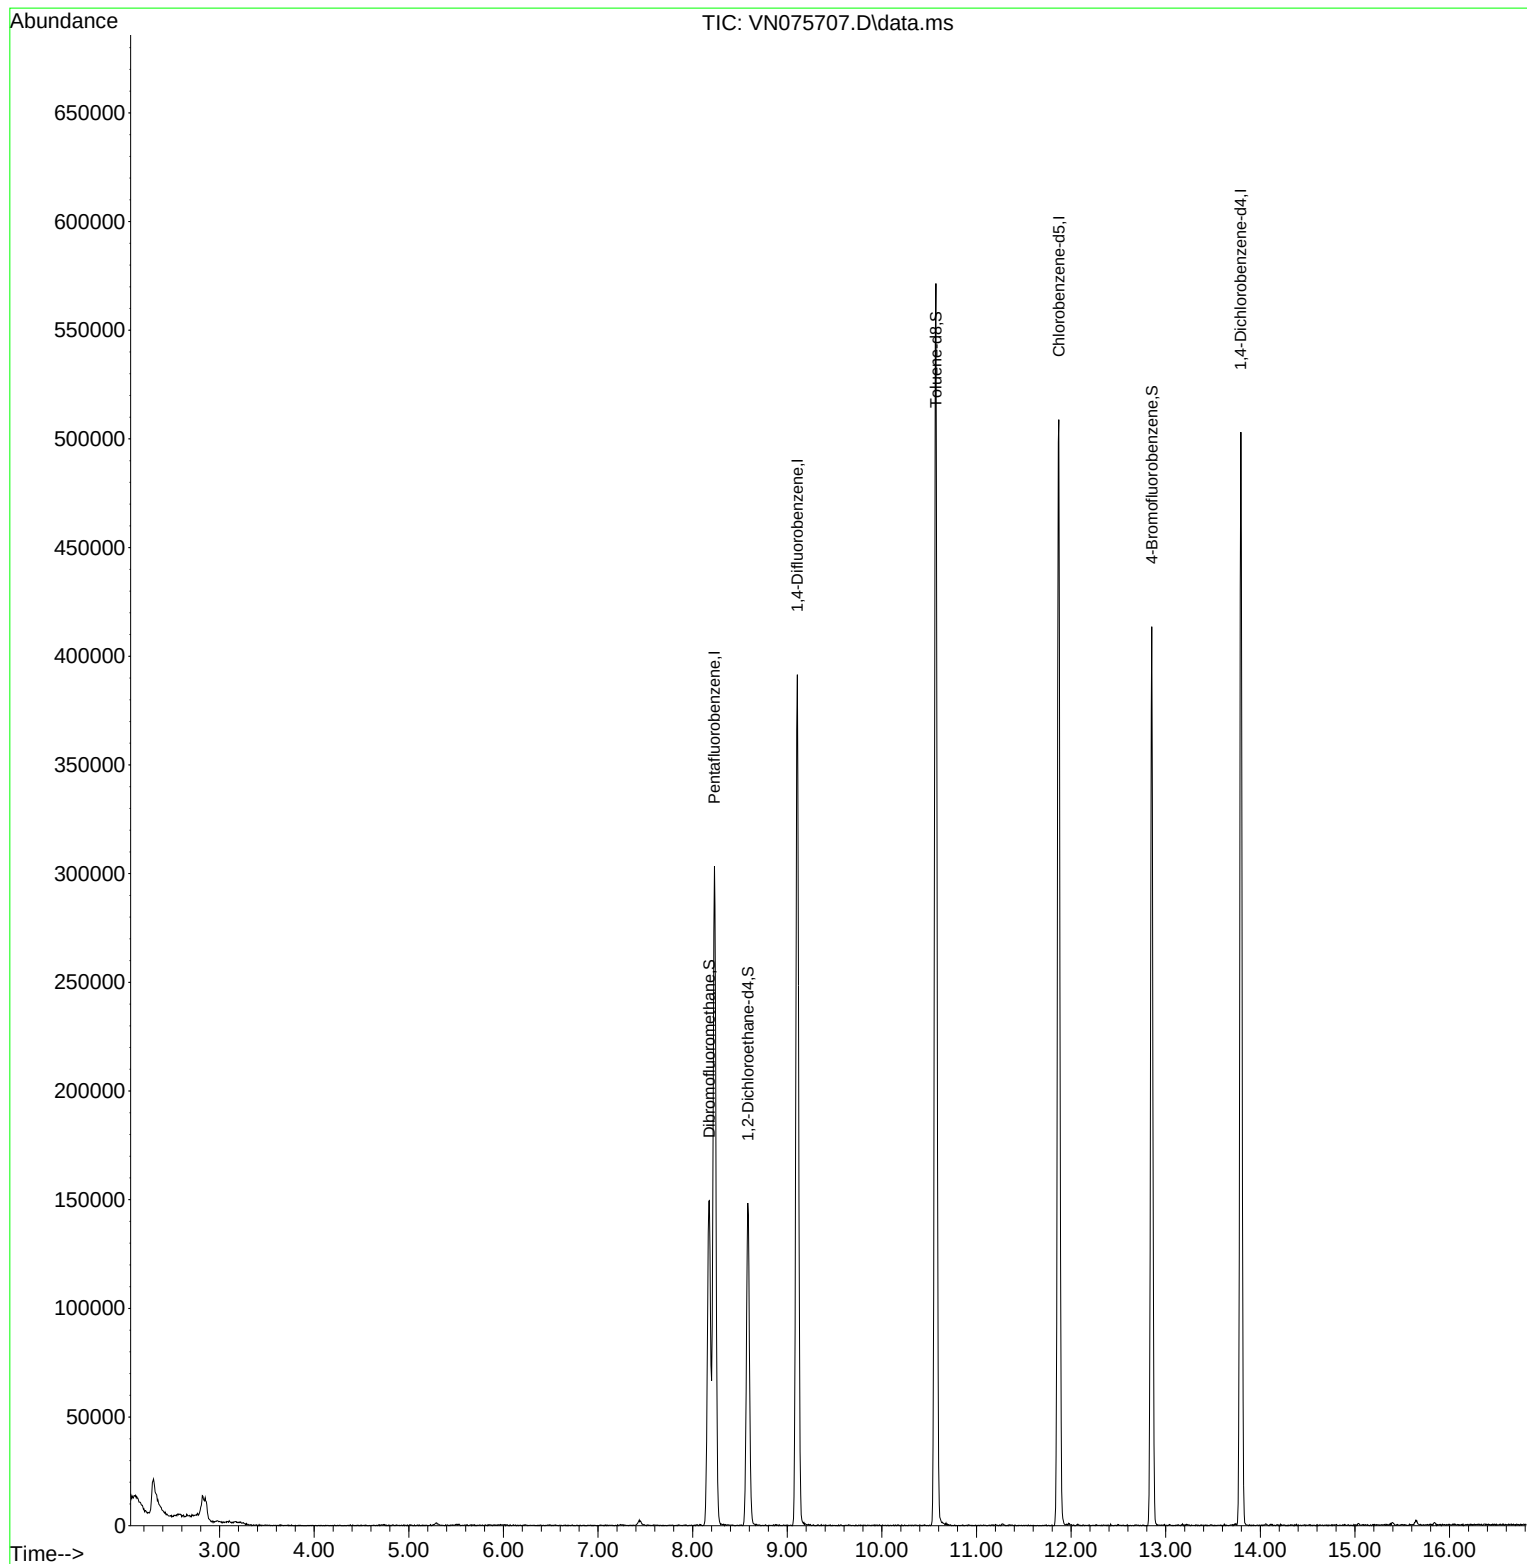


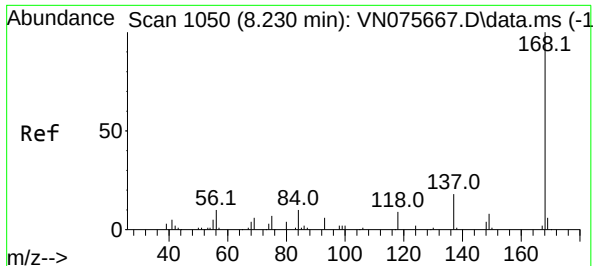

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.229 min Scan# 110
Delta R.T. -0.001 min
Lab File: VN075707.D
Acq: 12 Dec 2022 12:44




Instrument :
MSVOA_N
ClientSampleId :
VN1212WBL01


Tgt Ion:168 Resp: 234510
Ion Ratio Lower Upper
168 100
99 55.8 41.2 61.8

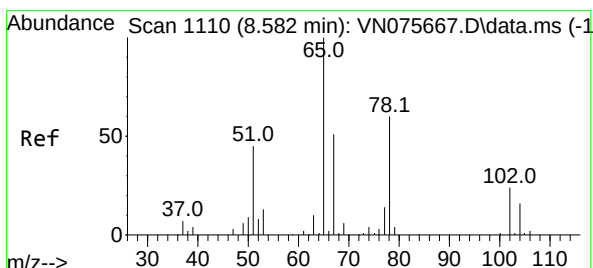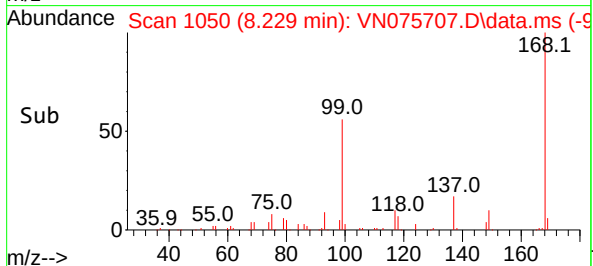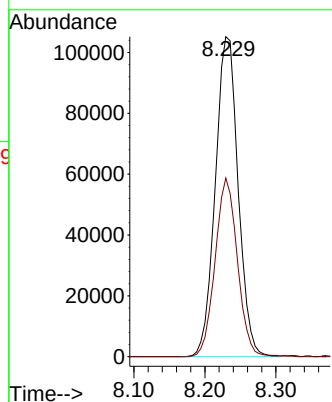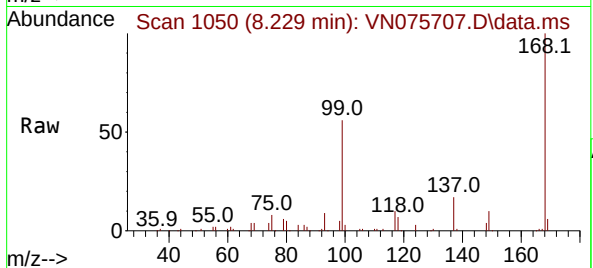

#33
1,2-Dichloroethane-d4
Concen: 48.057 ug/l
RT: 8.582 min Scan# 1110
Delta R.T. -0.000 min
Lab File: VN075707.D
Acq: 12 Dec 2022 12:44

Tgt Ion: 65 Resp: 119576
Ion Ratio Lower Upper
65 100
67 53.1 0.0 104.2

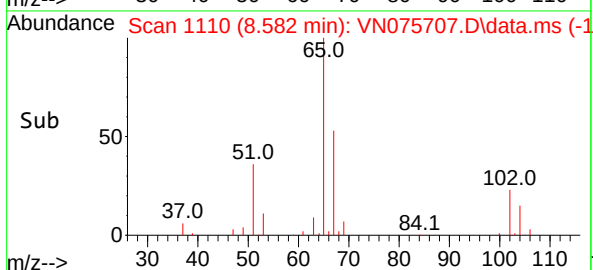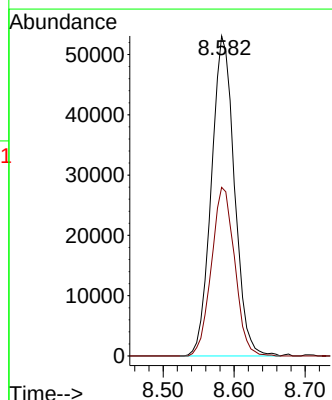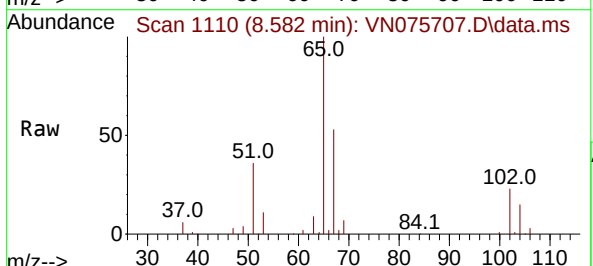

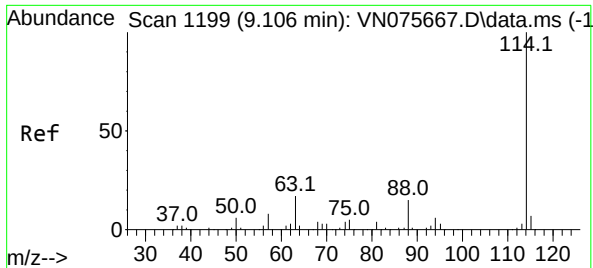

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1199

Delta R.T. -0.000 min

Lab File: VN075707.D

Acq: 12 Dec 2022 12:44

Instrument :

MSVOA_N

ClientSampleId :

VN1212WBL01





Tgt Ion:114 Resp: 364622

Ion Ratio Lower Upper

114 100

63 17.5 0.0 34.4

88 15.0 0.0 29.2

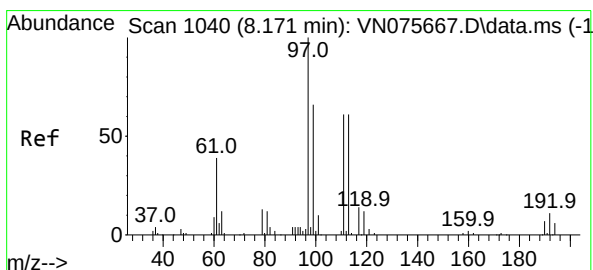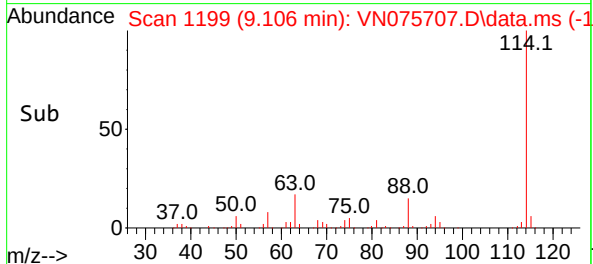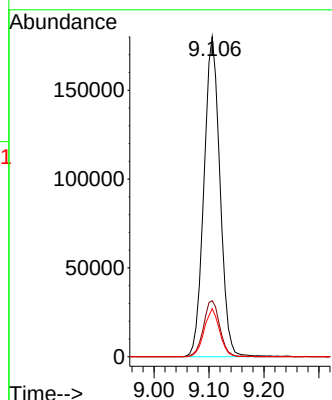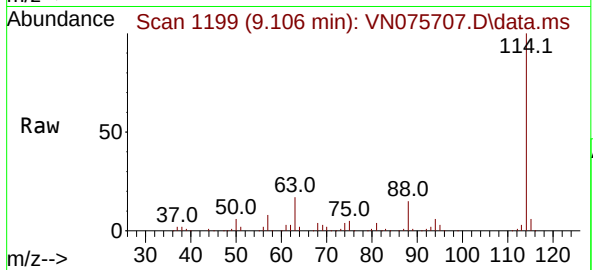

#35

Dibromofluoromethane

Concen: 49.102 ug/l

RT: 8.177 min Scan# 1041

Delta R.T. 0.006 min

Lab File: VN075707.D

Acq: 12 Dec 2022 12:44




Tgt Ion:113 Resp: 109233


Ion Ratio Lower Upper

113 100

111 102.7 81.0 121.6

192 19.9 16.2 24.2


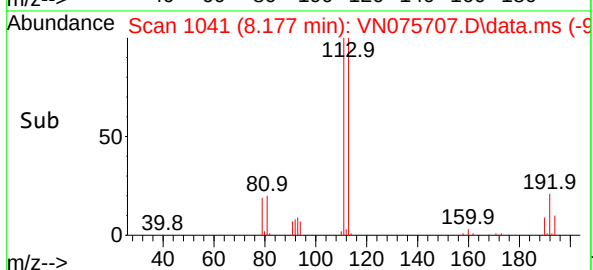
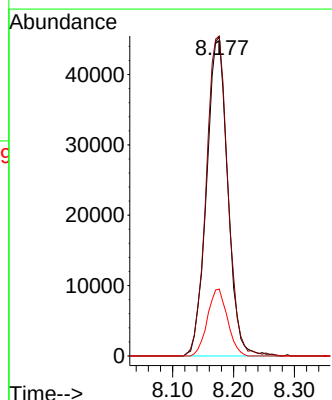
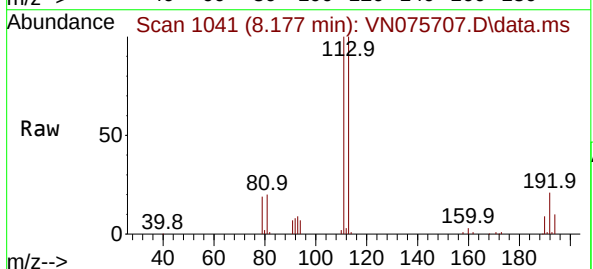


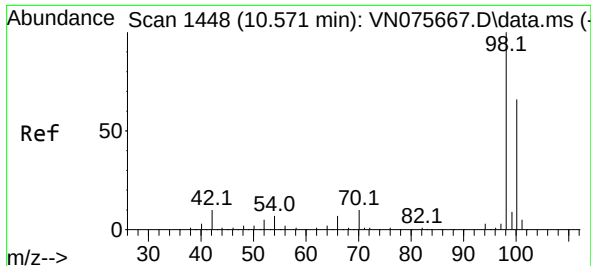

#50
Toluene-d8
Concen: 49.839 ug/l
RT: 10.570 min Scan# 1448
Delta R.T. -0.000 min
Lab File: VN075707.D
Acq: 12 Dec 2022 12:44




Instrument :
MSVOA_N
ClientSampleId :
VN1212WBL01


Tgt Ion: 98 Resp: 416375
Ion Ratio Lower Upper
98 100
100 65.5 52.6 78.8

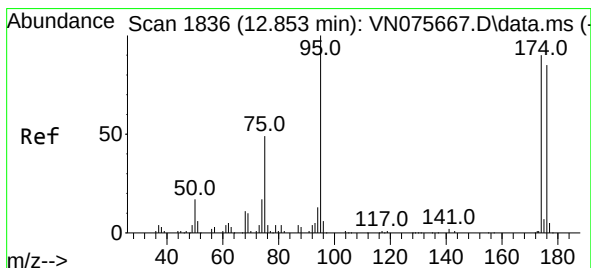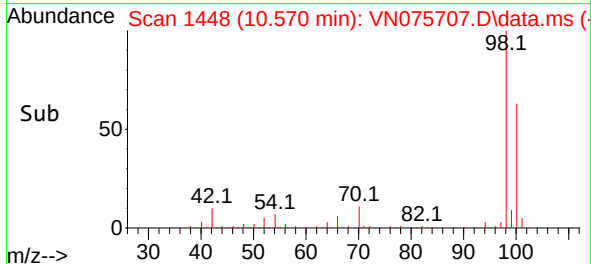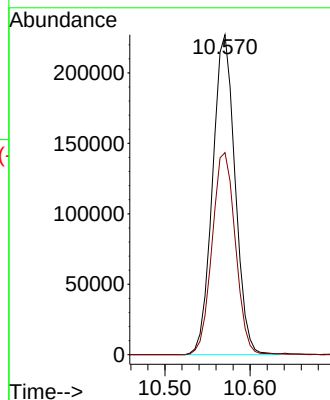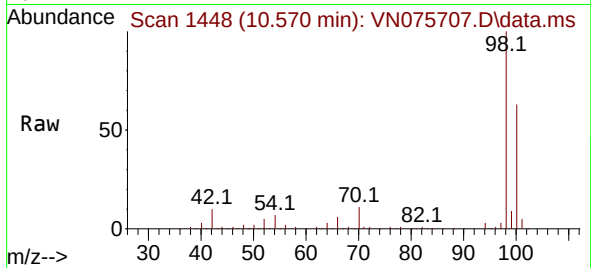

#62
4-Bromofluorobenzene
Concen: 46.850 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. -0.000 min
Lab File: VN075707.D
Acq: 12 Dec 2022 12:44

Tgt Ion: 95 Resp: 133825
Ion Ratio Lower Upper
95 100
174 89.5 0.0 178.6
176 85.4 0.0 170.8


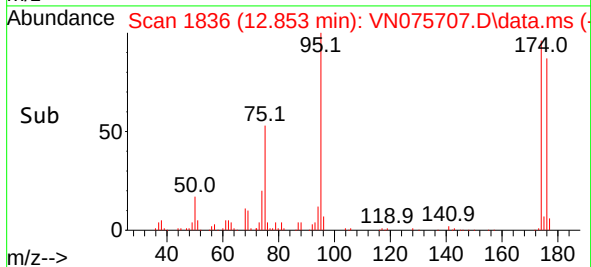
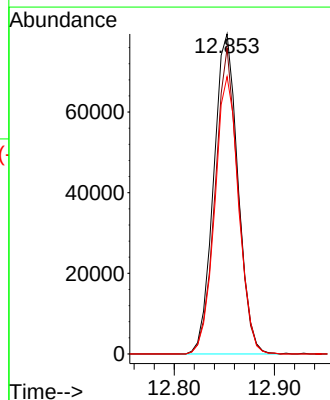
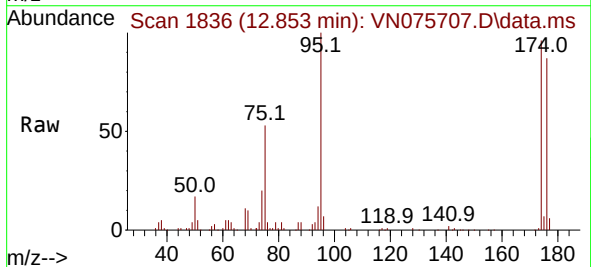


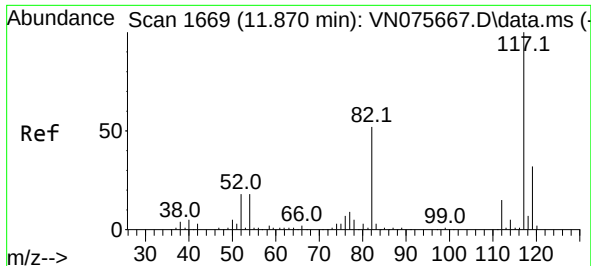

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 1669
Delta R.T. -0.000 min
Lab File: VN075707.D
Acq: 12 Dec 2022 12:44

Instrument :
MSVOA_N
ClientSampleId :
VN1212WBL01

Tgt Ion:117 Resp: 320790
Ion Ratio Lower Upper
117 100
82 50.7 41.8 62.8
119 31.9 25.8 38.6

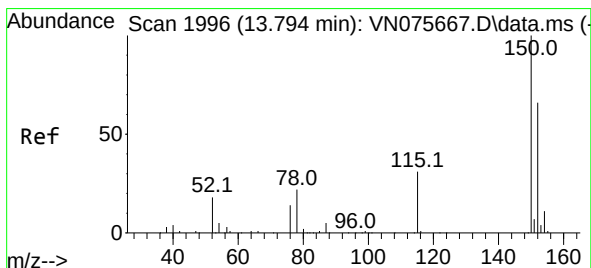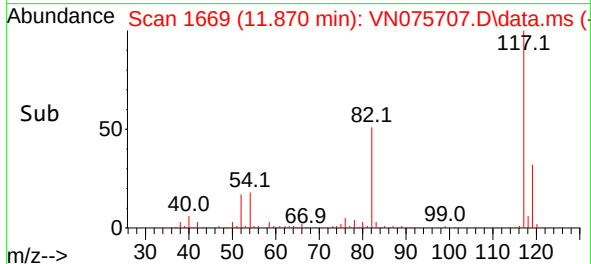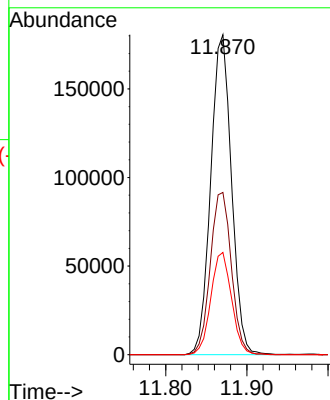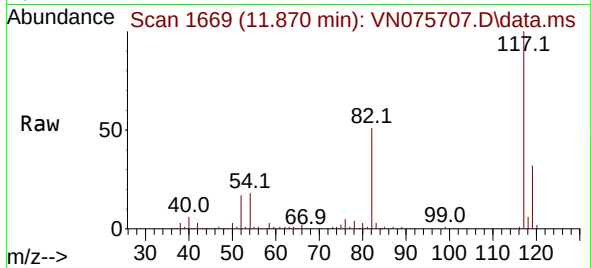

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. -0.000 min
Lab File: VN075707.D
Acq: 12 Dec 2022 12:44

Tgt Ion:152 Resp: 143772
Ion Ratio Lower Upper
152 100
115 56.6 28.4 85.2
150 155.1 0.0 347.6

