

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121222\
 Data File : VN075753.D
 Acq On : 13 Dec 2022 10:03
 Operator : JC\MD
 Sample : N5951-02
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-5

Quant Time: Dec 13 13:05:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120922W.M
 Quant Title : SW846 8260
 QLast Update : Mon Dec 12 07:54:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.230	168	247156	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	395847	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	336726	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	144385	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	125721	47.941	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	95.880%
35) Dibromofluoromethane	8.171	113	117063	48.471	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	96.940%
50) Toluene-d8	10.571	98	448214	49.418	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	98.840%
62) 4-Bromofluorobenzene	12.847	95	137564	44.361	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	88.720%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121222\
Data File : VN075753.D
Acq On : 13 Dec 2022 10:03
Operator : JC\MD
Sample : N5951-02
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Quant Time: Dec 13 13:05:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120922W.M
Quant Title : SW846 8260
QLast Update : Mon Dec 12 07:54:35 2022
Response via : Initial Calibration




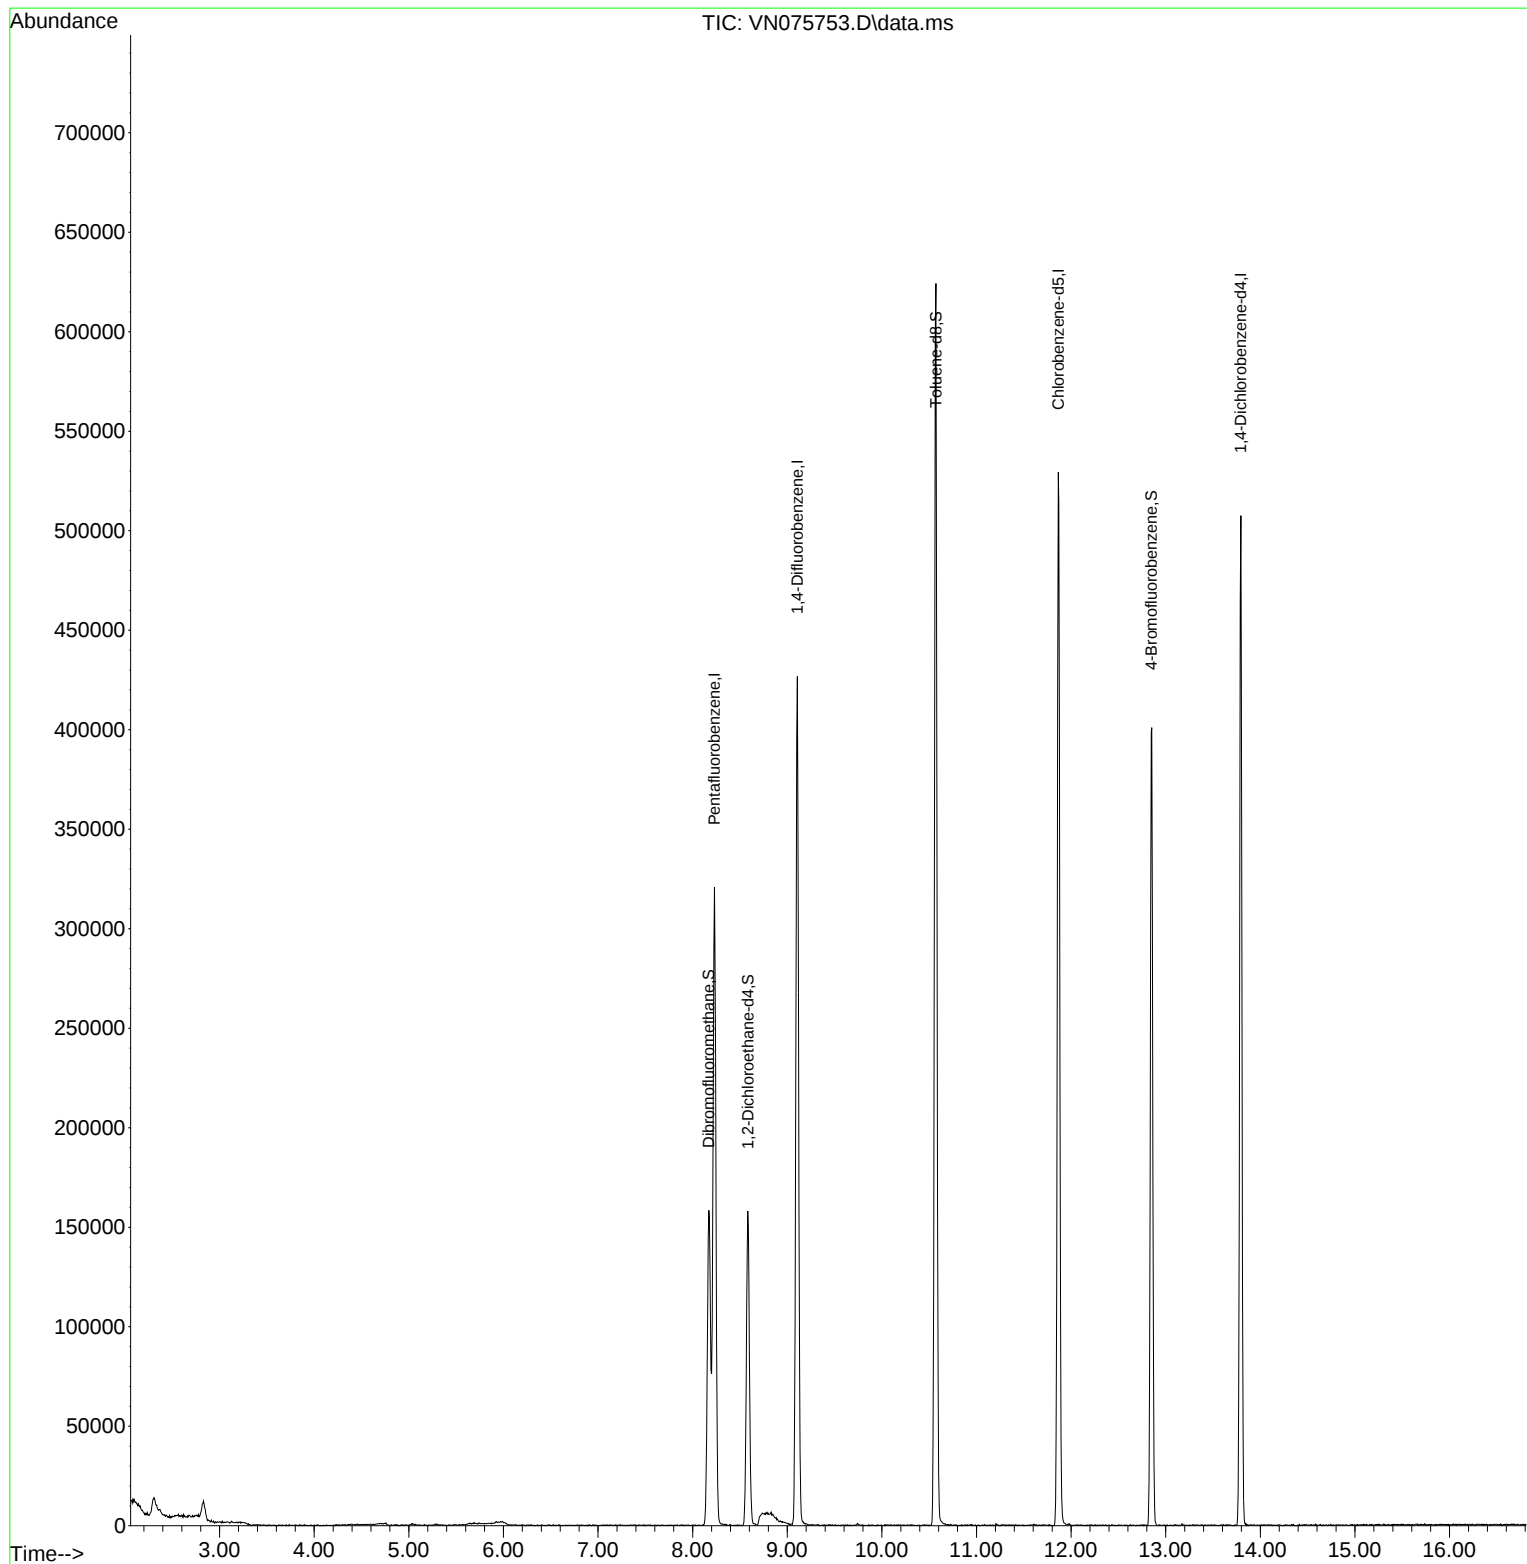


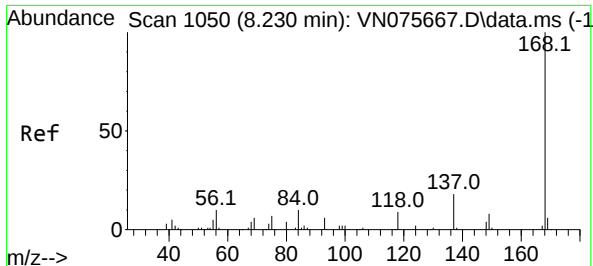

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1105
Delta R.T. -0.000 min
Lab File: VN075753.D
Acq: 13 Dec 2022 10:03




Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-WATER-REF-5


Tgt Ion:168 Resp: 247156
Ion Ratio Lower Upper
168 100
99 56.3 41.2 61.8

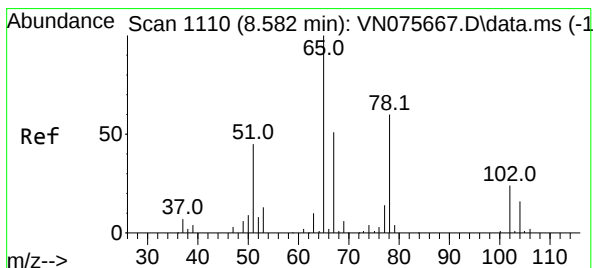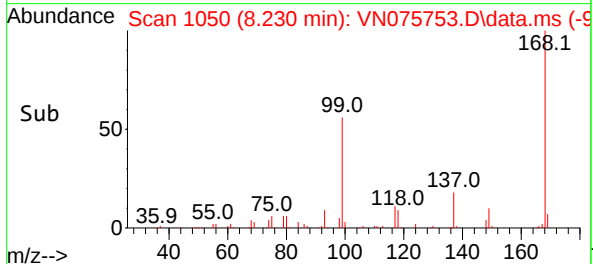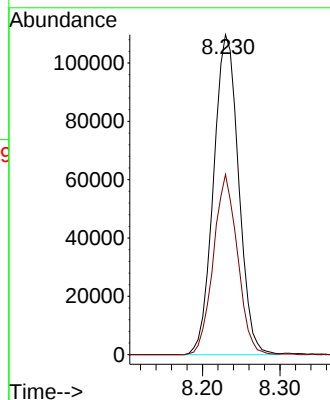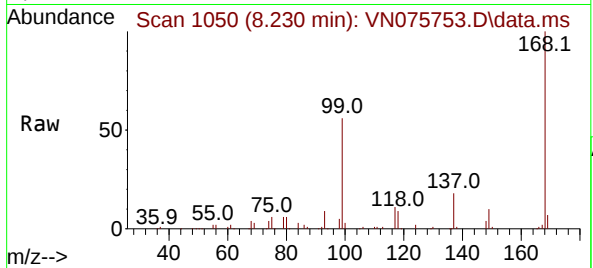

#33
1,2-Dichloroethane-d4
Concen: 47.941 ug/l
RT: 8.583 min Scan# 1110
Delta R.T. 0.000 min
Lab File: VN075753.D
Acq: 13 Dec 2022 10:03

Tgt Ion: 65 Resp: 125721
Ion Ratio Lower Upper
65 100
67 52.2 0.0 104.2

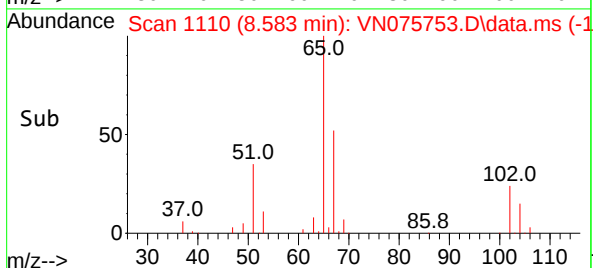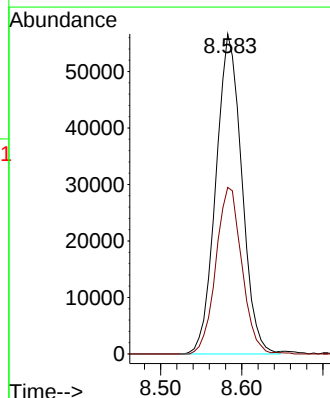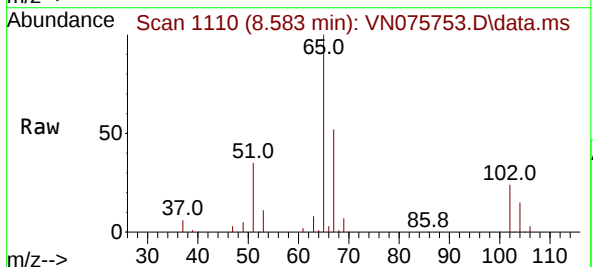

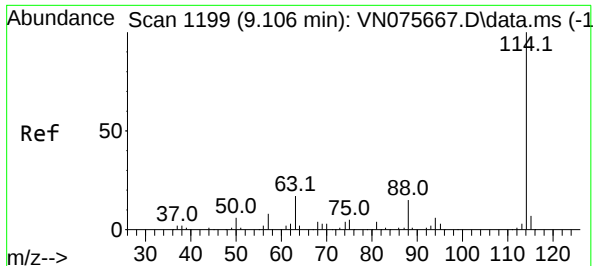

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1199

Delta R.T. 0.000 min

Lab File: VN075753.D

Acq: 13 Dec 2022 10:03

Instrument :

MSVOA_N

ClientSampleId :

STORAGE-BLANK-WATER-REF-5





Tgt Ion:114 Resp: 395847

Ion Ratio Lower Upper

114 100

63 17.3 0.0 34.4

88 13.8 0.0 29.2

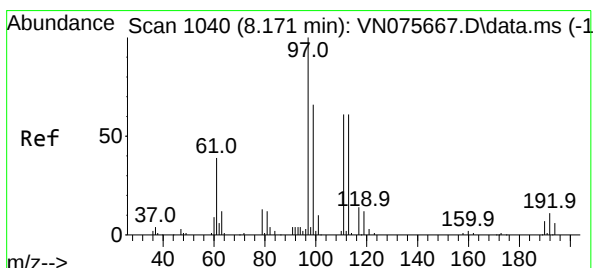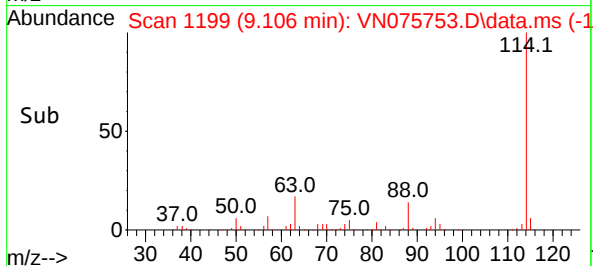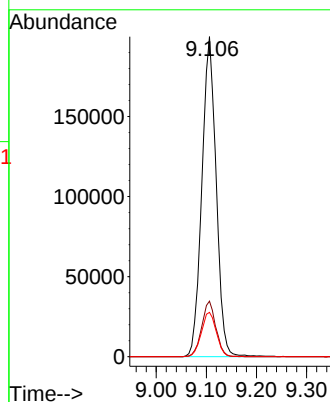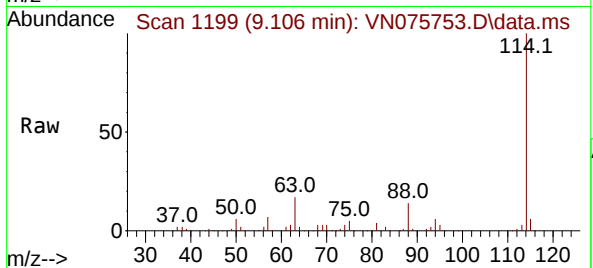

#35

Dibromofluoromethane

Concen: 48.471 ug/l

RT: 8.171 min Scan# 1040

Delta R.T. 0.000 min

Lab File: VN075753.D

Acq: 13 Dec 2022 10:03




Tgt Ion:113 Resp: 117063


Ion Ratio Lower Upper

113 100

111 101.4 81.0 121.6

192 20.1 16.2 24.2


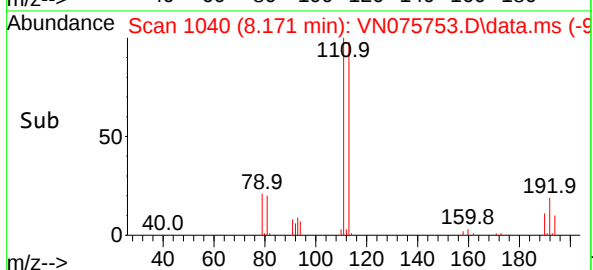
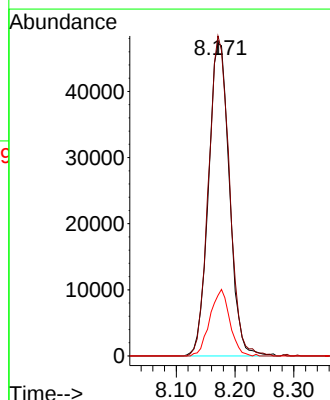
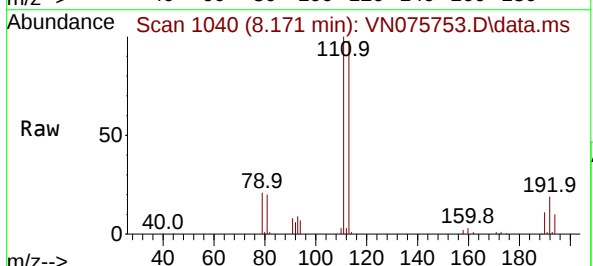


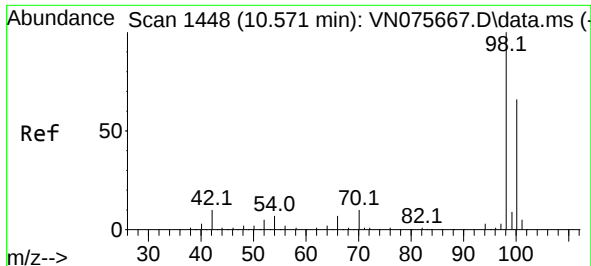

#50
Toluene-d8
Concen: 49.418 ug/l
RT: 10.571 min Scan# 1448
Delta R.T. 0.000 min
Lab File: VN075753.D
Acq: 13 Dec 2022 10:03




Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-WATER-REF-5


Tgt Ion: 98 Resp: 448214
Ion Ratio Lower Upper
98 100
100 65.0 52.6 78.8

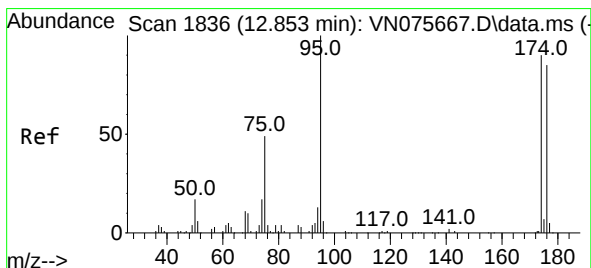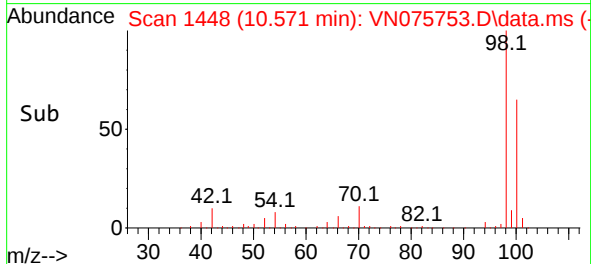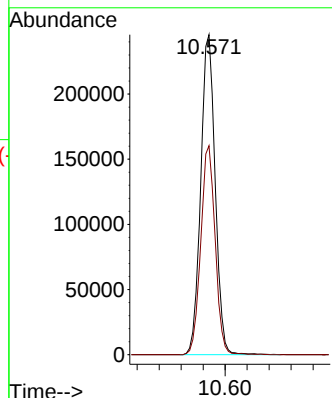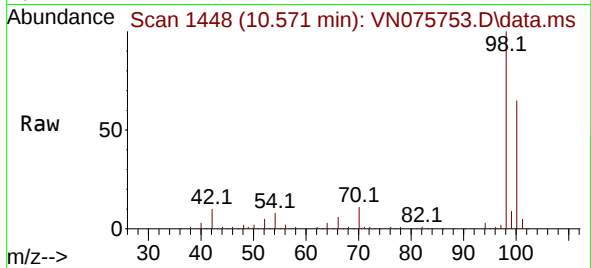

#62
4-Bromofluorobenzene
Concen: 44.361 ug/l
RT: 12.847 min Scan# 1835
Delta R.T. -0.006 min
Lab File: VN075753.D
Acq: 13 Dec 2022 10:03

Tgt Ion: 95 Resp: 137564
Ion Ratio Lower Upper
95 100
174 89.6 0.0 178.6
176 84.5 0.0 170.8


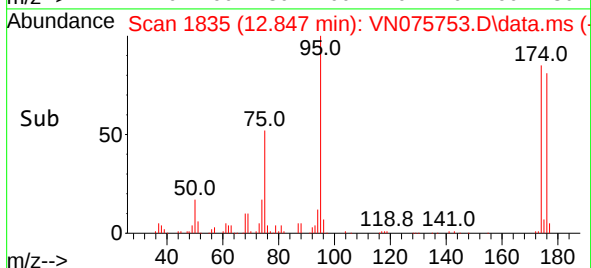
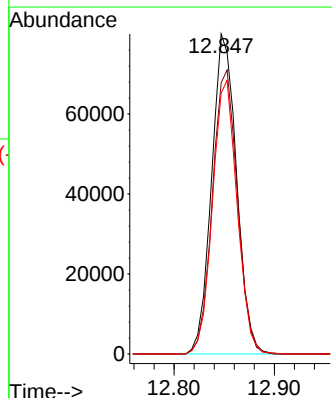
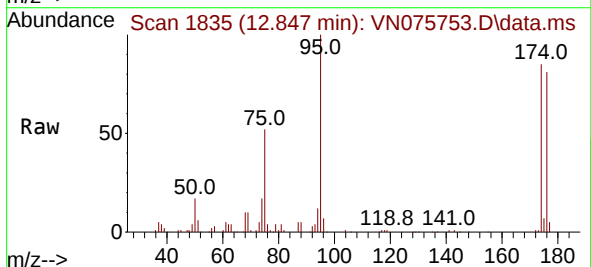


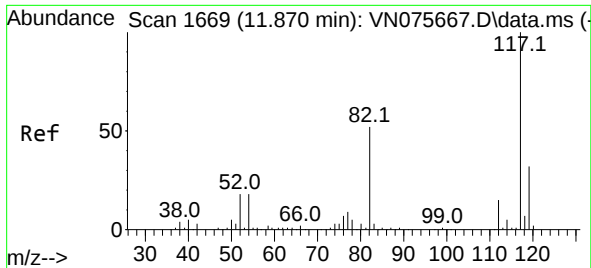

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. -0.006 min
Lab File: VN075753.D
Acq: 13 Dec 2022 10:03

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Tgt Ion:117 Resp: 336726
Ion Ratio Lower Upper
117 100
82 52.1 41.8 62.8
119 32.4 25.8 38.6

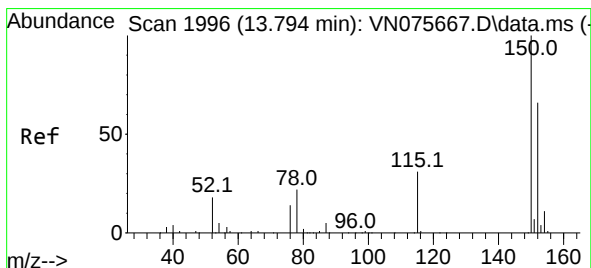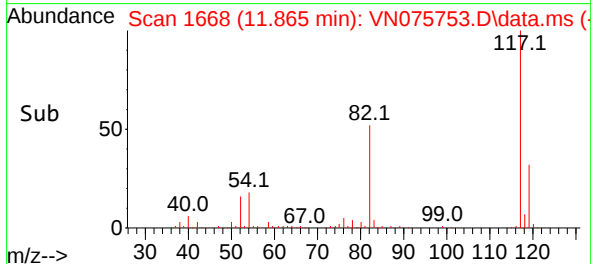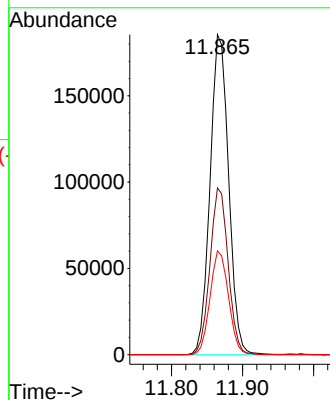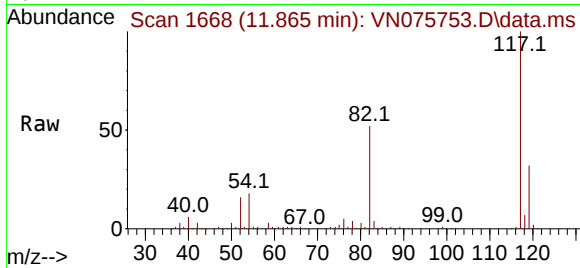

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. 0.000 min
Lab File: VN075753.D
Acq: 13 Dec 2022 10:03

Tgt Ion:152 Resp: 144385
Ion Ratio Lower Upper
152 100
115 57.9 28.4 85.2
150 160.4 0.0 347.6

