
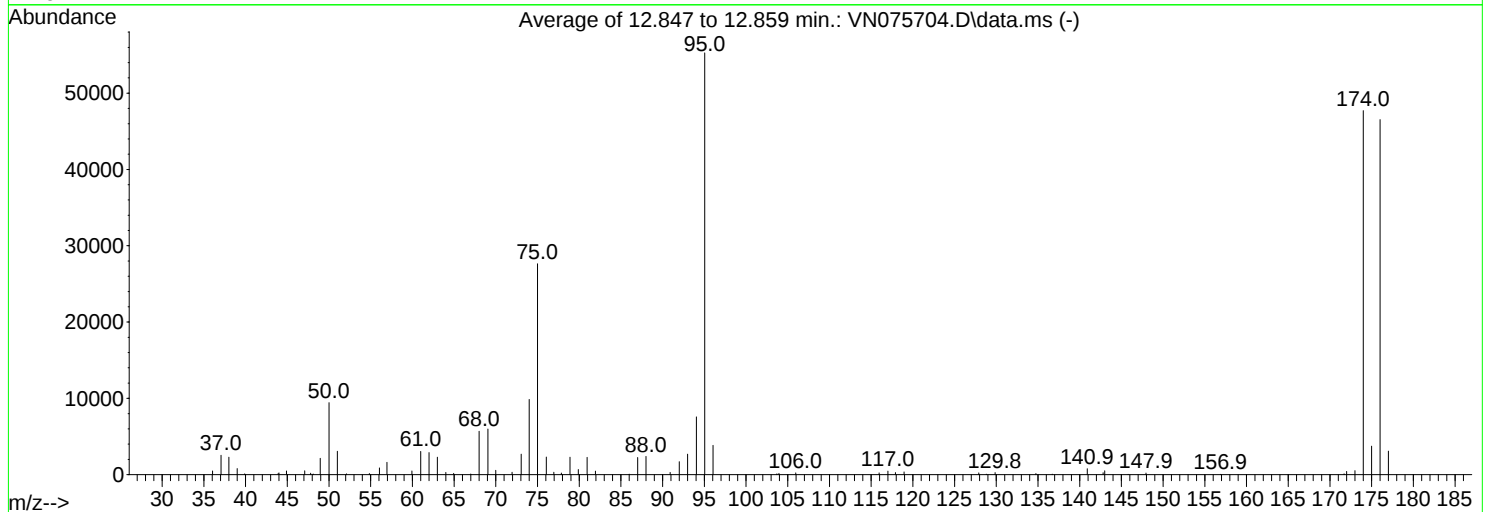


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121222\
Data File : VN075704.D
Acq On : 12 Dec 2022 11:12
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120922W.M
Title : SW846 8260
Last Update : Mon Dec 12 07:54:35 2022

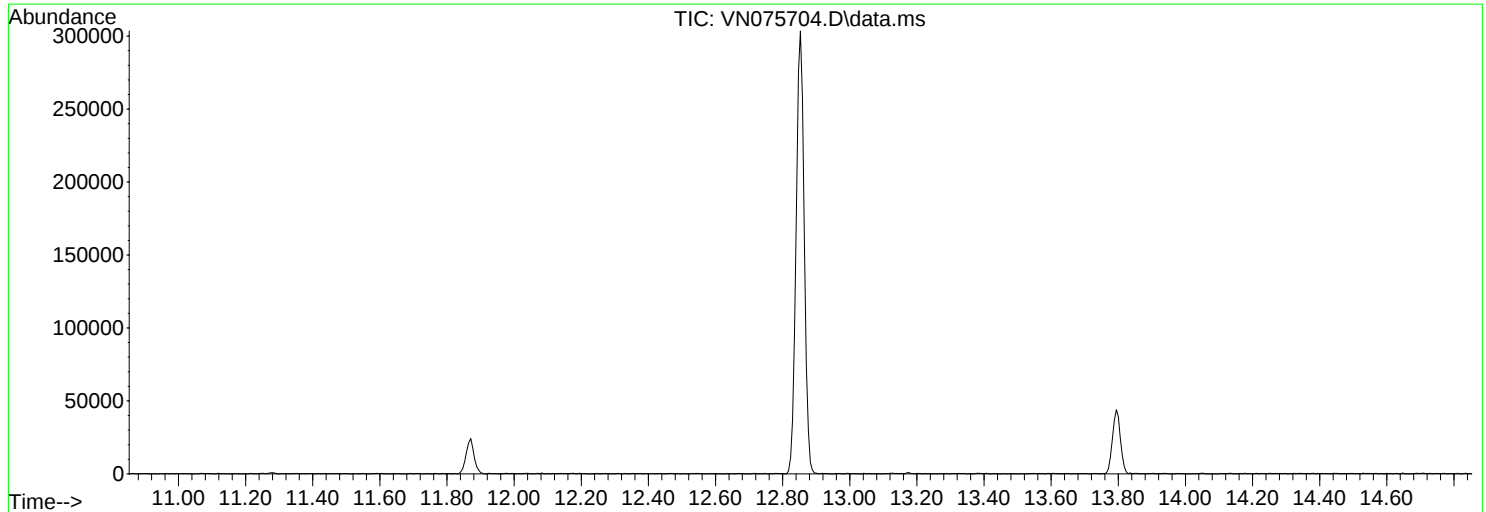

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	9445	PASS
75	95	30	60	50.0	27640	PASS
95	95	100	100	100.0	55285	PASS
96	95	5	9	6.9	3828	PASS
173	174	0.00	2	1.1	521	PASS
174	95	50	100	86.3	47704	PASS
175	174	5	9	7.8	3731	PASS
176	174	95	101	97.6	46539	PASS
177	176	5	9	6.6	3092	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	488	48.95	2133	64.00	299	76.95	321
37.05	2532	50.00	9445	64.95	163	77.85	211
38.00	2289	51.00	3070	67.00	89	78.90	228
39.00	807	52.10	109	68.00	5686	79.90	67
39.90	108	54.85	148	69.05	5976	80.95	2266
43.90	138	56.05	875	70.00	559	81.95	473
44.00	232	56.95	1620	71.95	310	86.00	56
44.90	479	59.95	493	73.05	2677	87.00	2244
47.10	504	61.00	3051	74.00	9857	88.00	2382
47.80	198	62.00	2899	75.00	27640	90.90	284
48.10	89	63.00	2279	76.05	2309	92.00	1692

Average of 12.847 to 12.859 min.: VN075704.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
93.00	2679	127.90	226	171.70	111		
94.05	7566	128.80	55	172.00	429		
95.05	55285	129.85	266	173.00	521		
96.05	3828	134.75	147	174.00	47704		
103.70	108	136.70	55	175.00	3731		
103.95	163	140.90	768	176.00	46539		
105.95	224	142.80	249	177.00	3092		
115.95	226	143.00	507				
117.00	462	145.80	52				
117.90	278	147.95	209				
118.95	350	156.90	51				

Instrument :

MSVOA_N

ClientSampleId :

BFB