


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121222\
Data File : VN075731.D
Acq On : 13 Dec 2022 00:52
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120922W.M
Title : SW846 8260
Last Update : Mon Dec 12 07:54:35 2022

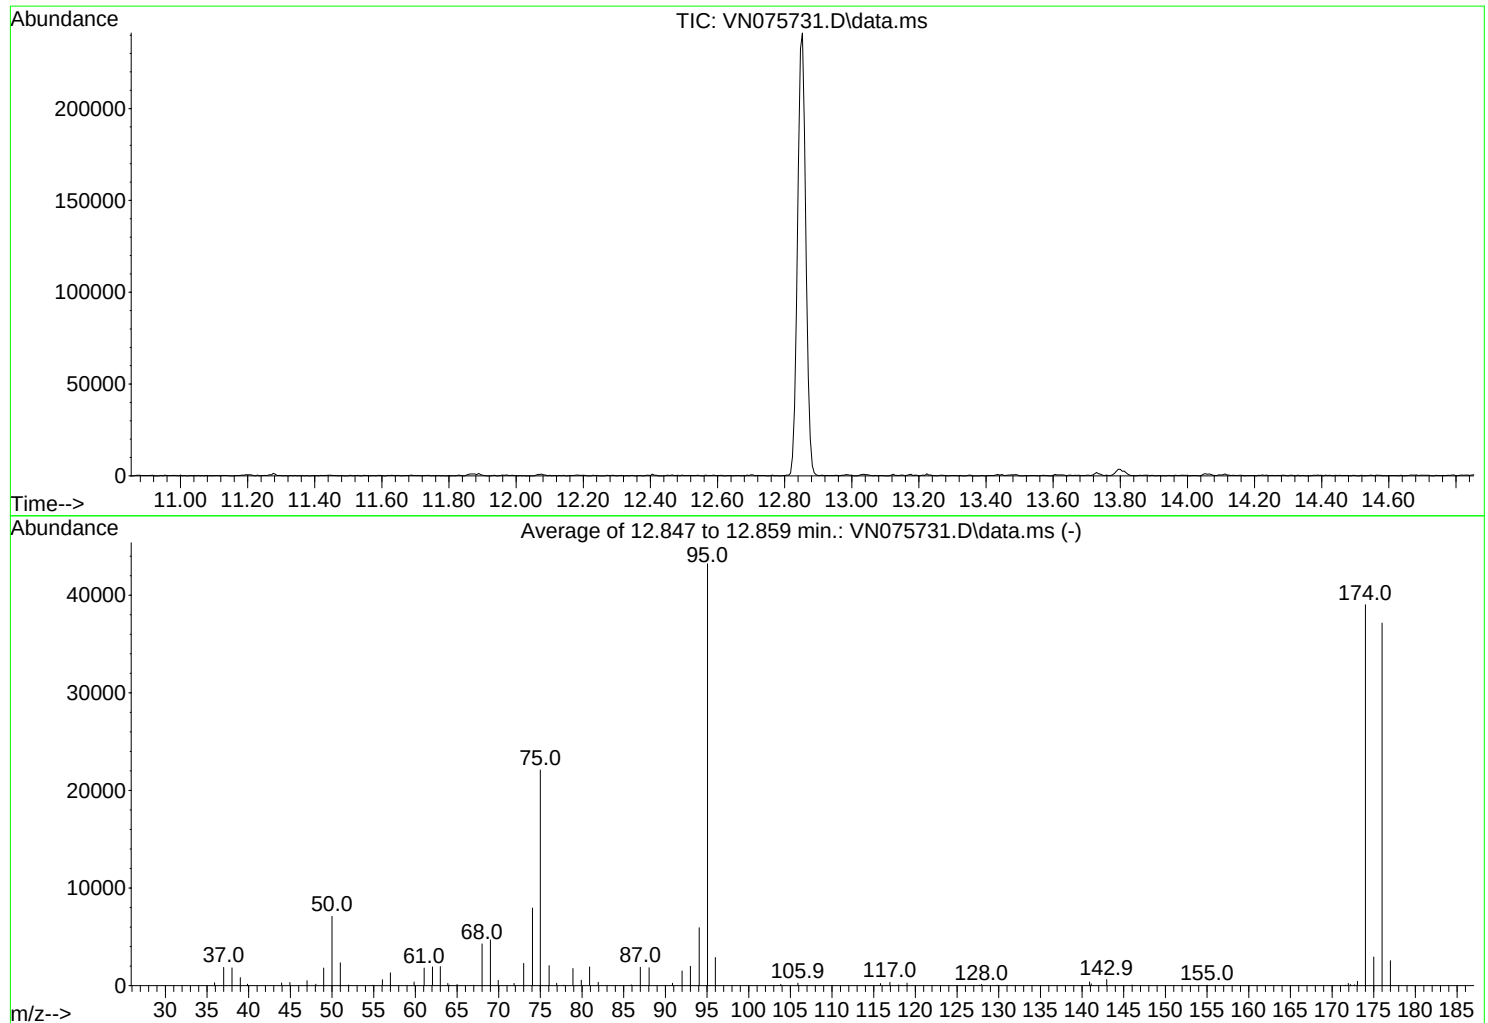

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	7103	PASS
75	95	30	60	51.1	22104	PASS
95	95	100	100	100.0	43221	PASS
96	95	5	9	6.7	2883	PASS
173	174	0.00	2	1.2	450	PASS
174	95	50	100	90.3	39045	PASS
175	174	5	9	7.5	2938	PASS
176	174	95	101	95.2	37160	PASS
177	176	5	9	6.9	2562	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	301	51.00	2338	65.00	135	77.80	5
37.00	1876	52.00	71	67.00	51	78.90	175
38.00	1816	54.90	54	68.00	4284	79.90	55
39.00	825	56.05	604	69.00	4686	80.90	191
39.85	149	57.00	1311	69.95	542	81.95	341
43.95	280	59.85	384	71.85	238	85.90	77
44.95	334	61.05	1812	73.00	2284	87.00	1890
47.00	511	62.05	1923	74.05	7961	88.05	1830
48.05	141	63.00	1946	75.00	22104	90.85	240
49.00	1802	63.90	224	76.05	2053	92.00	1517
50.00	7103	64.10	50	76.95	251	93.00	1987

Average of 12.847 to 12.859 min.: VN075731.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.05	5939	129.80	50	174.00	39045		
95.05	43221	140.90	380	175.00	2938		
96.00	2883	141.10	179	176.00	37160		
103.85	137	142.95	616	177.00	2562		
105.90	270	146.00	69				
115.80	211	155.00	53				
116.95	340	171.60	56				
118.00	87	171.95	230				
119.00	264	172.20	114				
127.70	50	172.70	90				
127.95	125	173.05	450				

Instrument :

MSVOA_N

ClientSampleId :

BFB