
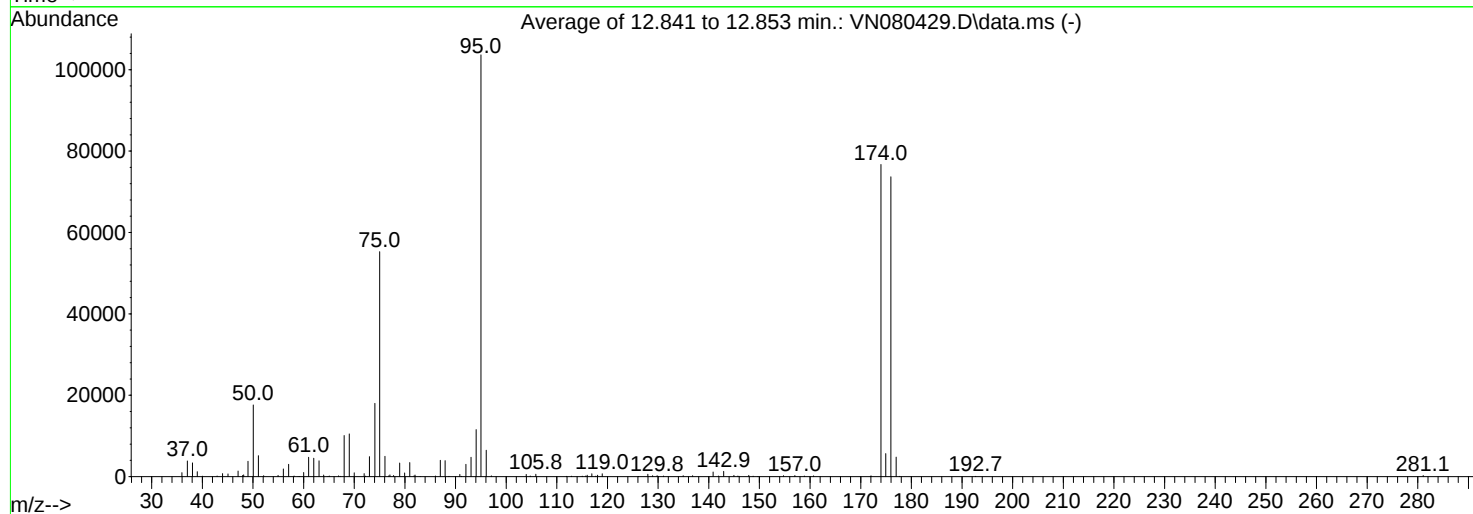


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121223\
Data File : VN080429.D
Acq On : 12 Dec 2023 08:32
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121223W.M
Title : SW846 8260
Last Update : Wed Dec 13 01:57:14 2023

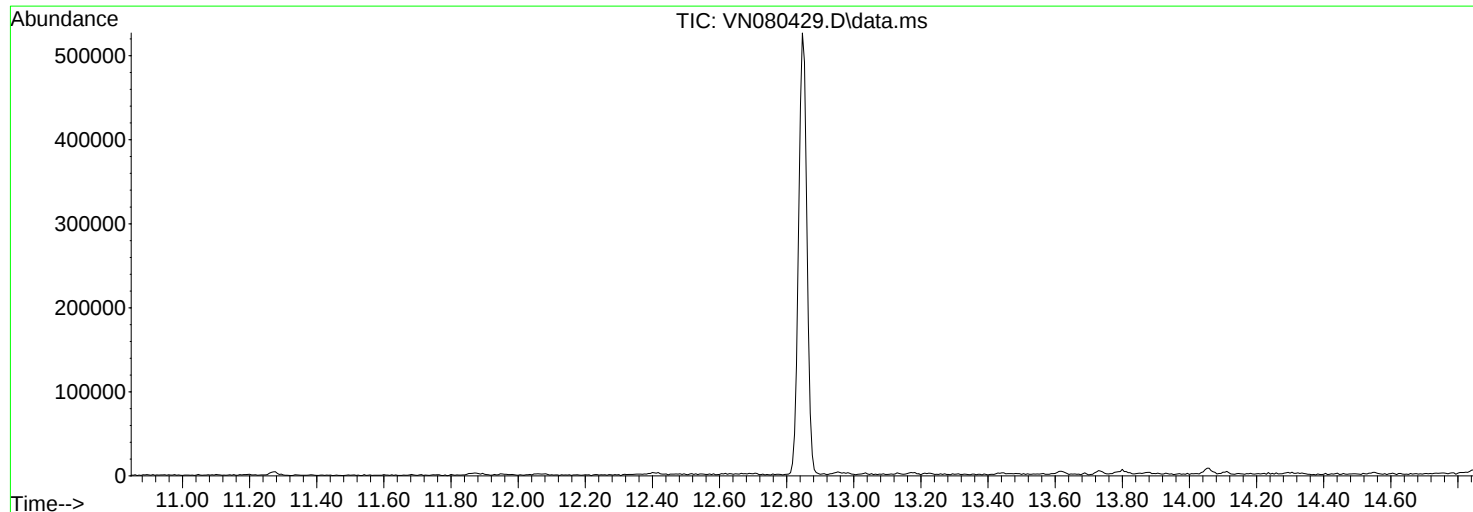

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1842

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	17614	PASS
75	95	30	60	53.3	55277	PASS
95	95	100	100	100.0	103651	PASS
96	95	5	9	6.2	6472	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	74.0	76715	PASS
175	174	5	9	7.4	5664	PASS
176	174	95	101	96.0	73677	PASS
177	176	5	9	6.5	4780	PASS

Average of 12.841 to 12.853 min.: VN080429.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	984	49.00	3788	61.00	4755	71.95	741
37.05	3852	50.05	17614	62.00	4541	72.20	111
38.05	3370	51.05	5170	63.05	3906	73.00	490
39.00	1224	52.10	241	63.95	391	74.05	1800
40.05	104	54.95	315	64.80	57	75.00	55277
42.90	160	56.00	1878	65.05	154	76.05	4997
44.00	739	57.05	3033	66.90	209	76.80	204
45.05	683	58.10	171	67.20	92	77.05	446
47.05	1387	58.90	56	68.00	10105	77.75	273
47.95	274	59.20	54	69.00	10502	78.95	3346
48.15	443	60.00	1038	70.00	949	79.95	901

Average of 12.841 to 12.853 min.: VN080429.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.95	3447	93.05	4743	115.70	170	131.05	160
81.80	198	94.05	11564	116.00	341	134.95	250
82.00	381	95.00	103651	116.90	698	136.80	225
83.00	60	96.05	6472	117.70	131	140.85	1159
86.05	160	97.05	215	118.05	349	141.90	158
87.00	4018	103.95	548	118.95	719	142.95	1291
87.95	3918	104.75	152	126.10	56	144.95	305
88.70	76	105.85	573	127.95	588	145.75	167
90.85	557	111.90	64	128.90	256	146.00	78
91.20	86	112.90	110	129.80	252	147.90	334
92.05	3047	115.00	126	130.00	91	148.75	122

Average of 12.841 to 12.853 min.: VN080429.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
149.70	61	177.70	79				
154.75	240	192.70	83				
157.00	261	281.05	282				
158.85	163						
160.70	217						
171.90	97						
172.05	180						
174.00	76715						
174.95	5664						
175.95	73677						
177.00	4780						

Instrument :

MSVOA_N

ClientSampleId :

BFB