
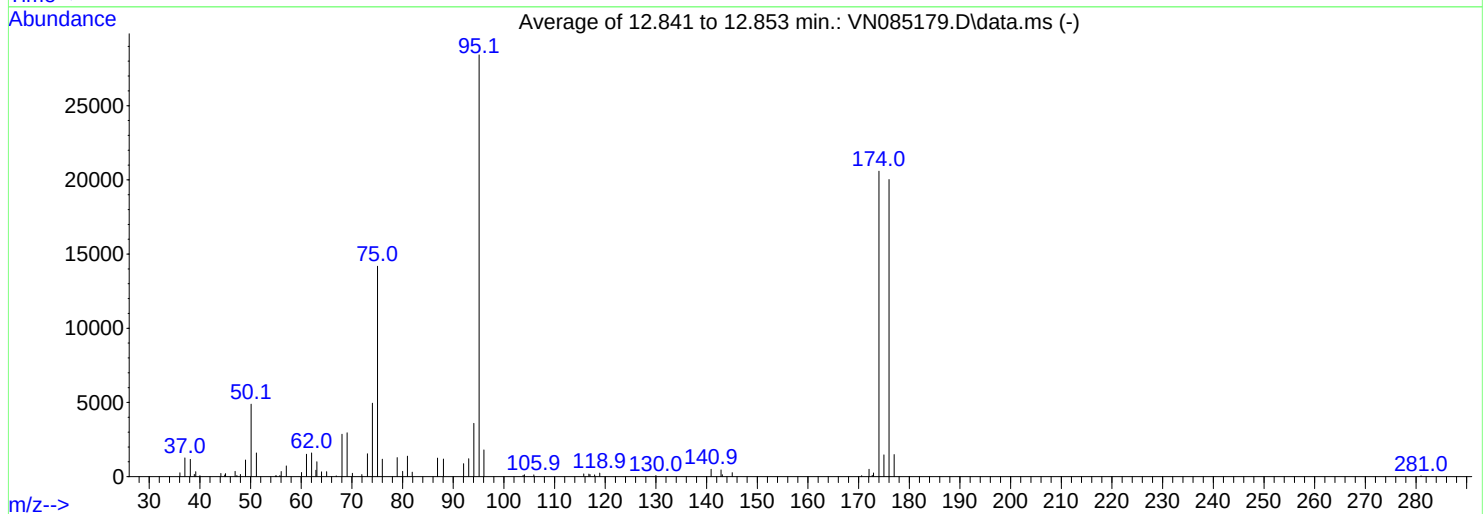


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121224\
Data File : VN085179.D
Acq On : 12 Dec 2024 09:39
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112224W.M
Title : SW846 8260
Last Update : Sat Nov 23 02:54:10 2024

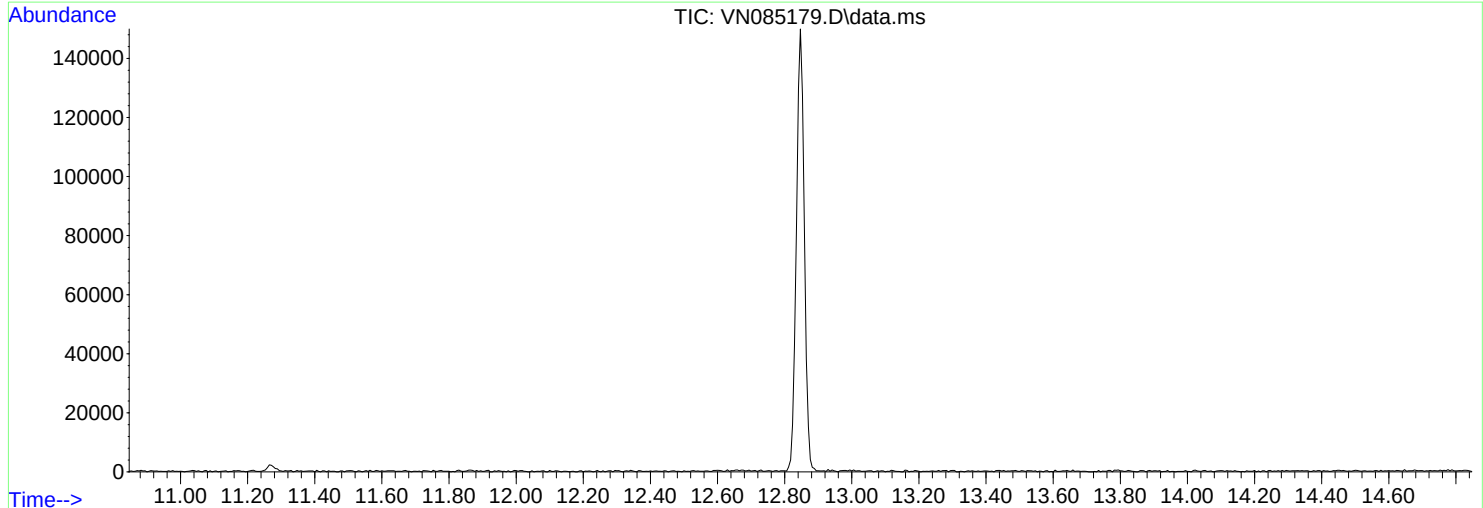

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	4886	PASS
75	95	30	60	49.9	14177	PASS
95	95	100	100	100.0	28427	PASS
96	95	5	9	6.3	1796	PASS
173	174	0.00	2	1.2	251	PASS
174	95	50	100	72.4	20584	PASS
175	174	5	9	7.1	1471	PASS
176	174	95	101	97.3	20027	PASS
177	176	5	9	7.4	1486	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	258	48.00	149	62.05	1591	74.05	494
37.05	1267	49.00	1119	62.90	434	75.05	1417
38.10	1165	50.10	4886	63.10	1003	76.00	117
38.90	156	51.15	1600	64.00	326	78.95	128
39.20	339	54.90	51	65.00	332	80.00	353
40.00	68	55.10	53	66.90	56	80.95	1384
44.15	214	55.80	71	68.05	2853	81.90	298
44.90	107	56.05	341	69.05	2958	86.90	1254
45.05	201	57.05	728	70.10	228	88.05	1182
46.95	353	60.05	284	71.95	138	92.05	871
47.30	77	61.05	1514	73.05	1547	93.05	1209

Average of 12.841 to 12.853 min.: VN085179.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.05	3590	130.00	74	176.00	20027		
95.10	28427	140.90	492	177.00	1486		
96.05	1796	142.85	452	281.00	56		
103.80	84	143.10	127				
104.05	133	145.05	268				
105.90	117	170.60	60				
115.75	182	172.05	500				
116.75	173	172.70	85				
117.00	136	172.95	251				
117.90	116	174.00	20584				
118.90	235	175.00	1471				

Instrument :

MSVOA_N

ClientSampleId :

BFB