



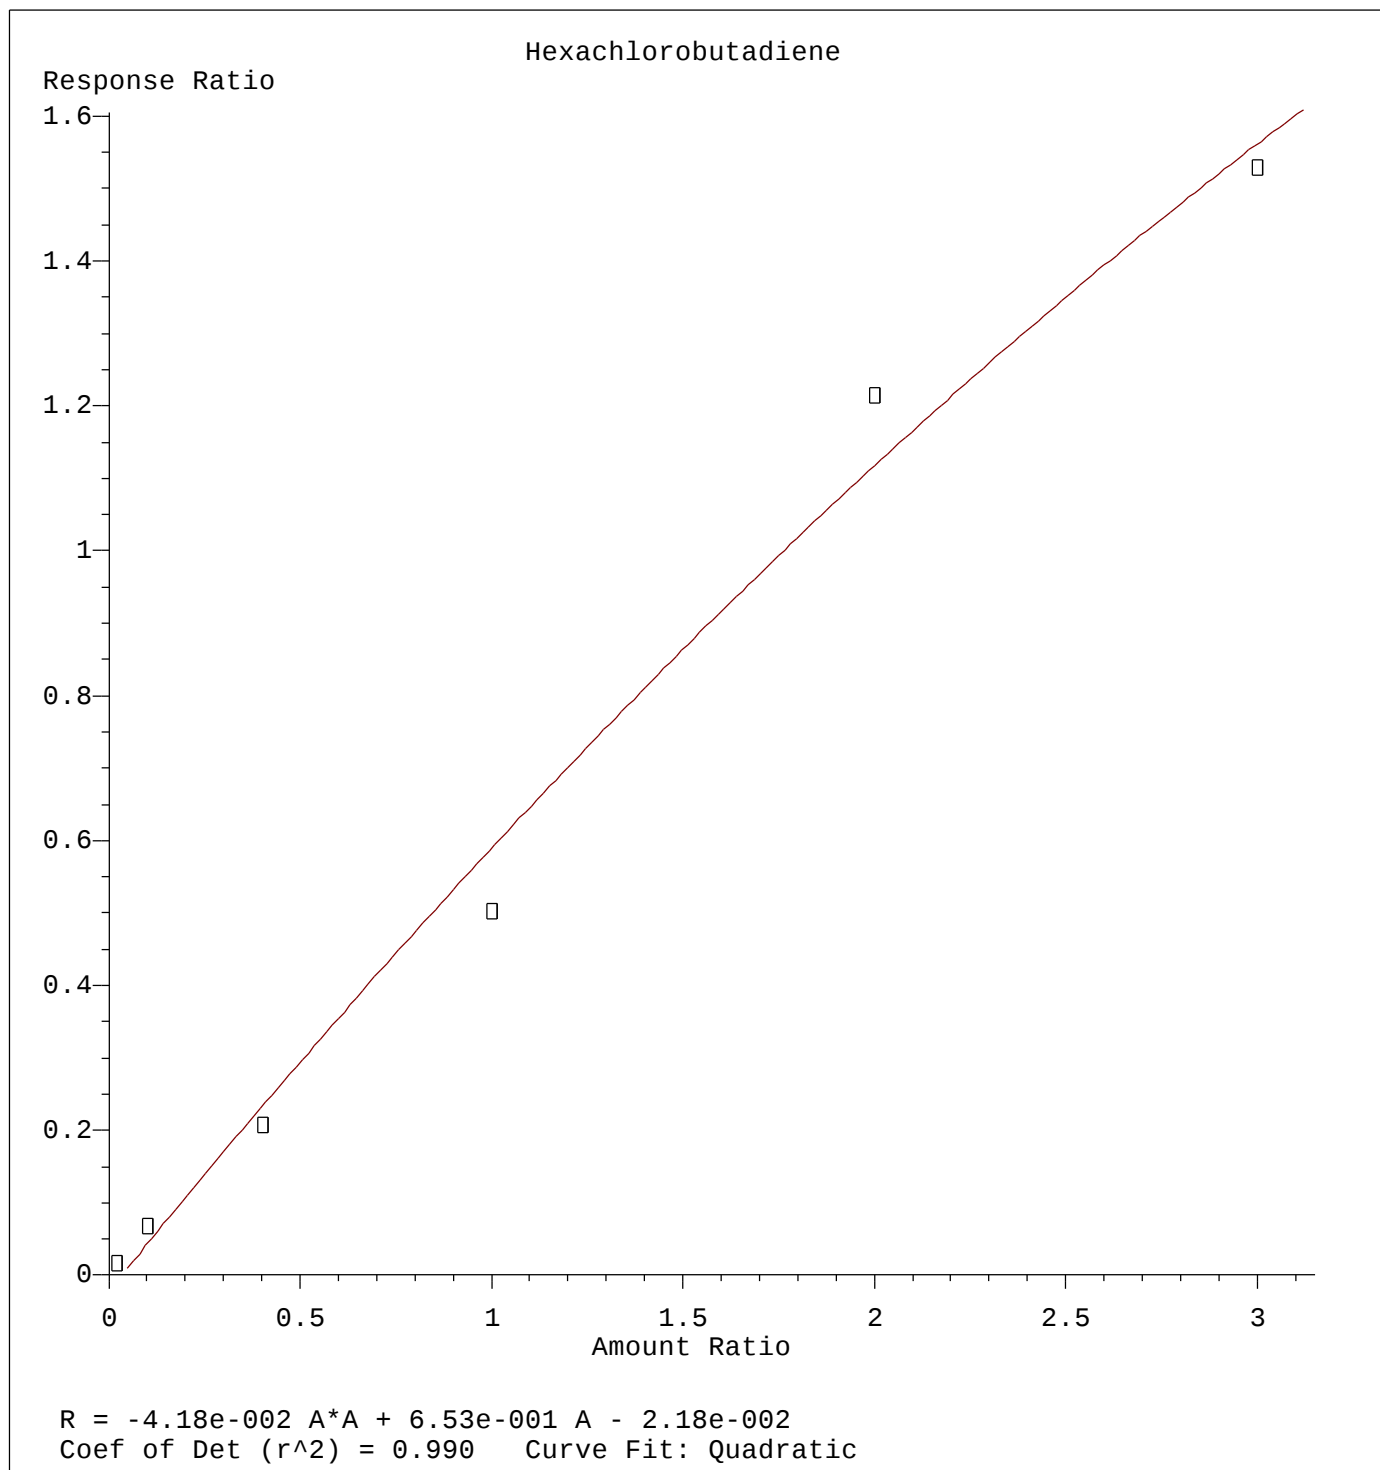


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121319W.M
Calibration Table Last Updated: Fri Dec 13 23:17:39 2019

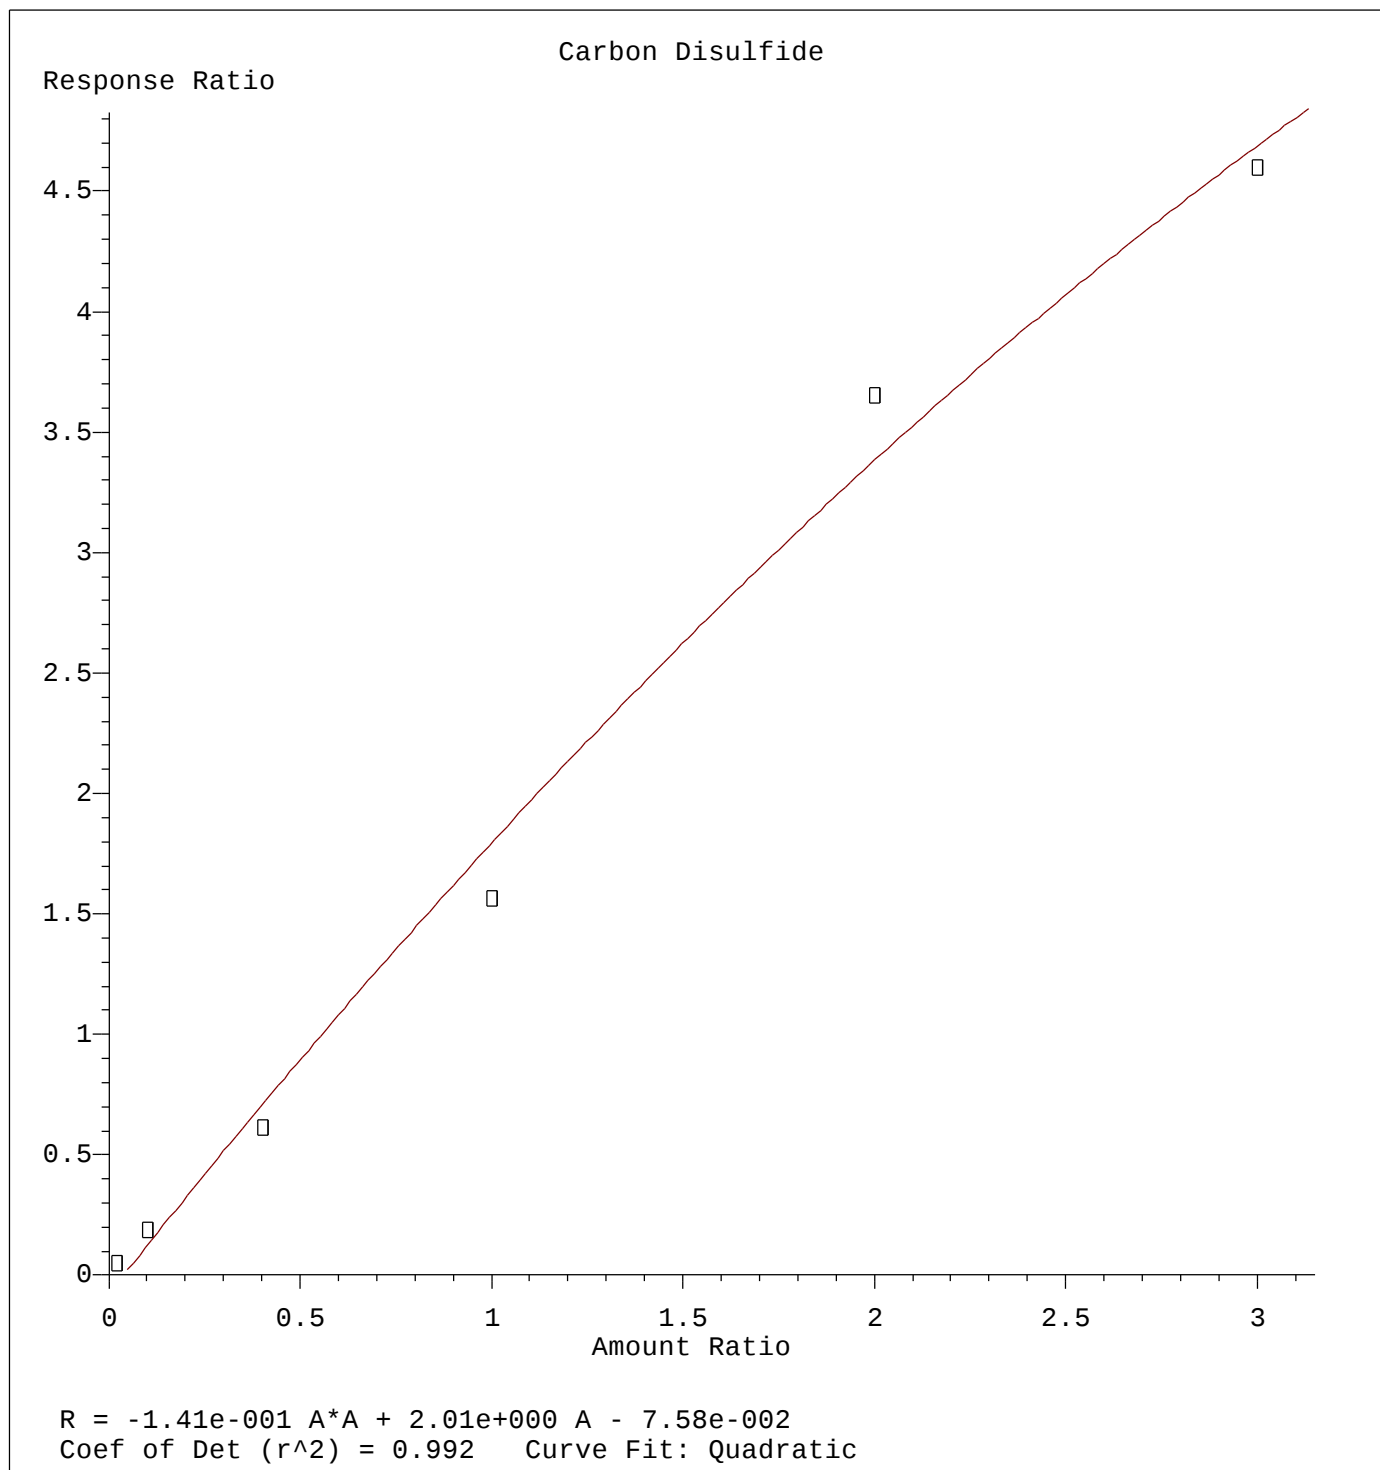

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121319W.M
Calibration Table Last Updated: Fri Dec 13 23:17:39 2019

Bromochloromethane

Response Ratio

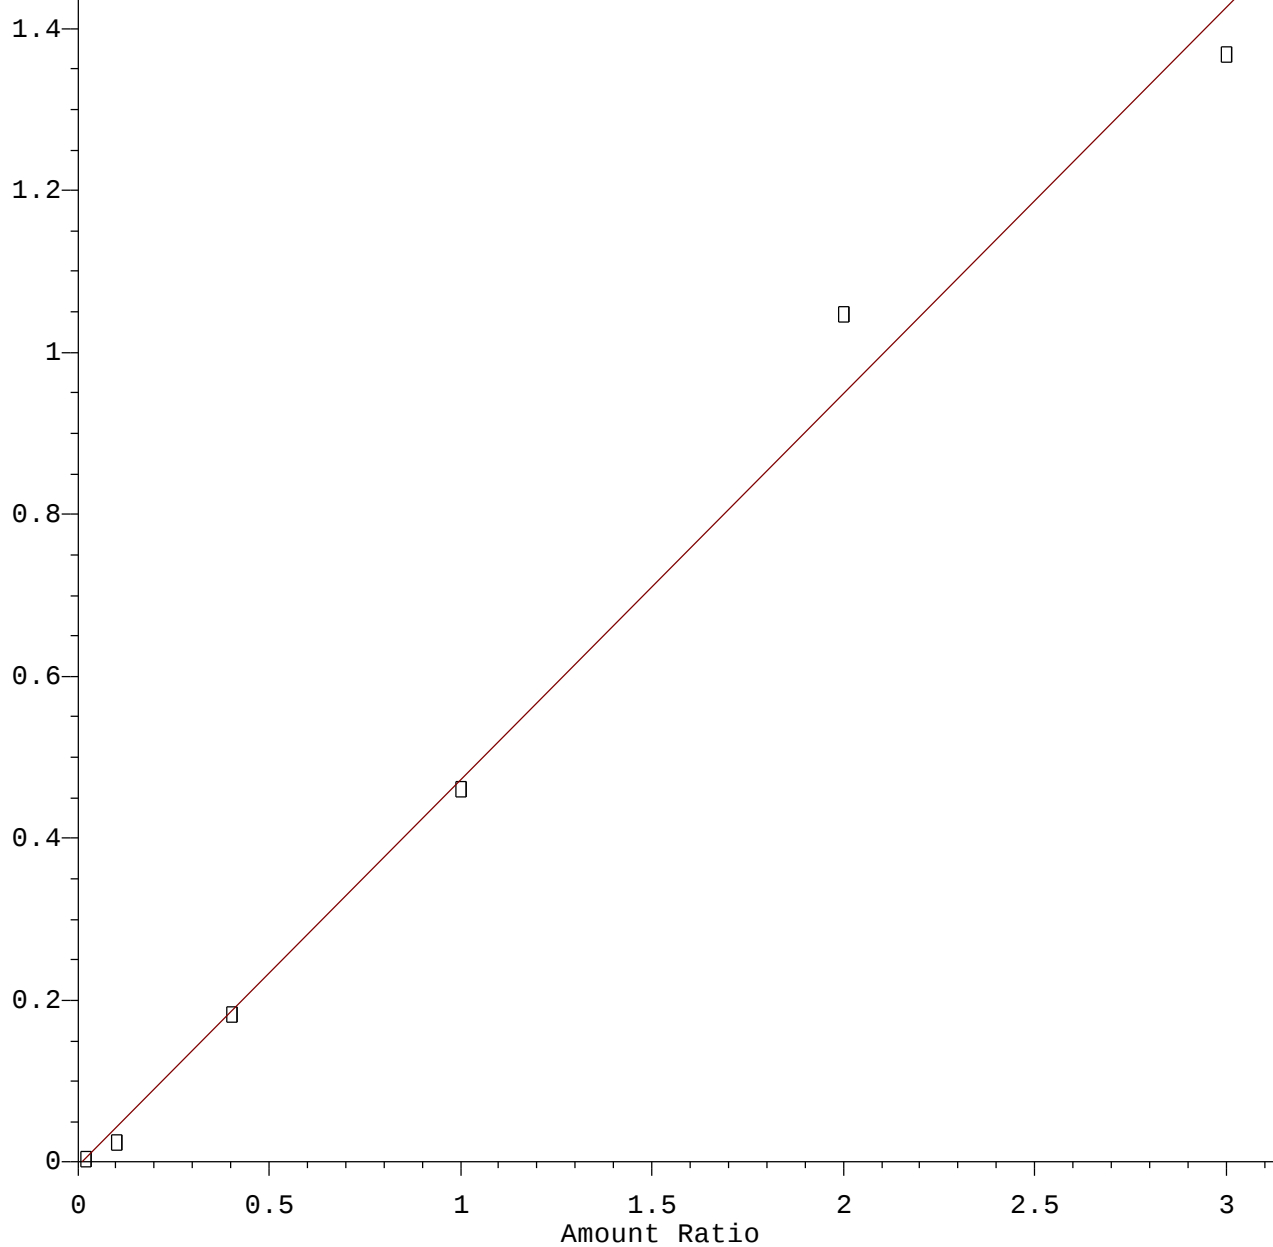


Resp Ratio = $4.77 \times 10^{-1} \times \text{Amt} - 4.48 \times 10^{-3}$
Coef of Det (r^2) = 0.992 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121319W.M
Calibration Table Last Updated: Fri Dec 13 23:17:39 2019

1,2-Dibromo-3-Chloropropane

Response Ratio

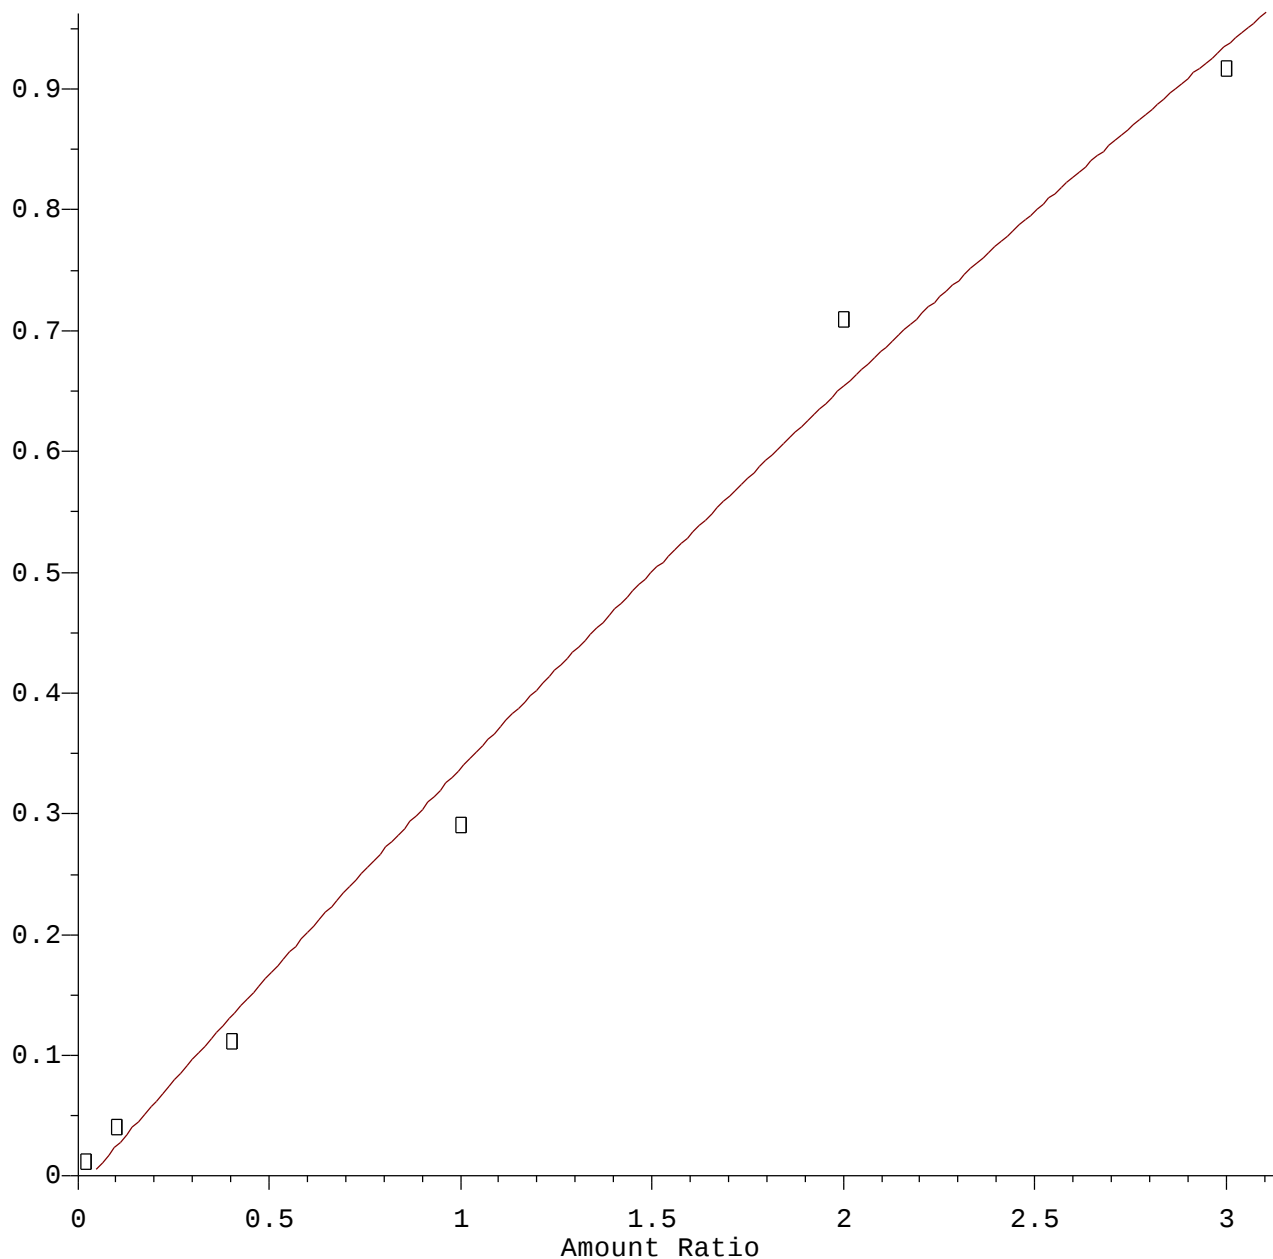

$R = -1.68e-002 A^2 + 3.66e-001 A - 1.19e-002$
Coef of Det (r^2) = 0.991 Curve Fit: Quadratic

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121319W.M
Calibration Table Last Updated: Fri Dec 13 23:17:39 2019