


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121321\
 Data File : VN070024.D
 Acq On : 13 Dec 2021 9:46
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N121321W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Tue Dec 14 00:59:04 2021

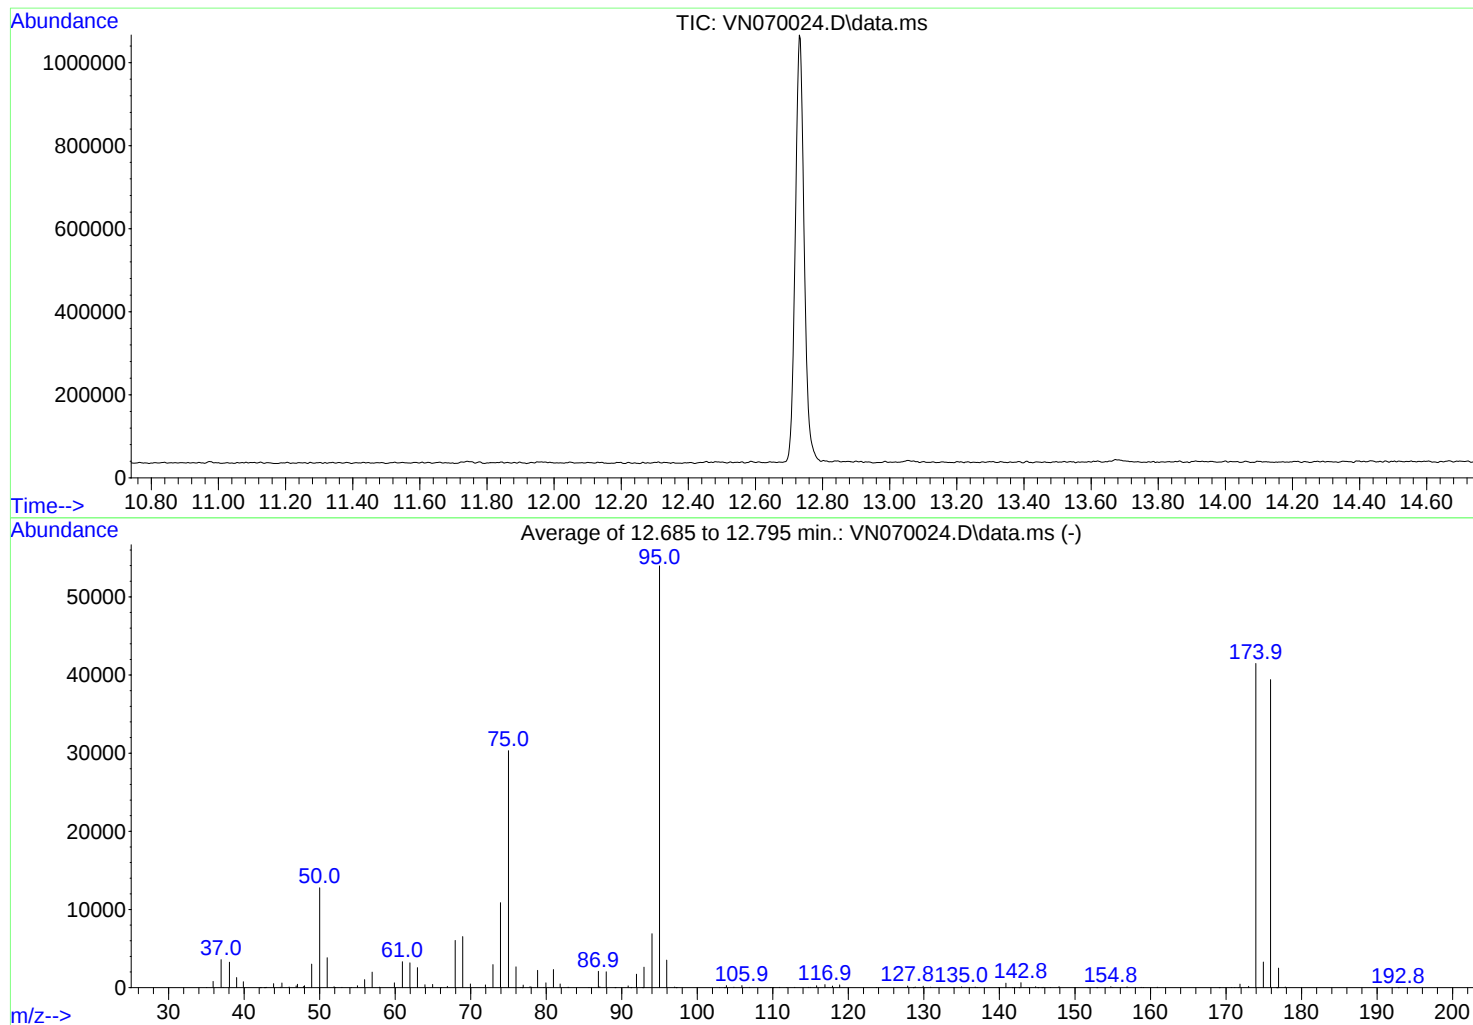

AutoFind: Averaged scan 3988 to 4029; Bkg corrected with scan 3987

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.7	12773	PASS
75	95	30	60	56.2	30315	PASS
95	95	100	100	100.0	53970	PASS
96	95	5	9	6.5	3515	PASS
173	174	0.00	2	0.4	159	PASS
174	95	50	100	76.9	41487	PASS
175	174	5	9	7.9	3268	PASS
176	174	95	101	95.0	39421	PASS
177	176	5	9	6.3	2497	PASS