


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121321\
 Data File : VN070042.D
 Acq On : 13 Dec 2021 19:53
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
 Title : SW846 8260
 Last Update : Fri Dec 03 08:46:47 2021

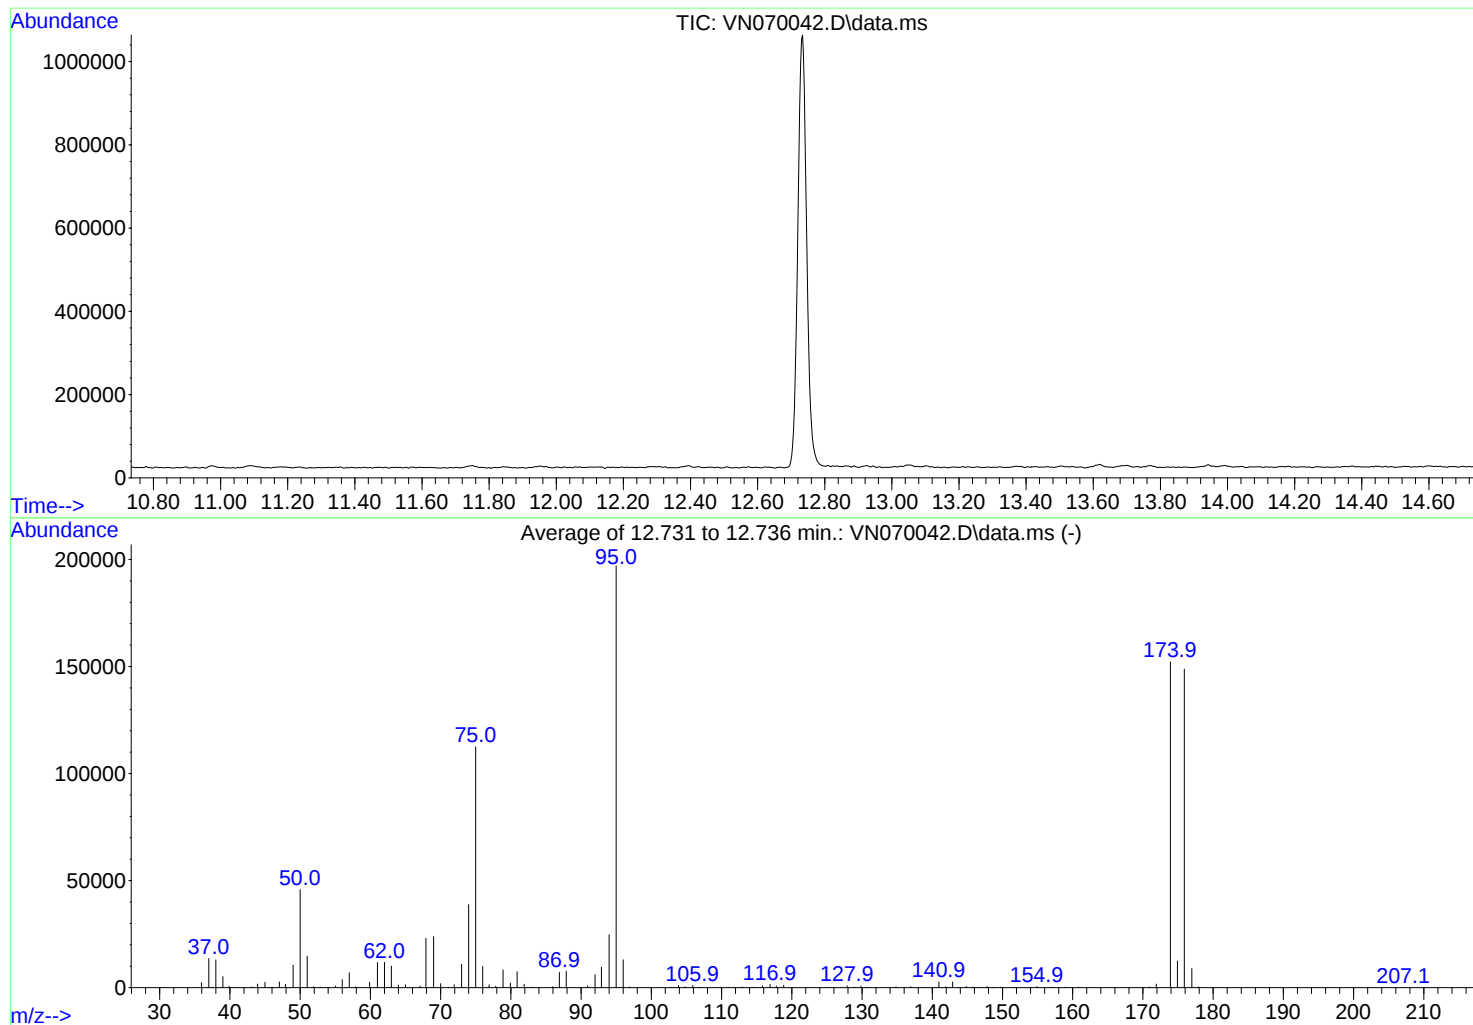

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3986

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.2	45773	PASS
75	95	30	60	57.1	112512	PASS
95	95	100	100	100.0	197035	PASS
96	95	5	9	6.6	13013	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	77.2	152192	PASS
175	174	5	9	8.2	12421	PASS
176	174	95	101	97.8	148821	PASS
177	176	5	9	6.0	8894	PASS