

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121323\
 Data File : VN080452.D
 Acq On : 13 Dec 2023 10:22
 Operator : JC\MD
 Sample : VN1213WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1213WBL01

Quant Time: Dec 14 04:02:53 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121223W.M
 Quant Title : SW846 8260
 QLast Update : Wed Dec 13 01:57:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	201438	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	362050	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	378844	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	170317	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	159295	61.914	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	123.820%
35) Dibromofluoromethane	8.165	113	135042	58.828	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	117.660%
50) Toluene-d8	10.565	98	482921	56.408	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	112.820%
62) 4-Bromofluorobenzene	12.847	95	192230	59.131	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	118.260%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121323\
Data File : VN080452.D
Acq On : 13 Dec 2023 10:22
Operator : JC\MD
Sample : VN1213WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1213WBL01

Quant Time: Dec 14 04:02:53 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121223W.M
Quant Title : SW846 8260
QLast Update : Wed Dec 13 01:57:14 2023
Response via : Initial Calibration




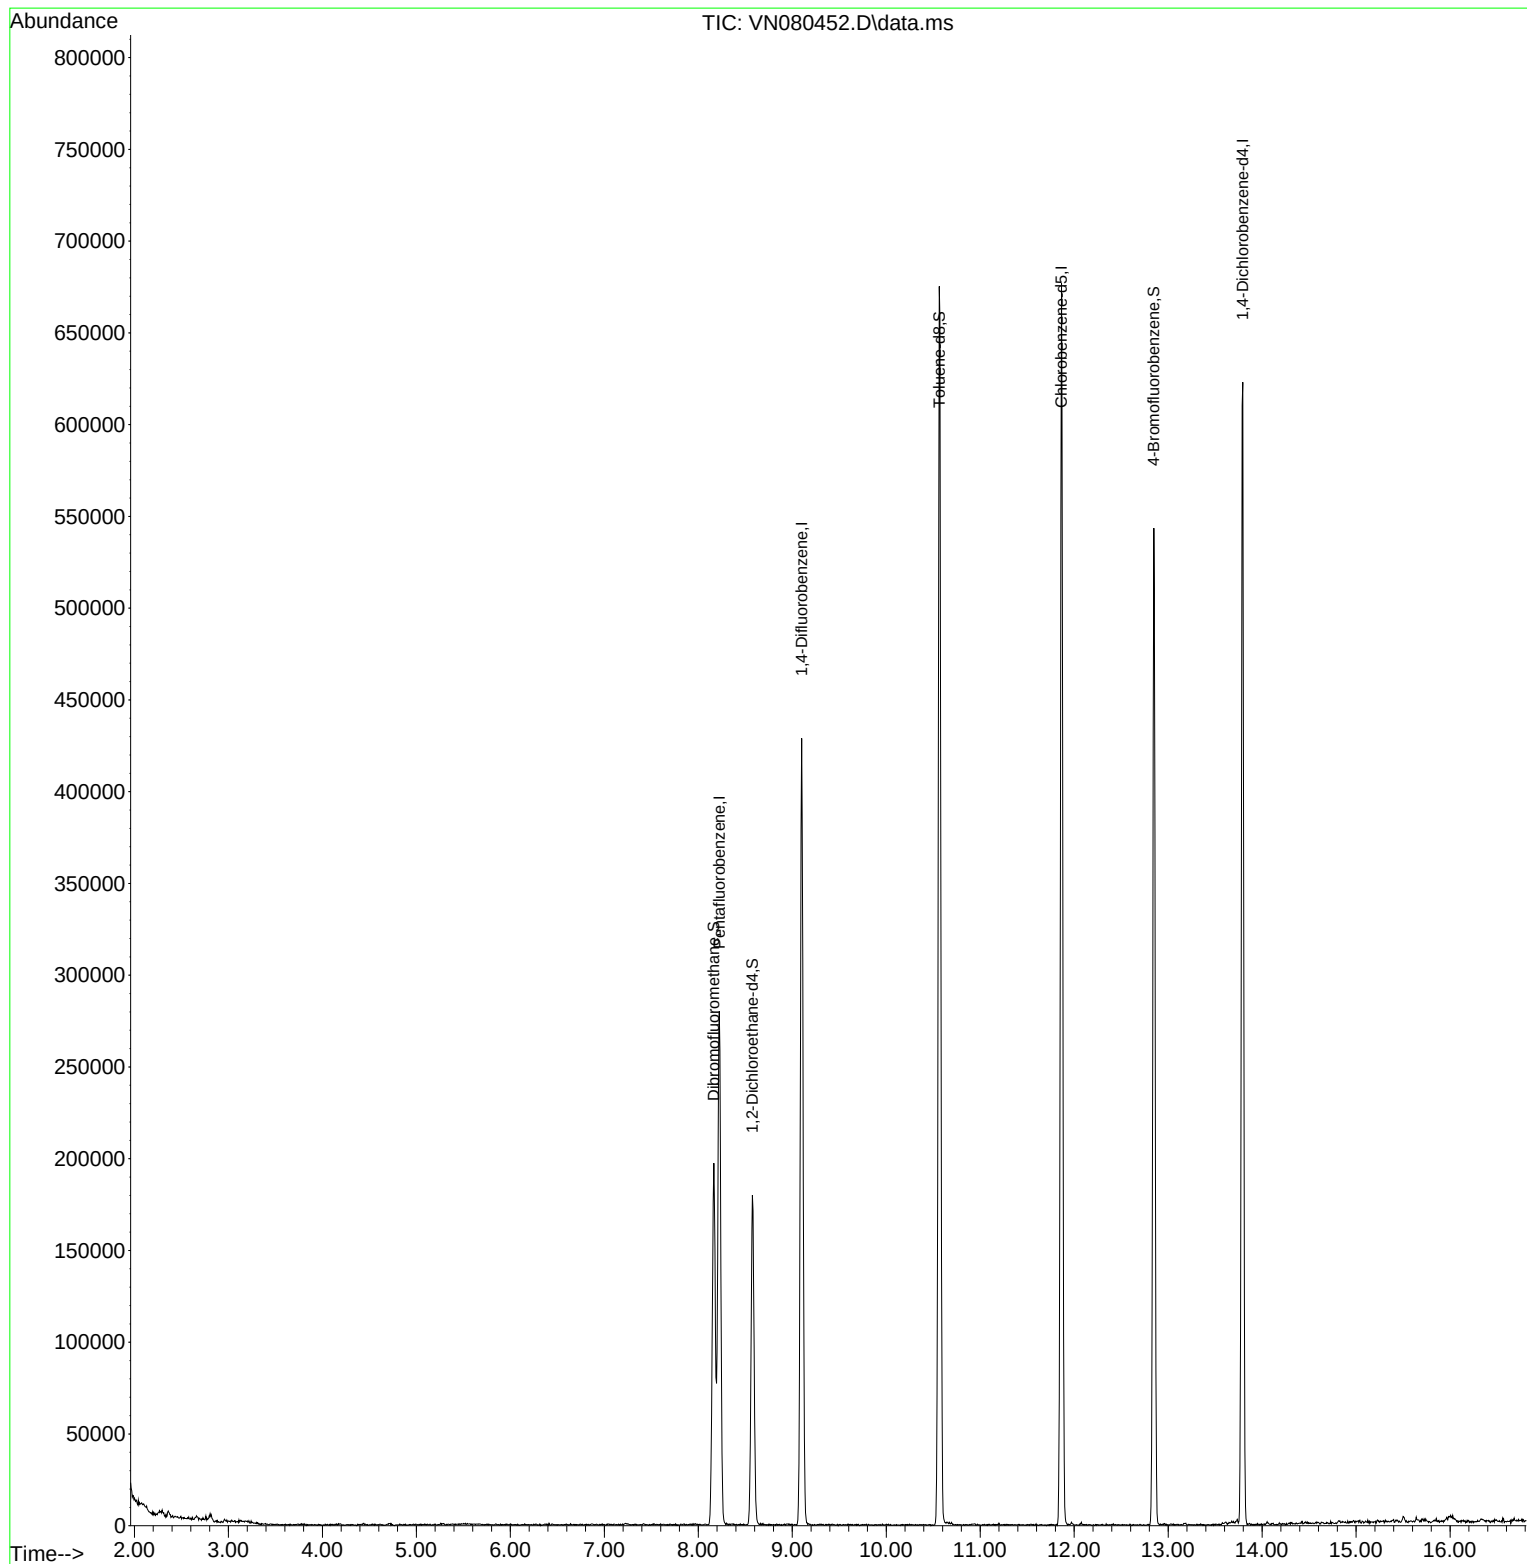


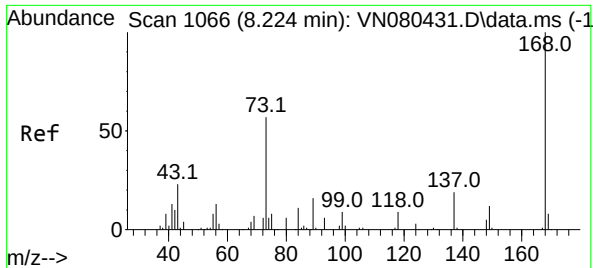

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN080452.D
Acq: 13 Dec 2023 10:22




Instrument :
MSVOA_N
ClientSampleId :
VN1213WBL01


Tgt Ion:168 Resp: 201438
Ion Ratio Lower Upper
168 100
99 65.6 53.0 79.6

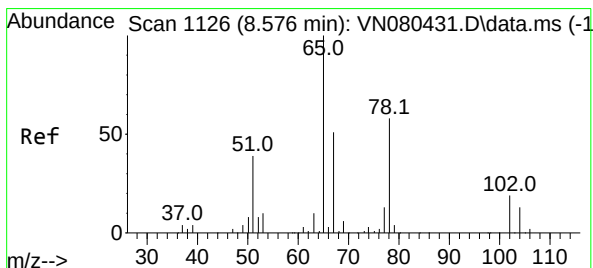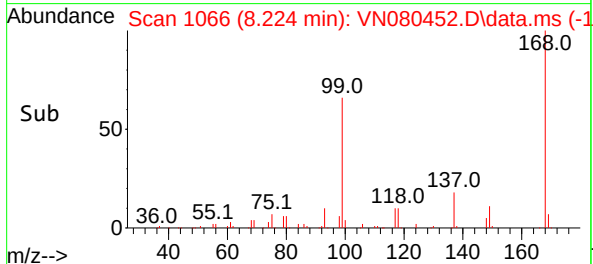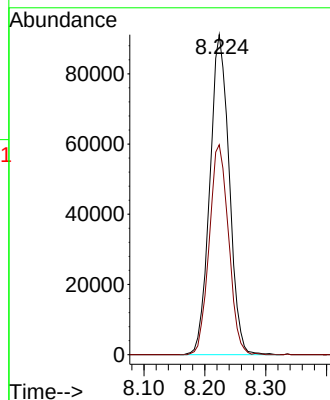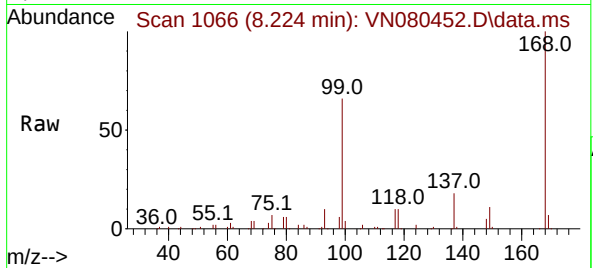

#33
1,2-Dichloroethane-d4
Concen: 61.914 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. 0.000 min
Lab File: VN080452.D
Acq: 13 Dec 2023 10:22

Tgt Ion: 65 Resp: 159295
Ion Ratio Lower Upper
65 100
67 49.0 0.0 106.6

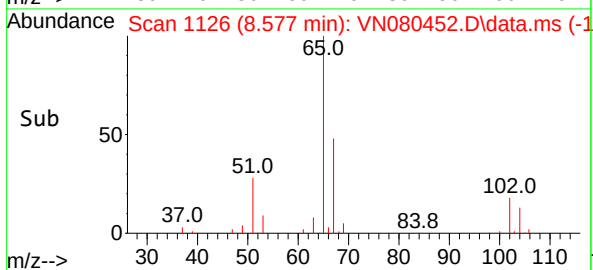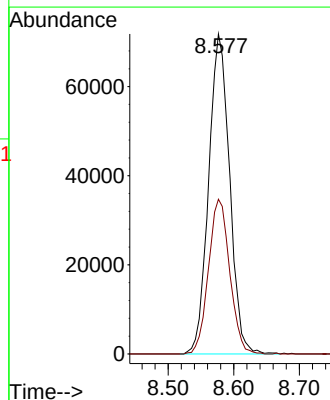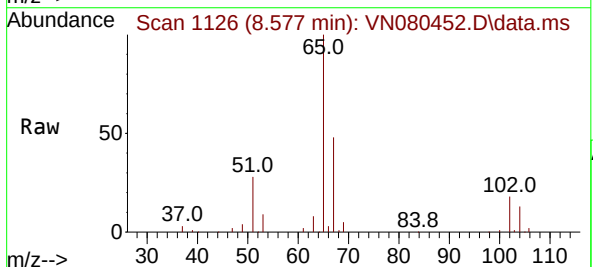

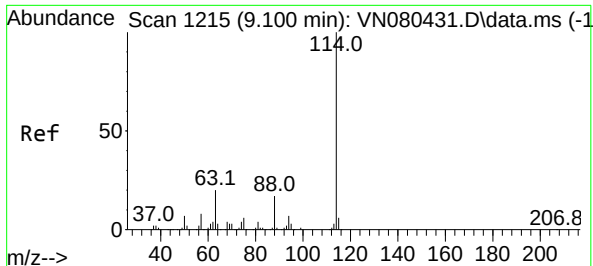

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1

Delta R.T. 0.000 min

Lab File: VN080452.D

Acq: 13 Dec 2023 10:22

Instrument :

MSVOA_N

ClientSampleId :

VN1213WBL01





Tgt Ion:114 Resp: 362050

Ion Ratio Lower Upper

114 100

63 21.8 0.0 36.4

88 17.9 0.0 30.6

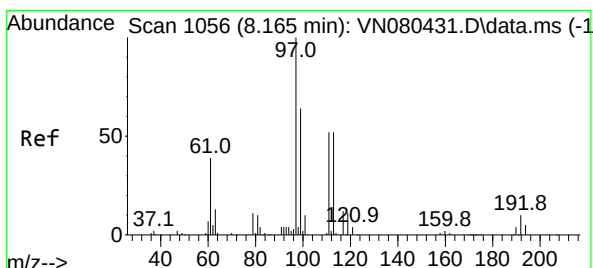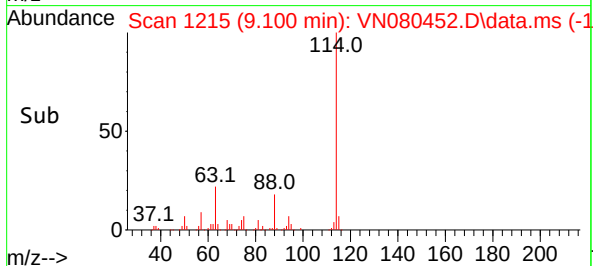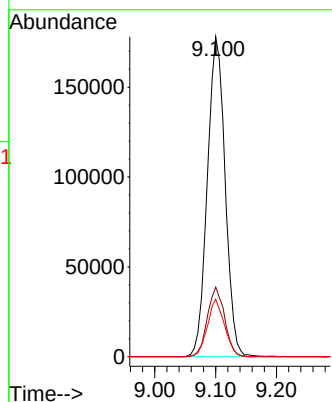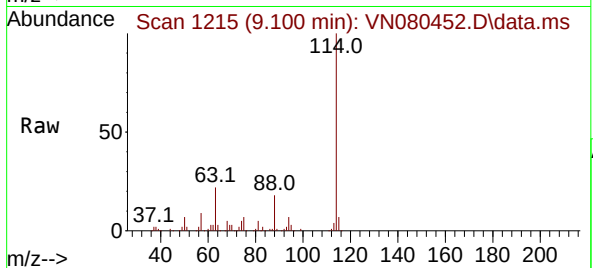

#35

Dibromofluoromethane

Concen: 58.828 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. 0.000 min

Lab File: VN080452.D

Acq: 13 Dec 2023 10:22




Tgt Ion:113 Resp: 135042


Ion Ratio Lower Upper

113 100

111 102.7 82.6 123.8

192 20.1 12.7 19.1#


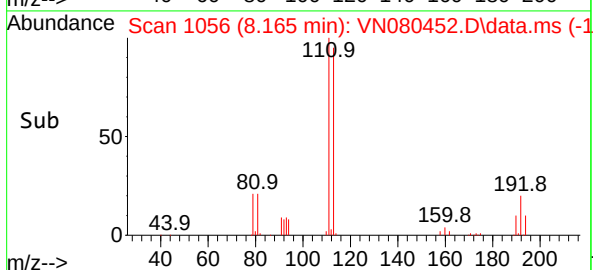
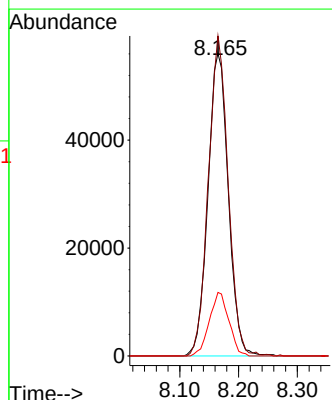
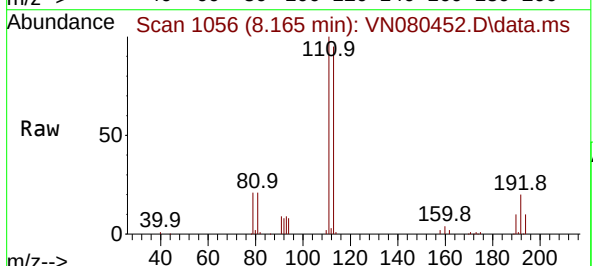


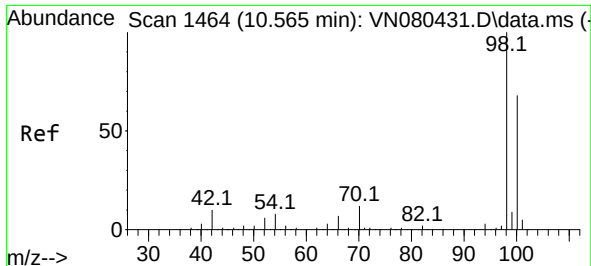

#50
Toluene-d8
Concen: 56.408 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. 0.000 min
Lab File: VN080452.D
Acq: 13 Dec 2023 10:22




Instrument :
MSVOA_N
ClientSampleId :
VN1213WBL01


Tgt Ion: 98 Resp: 482921
Ion Ratio Lower Upper
98 100
100 65.0 52.0 78.0

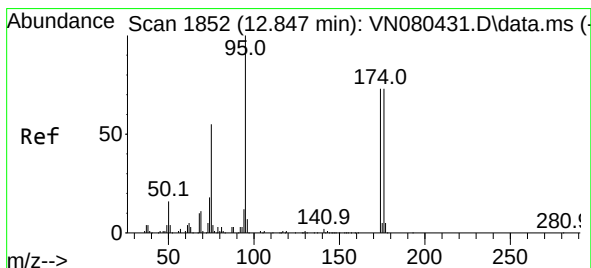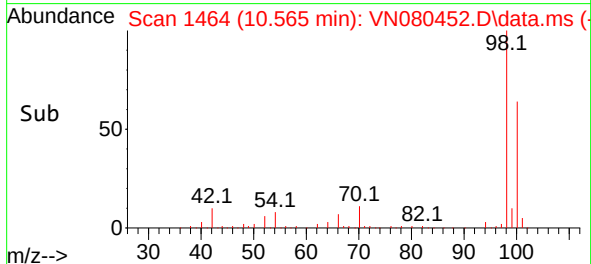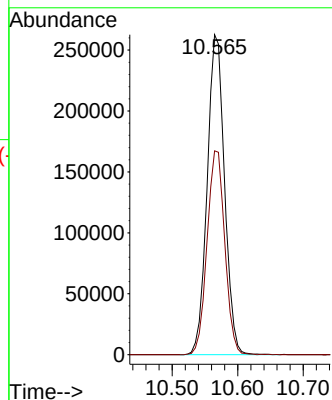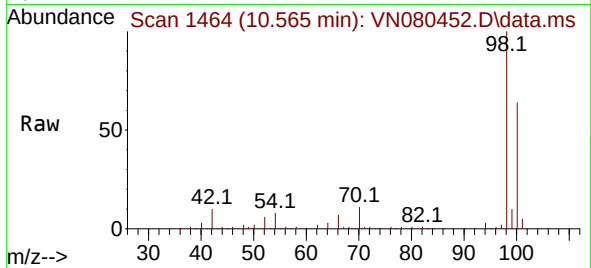

#62
4-Bromofluorobenzene
Concen: 59.131 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.000 min
Lab File: VN080452.D
Acq: 13 Dec 2023 10:22

Tgt Ion: 95 Resp: 192230
Ion Ratio Lower Upper
95 100
174 75.6 0.0 143.8
176 74.3 0.0 135.8


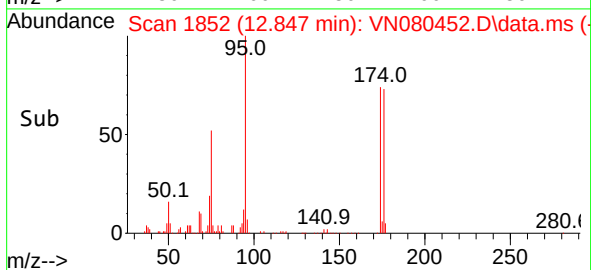
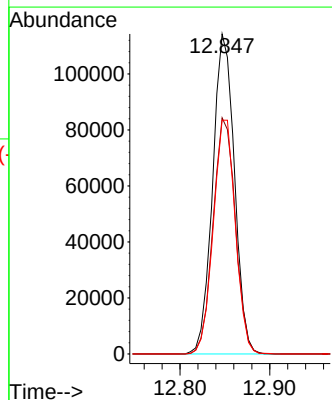
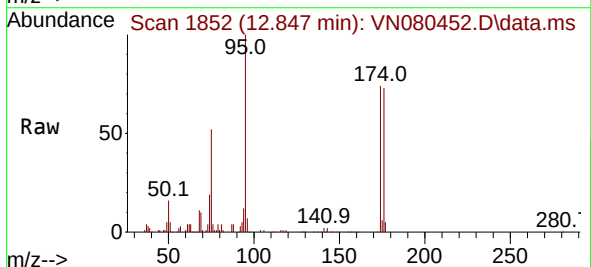


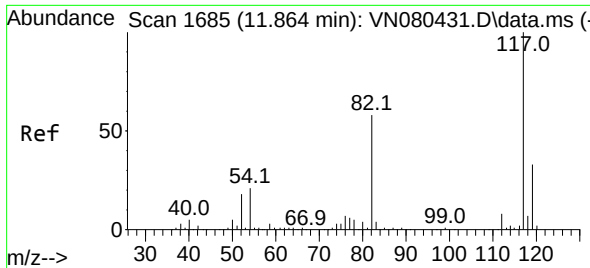

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN080452.D
Acq: 13 Dec 2023 10:22

Instrument :
MSVOA_N
ClientSampleId :
VN1213WBL01

Tgt Ion:117 Resp: 378844
Ion Ratio Lower Upper
117 100
82 58.6 44.0 66.0
119 32.6 25.6 38.4

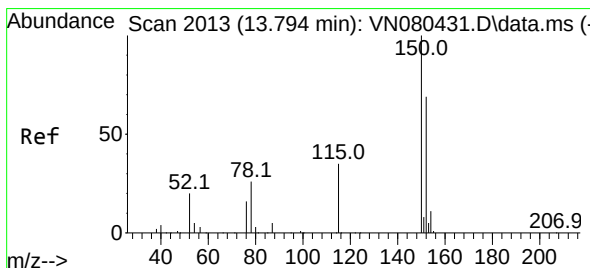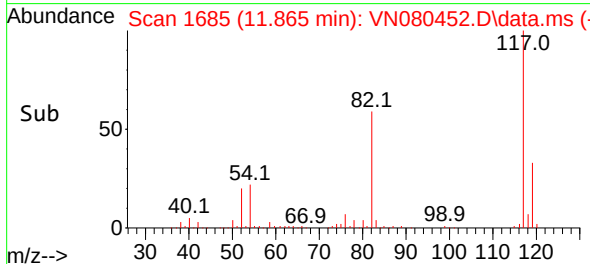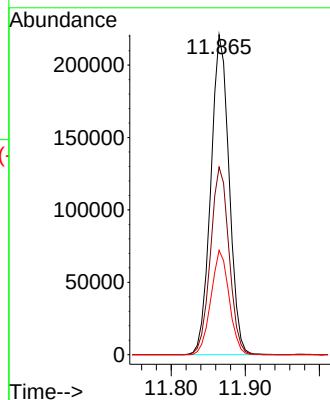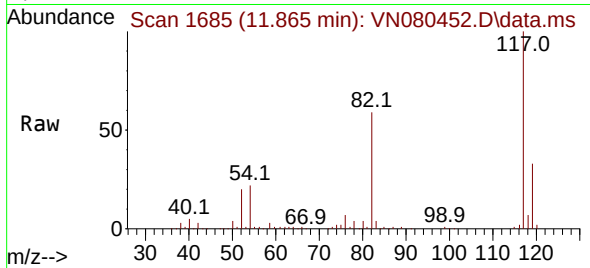

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. 0.000 min
Lab File: VN080452.D
Acq: 13 Dec 2023 10:22

Tgt Ion:152 Resp: 170317
Ion Ratio Lower Upper
152 100
115 65.1 32.3 96.8
150 157.8 0.0 355.8

