
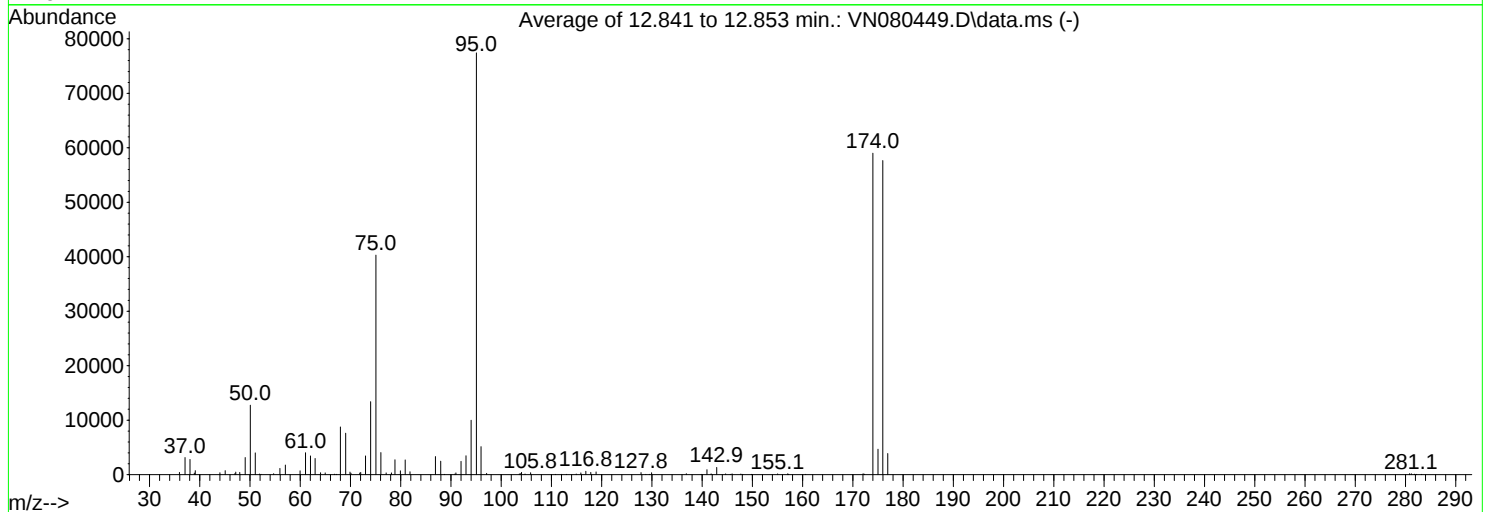


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121323\
Data File : VN080449.D
Acq On : 13 Dec 2023 08:35
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121223W.M
Title : SW846 8260
Last Update : Wed Dec 13 01:57:14 2023

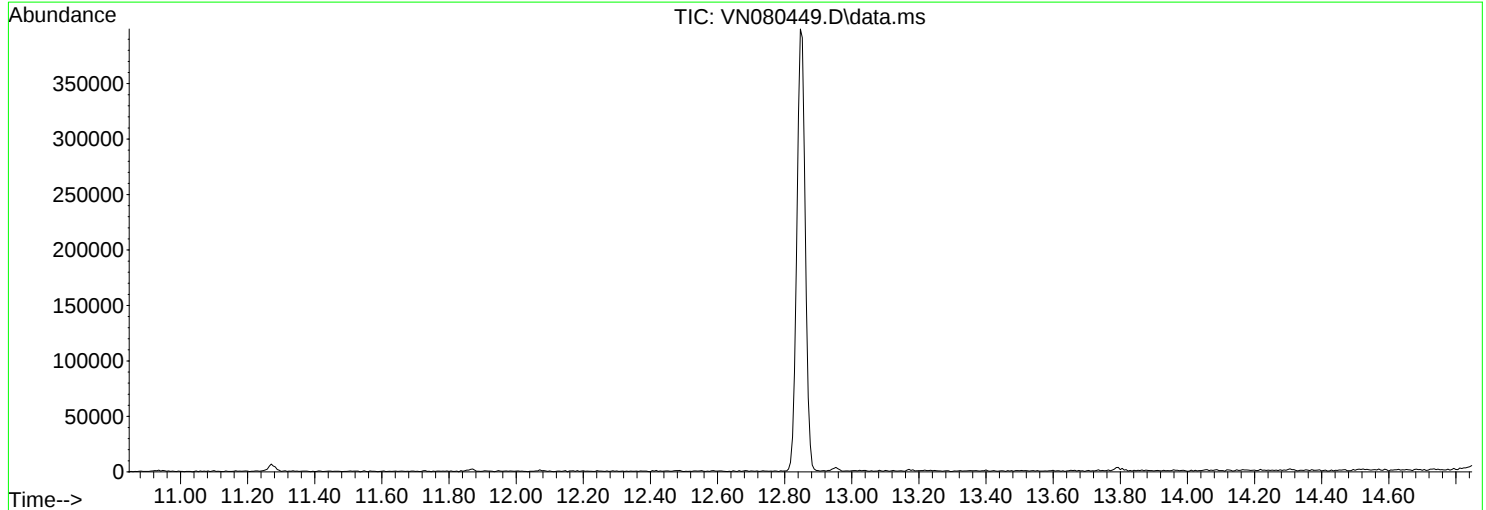

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	12738	PASS
75	95	30	60	52.0	40291	PASS
95	95	100	100	100.0	77429	PASS
96	95	5	9	6.6	5148	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	76.2	59011	PASS
175	174	5	9	7.9	4679	PASS
176	174	95	101	97.7	57656	PASS
177	176	5	9	6.7	3883	PASS

Average of 12.841 to 12.853 min.: VN080449.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	421	50.05	12738	64.05	364	74.00	1340
37.05	3145	51.05	4011	64.95	313	75.05	4029
38.05	2784	51.90	129	66.80	95	76.05	404
38.90	290	52.20	52	67.20	67	77.10	32
39.10	742	54.70	182	68.00	8766	78.15	319
44.00	368	55.95	1146	69.05	7622	78.85	2720
45.05	746	57.05	1769	69.90	461	79.95	696
47.00	209	59.95	710	70.10	263	80.90	2719
47.15	487	61.05	4018	71.85	308	81.85	539
47.95	414	62.05	3444	72.05	414	86.90	3318
49.05	3152	62.95	2977	73.00	3447	87.95	2481

Average of 12.841 to 12.853 min.: VN080449.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
88.70	58	104.05	404	127.85	391	145.95	144
90.80	109	104.75	124	128.80	52	147.70	135
91.00	328	105.85	369	129.50	55	148.10	75
92.00	2436	110.80	59	129.95	358	149.80	53
93.00	3480	112.00	56	136.85	165	155.05	154
94.00	9982	113.00	52	139.80	67	157.00	143
95.05	77429	114.95	107	140.95	901	157.20	85
96.00	5148	115.85	317	141.80	157	160.60	65
97.10	240	116.85	616	142.90	1338	172.05	180
103.60	108	117.85	413	144.70	137	172.30	96
103.80	204	118.90	507	145.60	60	174.00	59011

Average of 12.841 to 12.853 min.: VN080449.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
175.00	4679						
175.95	57656						
176.95	3883						
280.80	183						
281.15	189						
281.80	87						
282.20	51						
283.20	56						

Instrument :

MSVOA_N

ClientSampleId :

BFB