
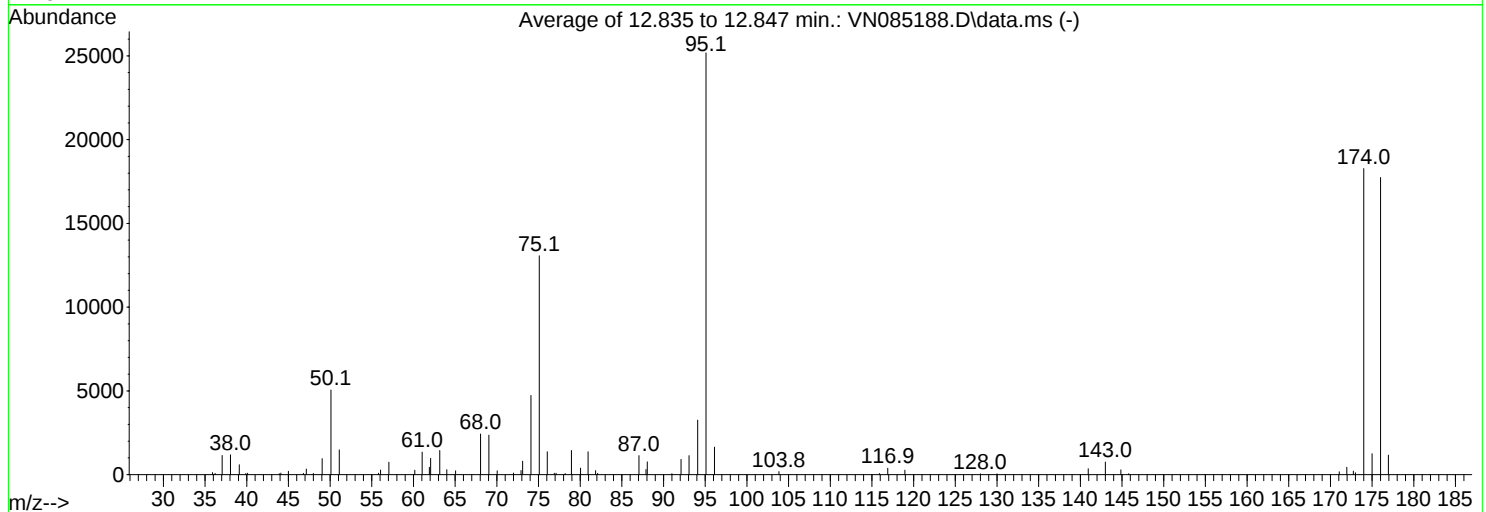


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121324\
Data File : VN085188.D
Acq On : 13 Dec 2024 08:38
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112224W.M
Title : SW846 8260
Last Update : Sat Nov 23 02:54:10 2024

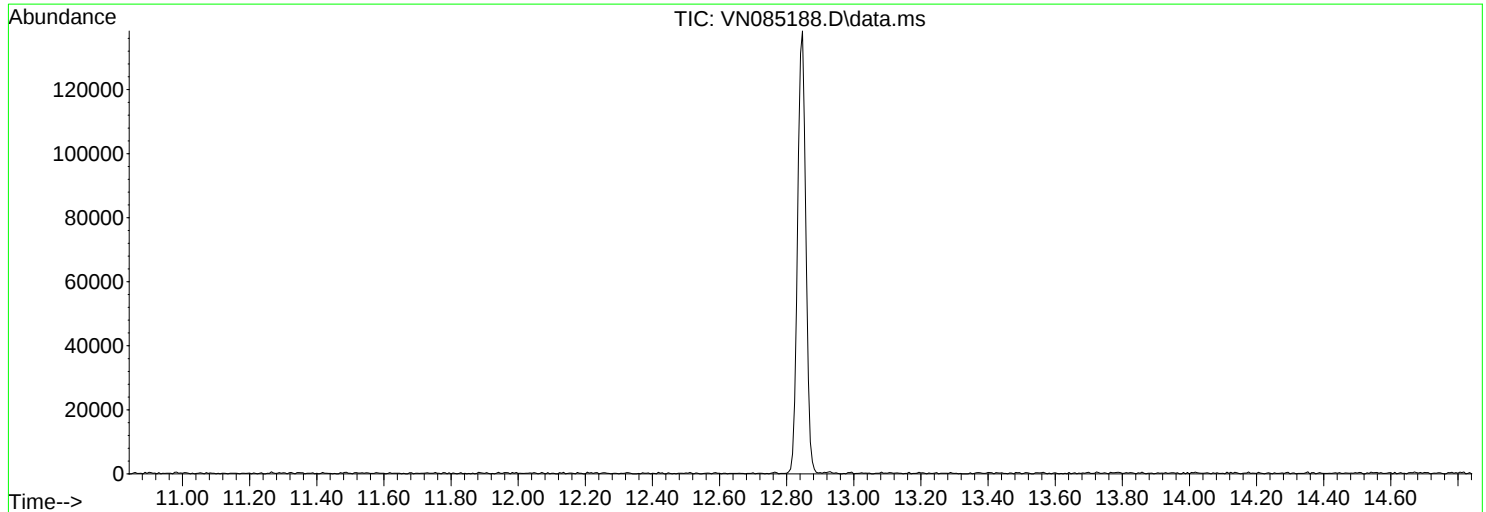

AutoFind: Scans 1850, 1851, 1852; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.1	5056	PASS
75	95	30	60	51.9	13072	PASS
95	95	100	100	100.0	25181	PASS
96	95	5	9	6.5	1642	PASS
173	174	0.00	2	1.1	206	PASS
174	95	50	100	72.6	18276	PASS
175	174	5	9	6.8	1249	PASS
176	174	95	101	97.1	17738	PASS
177	176	5	9	6.6	1164	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	123	47.15	336	62.05	970	75.10	1307
36.20	80	48.00	77	63.15	1438	76.05	1361
37.05	1147	49.05	960	64.00	296	76.90	8
38.05	1184	50.10	5056	65.05	230	77.10	9
39.10	588	51.10	1478	68.05	2429	78.20	69
39.90	65	55.80	83	69.05	2357	78.95	1440
40.10	89	56.05	275	70.05	227	80.05	392
43.90	58	57.05	743	72.00	95	80.95	1365
44.10	99	60.15	270	72.90	251	81.85	238
45.00	200	61.05	1344	73.10	805	82.10	73
46.80	74	61.90	440	74.10	4725	87.05	1139

Average of 12.835 to 12.847 min.: VN085188.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.90	309	118.95	263	174.00	18276		
88.05	763	128.00	52	175.00	1249		
91.00	56	130.00	52	176.00	17738		
92.10	903	140.95	352	176.95	1164		
93.05	1134	143.00	756				
94.10	3258	144.85	286				
95.10	25181	145.80	55				
96.10	1642	171.05	176				
103.85	181	171.95	441				
115.90	70	172.75	206				
116.90	380	173.00	117				

Instrument :

MSVOA_N

ClientSampleId :

BFB