


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN121418\
 Data File : VN052876.D
 Acq On : 14 Dec 2018 9:15
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N112618W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Tue Nov 27 00:48:33 2018

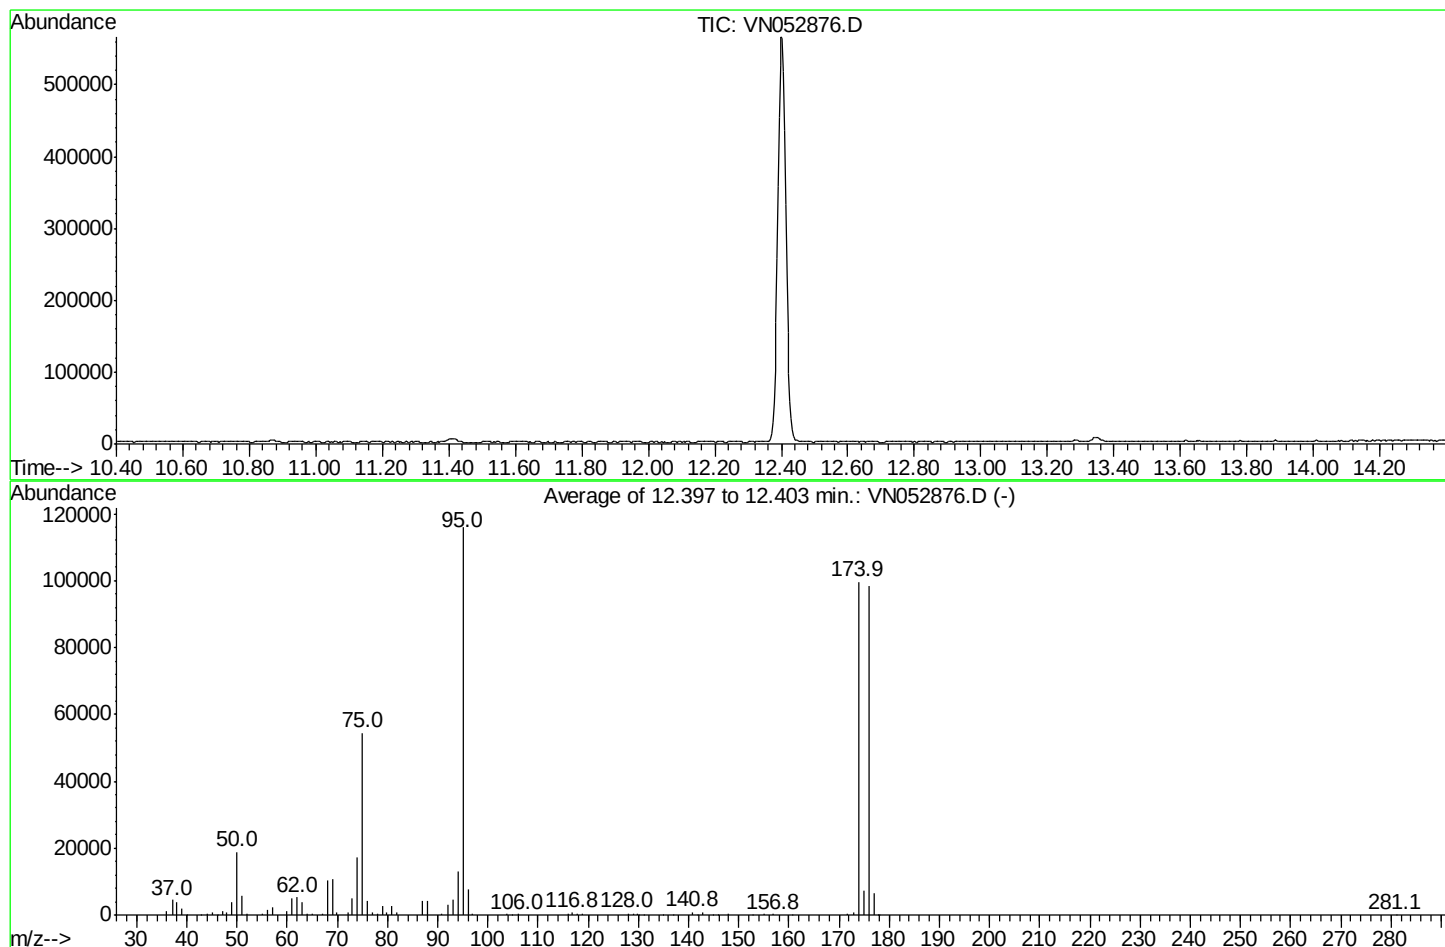

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	18845	PASS
75	95	30	60	47.0	54482	PASS
95	95	100	100	100.0	115946	PASS
96	95	5	9	6.5	7530	PASS
173	174	0.00	2	0.9	912	PASS
174	95	50	100	85.9	99624	PASS
175	174	5	9	7.4	7390	PASS
176	174	95	101	98.6	98208	PASS
177	176	5	9	6.6	6489	PASS