


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN121418\
Data File : VN052888.D
Acq On : 14 Dec 2018 14:50
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 13 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N112618W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Tue Nov 27 00:48:33 2018

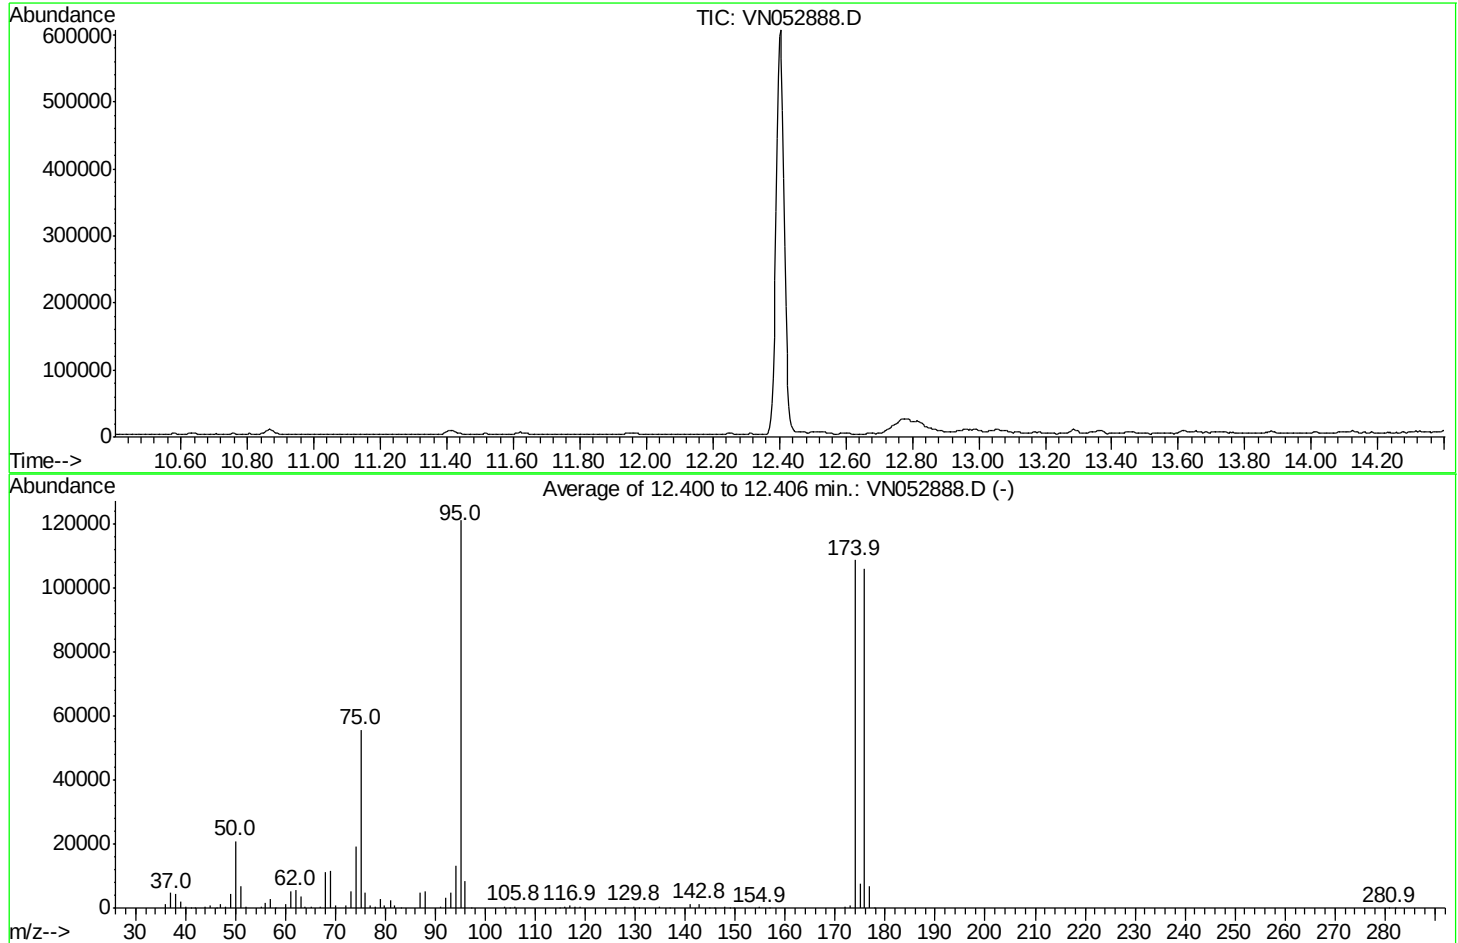

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	20784	PASS
75	95	30	60	45.9	55549	PASS
95	95	100	100	100.0	120941	PASS
96	95	5	9	6.9	8360	PASS
173	174	0.00	2	0.9	937	PASS
174	95	50	100	89.8	108597	PASS
175	174	5	9	6.9	7499	PASS
176	174	95	101	97.3	105704	PASS
177	176	5	9	6.5	6820	PASS