


Chloromethane

Response Ratio

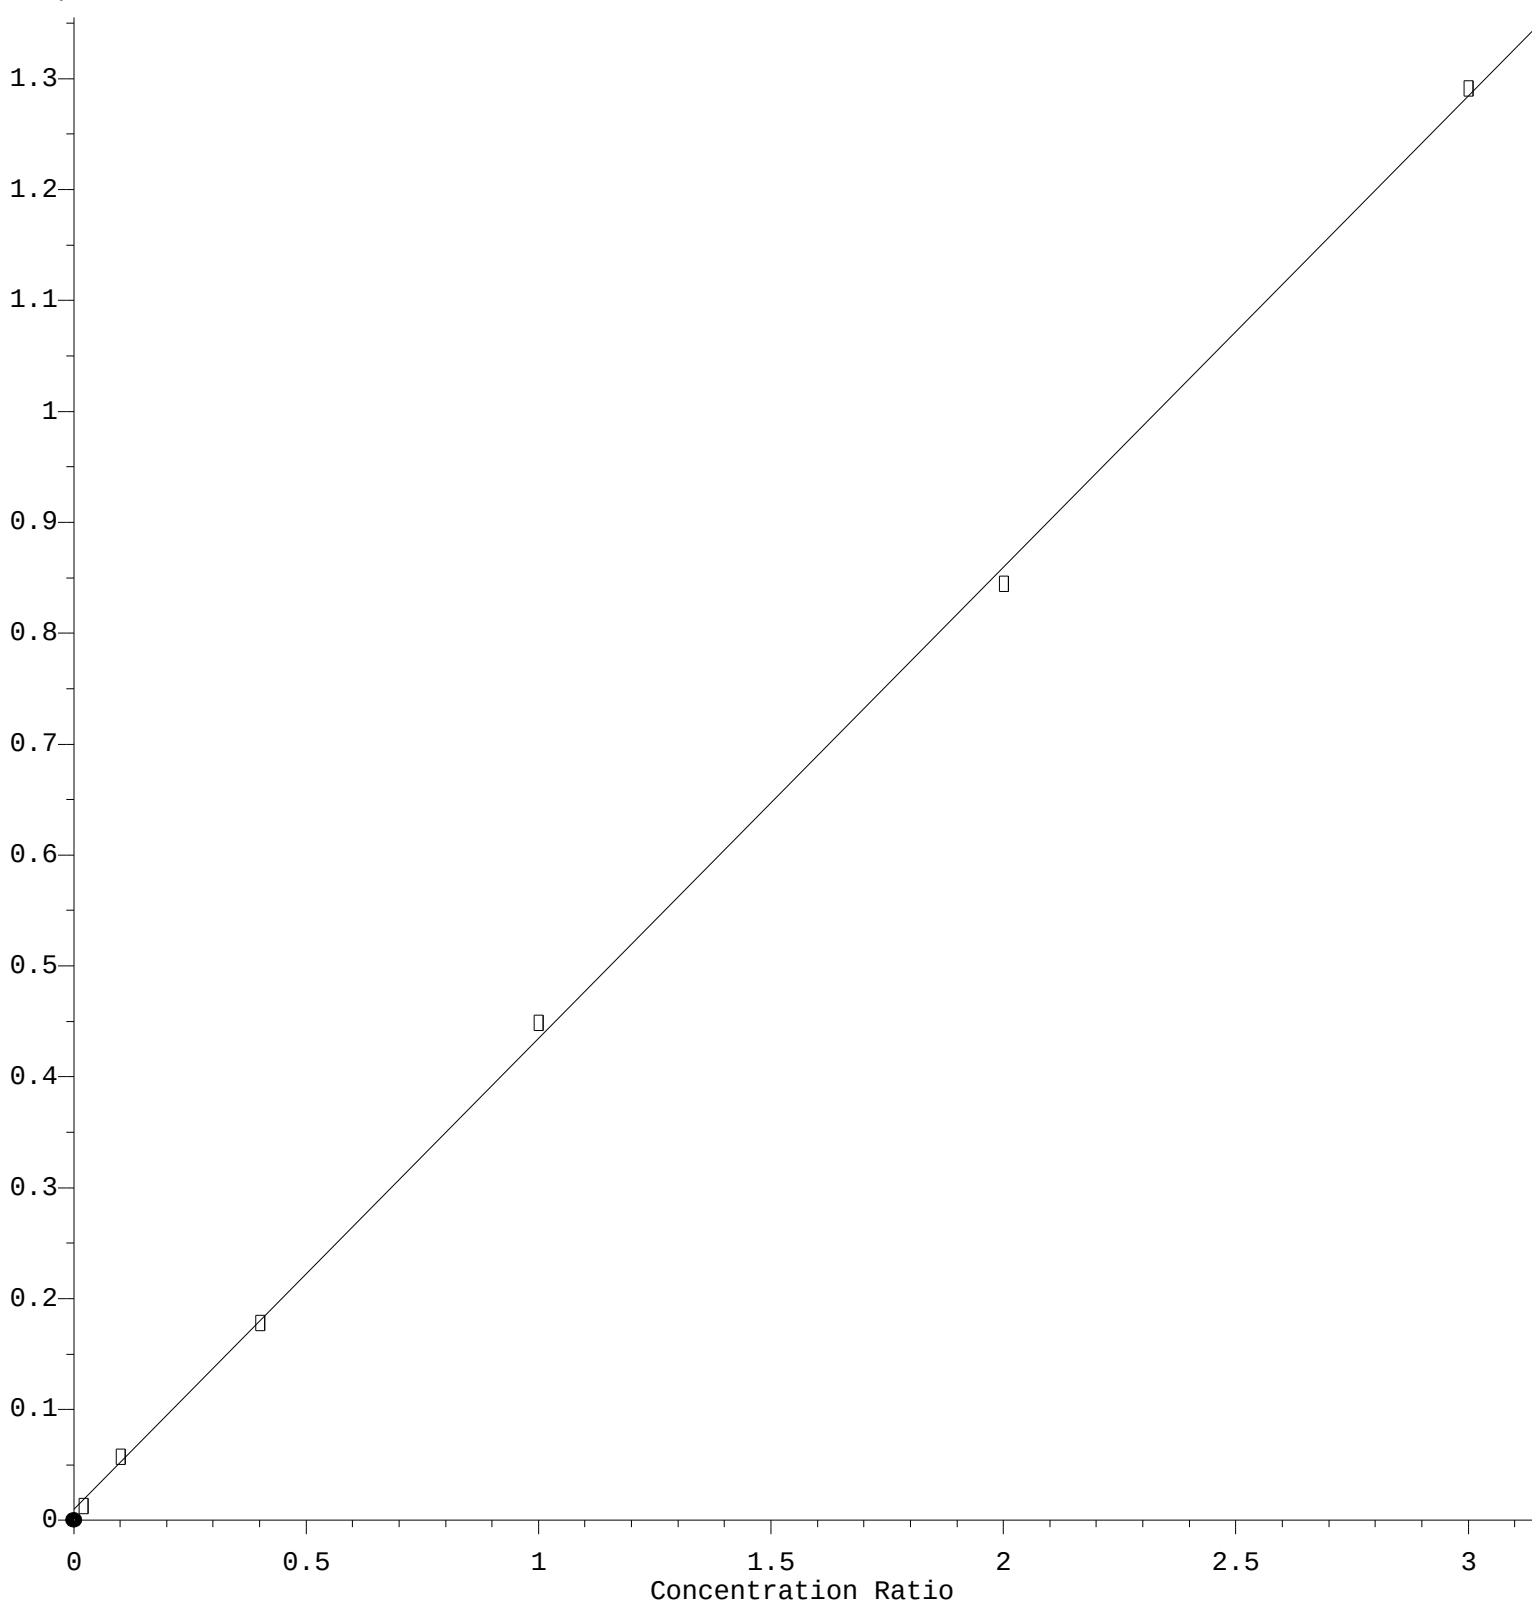


$$\text{Response} = 4.247\text{e-}001 * \text{Amt} + 1.027\text{e-}002$$

Coef of Det (r^2) = 0.999585 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121420W.M

Calibration Table Last Updated: Tue Dec 15 05:41:47 2020


Bromomethane

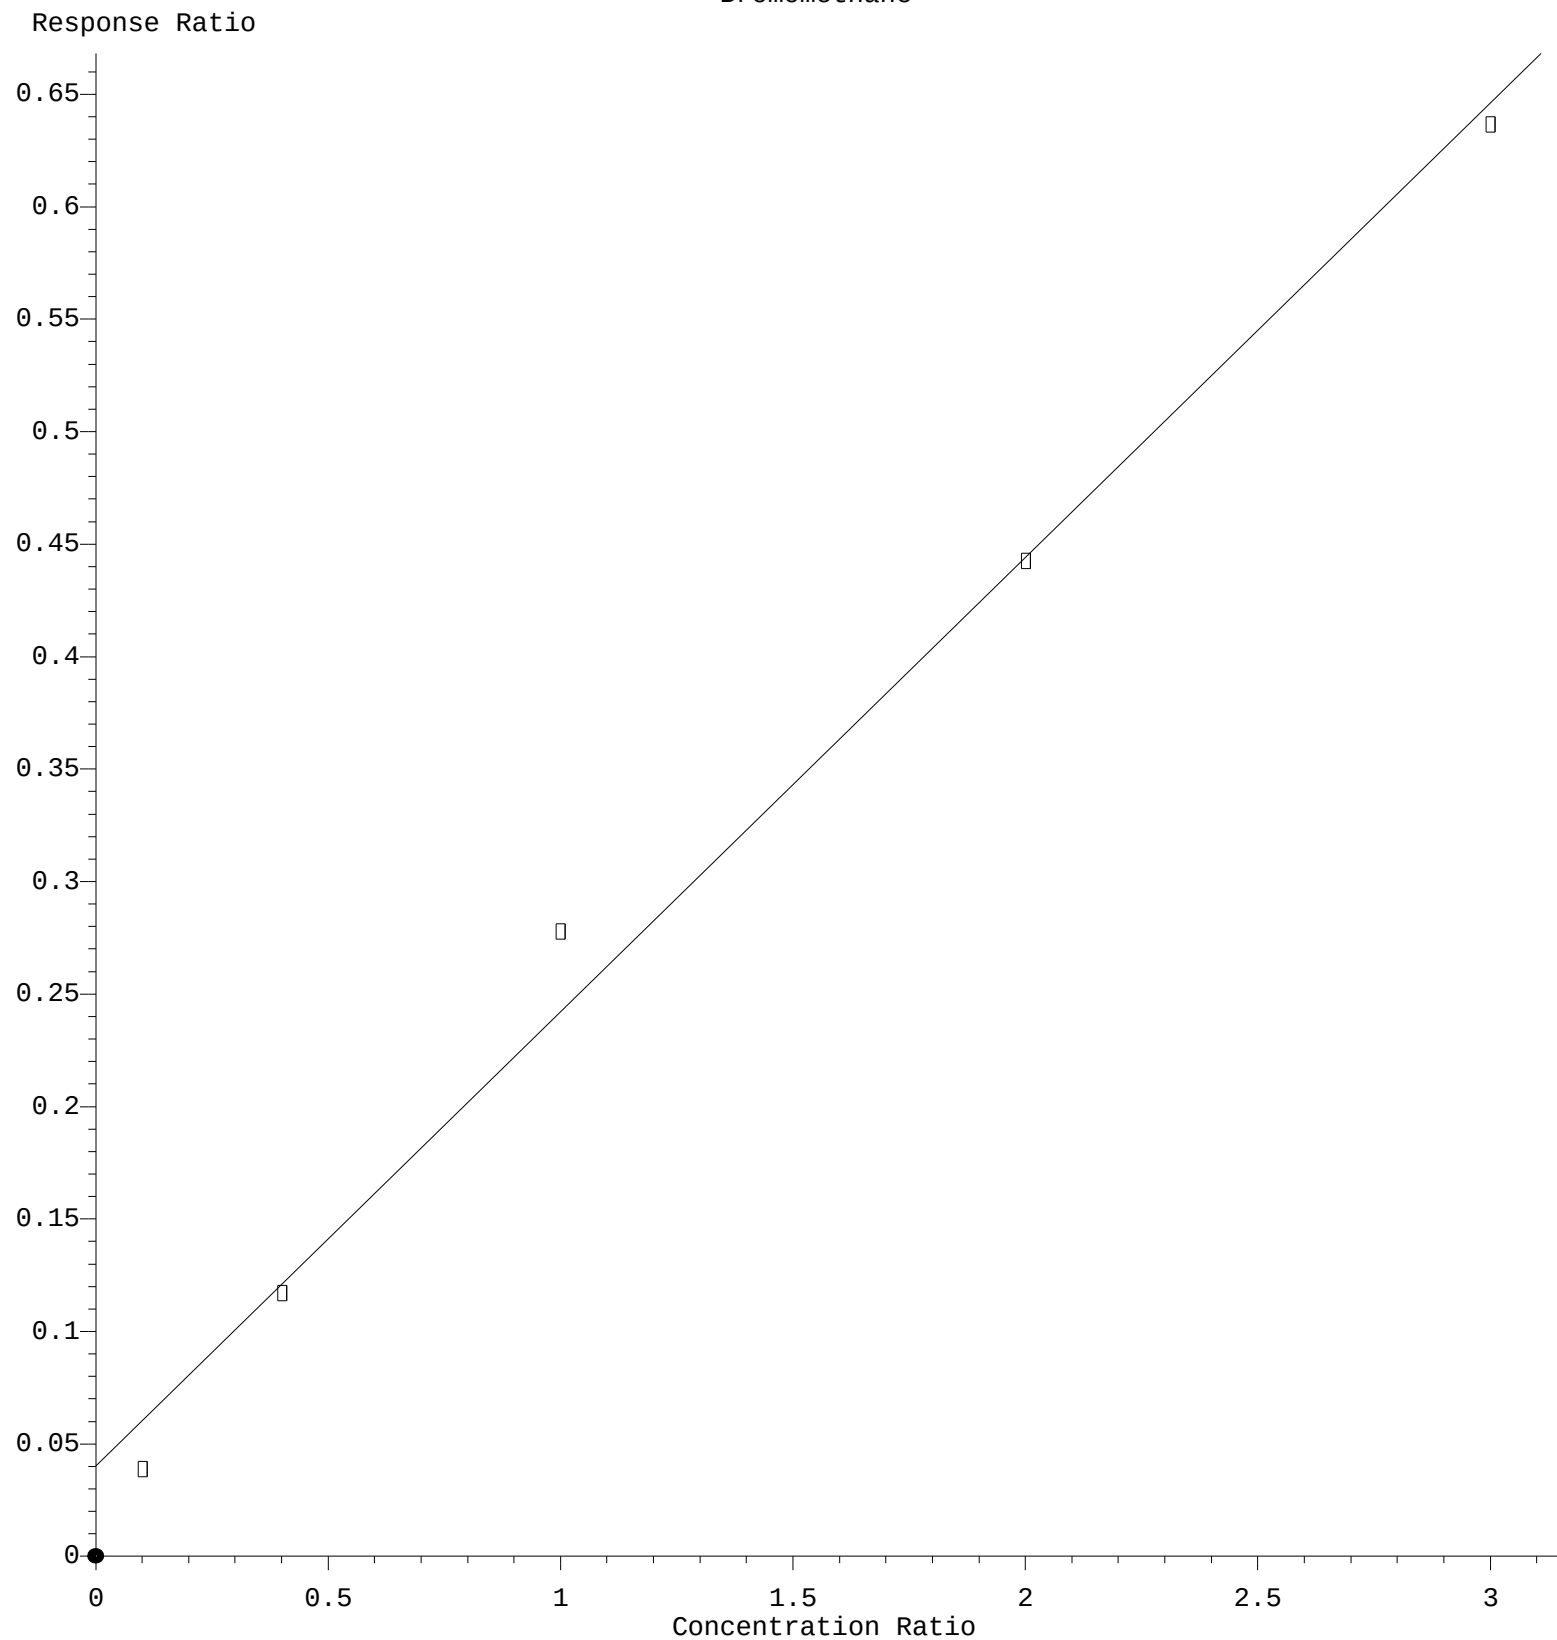

Response = 2.022e-001 * Amt + 3.954e-002
 Coef of Det (r^2) = 0.992131 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121420W.M
 Calibration Table Last Updated: Tue Dec 15 05:41:47 2020

Methyl Iodide

Response Ratio

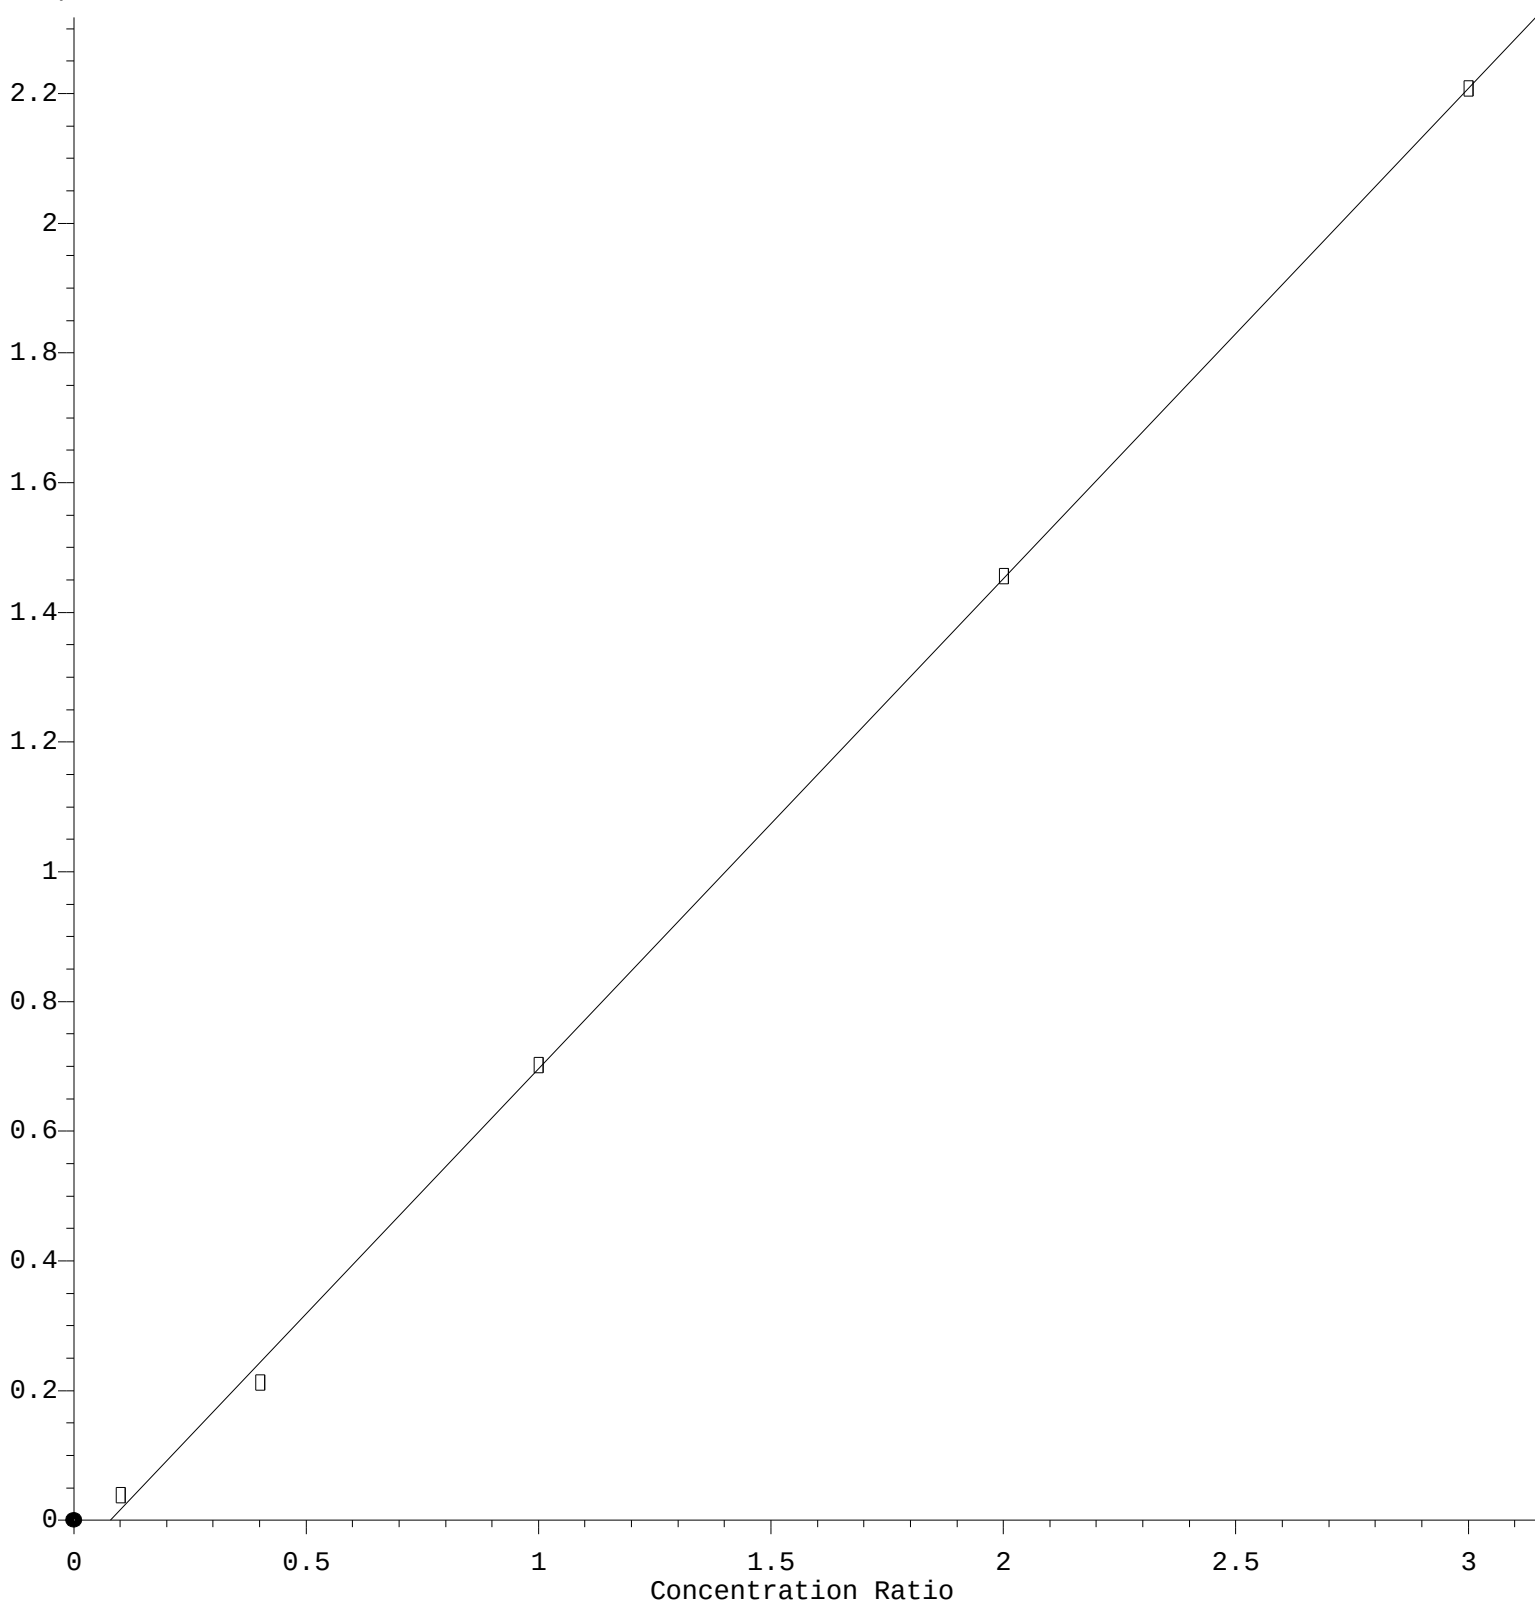

$$\text{Response} = 7.559\text{e-}001 * \text{Amt} - 5.955\text{e-}002$$


Coef of Det (r^2) = 0.999555 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121420W.M

Calibration Table Last Updated: Tue Dec 15 05:41:47 2020

Methylene Chloride

Response Ratio

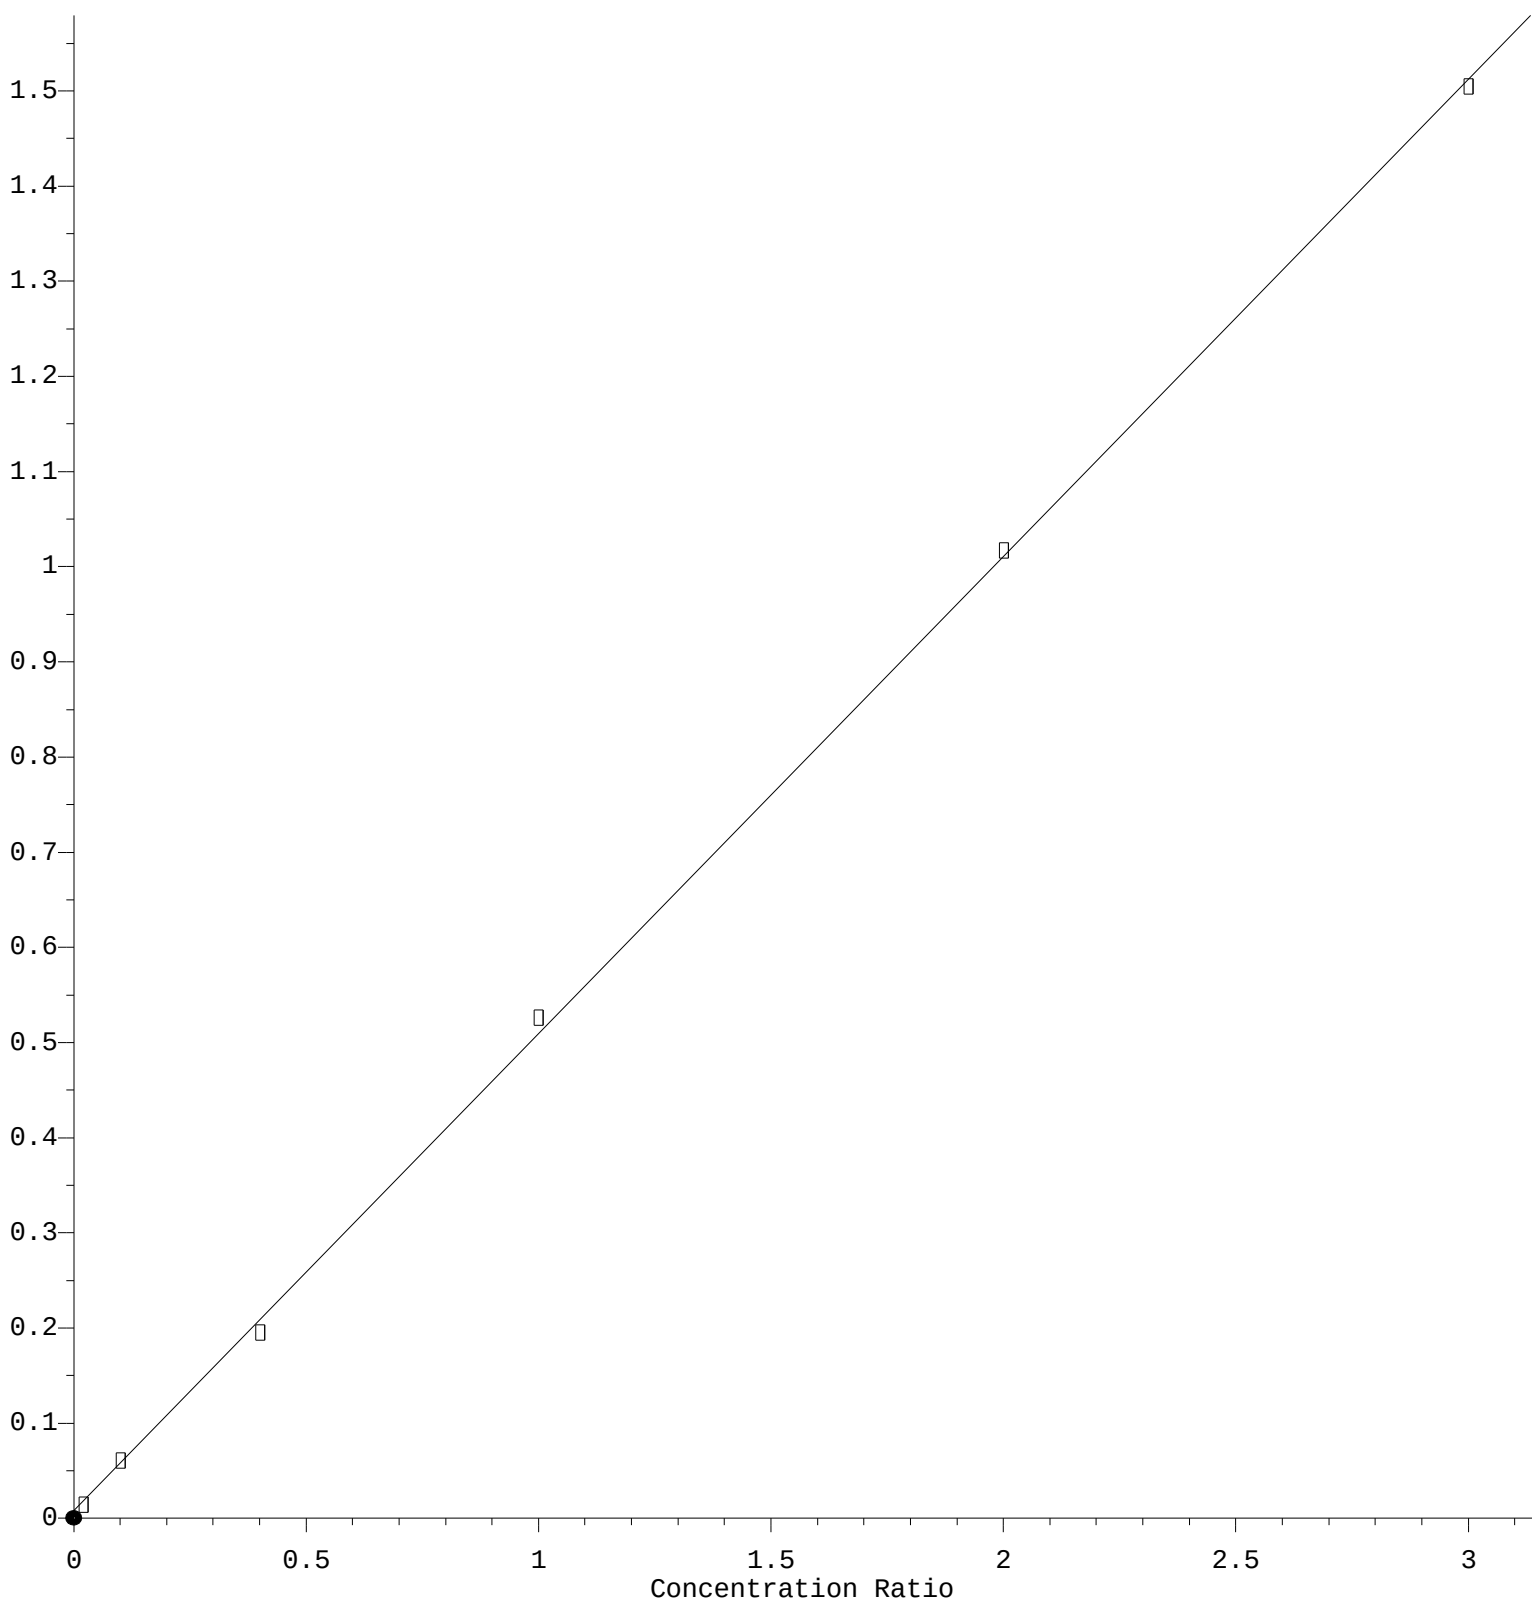

$$\text{Response} = 5.015\text{e-}001 * \text{Amt} + 7.865\text{e-}003$$


Coef of Det (r^2) = 0.999675 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121420W.M

Calibration Table Last Updated: Tue Dec 15 05:41:47 2020

Ethyl methacrylate

Response Ratio

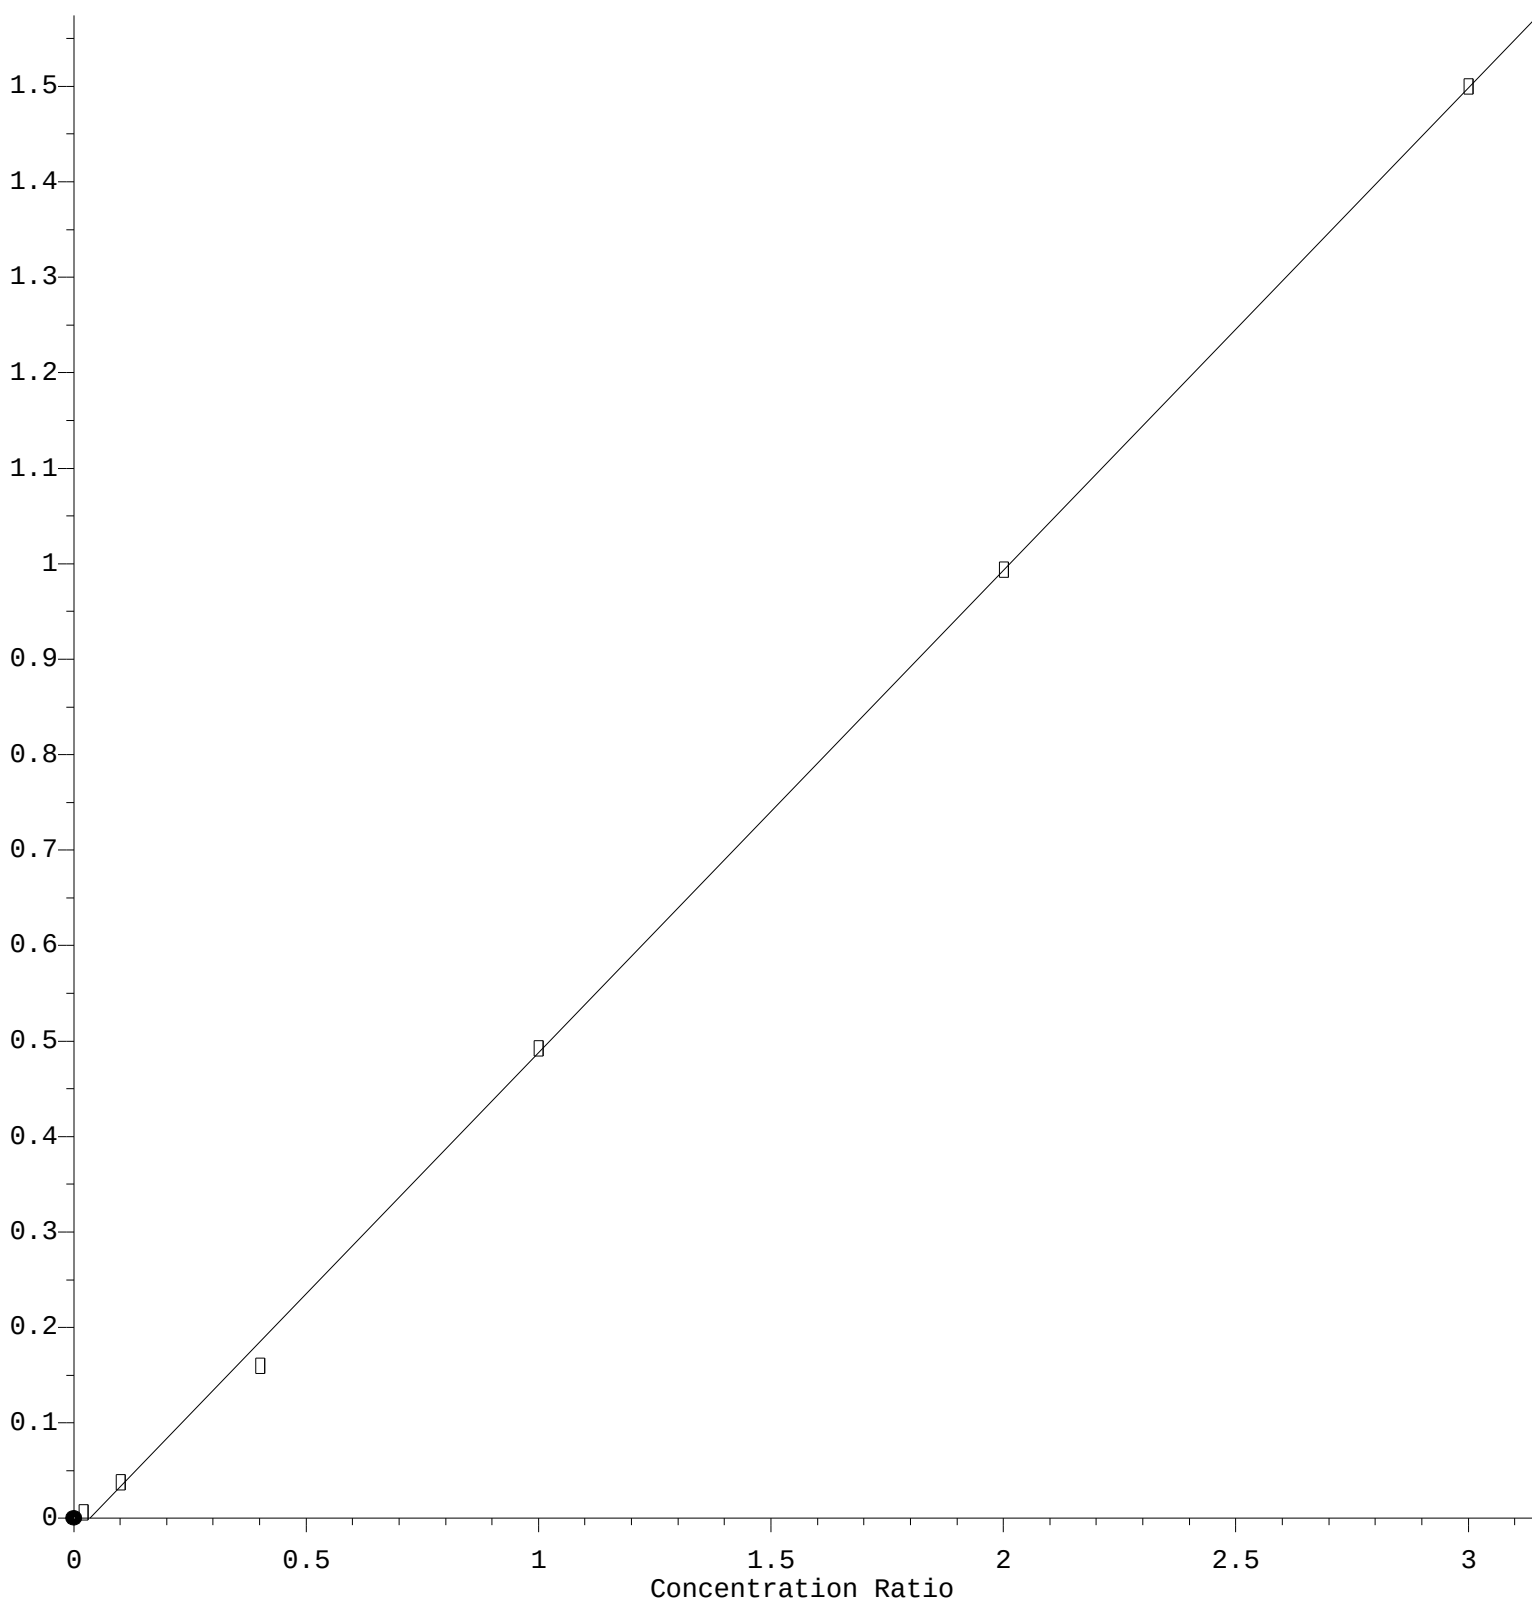

$$\text{Response} = 5.054\text{e-}001 * \text{Amt} - 1.789\text{e-}002$$


Coef of Det (r^2) = 0.999544 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121420W.M

Calibration Table Last Updated: Tue Dec 15 05:41:47 2020

Styrene

Response Ratio

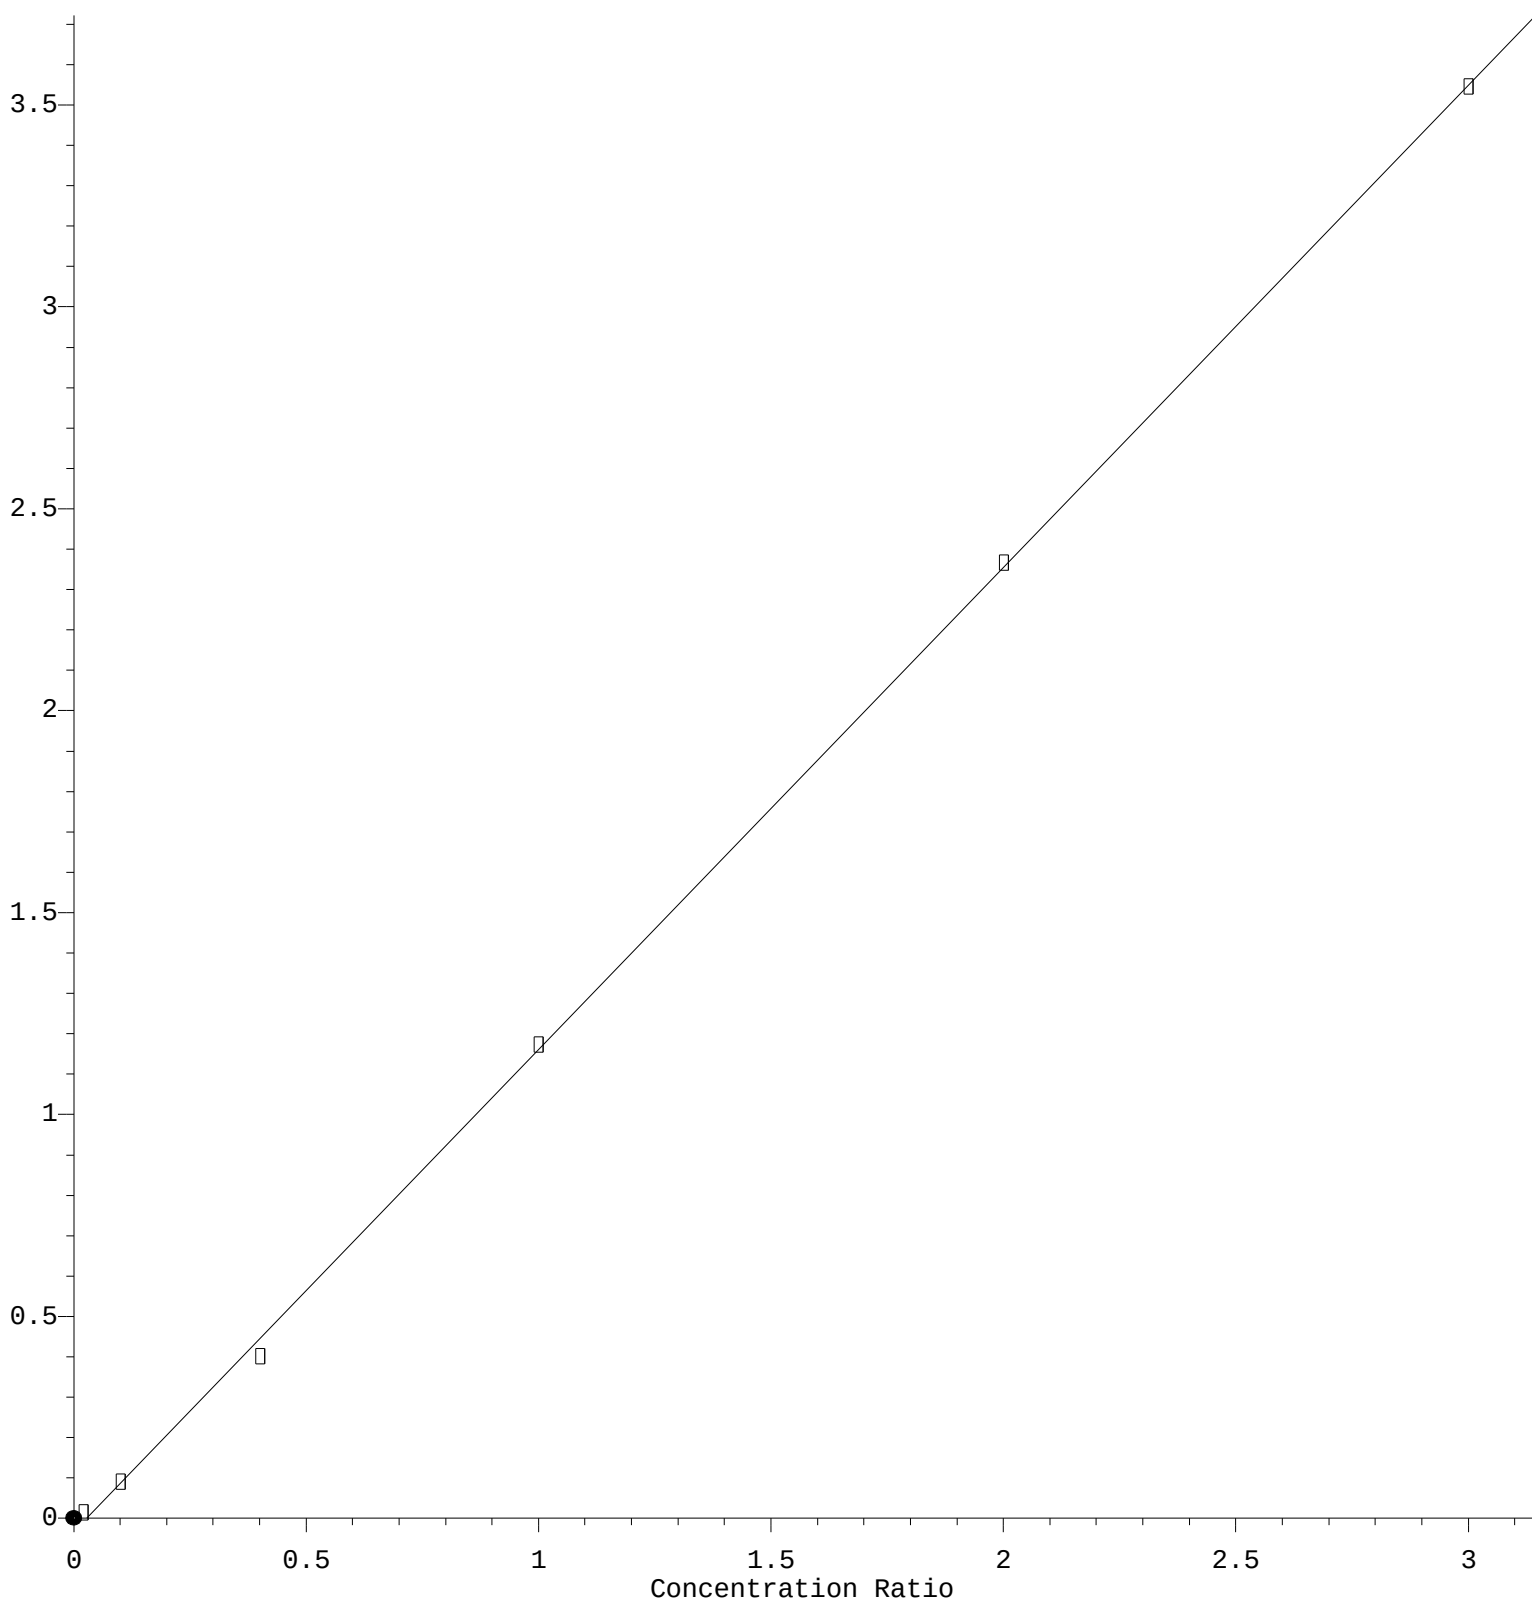

$$\text{Response} = 1.194\text{e}+000 * \text{Amt} - 3.293\text{e}-002$$


Coef of Det (r^2) = 0.999731 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121420W.M

Calibration Table Last Updated: Tue Dec 15 05:41:47 2020

p-Isopropyltoluene

Response Ratio

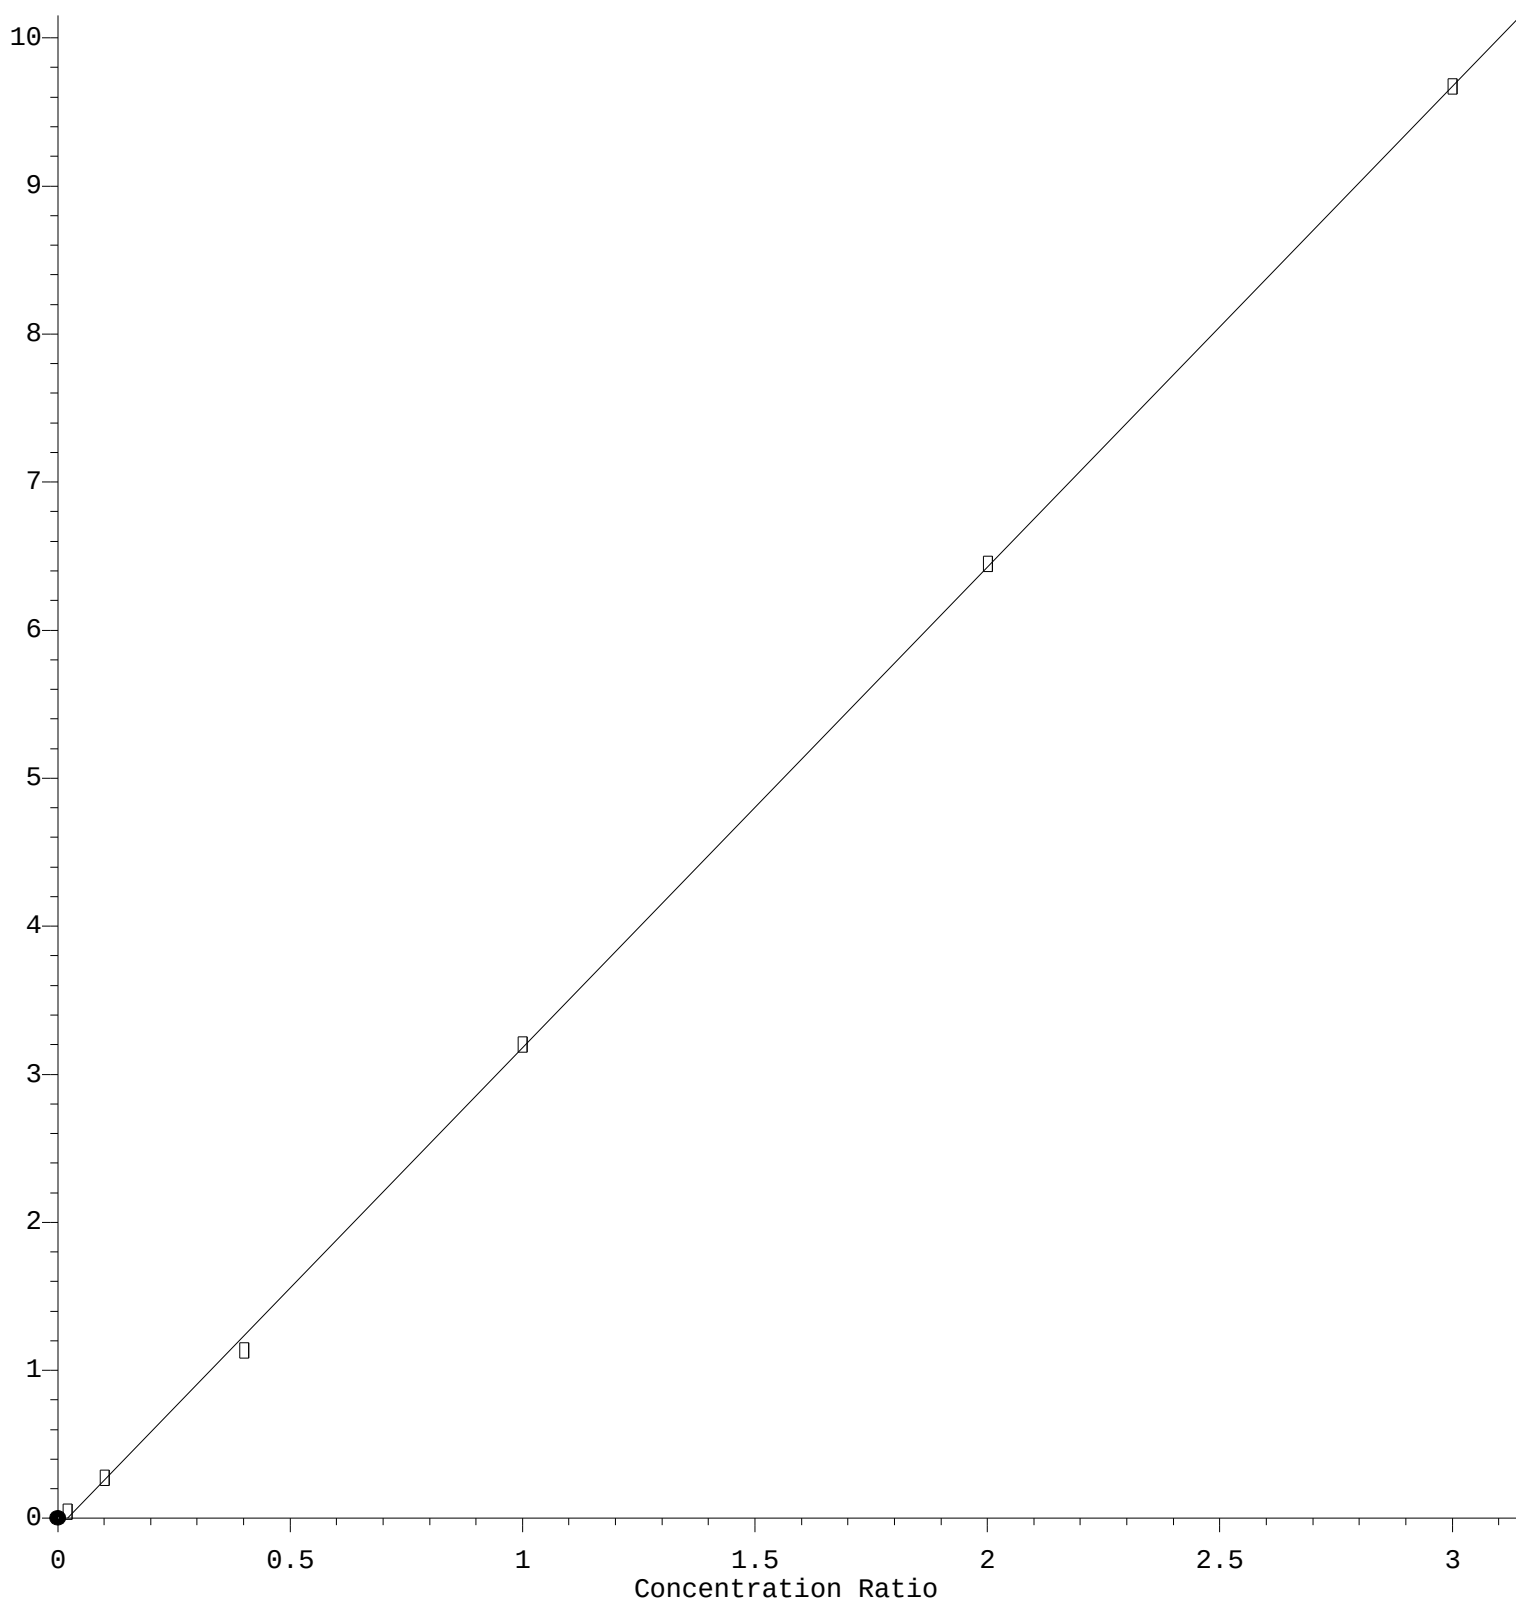

$$\text{Response} = 3.249\text{e}+000 * \text{Amt} - 6.923\text{e}-002$$


Coef of Det (r^2) = 0.999832 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121420W.M

Calibration Table Last Updated: Tue Dec 15 05:41:47 2020

1,2,4-Trichlorobenzene

Response Ratio

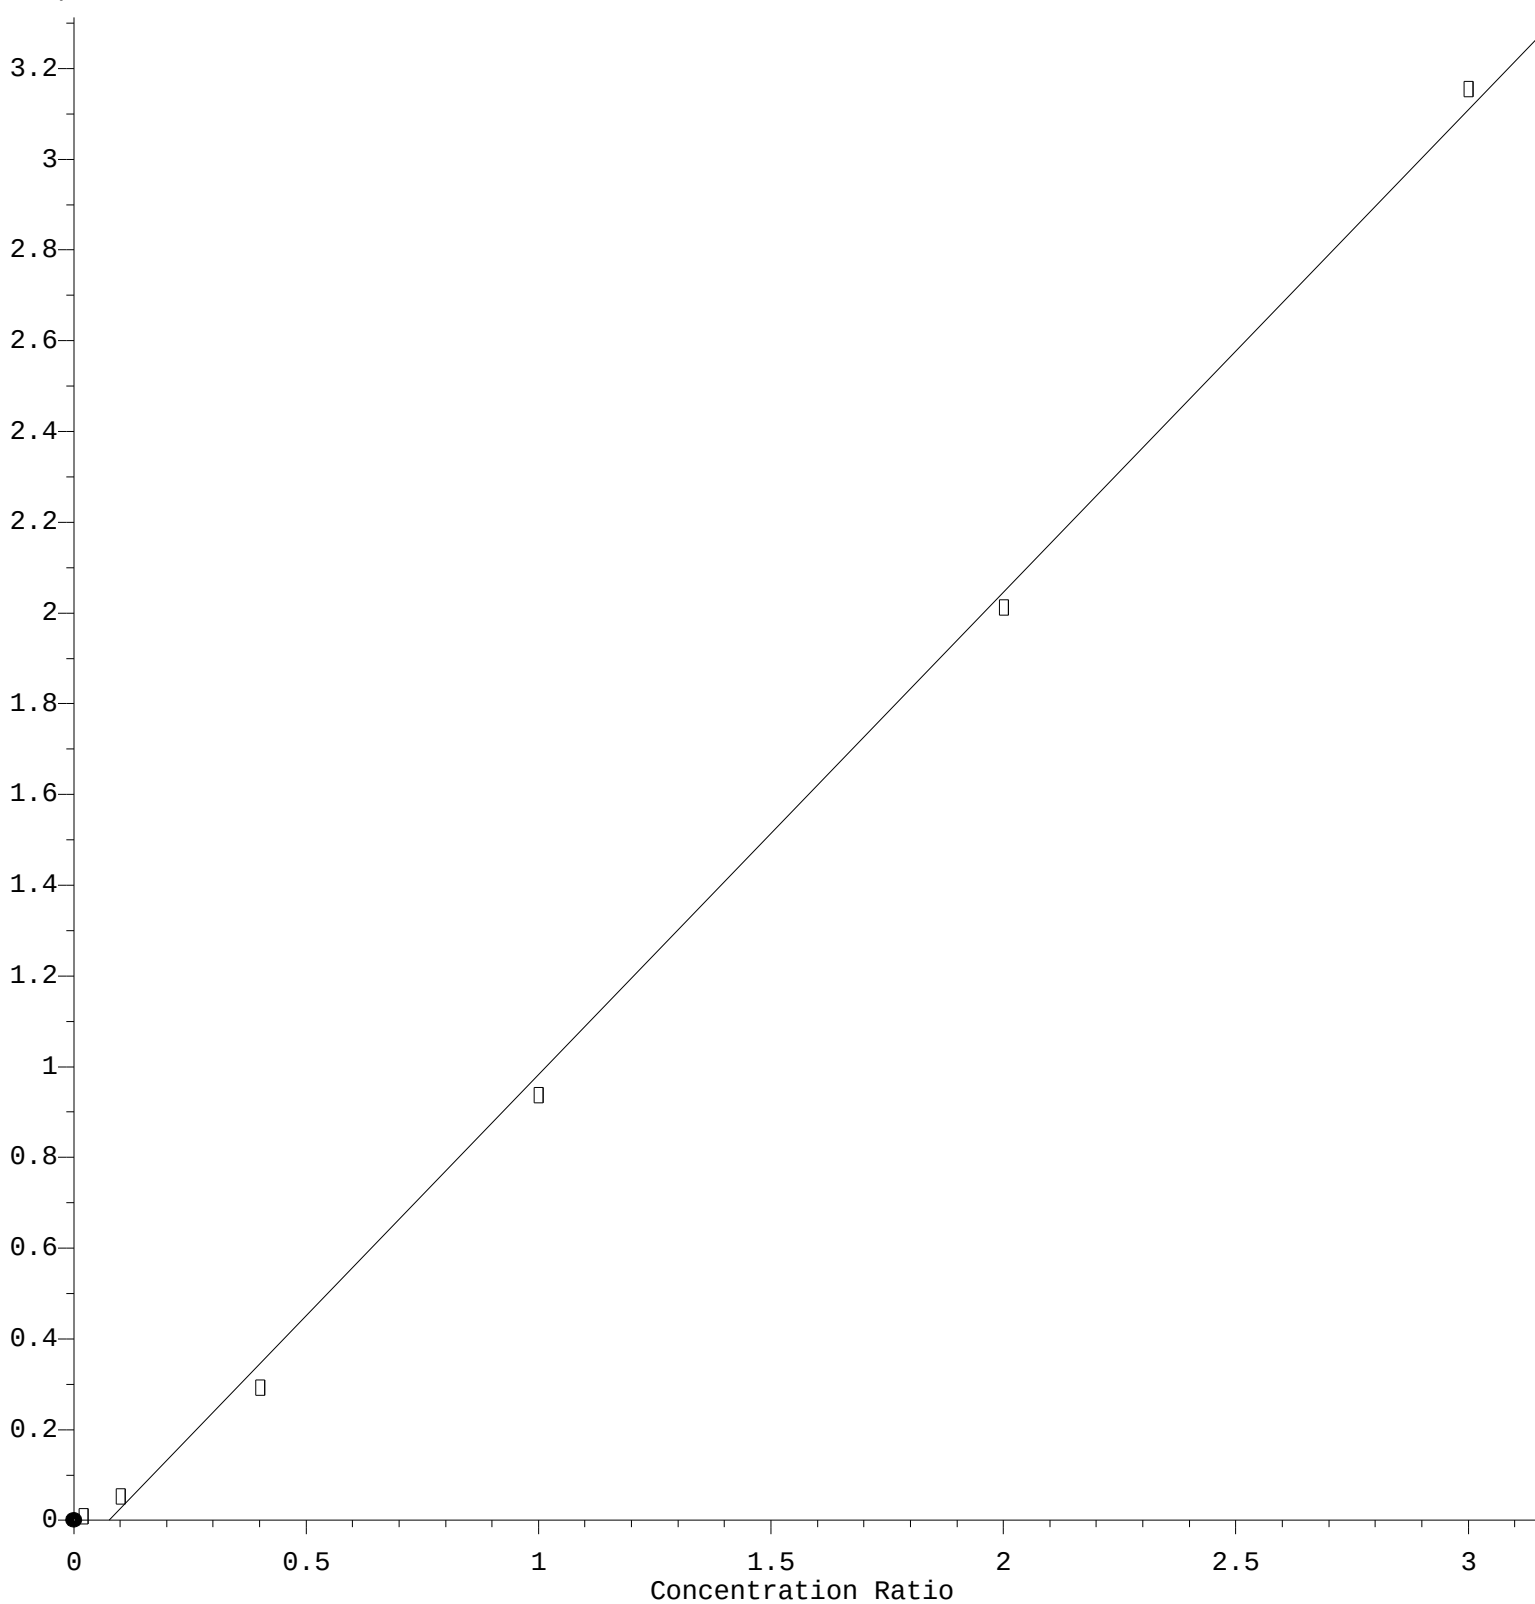

$$\text{Response} = 1.063\text{e}+000 * \text{Amt} - 7.929\text{e}-002$$


Coef of Det (r^2) = 0.998328 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121420W.M

Calibration Table Last Updated: Tue Dec 15 05:41:47 2020

1,2,4-Trichlorobenzene

Response Ratio

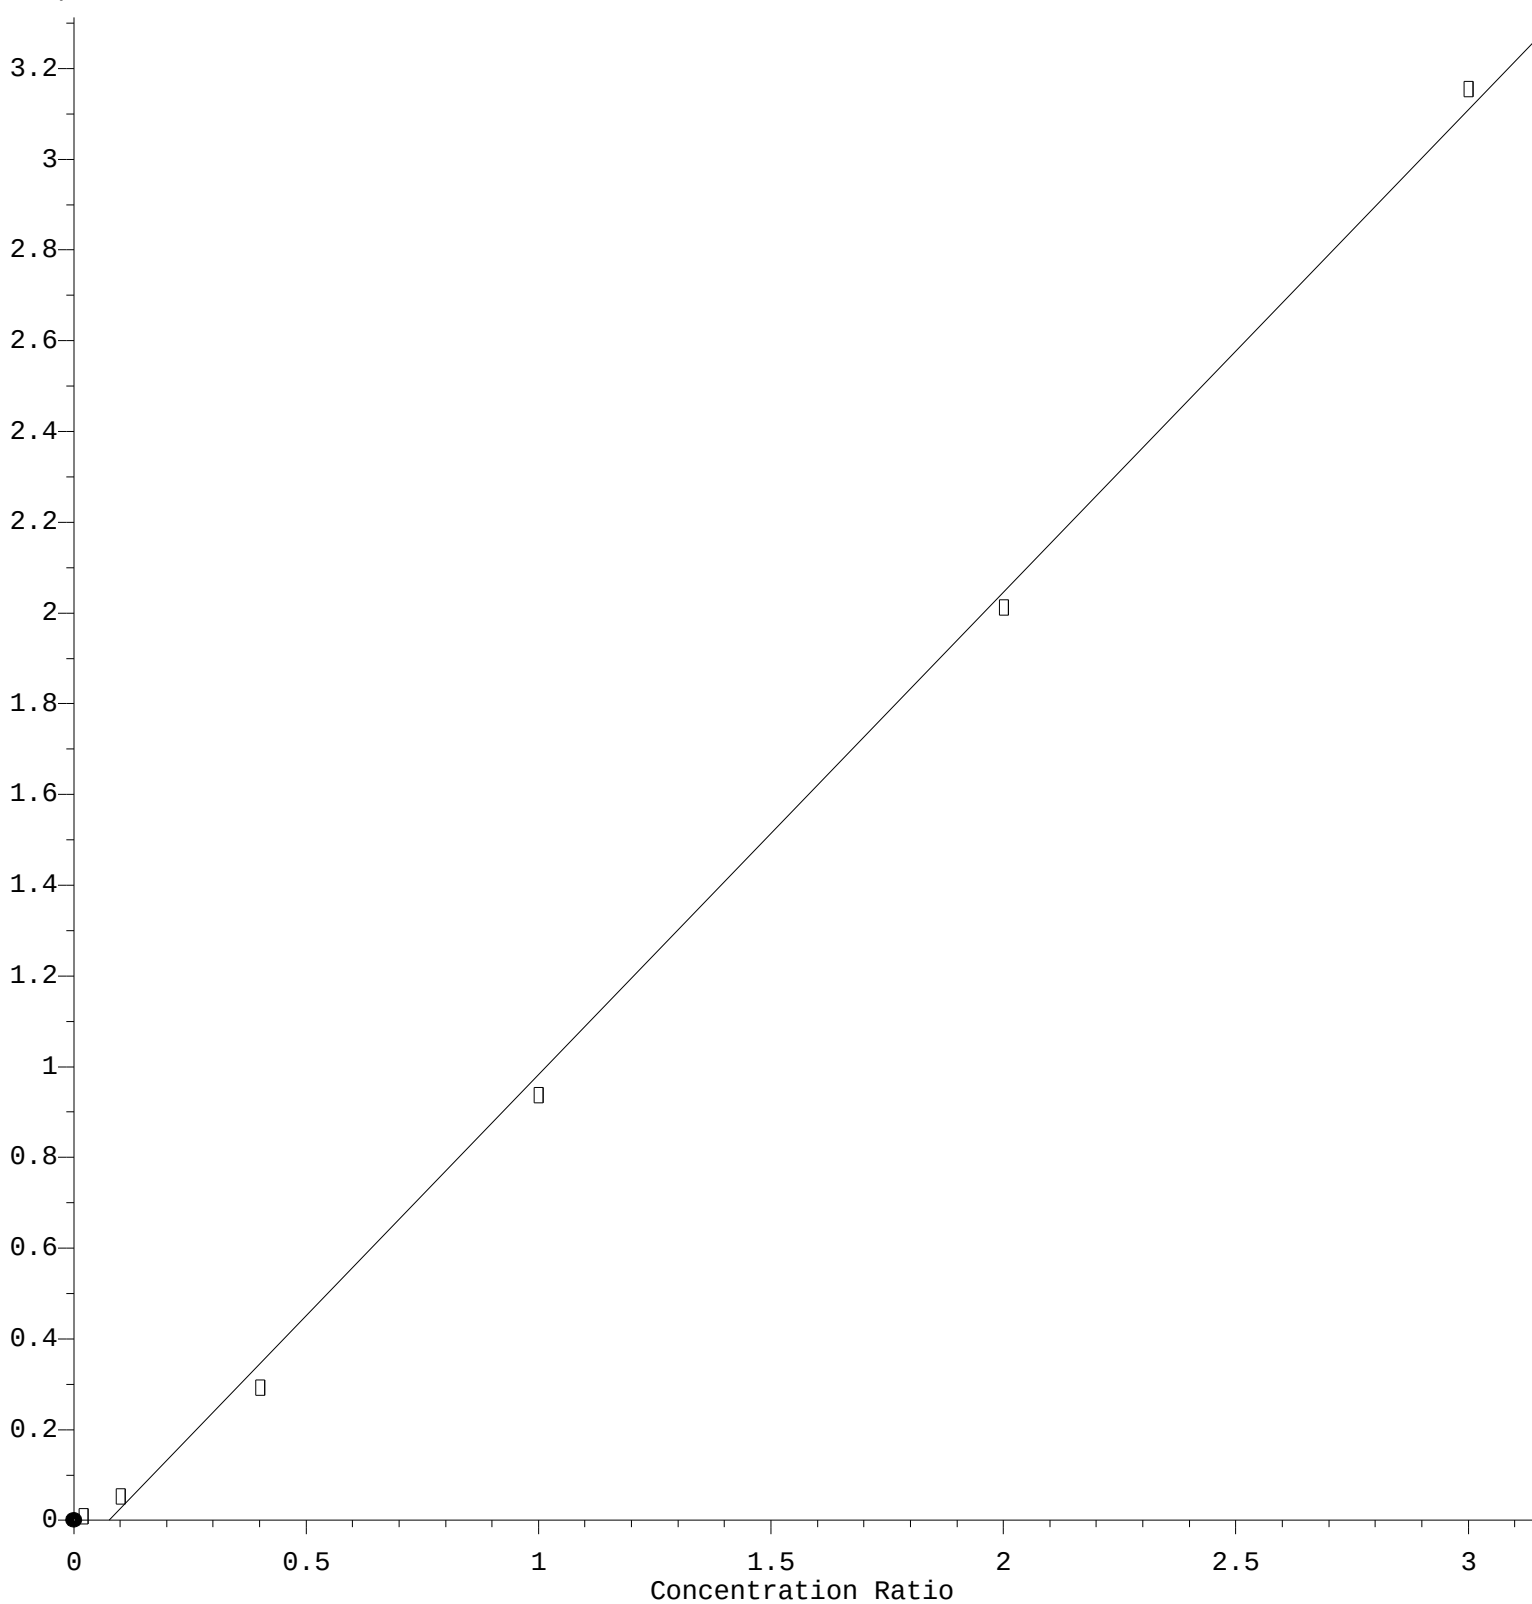

$$\text{Response} = 1.063\text{e}+000 * \text{Amt} - 7.929\text{e}-002$$


Coef of Det (r^2) = 0.998328 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121420W.M

Calibration Table Last Updated: Tue Dec 15 05:41:47 2020

Naphthalene

Response Ratio

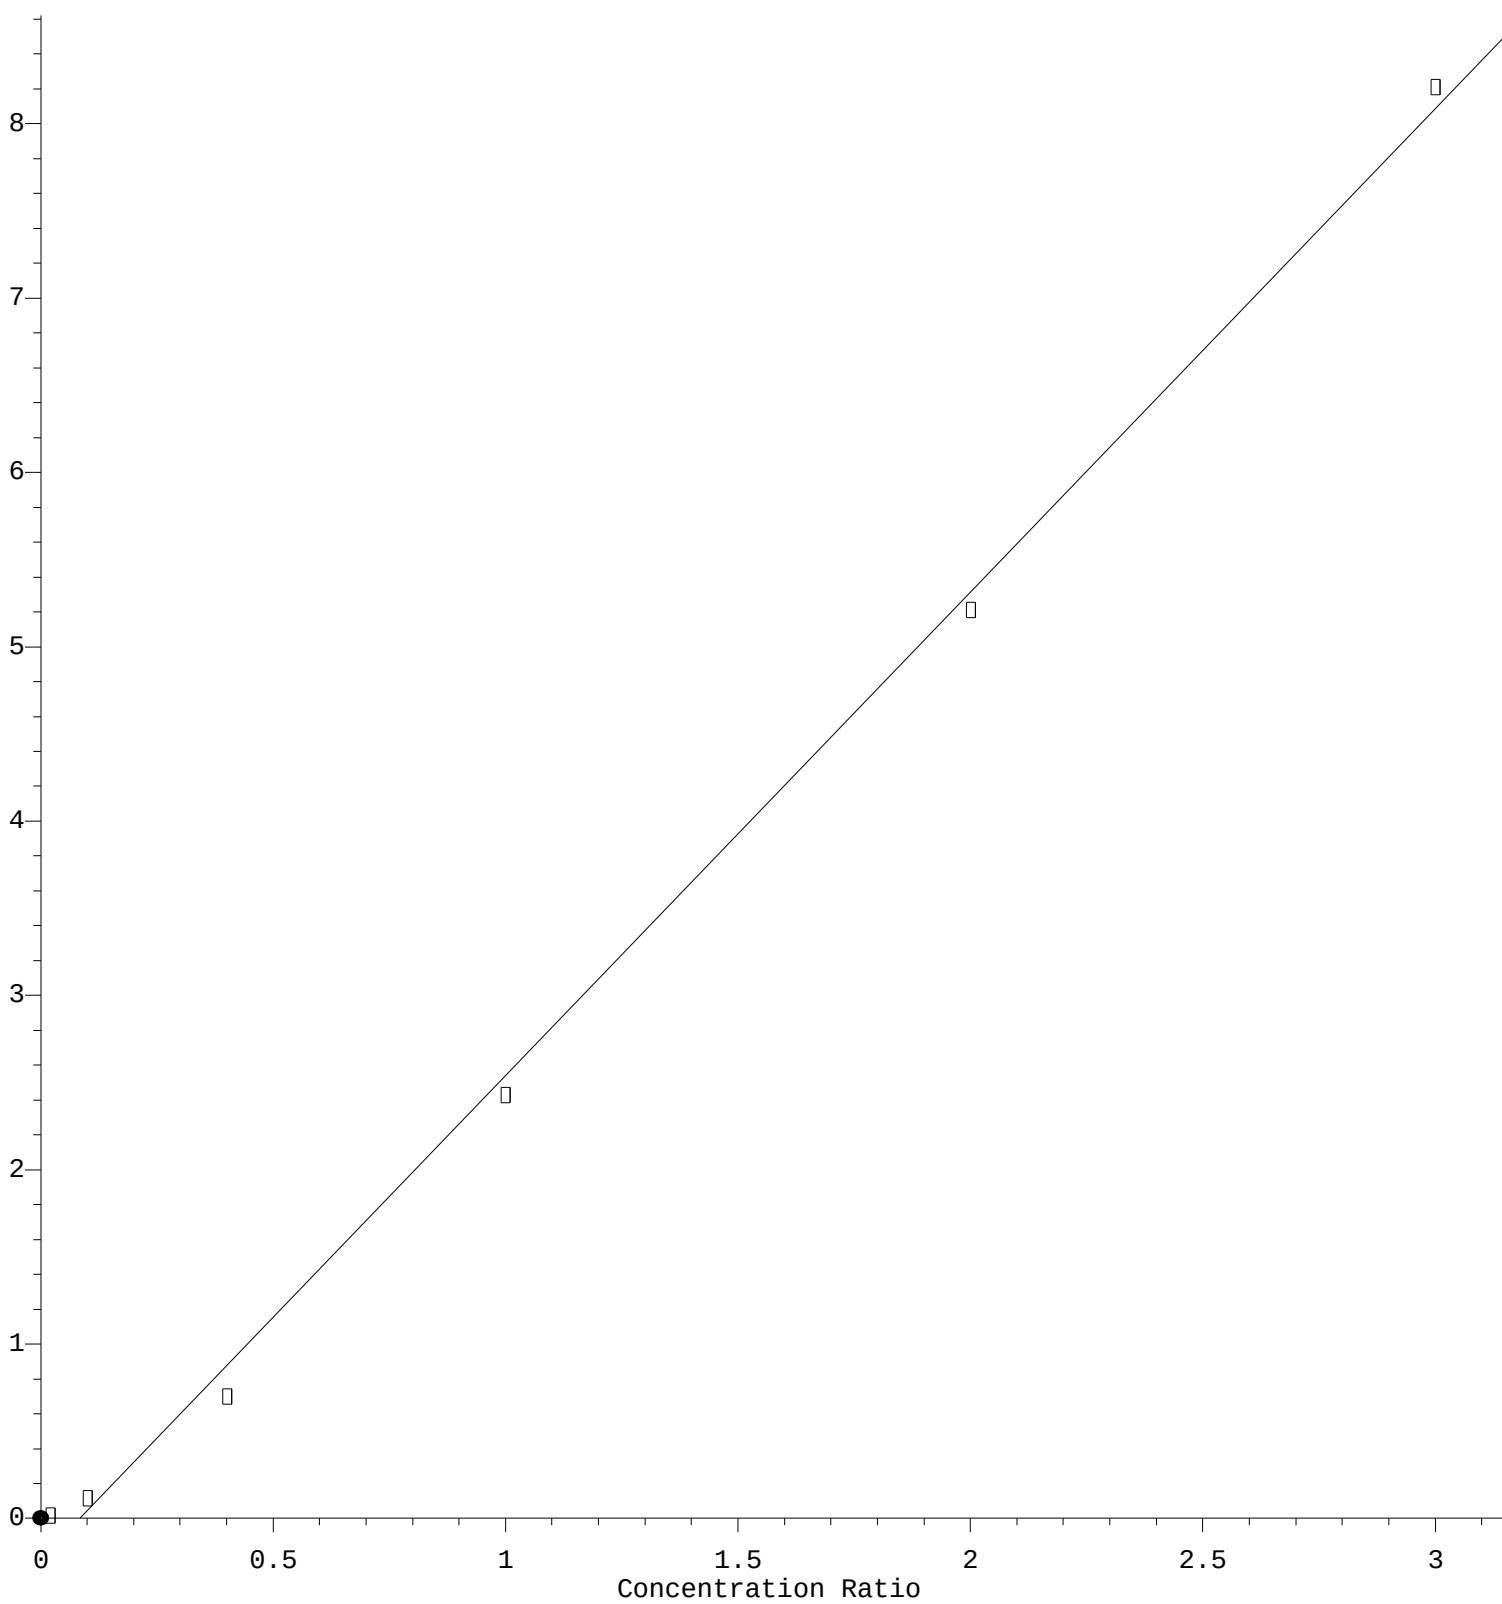

$$\text{Response} = 2.773\text{e}+000 * \text{Amt} - 2.338\text{e}-001$$


Coef of Det (r^2) = 0.997941 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121420W.M

Calibration Table Last Updated: Tue Dec 15 05:41:47 2020

Naphthalene

Response Ratio

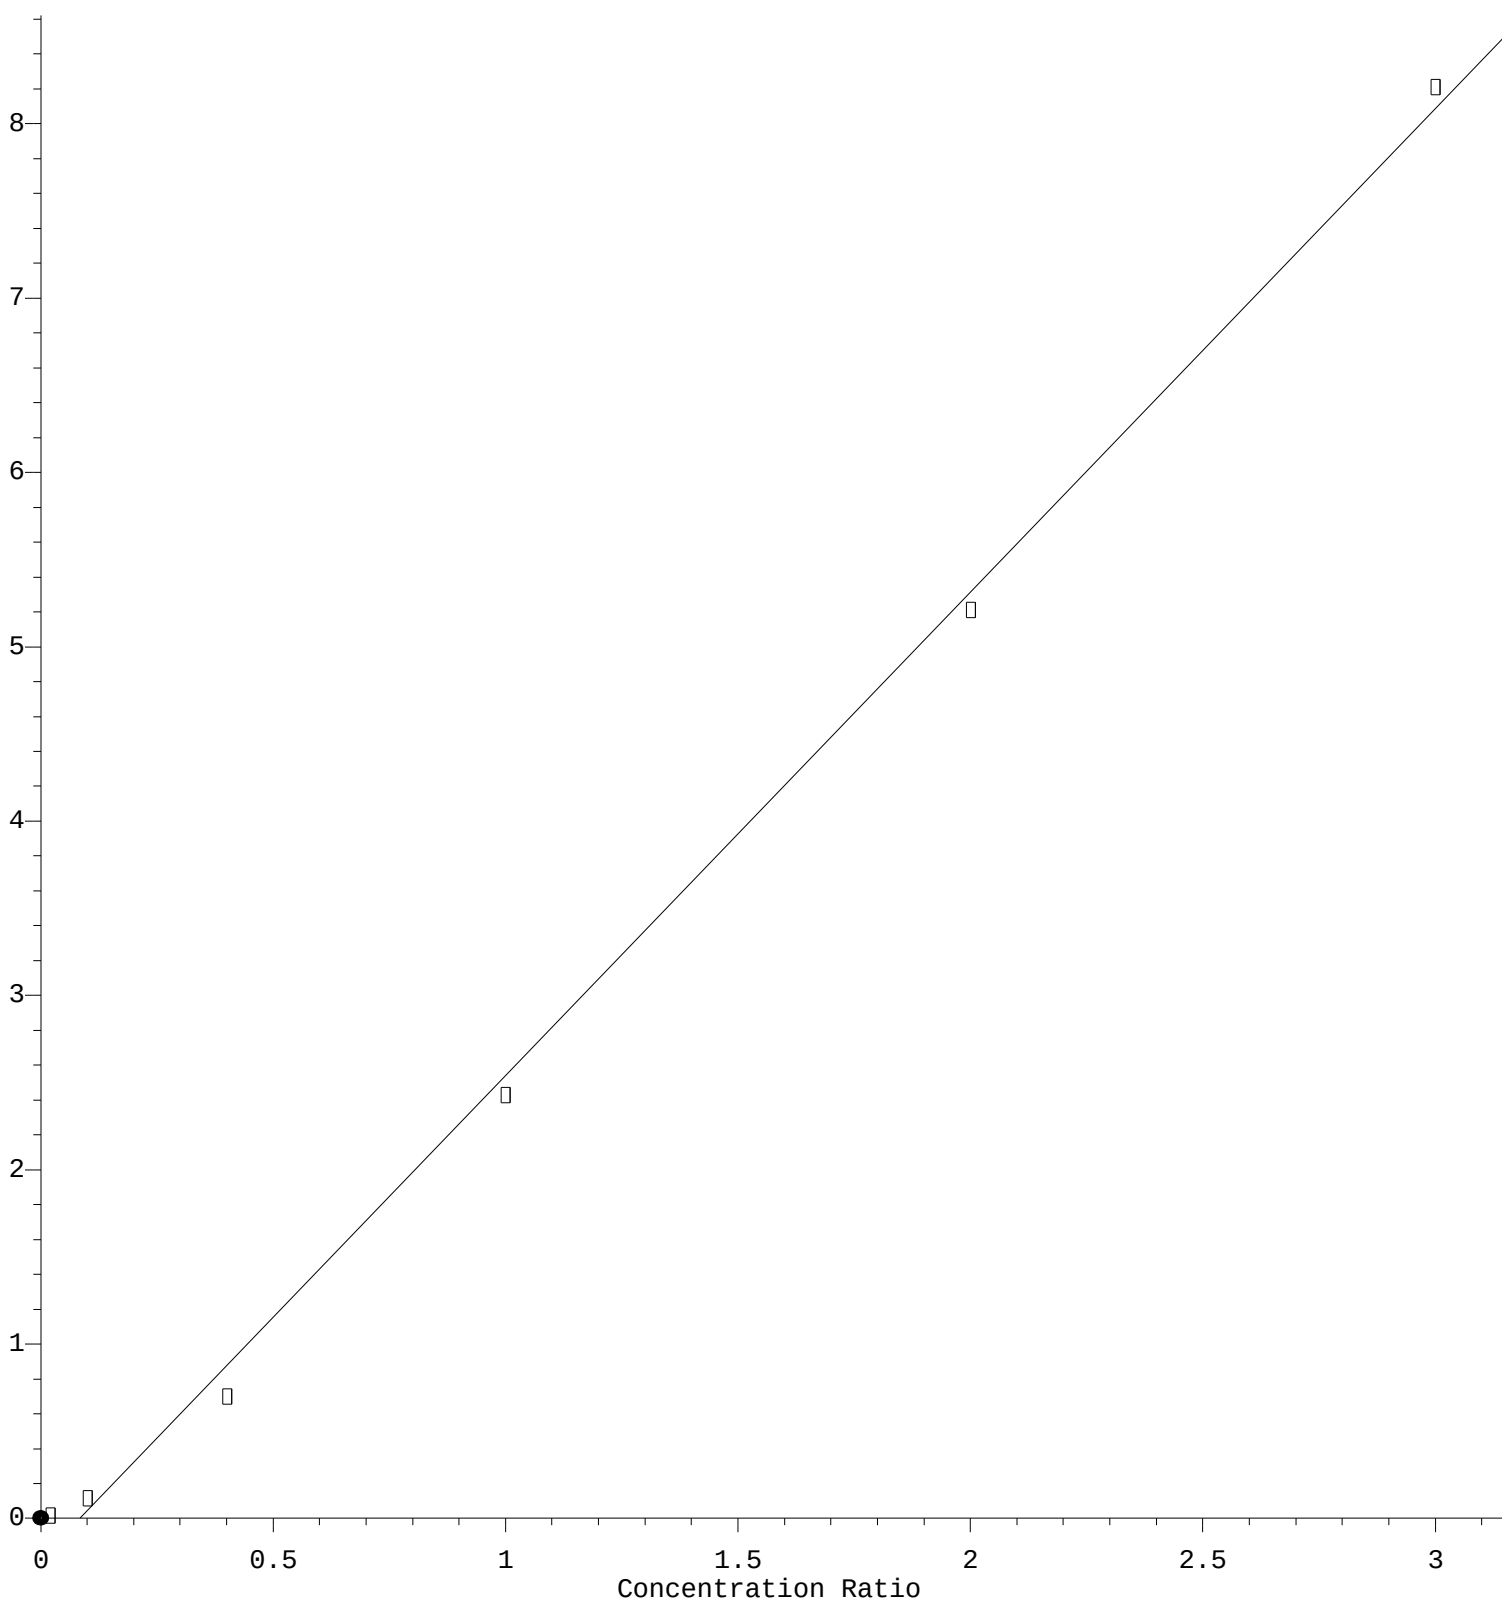

$$\text{Response} = 2.773\text{e}+000 * \text{Amt} - 2.338\text{e}-001$$


Coef of Det (r^2) = 0.997941 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121420W.M

Calibration Table Last Updated: Tue Dec 15 05:41:47 2020

1,2,3-Trichlorobenzene

Response Ratio

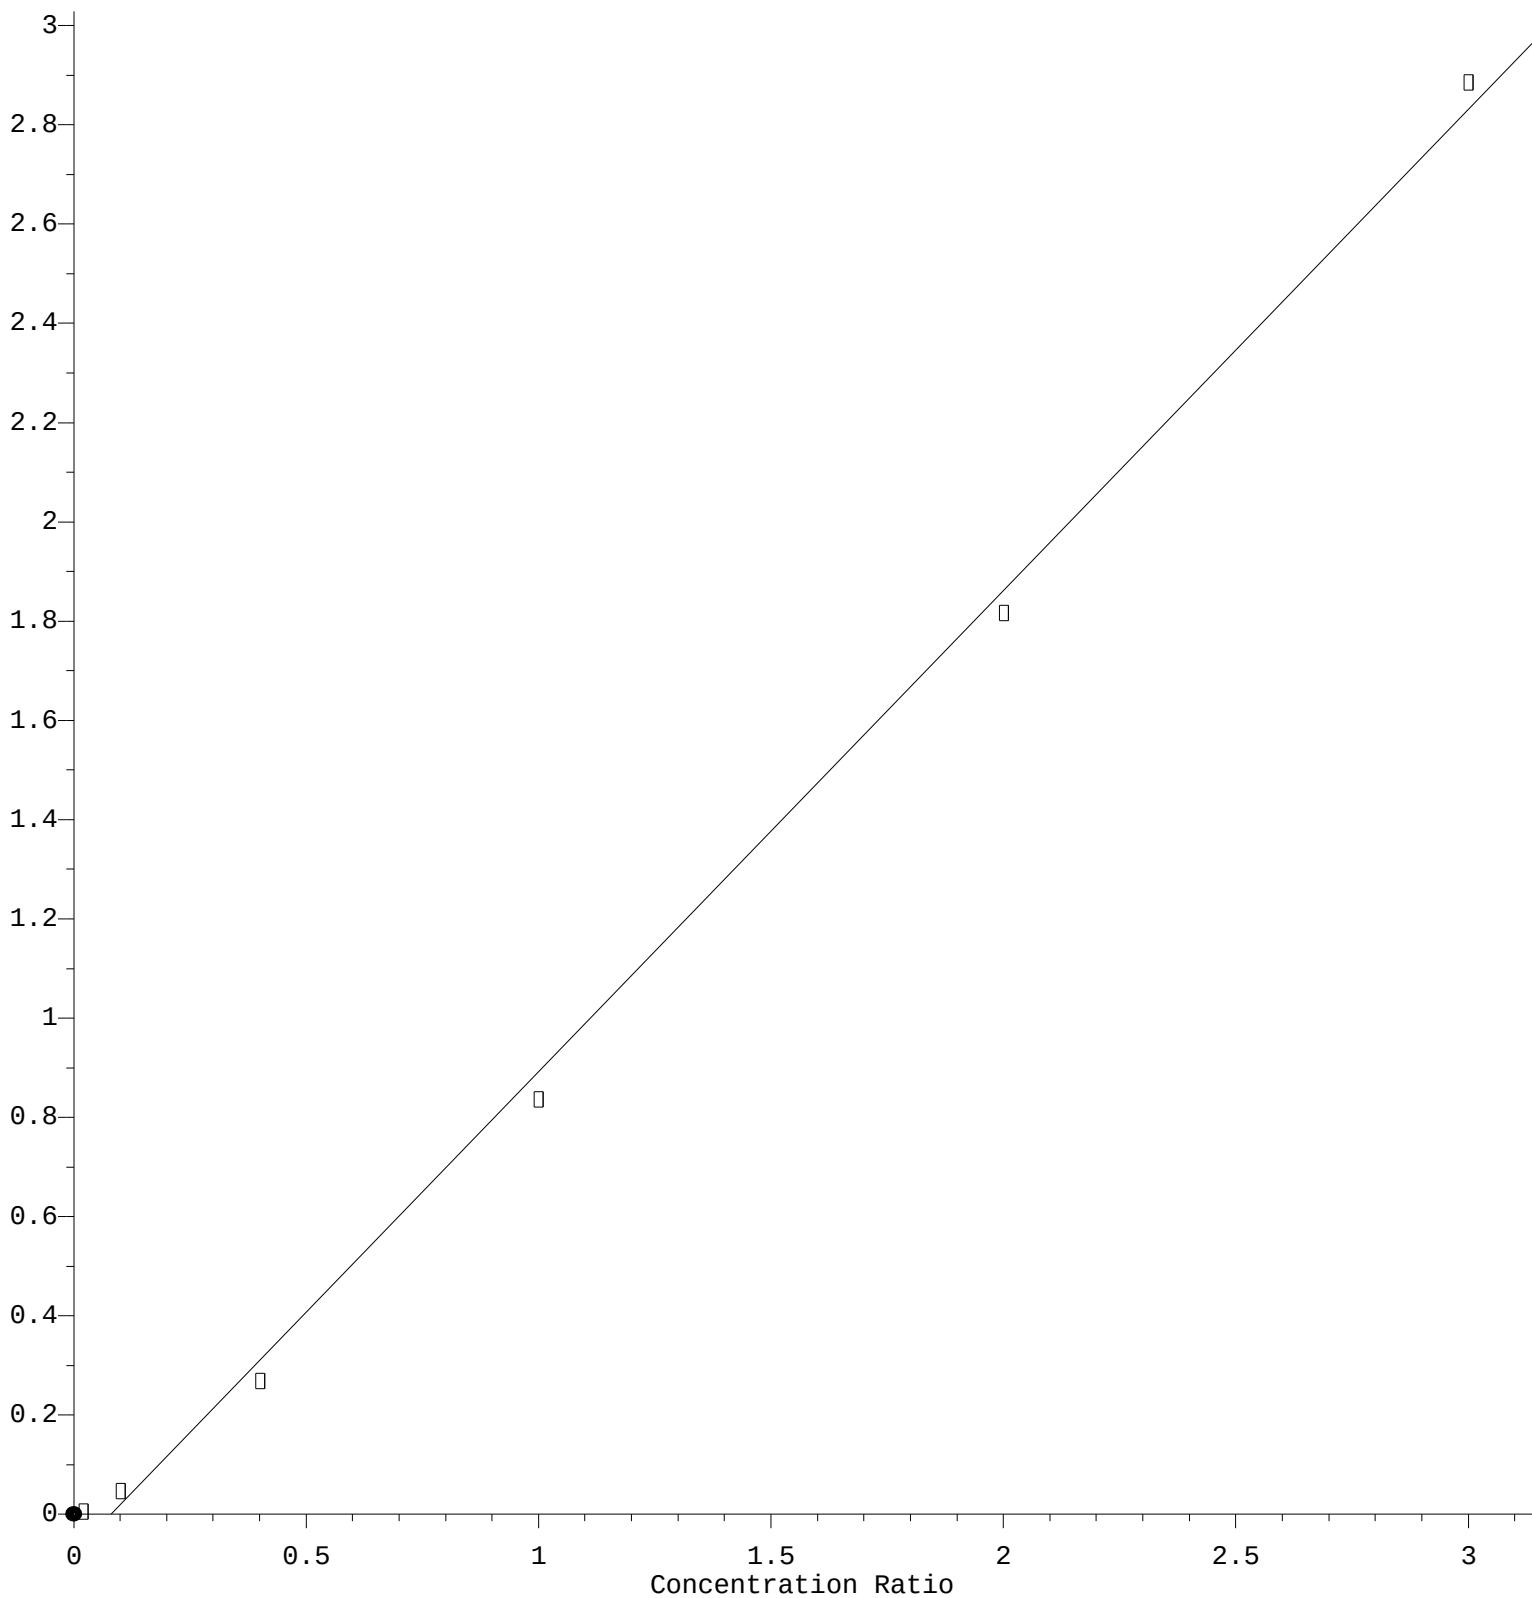

$$\text{Response} = 9.696\text{e-}001 * \text{Amt} - 7.781\text{e-}002$$

Coef of Det (r^2) = 0.997801 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121420W.M

Calibration Table Last Updated: Tue Dec 15 05:41:47 2020