


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121420\
 Data File : VN065114.D
 Acq On : 14 Dec 2020 21:02
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121420W.M
 Title : SW846 8260
 Last Update : Tue Dec 15 05:41:47 2020

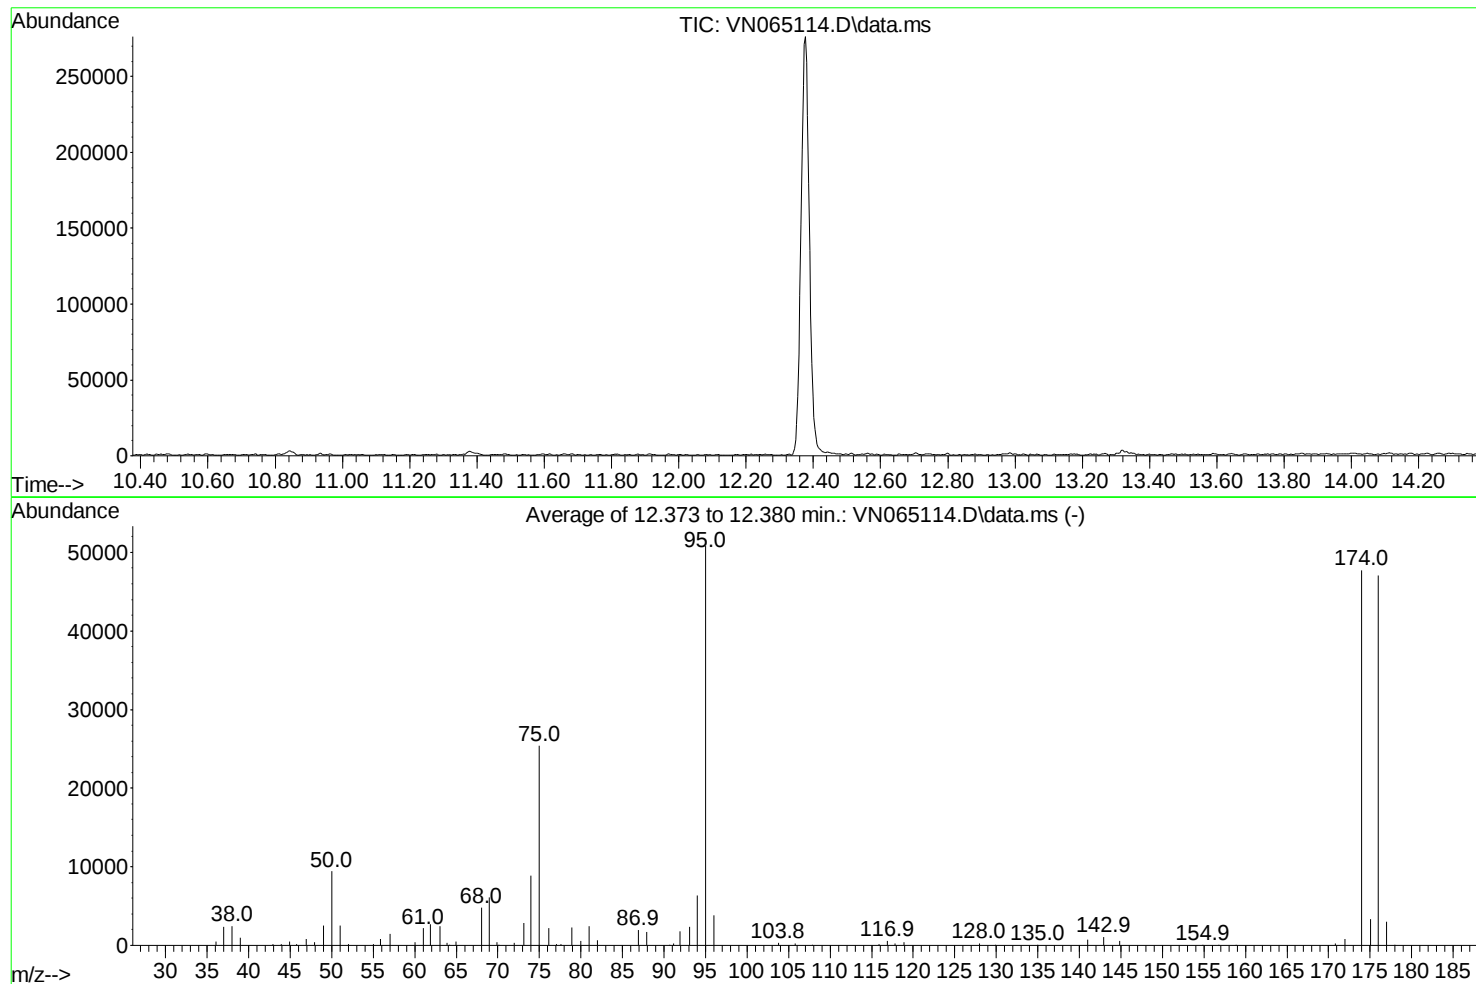

AutoFind: Scans 3307, 3308, 3309; Background Corrected with Scan 3294

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	9426	PASS
75	95	30	60	50.1	25435	PASS
95	95	100	100	100.0	50784	PASS
96	95	5	9	7.6	3839	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	94.0	47728	PASS
175	174	5	9	6.9	3310	PASS
176	174	95	101	98.6	47064	PASS
177	176	5	9	6.4	3029	PASS