

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121421\
 Data File : VN070095.D
 Acq On : 15 Dec 2021 2:03
 Operator : JC/MD
 Sample : M5011-05 10X
 Misc : 2.66g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Dec 15 05:29:06 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
 Quant Title : SW846 8260
 QLast Update : Fri Dec 03 08:46:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.083	168	1193037	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	2282922	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.744	117	2766038	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.675	152	1192264	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.434	65	962108	52.230	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 104.460%	
35) Dibromofluoromethane	8.021	113	659565	46.124	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 92.240%	
50) Toluene-d8	10.440	98	3071822	53.499	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 107.000%	
62) 4-Bromofluorobenzene	12.731	95	1430091	68.750	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 137.500%#	


Target Compounds				Qvalue		
11) Tert butyl alcohol	5.318	59	33933	9.745	ug/l #	72
16) Acetone	4.293	43	12333	1.113	ug/l	90
20) Methylene Chloride	5.095	84	5017	0.341	ug/l	93
25) 2-Butanone	7.340	43	14736	0.979	ug/l	96
31) Cyclohexane	8.080	56	36339	1.418	ug/l #	49
36) 1,1-Dichloropropene	8.083	75	103175	4.747	ug/l #	48
37) Ethyl Acetate	7.340	43	14736	0.456	ug/l #	68
38) Carbon Tetrachloride	8.083	117	123069	5.775	ug/l #	16
39) Methylcyclohexane	9.453	83	11820	0.457	ug/l	89
43) Isopropyl Acetate	8.611	43	21043	0.440	ug/l #	55
53) t-1,3-Dichloropropene	10.722	75	186	2.801	ug/l #	67
54) cis-1,3-Dichloropropene	10.191	75	83	2.002	ug/l #	52
55) 1,1,2-Trichloroethane	10.878	97	5423	0.331	ug/l #	34
56) Ethyl methacrylate	10.754	69	94	2.282	ug/l #	20
58) 2-Chloroethyl Vinyl ether	10.049	63	101	18.400	ug/l #	45
60) Dibromochloromethane	10.985	129	307	2.393	ug/l #	11
67) Ethyl Benzene	11.843	91	53574	0.526	ug/l	95
68) m/p-Xylenes	11.950	106	63725	1.717	ug/l	92
69) o-Xylene	12.280	106	18852	0.504	ug/l	92
71) Bromoform	12.704	173	222	2.743	ug/l #	29
76) 1,2,3-Trichloropropane	12.731	75	789977	23.105	ug/l #	1
78) n-propylbenzene	12.918	91	98876	0.838	ug/l	97
79) 2-Chlorotoluene	12.980	91	23744	0.318	ug/l #	38
80) 1,3,5-Trimethylbenzene	13.058	105	139301	1.632	ug/l	98
81) trans-1,4-Dichloro-2-b...	12.731	75	789977	73.538	ug/l #	5
83) tert-Butylbenzene	13.366	119	51984	0.688	ug/l #	61
84) 1,2,4-Trimethylbenzene	13.366	105	426281	5.242	ug/l	97
89) n-Butylbenzene	13.943	91	34420	0.529	ug/l #	73
90) Hexachloroethane	14.217	117	14322	1.018	ug/l #	6
93) 1,2,4-Trichlorobenzene	15.265	180	3156	3.030	ug/l #	86
95) Naphthalene	15.507	128	48017	4.744	ug/l #	95
96) 1,2,3-Trichlorobenzene	15.705	180	3483	2.609	ug/l #	54


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121421\
Data File : VN070095.D
Acq On : 15 Dec 2021 2:03
Operator : JC/MD
Sample : M5011-05 10X
Misc : 2.66g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :


Quant Time: Dec 15 05:29:06 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
Quant Title : SW846 8260
QLast Update : Fri Dec 03 08:46:47 2021
Response via : Initial Calibration

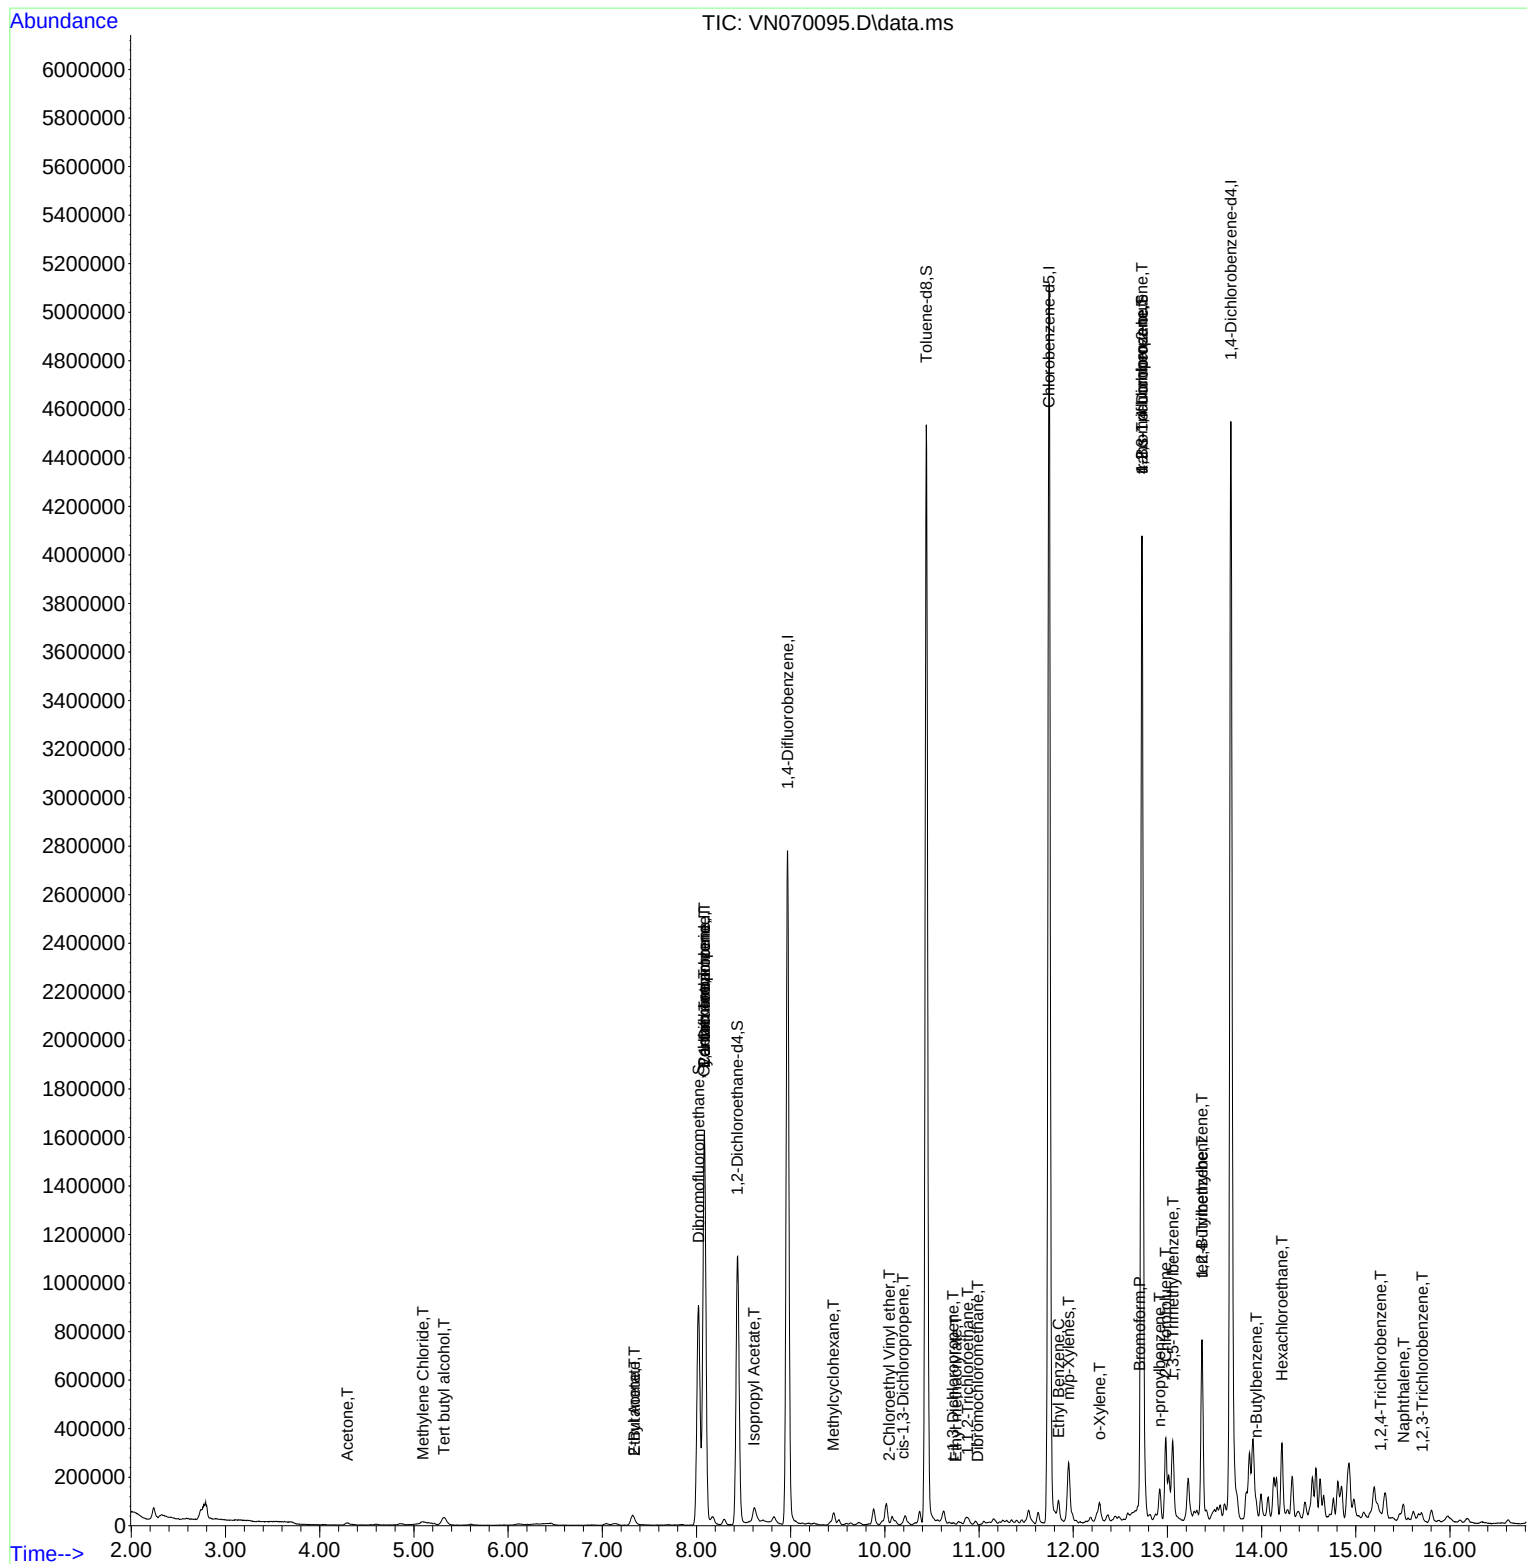



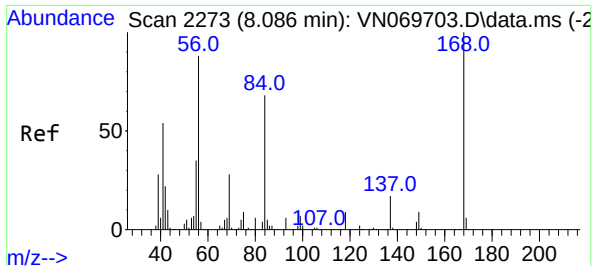


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.083 min Scan# 21
Delta R.T. -0.003 min
Lab File: VN070095.D
Acq: 15 Dec 2021 2:03

Instrument :
MSVOA_N
ClientSampleId :



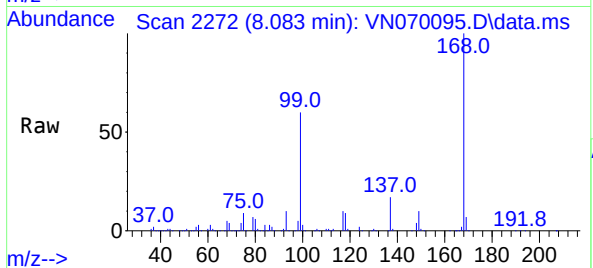



Tgt Ion:168 Resp: 1193037
Ion Ratio Lower Upper
168 100
99 59.8 41.3 61.9

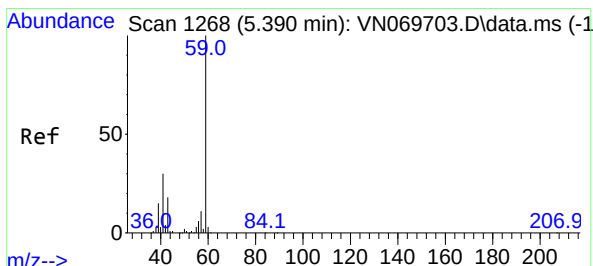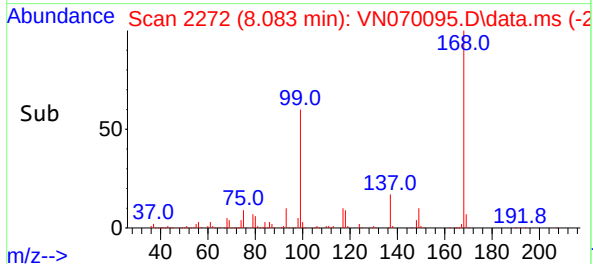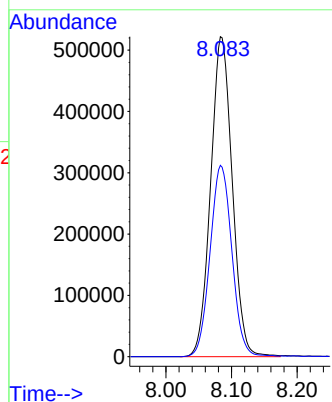

#11
Tert butyl alcohol
Concen: 9.745 ug/l
RT: 5.318 min Scan# 1241
Delta R.T. -0.072 min
Lab File: VN070095.D
Acq: 15 Dec 2021 2:03

Tgt Ion: 59 Resp: 33933
Ion Ratio Lower Upper
59 100
57 0.2 8.7 13.1#


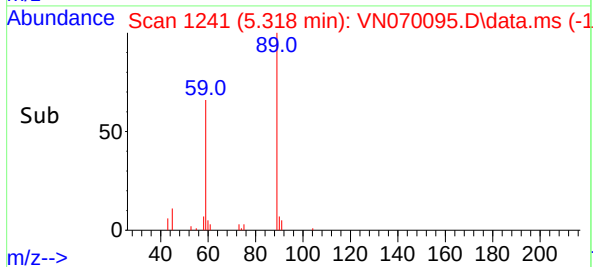
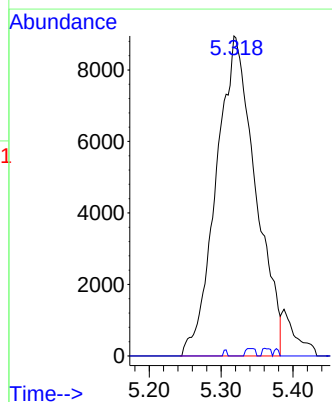
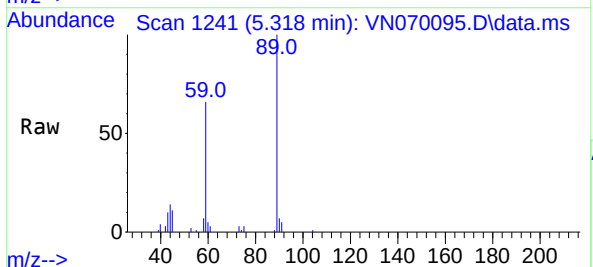




#16
Acetone
Concen: 1.113 ug/l
RT: 4.293 min Scan# 81
Delta R.T. 0.003 min
Lab File: VN070095.D
Acq: 15 Dec 2021 2:03




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 12333
Ion Ratio Lower Upper
43 100
58 23.5 23.1 34.7

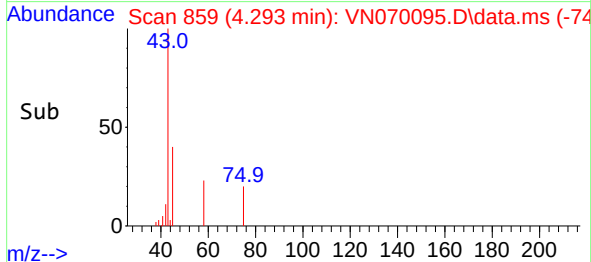

#20
Methylene Chloride
Concen: 0.341 ug/l
RT: 5.095 min Scan# 1158
Delta R.T. 0.003 min
Lab File: VN070095.D
Acq: 15 Dec 2021 2:03

Tgt Ion: 84 Resp: 5017
Ion Ratio Lower Upper
84 100
49 109.6 93.5 140.3
51 34.3 29.4 44.2
86 59.0 53.0 79.4


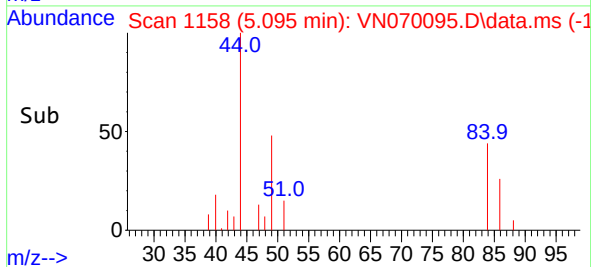

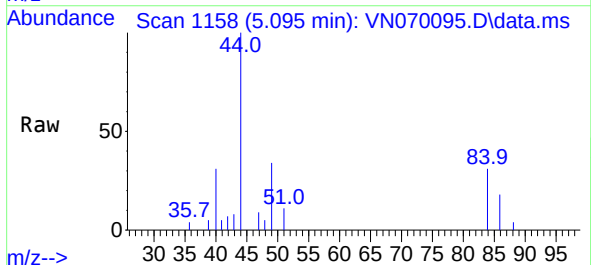


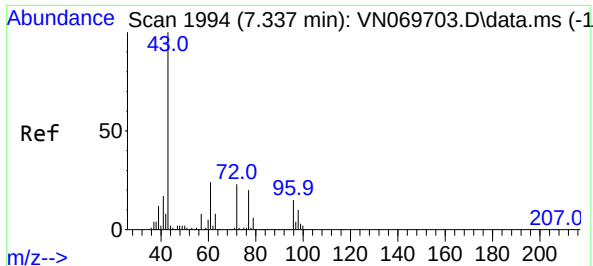

#25
2-Butanone
Concen: 0.979 ug/l
RT: 7.340 min Scan# 1994
Delta R.T. 0.003 min
Lab File: VN070095.D
Acq: 15 Dec 2021 2:03




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 14736
Ion Ratio Lower Upper
43 100
72 25.3 21.7 32.5

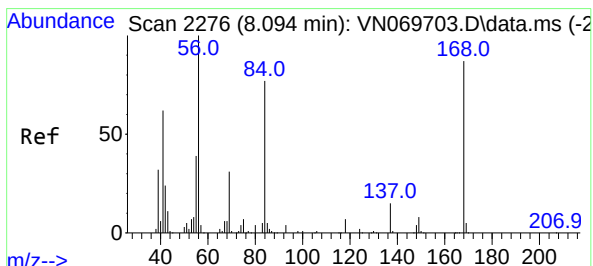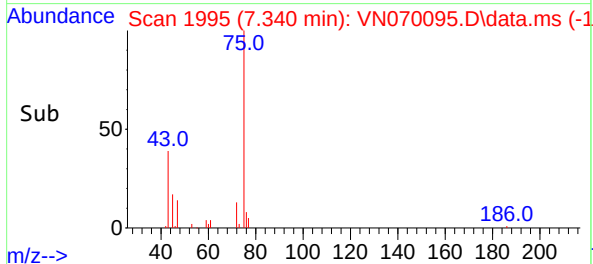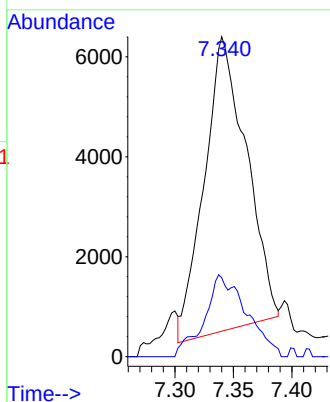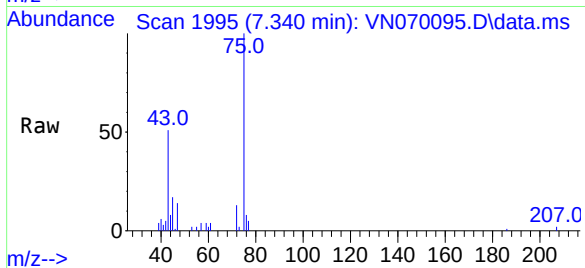

#31
Cyclohexane
Concen: 1.418 ug/l
RT: 8.080 min Scan# 2271
Delta R.T. -0.013 min
Lab File: VN070095.D
Acq: 15 Dec 2021 2:03

Tgt Ion: 56 Resp: 36339
Ion Ratio Lower Upper
56 100
69 131.5 27.1 40.7#
84 97.6 73.4 110.0


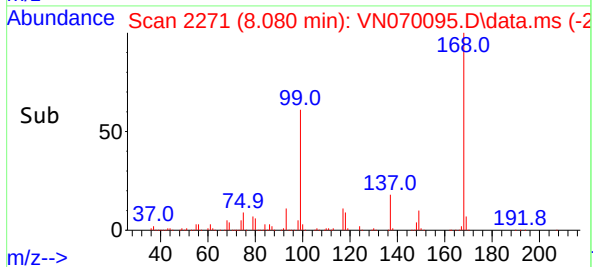

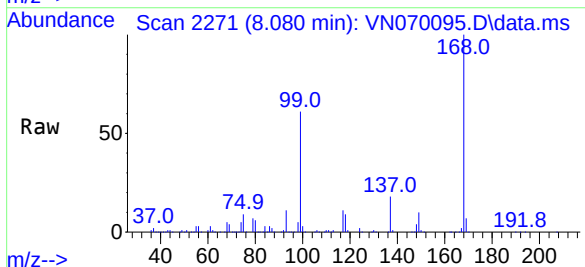




#33
1,2-Dichloroethane-d4
Concen: 52.230 ug/l
RT: 8.434 min Scan# 24
Delta R.T. -0.003 min
Lab File: VN070095.D
Acq: 15 Dec 2021 2:03




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 65 Resp: 962108
Ion Ratio Lower Upper
65 100
67 51.1 0.0 103.0



#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.968 min Scan# 2602
Delta R.T. -0.000 min
Lab File: VN070095.D
Acq: 15 Dec 2021 2:03


Tgt Ion: 114 Resp: 2282922
Ion Ratio Lower Upper
114 100
63 23.8 0.0 37.8
88 16.4 0.0 27.4

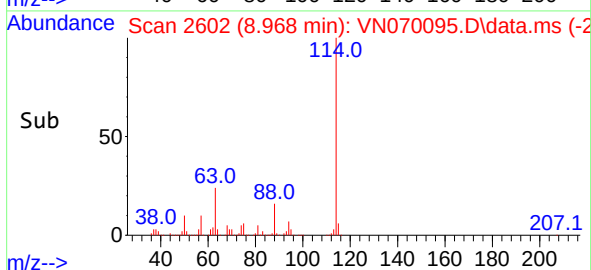



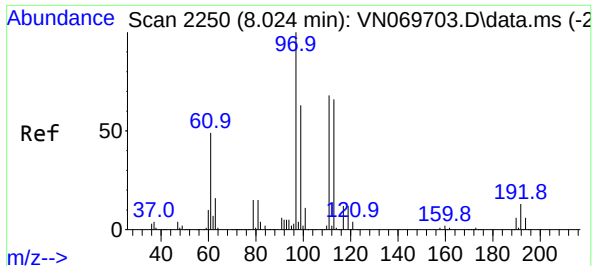


#35
Dibromofluoromethane
Concen: 46.124 ug/l
RT: 8.021 min Scan# 2113
Delta R.T. -0.003 min
Lab File: VN070095.D
Acq: 15 Dec 2021 2:03

Instrument :
MSVOA_N
ClientSampleId :



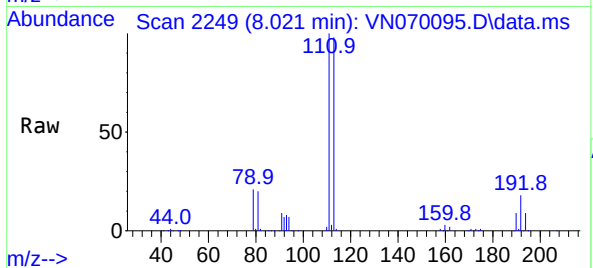



Tgt Ion:113 Resp: 659565
Ion Ratio Lower Upper
113 100
111 103.8 82.2 123.2
192 18.8 16.9 25.3

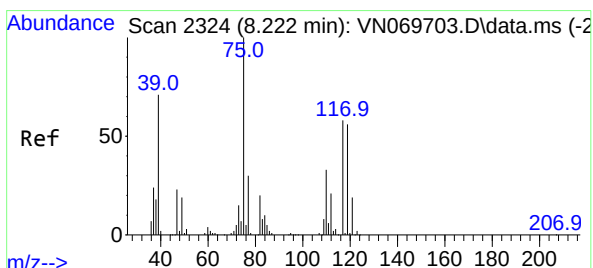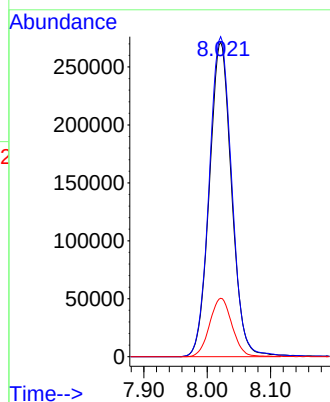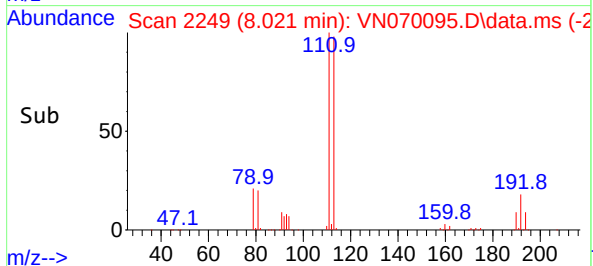

#36
1,1-Dichloropropene
Concen: 4.747 ug/l
RT: 8.083 min Scan# 2272
Delta R.T. -0.139 min
Lab File: VN070095.D
Acq: 15 Dec 2021 2:03

Tgt Ion: 75 Resp: 103175
Ion Ratio Lower Upper
75 100
110 7.9 18.4 55.2#
77 0.0 24.4 36.6#


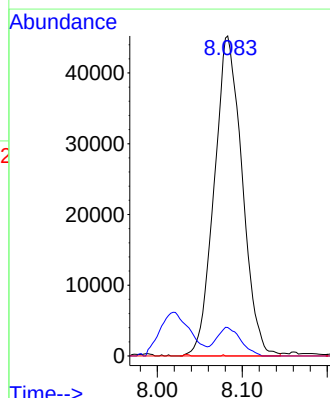
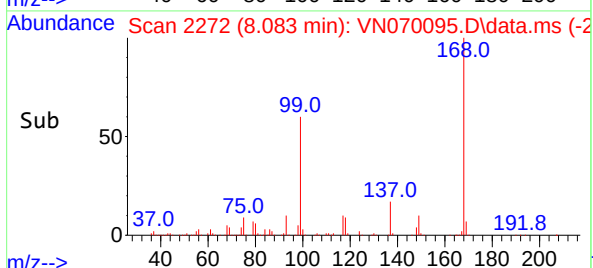
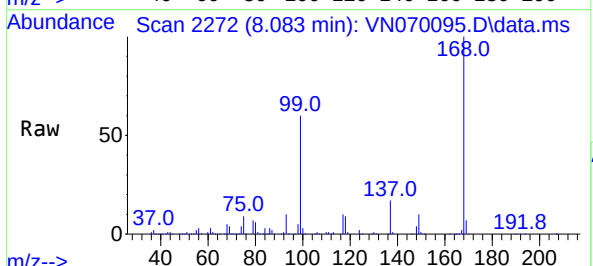


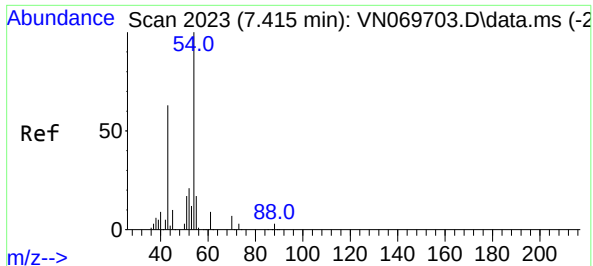

#37
Ethyl Acetate
Concen: 0.456 ug/l
RT: 7.340 min Scan# 19
Delta R.T. -0.075 min
Lab File: VN070095.D
Acq: 15 Dec 2021 2:03




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 14736
Ion Ratio Lower Upper
43 100
61 0.0 11.5 17.3#
70 0.0 7.9 11.9#

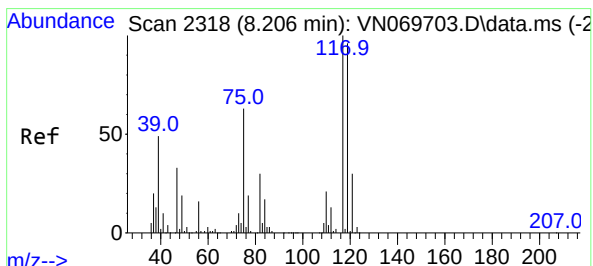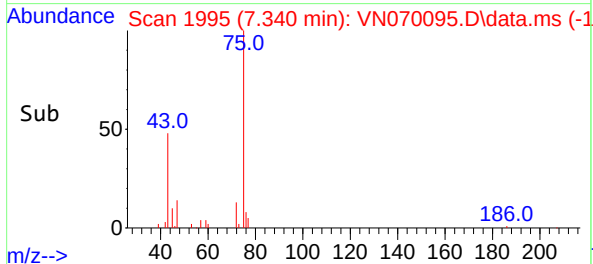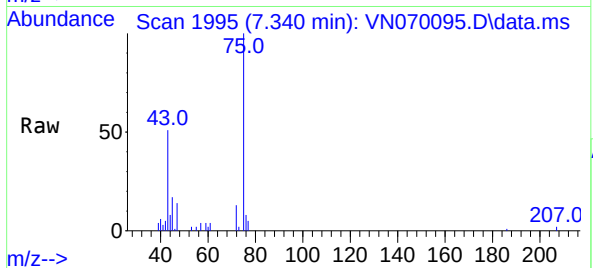

#38
Carbon Tetrachloride
Concen: 5.775 ug/l
RT: 8.083 min Scan# 2272
Delta R.T. -0.123 min
Lab File: VN070095.D
Acq: 15 Dec 2021 2:03


Tgt Ion: 117 Resp: 123069
Ion Ratio Lower Upper
117 100
119 5.0 76.1 114.1#
121 0.0 24.2 36.2#

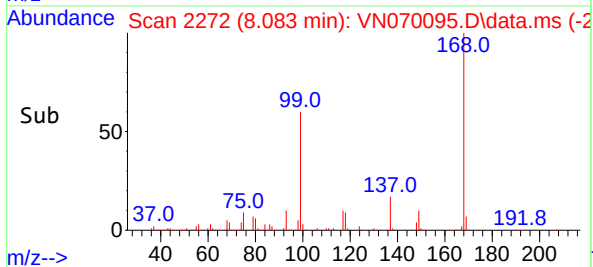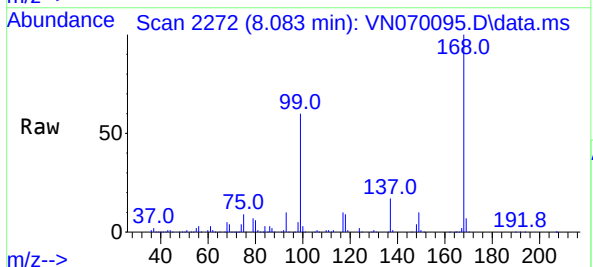






#39
Methylcyclohexane
Concen: 0.457 ug/l
RT: 9.453 min Scan# 21
Delta R.T. -0.008 min
Lab File: VN070095.D
Acq: 15 Dec 2021 2:03

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 83 Resp: 11820
Ion Ratio Lower Upper
83 100
55 83.8 58.1 87.1
98 43.2 38.4 57.6



#43
Isopropyl Acetate
Concen: 0.440 ug/l
RT: 8.611 min Scan# 2469
Delta R.T. 0.048 min
Lab File: VN070095.D
Acq: 15 Dec 2021 2:03

Tgt Ion: 43 Resp: 21043
Ion Ratio Lower Upper
43 100
61 0.0 20.4 30.6#
87 0.0 11.2 16.8#


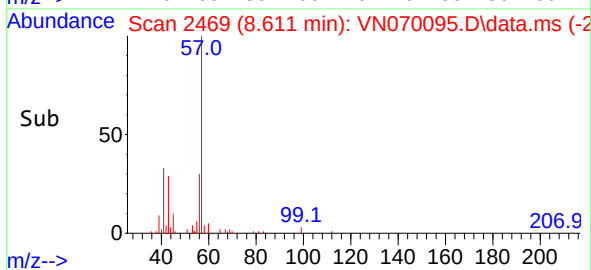




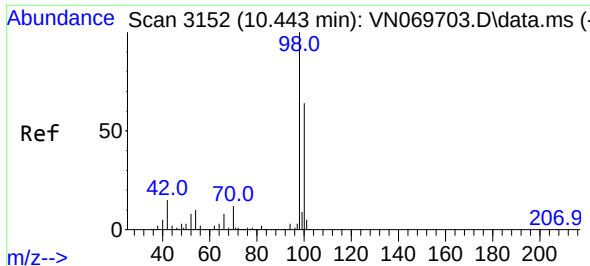

#50
Toluene-d8
Concen: 53.499 ug/l
RT: 10.440 min Scan# 3152
Delta R.T. -0.003 min
Lab File: VN070095.D
Acq: 15 Dec 2021 2:03




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 98 Resp: 3071822
Ion Ratio Lower Upper
98 100
100 64.4 50.4 75.6

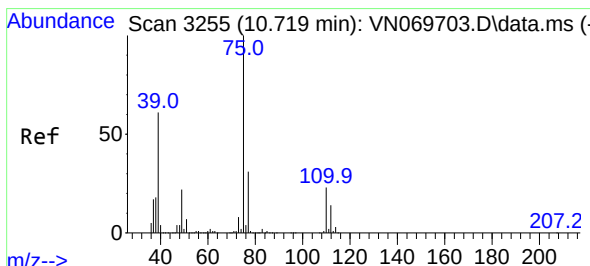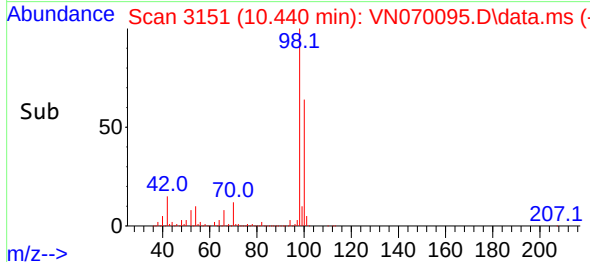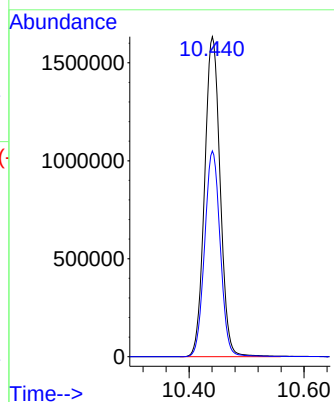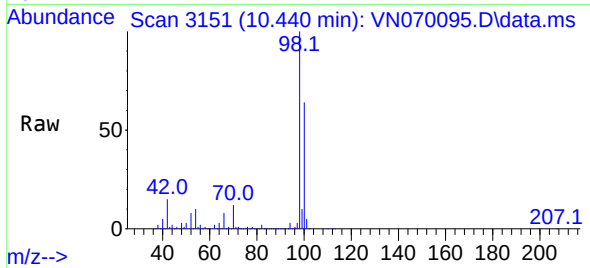

#53
t-1,3-Dichloropropene
Concen: 2.801 ug/l
RT: 10.722 min Scan# 3256
Delta R.T. 0.003 min
Lab File: VN070095.D
Acq: 15 Dec 2021 2:03


Tgt Ion: 75 Resp: 186
Ion Ratio Lower Upper
75 100
77 13.8 25.6 38.4#

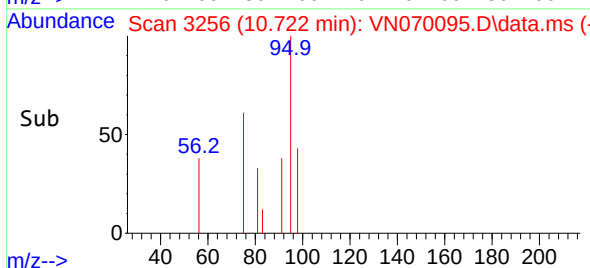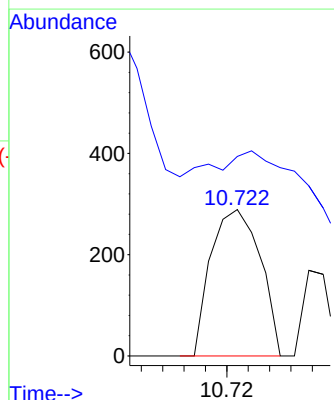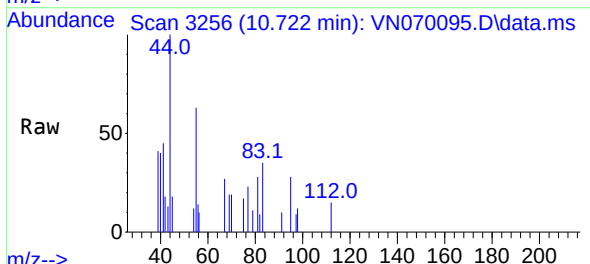



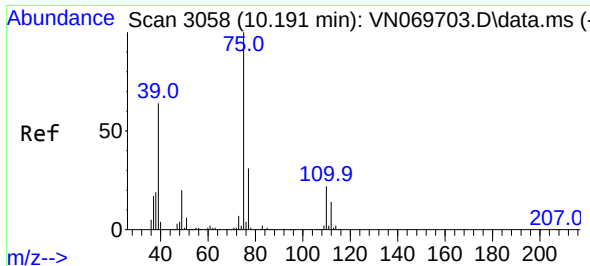


#54
 cis-1,3-Dichloropropene
 Concen: 2.002 ug/l
 RT: 10.191 min Scan# 3058
 Delta R.T. -0.000 min
 Lab File: VN070095.D
 Acq: 15 Dec 2021 2:03

Instrument :
 MSVOA_N
 ClientSampleId :



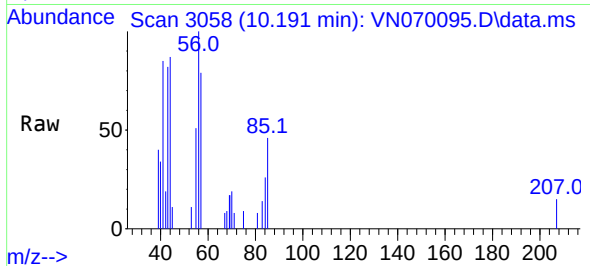



Tgt Ion:	75	Resp:	83
Ion	Ratio	Lower	Upper
75	100		
77	0.0	26.4	39.6#
39	82.7	42.5	63.7#

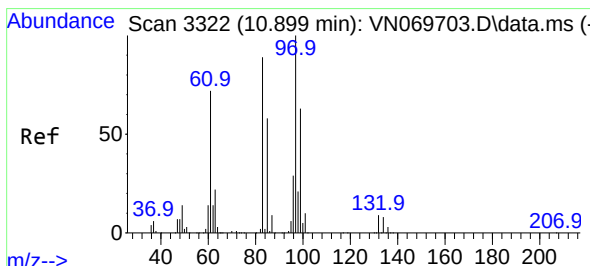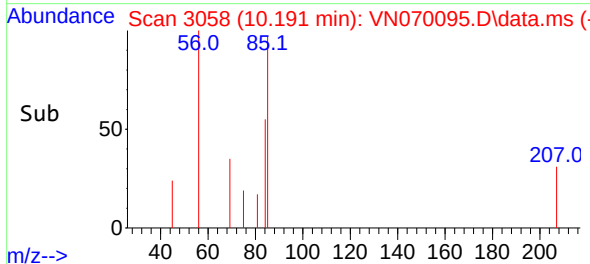

#55
 1,1,2-Trichloroethane
 Concen: 0.331 ug/l
 RT: 10.878 min Scan# 3314
 Delta R.T. -0.021 min
 Lab File: VN070095.D
 Acq: 15 Dec 2021 2:03


Tgt Ion:	97	Resp:	5423
Ion	Ratio	Lower	Upper
97	100		
83	13.7	67.8	101.6#
85	32.6	45.4	68.2#
99	0.0	49.4	74.0#

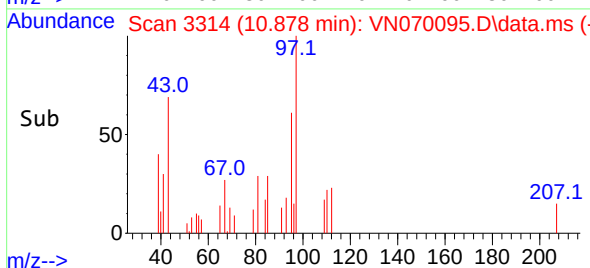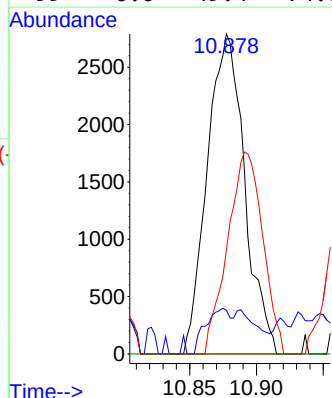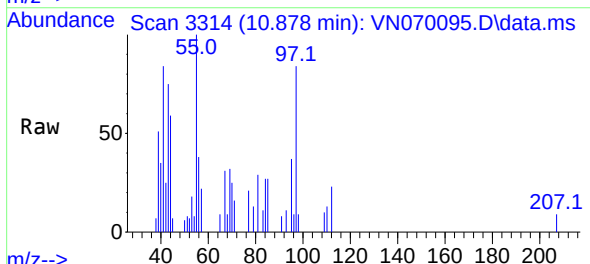






#56
Ethyl methacrylate
Concen: 2.282 ug/l
RT: 10.754 min Scan# 31
Delta R.T. -0.008 min
Lab File: VN070095.D
Acq: 15 Dec 2021 2:03

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 69 Resp: 94
Ion Ratio Lower Upper
69 100
41 0.0 51.4 77.0#
39 92.6 34.6 52.0#

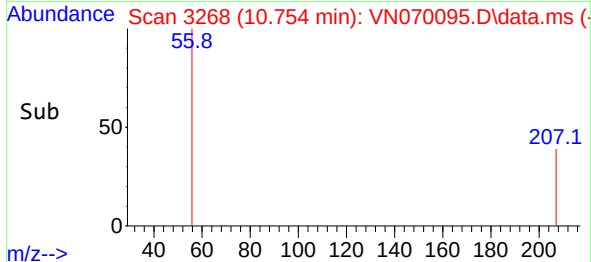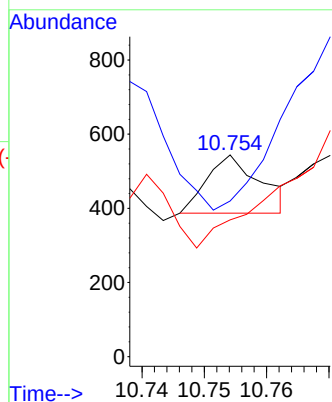

#58
2-Chloroethyl Vinyl ether
Concen: 18.400 ug/l
RT: 10.049 min Scan# 3005
Delta R.T. 0.006 min
Lab File: VN070095.D
Acq: 15 Dec 2021 2:03

Tgt Ion: 63 Resp: 101
Ion Ratio Lower Upper
63 100
106 0.0 23.9 35.9#



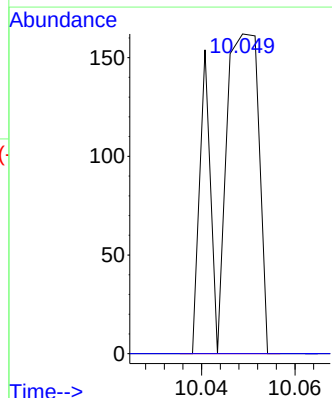





#60
Dibromochloromethane
Concen: 2.393 ug/l
RT: 10.985 min Scan# 31
Delta R.T. -0.255 min
Lab File: VN070095.D
Acq: 15 Dec 2021 2:03




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:129 Resp: 307
Ion Ratio Lower Upper
129 100
127 0.0 38.6 116.0#

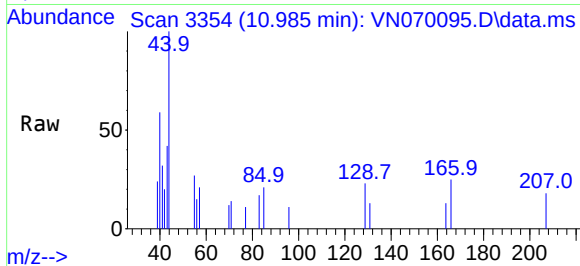

#62
4-Bromofluorobenzene
Concen: 68.750 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. -0.000 min
Lab File: VN070095.D
Acq: 15 Dec 2021 2:03


Tgt Ion: 95 Resp: 1430091
Ion Ratio Lower Upper
95 100
174 74.5 0.0 187.2
176 72.0 0.0 181.4

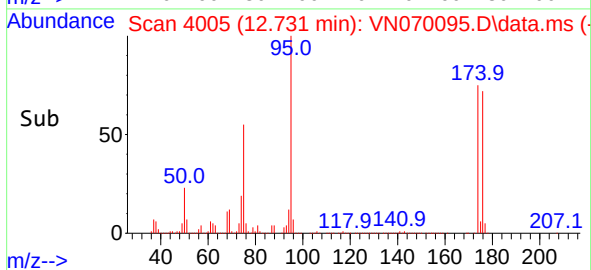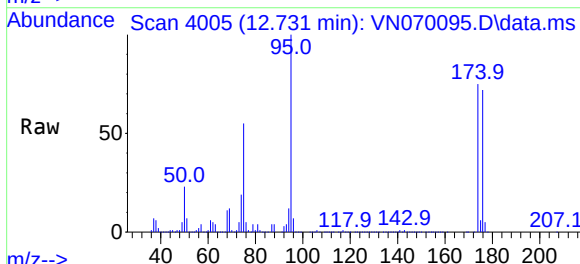

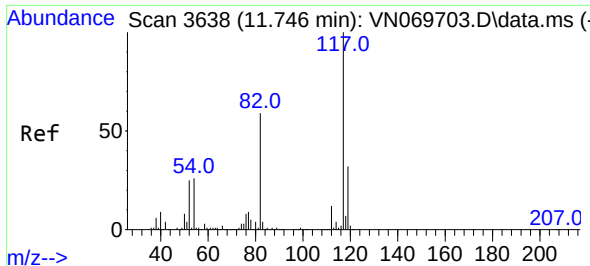




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.744 min Scan# 3638
Delta R.T. -0.002 min
Lab File: VN070095.D
Acq: 15 Dec 2021 2:03

Instrument :
MSVOA_N
ClientSampleId :

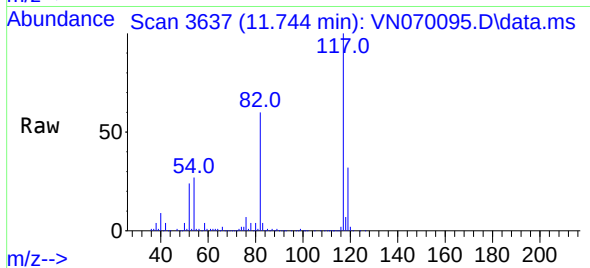

Tgt Ion:117 Resp: 2766038




Ion	Ratio	Lower	Upper
117	100		
82	60.2	42.4	63.6
119	32.3	25.4	38.2

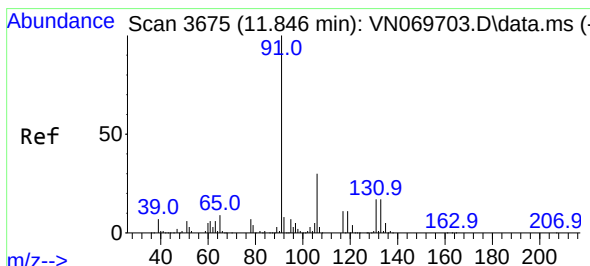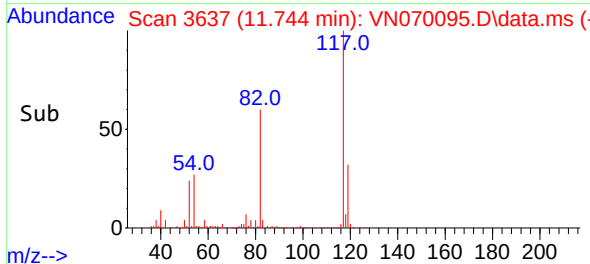


#67
Ethyl Benzene
Concen: 0.526 ug/l
RT: 11.843 min Scan# 3674
Delta R.T. -0.003 min
Lab File: VN070095.D
Acq: 15 Dec 2021 2:03

Tgt Ion: 91 Resp: 53574

Ion	Ratio	Lower	Upper
91	100		
106	29.4	25.7	38.5


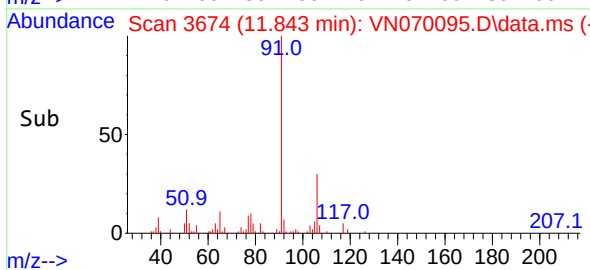

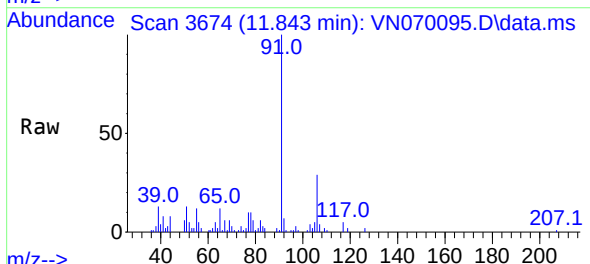




#68
m/p-Xylenes
Concen: 1.717 ug/l
RT: 11.950 min Scan# 31
Delta R.T. -0.003 min
Lab File: VN070095.D
Acq: 15 Dec 2021 2:03




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:106 Resp: 63725
Ion Ratio Lower Upper
106 100
91 213.2 160.6 240.8

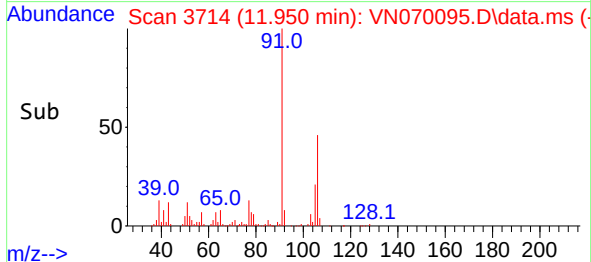

#69
o-Xylene
Concen: 0.504 ug/l
RT: 12.280 min Scan# 3837
Delta R.T. -0.003 min
Lab File: VN070095.D
Acq: 15 Dec 2021 2:03

Tgt Ion:106 Resp: 18852
Ion Ratio Lower Upper
106 100
91 224.4 105.8 317.3


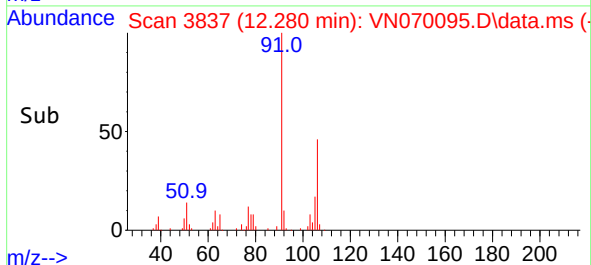
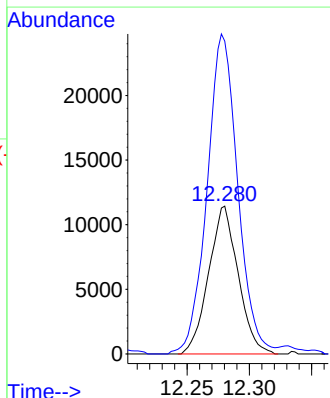
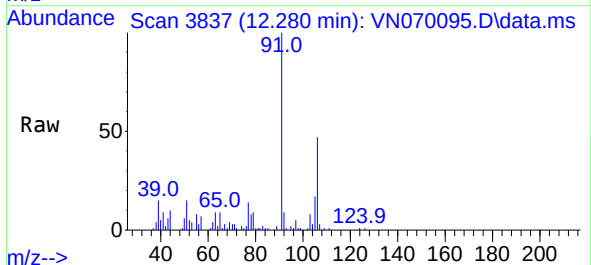




#71
Bromoform
Concen: 2.743 ug/l
RT: 12.704 min Scan# 3904
Delta R.T. 0.244 min
Lab File: VN070095.D
Acq: 15 Dec 2021 2:03




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:173 Resp: 222
Ion Ratio Lower Upper
173 100
175 0.0 24.2 72.6#
254 0.0 0.0 0.0



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.675 min Scan# 4357
Delta R.T. -0.003 min
Lab File: VN070095.D
Acq: 15 Dec 2021 2:03

Tgt Ion:152 Resp: 1192264
Ion Ratio Lower Upper
152 100
115 62.1 27.5 82.5
150 158.1 0.0 344.4


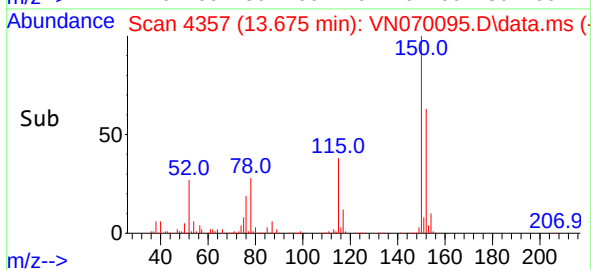






#76
1,2,3-Trichloropropane
Concen: 23.105 ug/l
RT: 12.731 min Scan# 4061
Delta R.T. -0.150 min
Lab File: VN070095.D
Acq: 15 Dec 2021 2:03




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 789977
Ion Ratio Lower Upper
75 100
77 1.1 82.6 247.8#



#78
n-propylbenzene
Concen: 0.838 ug/l
RT: 12.918 min Scan# 4075
Delta R.T. -0.003 min
Lab File: VN070095.D
Acq: 15 Dec 2021 2:03

Tgt Ion: 91 Resp: 98876
Ion Ratio Lower Upper
91 100
120 22.4 11.9 35.9





#79

2-Chlorotoluene

Concen: 0.318 ug/l

RT: 12.980 min Scan# 4098

Delta R.T. -0.029 min

Lab File: VN070095.D

Acq: 15 Dec 2021 2:03

Instrument :

MSVOA_N


ClientSampleId :

Tgt Ion: 91 Resp: 23744




Ion Ratio Lower Upper

91 100

126 0.0 18.3 54.8#

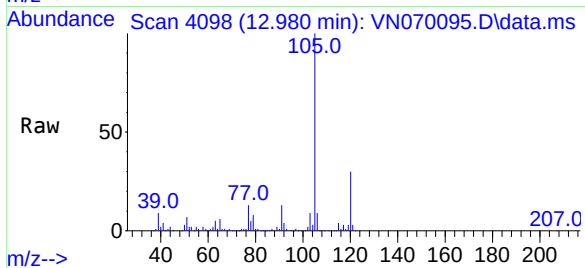

Abundance

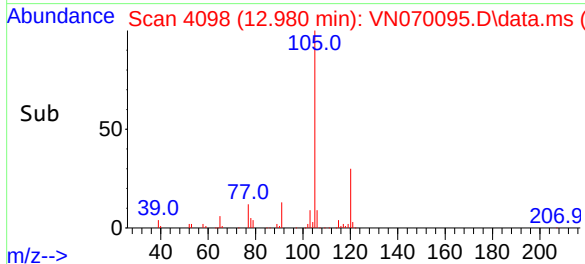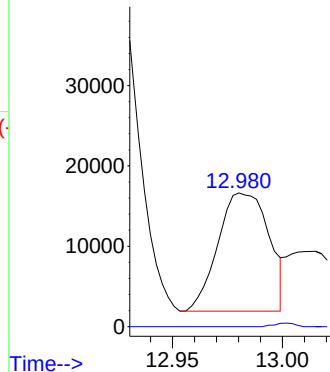

#80

1,3,5-Trimethylbenzene

Concen: 1.632 ug/l

RT: 13.058 min Scan# 4127

Delta R.T. -0.003 min

Lab File: VN070095.D


Acq: 15 Dec 2021 2:03

Tgt Ion: 105 Resp: 139301



Ion Ratio Lower Upper


105 100

120 47.8 24.6 73.6

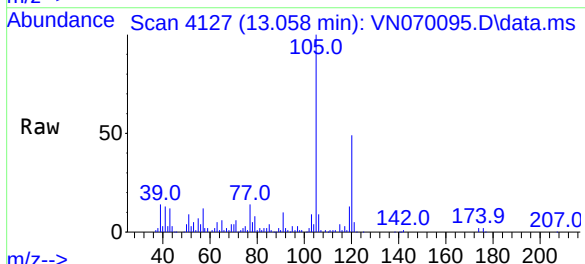


Abundance

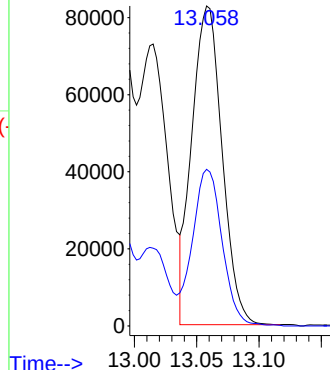



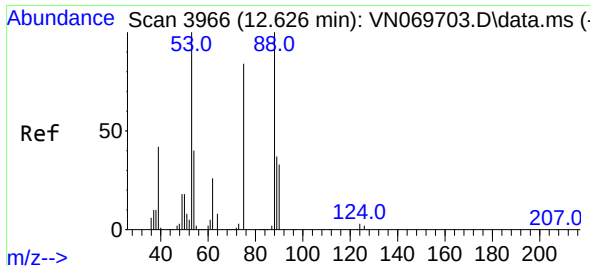


#81
 trans-1,4-Dichloro-2-butene
 Concen: 73.538 ug/l
 RT: 12.731 min Scan# 4005
 Delta R.T. 0.105 min
 Lab File: VN070095.D
 Acq: 15 Dec 2021 2:03


Instrument :
 MSVOA_N
 ClientSampleId :

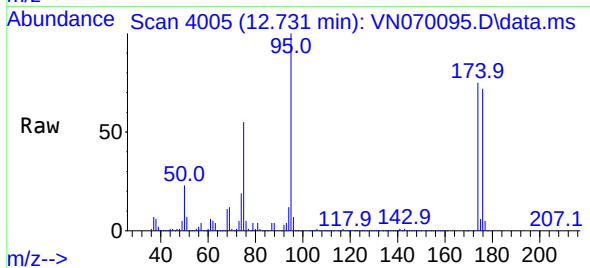



Tgt Ion: 75 Resp: 789977
 Ion Ratio Lower Upper
 75 100
 53 0.1 90.5 135.7#
 89 0.0 38.2 57.4#

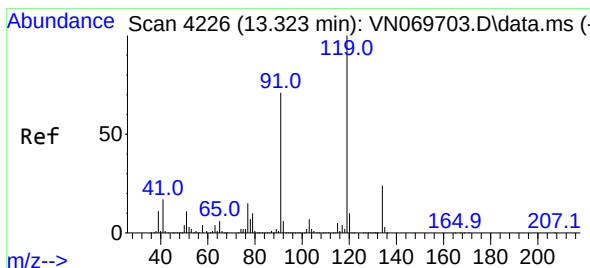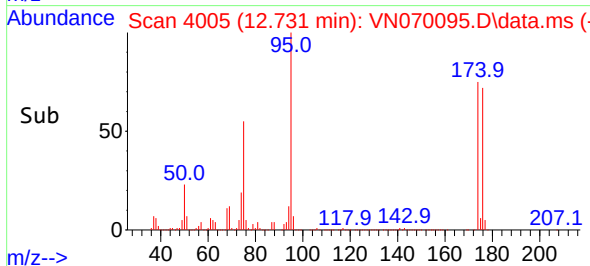


#83
 tert-Butylbenzene
 Concen: 0.688 ug/l
 RT: 13.366 min Scan# 4242
 Delta R.T. 0.043 min
 Lab File: VN070095.D
 Acq: 15 Dec 2021 2:03

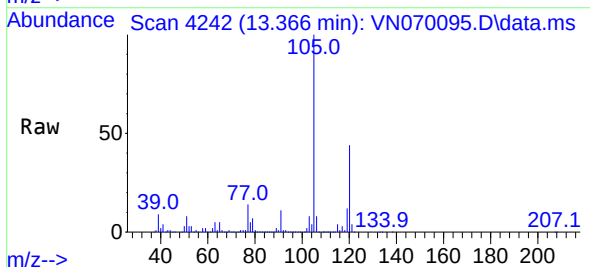


Tgt Ion: 119 Resp: 51984
 Ion Ratio Lower Upper
 119 100
 91 89.8 31.5 94.5
 134 0.0 12.4 37.4#

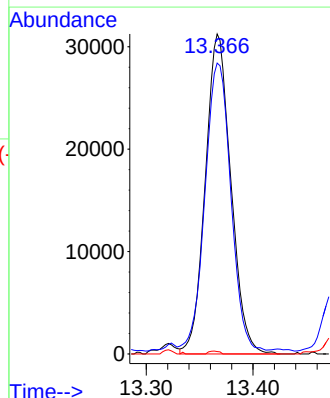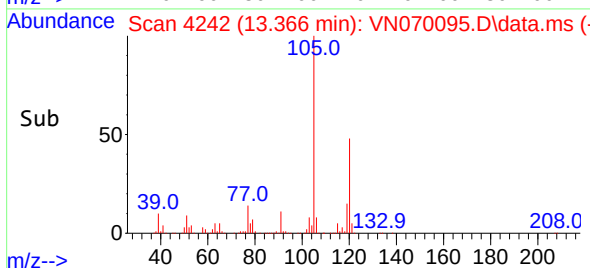






#84
1,2,4-Trimethylbenzene
Concen: 5.242 ug/l
RT: 13.366 min Scan# 41
Delta R.T. -0.003 min
Lab File: VN070095.D
Acq: 15 Dec 2021 2:03

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:105 Resp: 426281
Ion Ratio Lower Upper
105 100
120 43.9 22.8 68.4

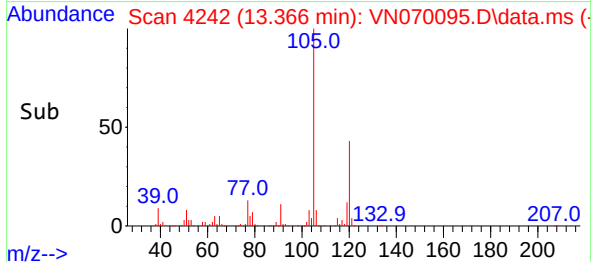

#89
n-Butylbenzene
Concen: 0.529 ug/l
RT: 13.943 min Scan# 4457
Delta R.T. 0.000 min
Lab File: VN070095.D
Acq: 15 Dec 2021 2:03

Tgt Ion: 91 Resp: 34420
Ion Ratio Lower Upper
91 100
92 60.4 25.4 76.0
134 0.0 13.6 40.8#


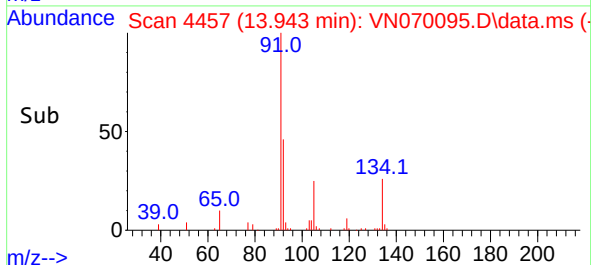
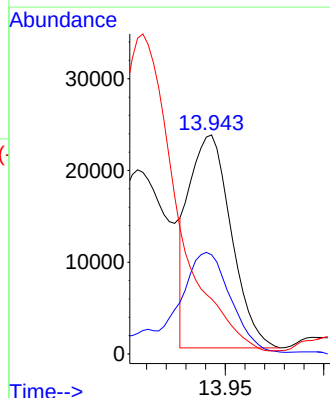
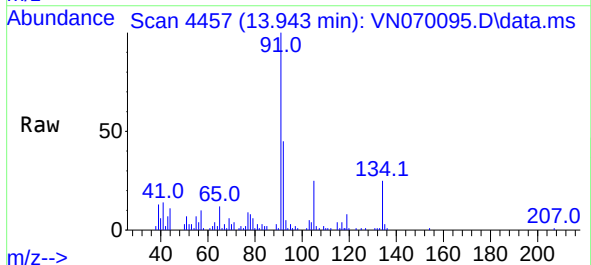




#90
Hexachloroethane
Concen: 1.018 ug/l
RT: 14.217 min Scan# 411
Delta R.T. 0.005 min
Lab File: VN070095.D
Acq: 15 Dec 2021 2:03




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:117 Resp: 14322
Ion Ratio Lower Upper
117 100
201 0.0 43.9 131.6#

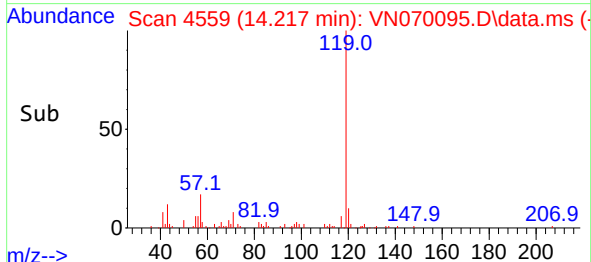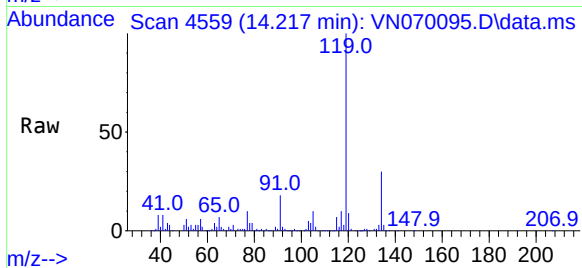

#93
1,2,4-Trichlorobenzene
Concen: 3.030 ug/l
RT: 15.265 min Scan# 4950
Delta R.T. 0.000 min
Lab File: VN070095.D
Acq: 15 Dec 2021 2:03


Tgt Ion:180 Resp: 3156
Ion Ratio Lower Upper
180 100
182 95.0 48.3 144.9
145 0.0 14.5 43.5#

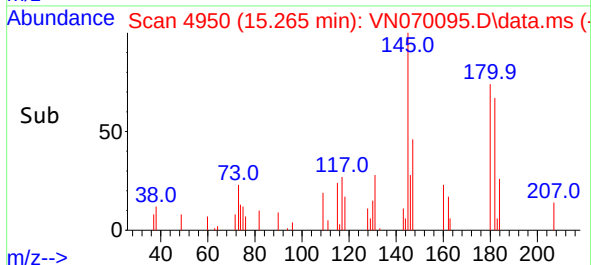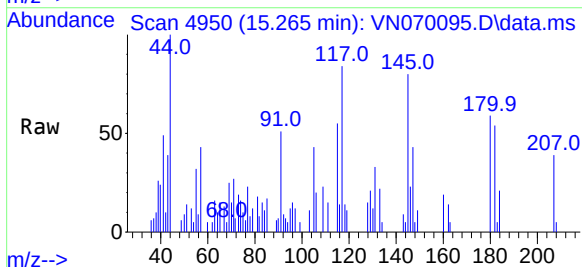






#95
Naphthalene
Concen: 4.744 ug/l
RT: 15.507 min Scan# 5040
Delta R.T. -0.000 min
Lab File: VN070095.D
Acq: 15 Dec 2021 2:03

Instrument :
MSVOA_N
ClientSampleId :



Tgt Ion:128 Resp: 48017
Ion Ratio Lower Upper
128 100
127 14.3 10.5 15.7
129 13.6 8.7 13.1#

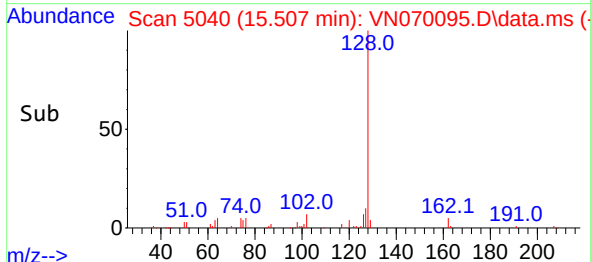

#96
1,2,3-Trichlorobenzene
Concen: 2.609 ug/l
RT: 15.705 min Scan# 5114
Delta R.T. 0.003 min
Lab File: VN070095.D
Acq: 15 Dec 2021 2:03

Tgt Ion:180 Resp: 3483
Ion Ratio Lower Upper
180 100
182 97.5 47.4 142.2
145 128.9 15.0 45.1#

