

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121421\
 Data File : VN070072.D
 Acq On : 14 Dec 2021 15:35
 Operator : JC/MD
 Sample : M5029-03
 Misc : 4.05g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PSC-124019

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M

Title : SW846 8260

Signal : TIC: VN070072.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.228	75	89	132	rBV2	153803	574170	7.26%	1.336%
2	7.351	1975	1999	2025	rBV	76407	236451	2.99%	0.550%
3	8.016	2224	2247	2258	rBV	767713	1872657	23.68%	4.357%
4	8.078	2259	2270	2307	rVB	1412796	3250683	41.11%	7.563%
5	8.432	2379	2402	2432	rBV	1005251	2317471	29.31%	5.392%
6	8.649	2468	2483	2507	rBV2	54142	131022	1.66%	0.305%
7	8.963	2580	2600	2630	rBV	2453078	5159651	65.25%	12.005%
8	10.440	3128	3151	3170	rBV	4183408	7818635	98.88%	18.191%
9	11.744	3618	3637	3671	rBV	4421078	7907366	100.00%	18.397%
10	12.733	3987	4006	4028	rBV	3546722	6074861	76.83%	14.134%
11	13.675	4340	4357	4385	rBV	4384913	7409982	93.71%	17.240%
12	15.504	5017	5039	5057	rBV	109656	227890	2.88%	0.530%




Sum of corrected areas: 42980839

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121421\
Data File : VN070072.D
Acq On : 14 Dec 2021 15:35
Operator : JC/MD
Sample : M5029-03
Misc : 4.05g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PSC-124019

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

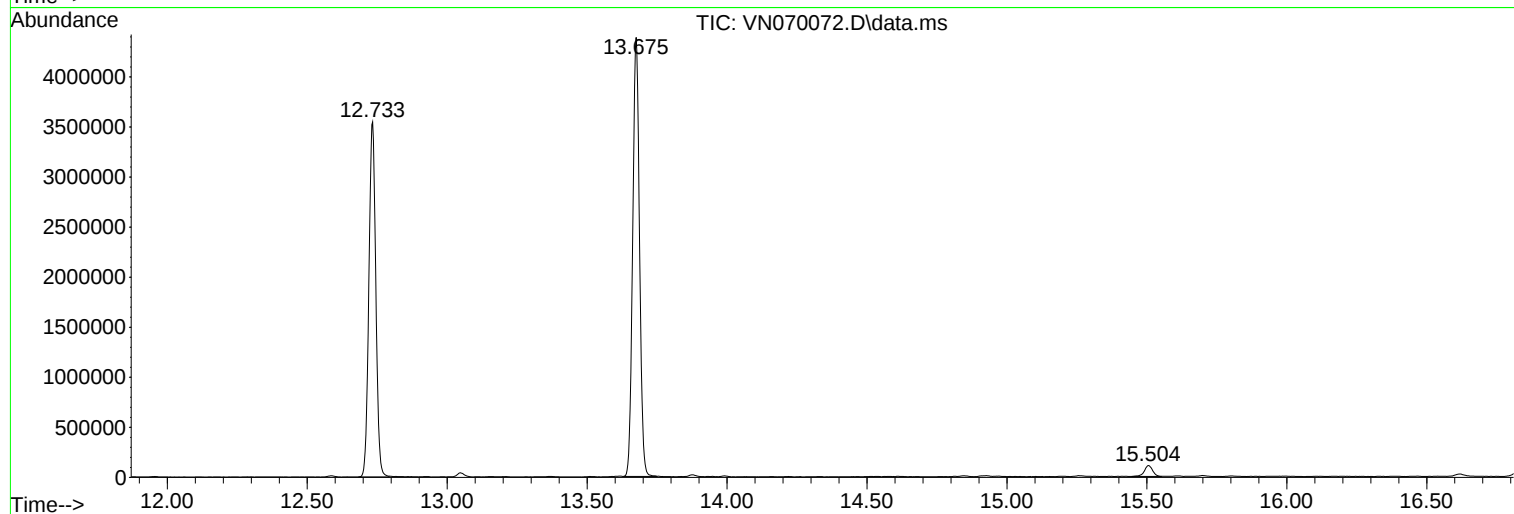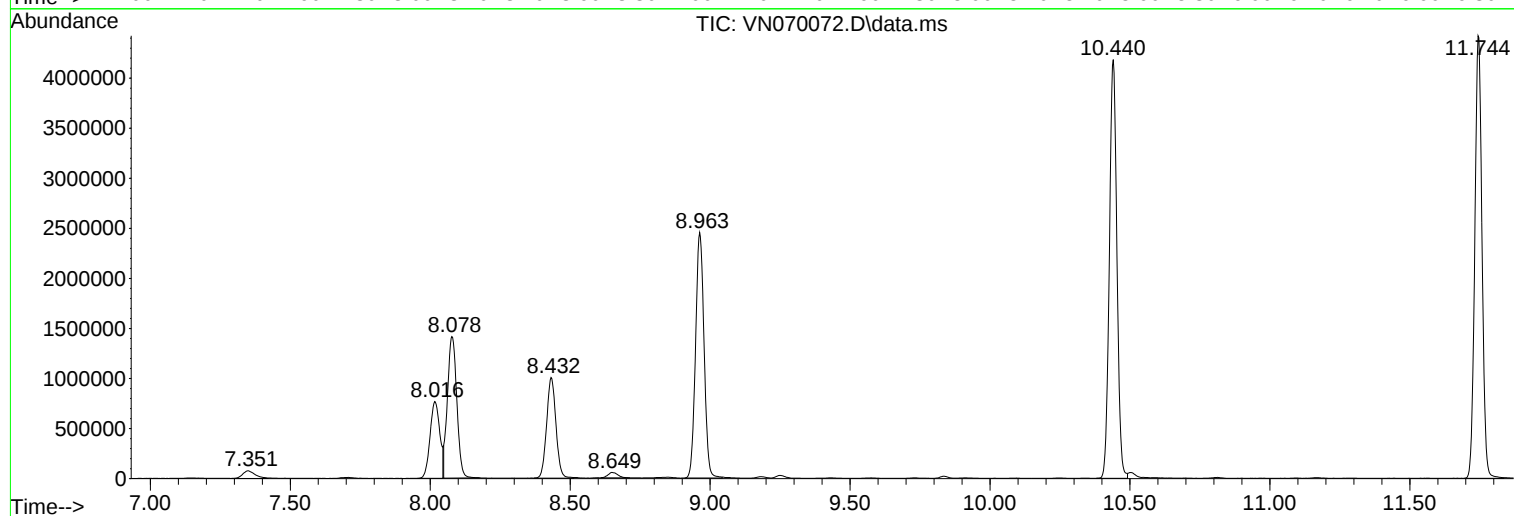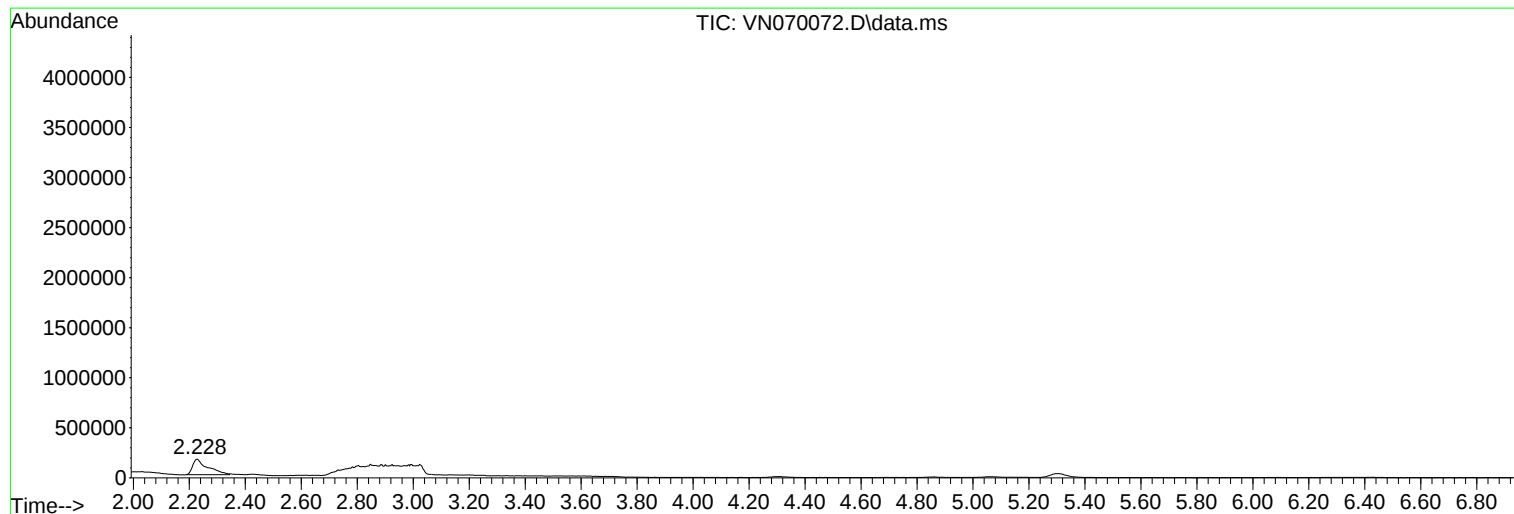

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121421\
Data File : VN070072.D
Acq On : 14 Dec 2021 15:35
Operator : JC/MD
Sample : M5029-03
Misc : 4.05g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PSC-124019

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	2.228	8.8	ug/l	574170	1	8.078	3250680	50.0