


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121421\
Data File : VN070087.D
Acq On : 14 Dec 2021 22:39
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
Title : SW846 8260
Last Update : Fri Dec 03 08:46:47 2021

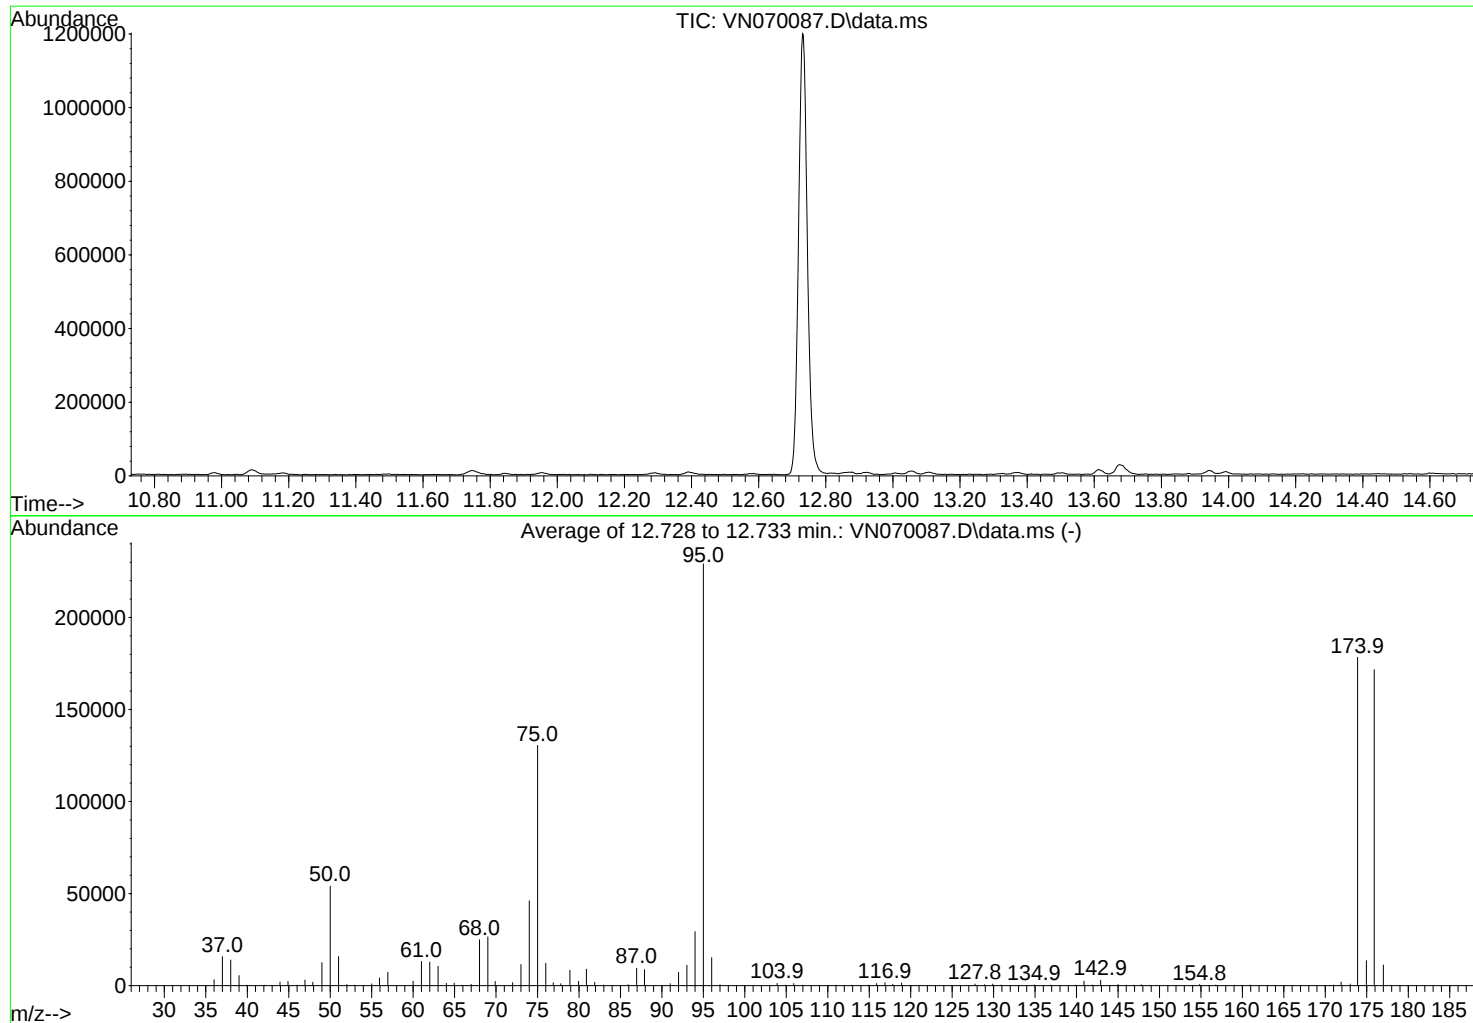

AutoFind: Scans 4004, 4005, 4006; Background Corrected with Scan 3987

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.6	54099	PASS
75	95	30	60	56.9	130448	PASS
95	95	100	100	100.0	229120	PASS
96	95	5	9	6.7	15245	PASS
173	174	0.00	2	0.5	895	PASS
174	95	50	100	77.8	178347	PASS
175	174	5	9	7.6	13547	PASS
176	174	95	101	96.3	171669	PASS
177	176	5	9	6.5	11209	PASS