
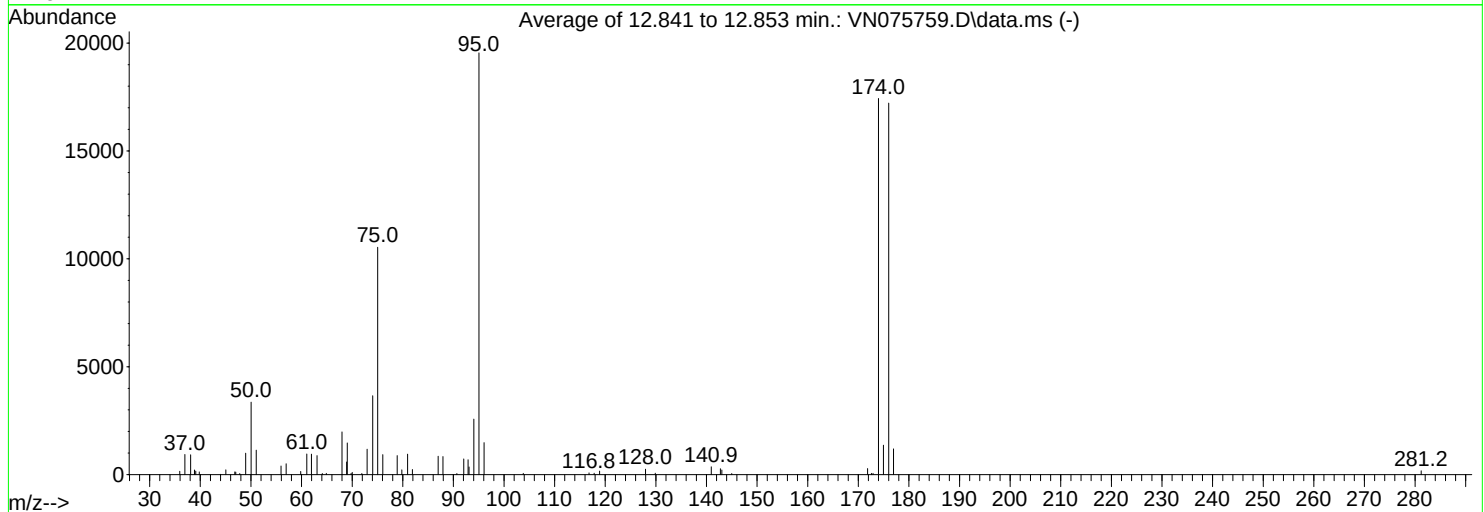


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121422\
 Data File : VN075759.D
 Acq On : 14 Dec 2022 08:28
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
 Title : SW846 8260
 Last Update : Wed Dec 14 13:03:41 2022

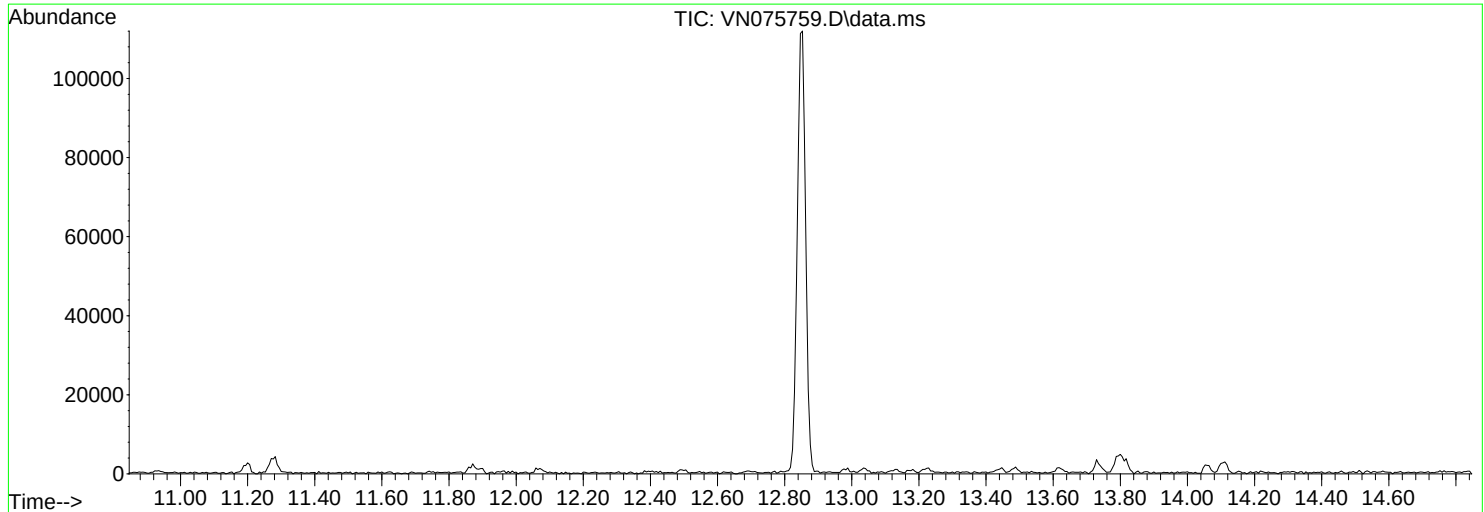

AutoFind: Scans 1834, 1835, 1836; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	3360	PASS
75	95	30	60	53.9	10535	PASS
95	95	100	100	100.0	19547	PASS
96	95	5	9	7.6	1481	PASS
173	174	0.00	2	0.3	57	PASS
174	95	50	100	89.2	17432	PASS
175	174	5	9	7.8	1368	PASS
176	174	95	101	98.8	17215	PASS
177	176	5	9	6.9	1194	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	157	48.95	995	68.00	1980	79.80	211
36.95	936	50.05	3360	68.90	589	80.95	95
38.10	922	51.05	1138	69.05	1472	81.90	23
38.85	215	55.95	398	69.80	62	87.00	85
39.10	165	56.95	504	70.00	102	87.95	840
39.80	123	59.85	146	71.90	55	90.70	53
44.00	13	61.05	956	72.95	1181	92.05	729
45.05	219	61.95	946	74.05	3653	92.90	693
46.80	127	63.05	885	75.05	10535	93.10	357
47.00	121	64.10	54	76.05	926	94.05	2572
47.80	50	64.90	60	78.90	882	95.05	19547

Average of 12.841 to 12.853 min.: VN075759.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
96.05	1481	171.85	284				
103.80	62	172.60	58				
116.80	84	172.90	57				
117.80	67	174.00	17432				
118.90	161	174.95	1368				
127.95	251	176.00	17215				
129.90	67	176.95	1194				
140.95	361	281.20	176				
142.75	274						
143.05	213						
145.00	52						

Instrument :

MSVOA_N

ClientSampleId :

BFB