


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121422\
Data File : VN075783.D
Acq On : 14 Dec 2022 22:04
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
Title : SW846 8260
Last Update : Wed Dec 14 13:03:41 2022

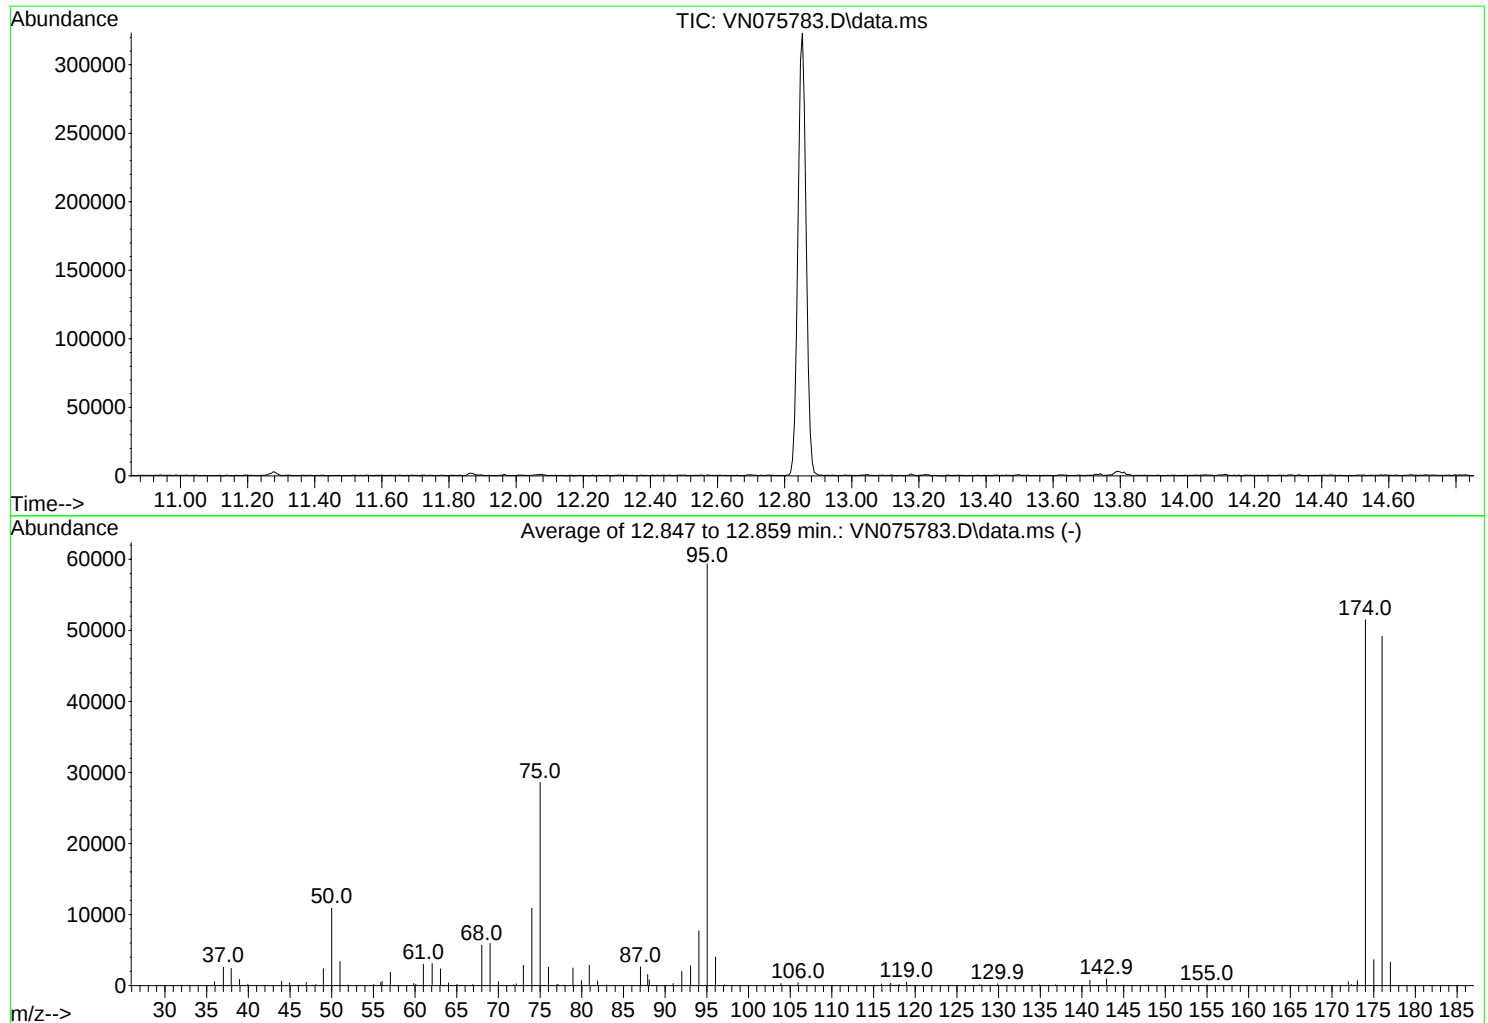

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	10910	PASS
75	95	30	60	48.2	28592	PASS
95	95	100	100	100.0	59360	PASS
96	95	5	9	6.8	4027	PASS
173	174	0.00	2	1.3	694	PASS
174	95	50	100	86.8	51504	PASS
175	174	5	9	7.1	3647	PASS
176	174	95	101	95.5	49181	PASS
177	176	5	9	6.8	3323	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	547	50.00	10910	63.05	2341	75.00	2859
37.00	2616	51.00	3401	64.00	389	76.00	260
37.95	2438	51.95	113	65.05	193	77.00	14
38.95	885	55.05	187	66.95	155	77.15	18
39.95	214	55.90	422	68.00	5698	77.90	61
44.00	610	56.05	608	69.00	5942	78.95	2470
44.95	416	57.05	1876	70.00	560	79.95	729
46.95	460	59.85	306	71.80	127	80.90	2863
47.70	65	60.10	183	72.15	240	81.90	656
48.10	171	61.00	3018	73.00	2862	82.95	121
49.00	2386	62.05	3119	74.00	10900	87.05	2627

Average of 12.847 to 12.859 min.: VN075783.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.90	1546	115.95	256	140.95	742	172.30	160
88.10	815	116.90	98	142.20	52	173.05	694
90.95	301	117.05	331	142.95	951	174.00	51504
92.00	2004	117.70	91	144.80	56	175.00	3647
93.05	2816	118.05	182	145.00	96	176.00	49181
94.05	7696	118.95	468	147.70	70	177.00	3323
95.05	59360	127.75	126	148.00	81		
96.05	4027	128.00	83	155.00	124		
97.10	132	129.90	274	157.00	54		
103.90	286	134.90	124	159.10	72		
105.95	415	136.85	136	171.95	552		

Instrument :

MSVOA_N

ClientSampleId :

BFB