

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121423\
 Data File : VN080488.D
 Acq On : 14 Dec 2023 17:26
 Operator : JC\MD
 Sample : 05831-03
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Dec 15 00:30:55 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121223W.M
 Quant Title : SW846 8260
 QLast Update : Wed Dec 13 01:57:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	220608	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	398608	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	415744	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	193840	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	156316	55.477	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 110.960%	
35) Dibromofluoromethane	8.165	113	132304	52.349	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 104.700%	
50) Toluene-d8	10.565	98	462104	49.026	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 98.060%	
62) 4-Bromofluorobenzene	12.847	95	189602	52.974	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 105.940%	


Target Compounds					Qvalue	
3) Chloromethane	2.365	50	3133	0.664	ug/l	98
6) Chloroethane	3.136	64	613	0.396	ug/l #	43
11) Tert butyl alcohol	5.500	59	1017	3.065	ug/l #	88
13) Acrolein	4.189	56	663	1.824	ug/l	91
16) Acetone	4.447	43	3995	7.996	ug/l #	71
25) 2-Butanone	7.559	43	345599	359.083	ug/l #	37
29) Tetrahydrofuran	7.553	42	18521	26.874	ug/l #	26
31) Cyclohexane	8.224	56	5228	1.364	ug/l #	5
36) 1,1-Dichloropropene	8.229	75	17992	4.354	ug/l #	51
37) Ethyl Acetate	7.559	43	345599	133.555	ug/l	99
38) Carbon Tetrachloride	8.224	117	24827	5.028	ug/l #	18
39) Methylcyclohexane	9.606	83	1268	0.295	ug/l #	74
40) Benzene	8.612	78	3351	0.281	ug/l	97
41) Methacrylonitrile	7.559	41	3657	2.451	ug/l #	16
52) Toluene	10.629	92	10229	1.357	ug/l	95
59) 2-Hexanone	11.288	43	195396	103.290	ug/l #	22
67) Ethyl Benzene	11.964	91	14648	0.861	ug/l	92
68) m/p-Xylenes	12.064	106	13314	2.119	ug/l	88
69) o-Xylene	12.400	106	8867	1.443	ug/l	94
73) Isopropylbenzene	12.694	105	4784	0.307	ug/l	95
76) 1,2,3-Trichloropropane	12.847	75	104600	27.049	ug/l #	1
78) n-propylbenzene	13.041	91	11025	0.642	ug/l	98
79) 2-Chlorotoluene	13.094	91	6711	0.599	ug/l #	42
80) 1,3,5-Trimethylbenzene	13.176	105	17800	1.327	ug/l	98
81) trans-1,4-Dichloro-2-b...	12.847	75	104600	71.020	ug/l #	15
83) tert-Butylbenzene	13.482	119	4696	0.428	ug/l #	64
84) 1,2,4-Trimethylbenzene	13.482	105	34514	2.587	ug/l	100
85) sec-Butylbenzene	13.611	105	3659	0.260	ug/l	97
86) p-Isopropyltoluene	13.729	119	3552	0.280	ug/l	94
89) n-Butylbenzene	14.053	91	2757	0.260	ug/l #	82
90) Hexachloroethane	14.335	117	1364	0.677	ug/l #	21
95) Naphthalene	15.647	128	2502	0.232	ug/l #	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121423\
Data File : VN080488.D
Acq On : 14 Dec 2023 17:26
Operator : JC\MD
Sample : 05831-03
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Dec 15 00:30:55 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121223W.M
Quant Title : SW846 8260
QLast Update : Wed Dec 13 01:57:14 2023
Response via : Initial Calibration




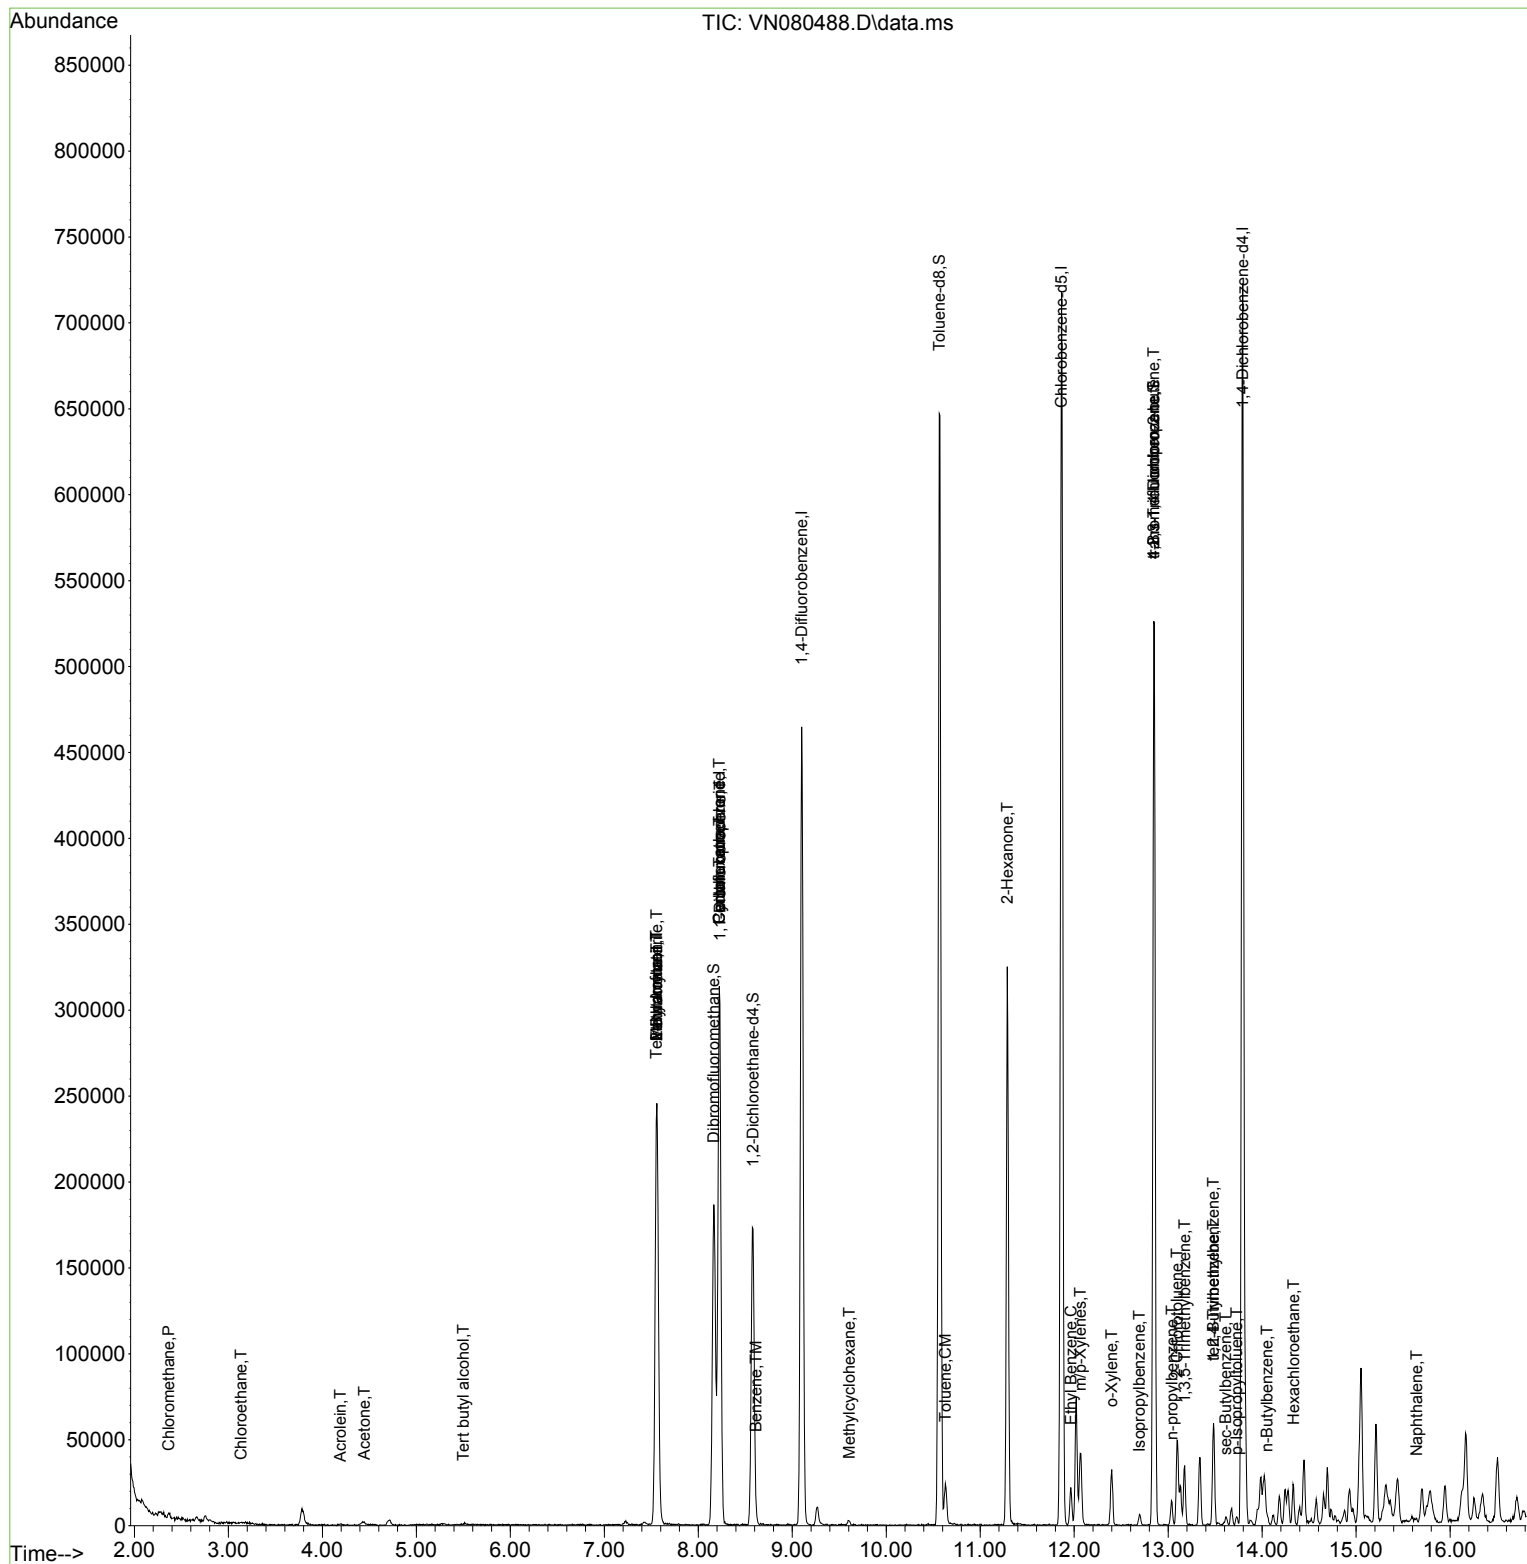




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 10
Delta R.T. -0.000 min
Lab File: VN080488.D
Acq: 14 Dec 2023 17:26




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:168 Resp: 220608
Ion Ratio Lower Upper
168 100
99 67.2 53.0 79.6

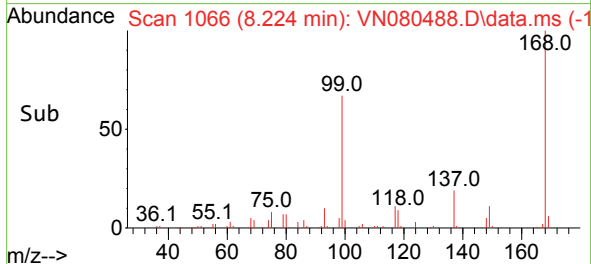

#3
Chloromethane
Concen: 0.664 ug/l
RT: 2.365 min Scan# 70
Delta R.T. 0.006 min
Lab File: VN080488.D
Acq: 14 Dec 2023 17:26

Tgt Ion: 50 Resp: 3133
Ion Ratio Lower Upper
50 100
52 32.1 26.5 39.7


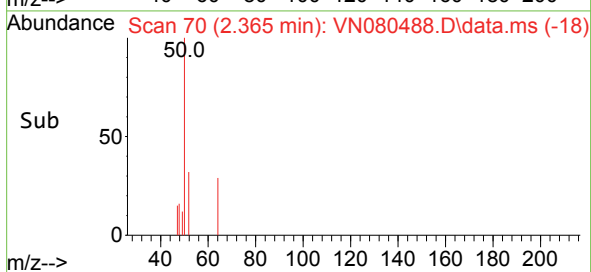






#6
Chloroethane
Concen: 0.396 ug/l
RT: 3.136 min Scan# 201
Delta R.T. 0.012 min
Lab File: VN080488.D
Acq: 14 Dec 2023 17:26




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 64 Resp: 613
Ion Ratio Lower Upper
64 100
66 0.0 25.4 38.2#

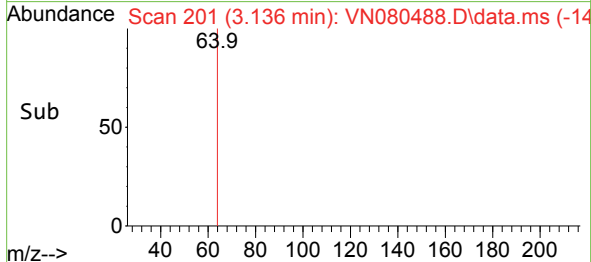

#11
Tert butyl alcohol
Concen: 3.065 ug/l
RT: 5.500 min Scan# 603
Delta R.T. -0.012 min
Lab File: VN080488.D
Acq: 14 Dec 2023 17:26

Tgt Ion: 59 Resp: 1017
Ion Ratio Lower Upper
59 100
57 5.7 8.2 12.4#




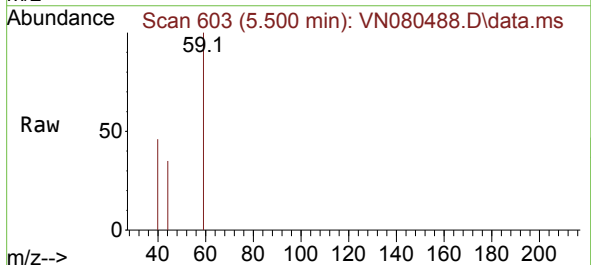




#13
Acrolein
Concen: 1.824 ug/l
RT: 4.189 min Scan# 31
Delta R.T. 0.012 min
Lab File: VN080488.D
Acq: 14 Dec 2023 17:26




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 56 Resp: 663
Ion Ratio Lower Upper
56 100
55 75.6 54.5 81.7

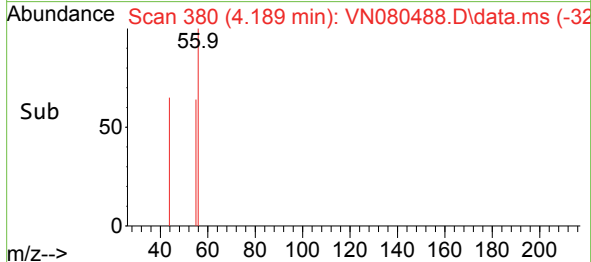

#16
Acetone
Concen: 7.996 ug/l
RT: 4.447 min Scan# 424
Delta R.T. 0.029 min
Lab File: VN080488.D
Acq: 14 Dec 2023 17:26

Tgt Ion: 43 Resp: 3995
Ion Ratio Lower Upper
43 100
58 17.9 28.0 42.0#




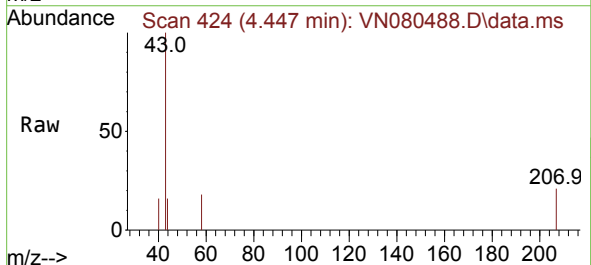




#25
2-Butanone
Concen: 359.083 ug/l
RT: 7.559 min Scan# 91
Delta R.T. 0.082 min
Lab File: VN080488.D
Acq: 14 Dec 2023 17:26




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 345599
Ion Ratio Lower Upper
43 100
72 0.0 30.2 45.2#

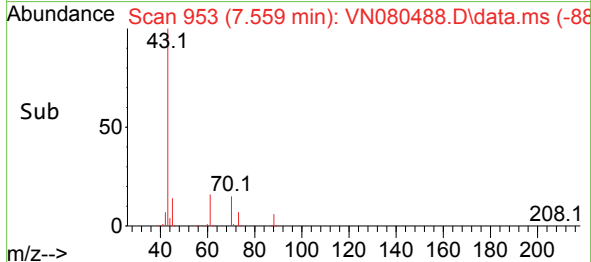

#29
Tetrahydrofuran
Concen: 26.874 ug/l
RT: 7.553 min Scan# 952
Delta R.T. -0.282 min
Lab File: VN080488.D
Acq: 14 Dec 2023 17:26

Tgt Ion: 42 Resp: 18521
Ion Ratio Lower Upper
42 100
72 0.6 49.8 74.6#
71 8.3 47.4 71.2#

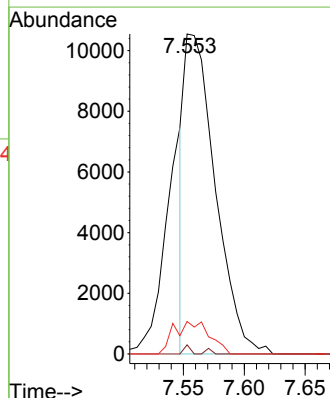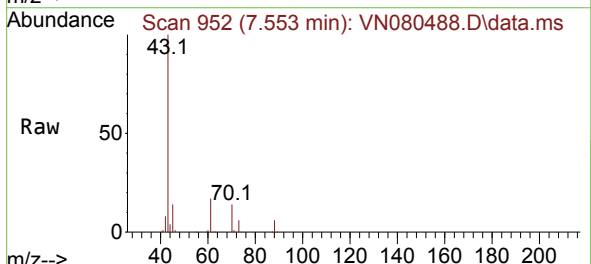



#31

Cyclohexane

Concen: 1.364 ug/l

RT: 8.224 min Scan# 1066

Delta R.T. -0.029 min


Lab File: VN080488.D

Acq: 14 Dec 2023 17:26

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion: 56 Resp: 5228

Ion Ratio Lower Upper

56 100

69 197.2 26.8 40.2#

84 134.7 81.8 122.6#

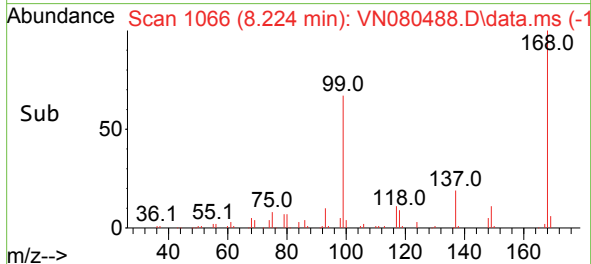

#33

1,2-Dichloroethane-d4

Concen: 55.477 ug/l

RT: 8.582 min Scan# 1127

Delta R.T. 0.006 min

Lab File: VN080488.D




Acq: 14 Dec 2023 17:26


Tgt Ion: 65 Resp: 156316

Ion Ratio Lower Upper

65 100


67 49.5 0.0 106.6








#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.100 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN080488.D
Acq: 14 Dec 2023 17:26

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:114 Resp: 398608
Ion Ratio Lower Upper
114 100
63 21.4 0.0 36.4
88 18.2 0.0 30.6

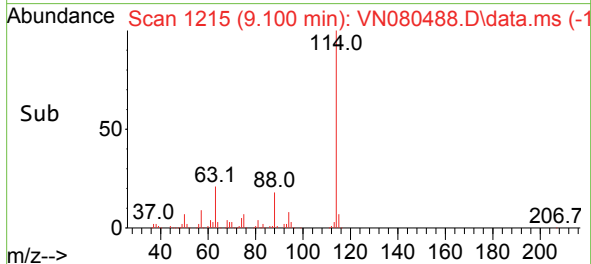

#35
Dibromofluoromethane
Concen: 52.349 ug/l
RT: 8.165 min Scan# 1056
Delta R.T. 0.000 min
Lab File: VN080488.D
Acq: 14 Dec 2023 17:26

Tgt Ion:113 Resp: 132304
Ion Ratio Lower Upper
113 100
111 102.0 82.6 123.8
192 18.2 12.7 19.1

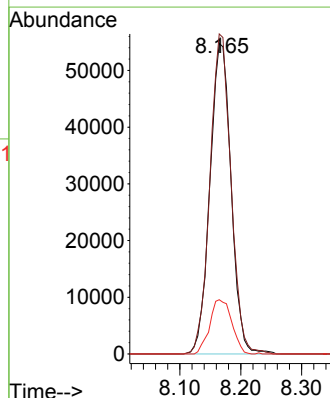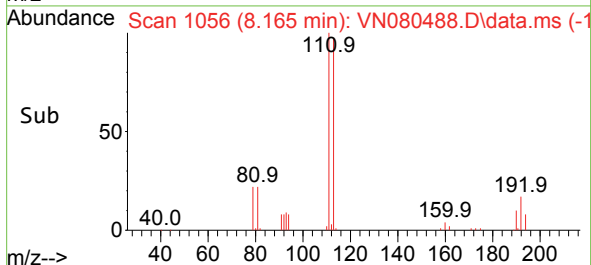



#36

1,1-Dichloropropene

Concen: 4.354 ug/l

RT: 8.229 min Scan# 1067

Delta R.T. -0.141 min


Lab File: VN080488.D

Acq: 14 Dec 2023 17:26

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion: 75 Resp: 17992

Ion Ratio Lower Upper

75 100

110 12.6 19.1 57.3#

77 0.0 25.0 37.4#



#37

Ethyl Acetate

Concen: 133.555 ug/l

RT: 7.559 min Scan# 953

Delta R.T. 0.006 min

Lab File: VN080488.D

Acq: 14 Dec 2023 17:26




Tgt Ion: 43 Resp: 345599


Ion Ratio Lower Upper

43 100

61 16.8 13.2 19.8


70 15.0 11.3 16.9








#38
Carbon Tetrachloride
Concen: 5.028 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.135 min
Lab File: VN080488.D
Acq: 14 Dec 2023 17:26

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:117 Resp: 24827
Ion Ratio Lower Upper
117 100
119 8.5 77.3 115.9#
121 0.0 23.3 34.9#

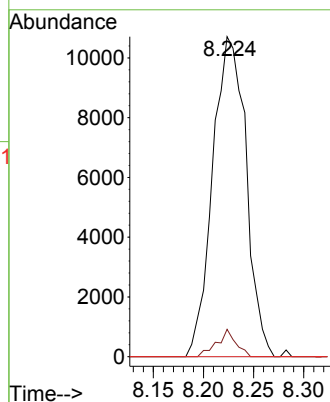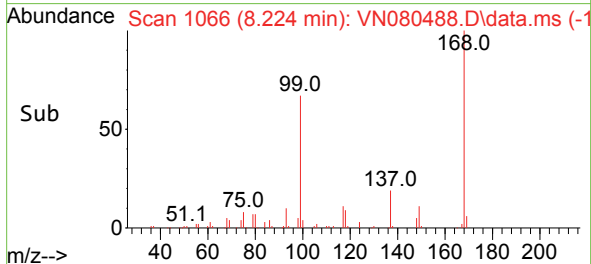

#39
Methylcyclohexane
Concen: 0.295 ug/l
RT: 9.606 min Scan# 1301
Delta R.T. 0.006 min
Lab File: VN080488.D
Acq: 14 Dec 2023 17:26

Tgt Ion: 83 Resp: 1268
Ion Ratio Lower Upper
83 100
55 44.9 49.1 73.7#
98 28.8 40.6 61.0#



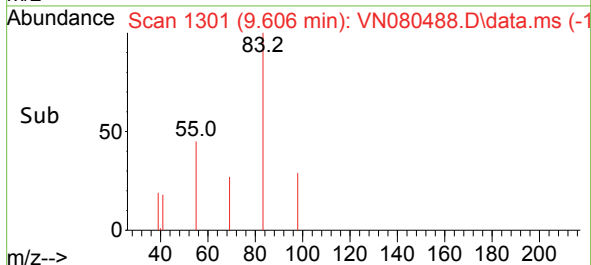





#40
Benzene
Concen: 0.281 ug/l
RT: 8.612 min Scan# 1131
Delta R.T. 0.006 min
Lab File: VN080488.D
Acq: 14 Dec 2023 17:26




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 78 Resp: 3351
Ion Ratio Lower Upper
78 100
77 22.3 19.0 28.6

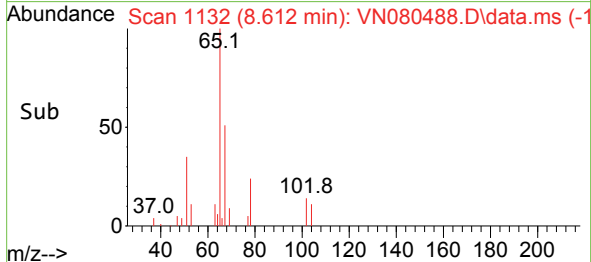

#41
Methacrylonitrile
Concen: 2.451 ug/l
RT: 7.559 min Scan# 953
Delta R.T. -0.212 min
Lab File: VN080488.D
Acq: 14 Dec 2023 17:26

Tgt Ion: 41 Resp: 3657
Ion Ratio Lower Upper
41 100
39 2.1 42.6 64.0#
67 0.0 77.5 116.3#
52 0.0 28.9 43.3#





#50

Toluene-d8

Concen: 49.026 ug/l

RT: 10.565 min Scan# 1464

Delta R.T. 0.000 min

Lab File: VN080488.D

Acq: 14 Dec 2023 17:26

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 98 Resp: 462104

Ion Ratio Lower Upper

98 100

100 64.7 52.0 78.0

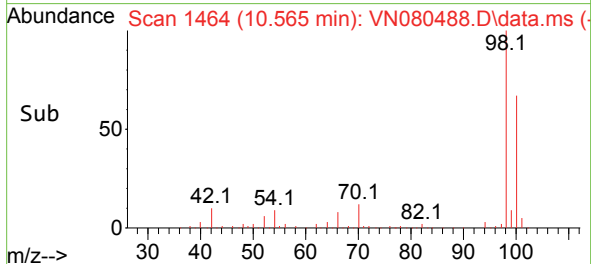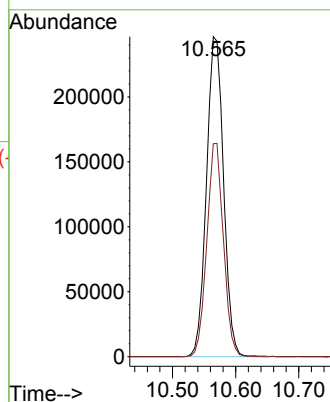

#52

Toluene

Concen: 1.357 ug/l

RT: 10.629 min Scan# 1475

Delta R.T. 0.000 min

Lab File: VN080488.D




Acq: 14 Dec 2023 17:26


Tgt Ion: 92 Resp: 10229

Ion Ratio Lower Upper

92 100

91 177.9 137.4 206.0




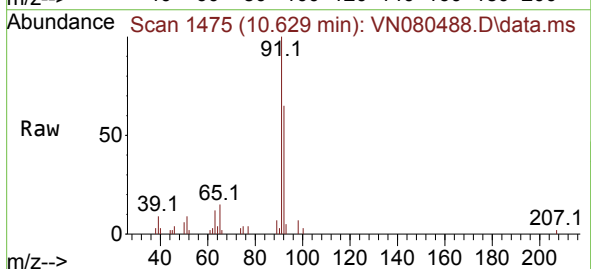




#59
2-Hexanone
Concen: 103.290 ug/l
RT: 11.288 min Scan# 1587
Delta R.T. 0.094 min
Lab File: VN080488.D
Acq: 14 Dec 2023 17:26




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 195396
Ion Ratio Lower Upper
43 100
58 2.3 31.7 95.1#

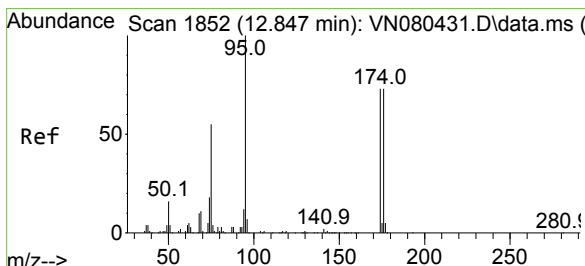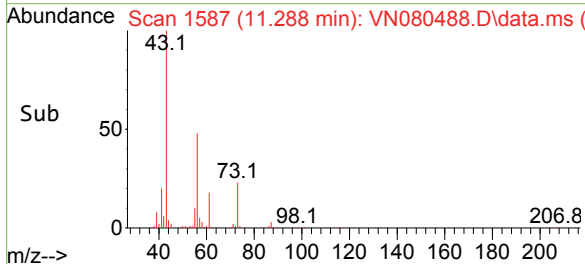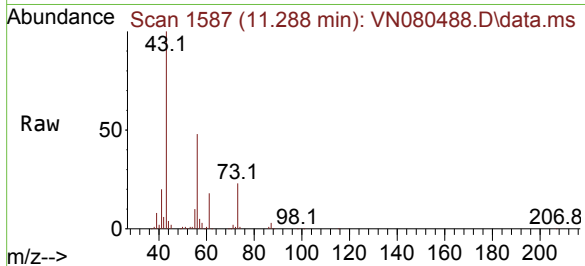

#62
4-Bromofluorobenzene
Concen: 52.974 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.000 min
Lab File: VN080488.D
Acq: 14 Dec 2023 17:26

Tgt Ion: 95 Resp: 189602
Ion Ratio Lower Upper
95 100
174 76.2 0.0 143.8
176 73.3 0.0 135.8


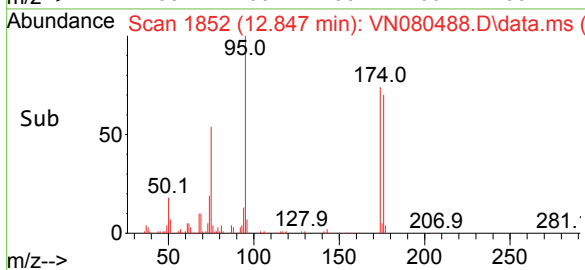

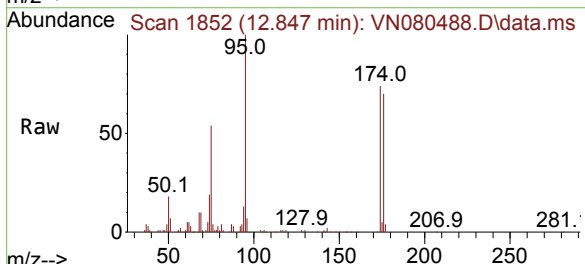




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN080488.D
Acq: 14 Dec 2023 17:26




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:117 Resp: 415744
Ion Ratio Lower Upper
117 100
82 57.8 44.0 66.0
119 31.8 25.6 38.4

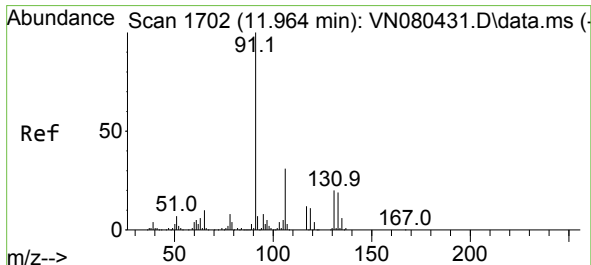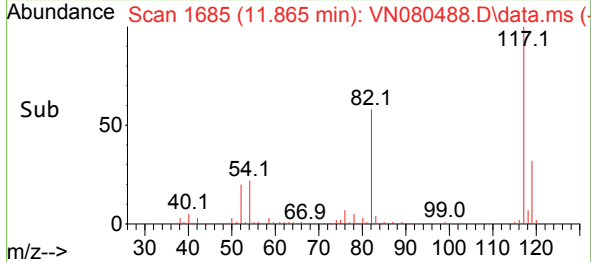

#67
Ethyl Benzene
Concen: 0.861 ug/l
RT: 11.964 min Scan# 1702
Delta R.T. 0.000 min
Lab File: VN080488.D
Acq: 14 Dec 2023 17:26

Tgt Ion: 91 Resp: 14648
Ion Ratio Lower Upper
91 100
106 36.5 25.6 38.4




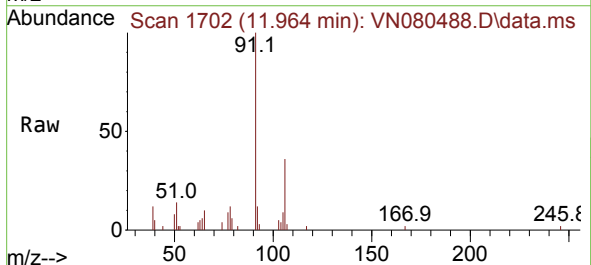




#68
m/p-Xylenes
Concen: 2.119 ug/l
RT: 12.064 min Scan# 1719
Delta R.T. -0.006 min
Lab File: VN080488.D
Acq: 14 Dec 2023 17:26




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:106 Resp: 13314
Ion Ratio Lower Upper
106 100
91 217.7 159.6 239.4

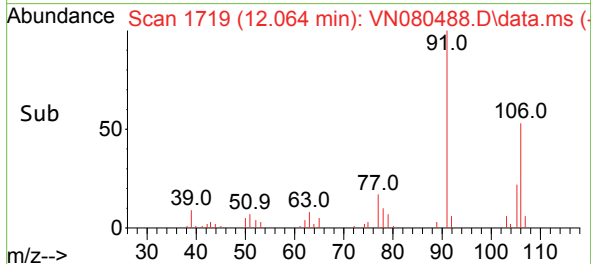

#69
o-Xylene
Concen: 1.443 ug/l
RT: 12.400 min Scan# 1776
Delta R.T. 0.000 min
Lab File: VN080488.D
Acq: 14 Dec 2023 17:26

Tgt Ion:106 Resp: 8867
Ion Ratio Lower Upper
106 100
91 220.1 105.2 315.5





#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.794 min Scan# 2013

Delta R.T. 0.000 min


Lab File: VN080488.D

Acq: 14 Dec 2023 17:26

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion:152 Resp: 193840

Ion Ratio Lower Upper

152 100

115 66.3 32.3 96.8

150 157.8 0.0 355.8

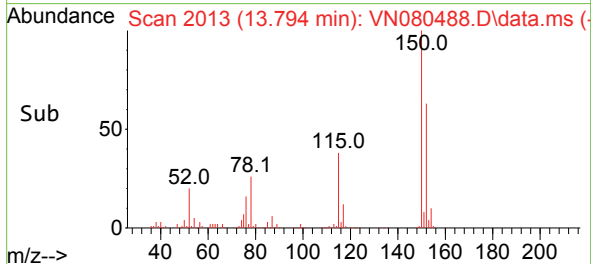

#73

Isopropylbenzene

Concen: 0.307 ug/l

RT: 12.694 min Scan# 1826

Delta R.T. 0.000 min

Lab File: VN080488.D




Acq: 14 Dec 2023 17:26


Tgt Ion:105 Resp: 4784

Ion Ratio Lower Upper

105 100

120 28.5 13.1 39.1





#76

1,2,3-Trichloropropane

Concen: 27.049 ug/l

RT: 12.847 min Scan# 1852

Delta R.T. -0.147 min

Lab File: VN080488.D

Acq: 14 Dec 2023 17:26

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 75 Resp: 104600

Ion Ratio Lower Upper

75 100

77 1.3 84.5 253.5#



#78

n-propylbenzene

Concen: 0.642 ug/l

RT: 13.041 min Scan# 1885

Delta R.T. 0.006 min

Lab File: VN080488.D




Acq: 14 Dec 2023 17:26


Tgt Ion: 91 Resp: 11025

Ion Ratio Lower Upper

91 100

120 22.0 11.5 34.4







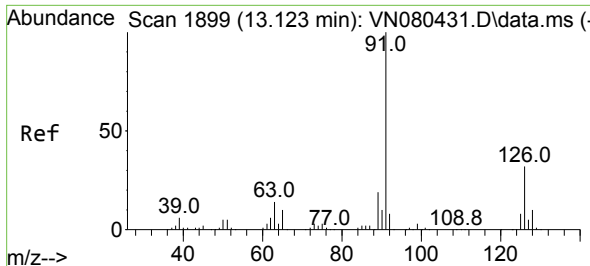

#79
2-Chlorotoluene
Concen: 0.599 ug/l
RT: 13.094 min Scan# 1899
Delta R.T. -0.029 min
Lab File: VN080488.D
Acq: 14 Dec 2023 17:26




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 91 Resp: 6711
Ion Ratio Lower Upper
91 100
126 0.0 16.3 48.8#

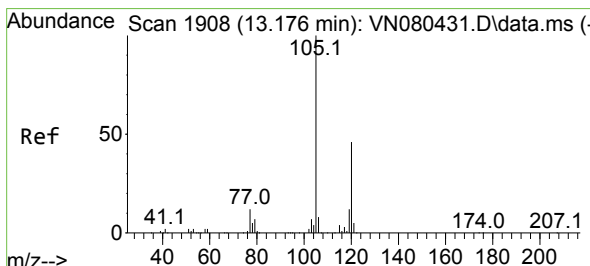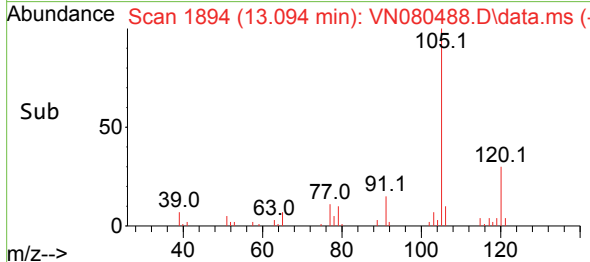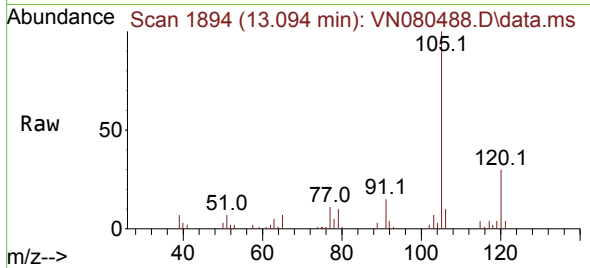

#80
1,3,5-Trimethylbenzene
Concen: 1.327 ug/l
RT: 13.176 min Scan# 1908
Delta R.T. 0.000 min
Lab File: VN080488.D
Acq: 14 Dec 2023 17:26

Tgt Ion: 105 Resp: 17800
Ion Ratio Lower Upper
105 100
120 47.2 24.1 72.3


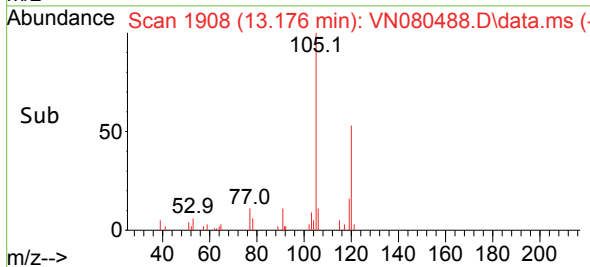

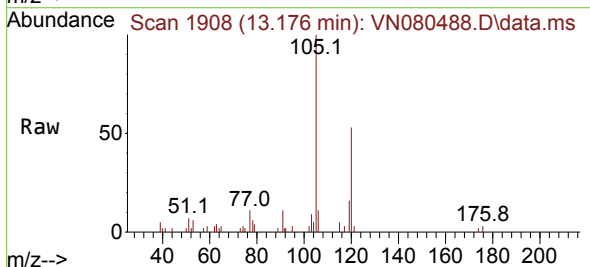


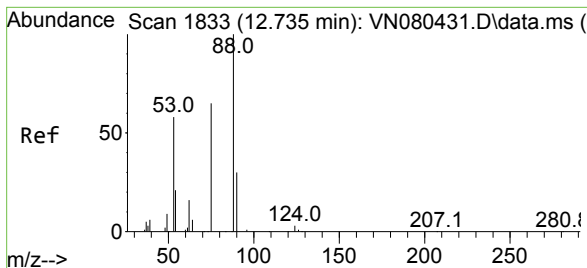

#81
 trans-1,4-Dichloro-2-butene
 Concen: 71.020 ug/l
 RT: 12.847 min Scan# 1852
 Delta R.T. 0.112 min
 Lab File: VN080488.D
 Acq: 14 Dec 2023 17:26




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion: 75 Resp: 104600
 Ion Ratio Lower Upper
 75 100
 53 0.0 67.4 101.2#
 89 0.0 38.8 58.2#

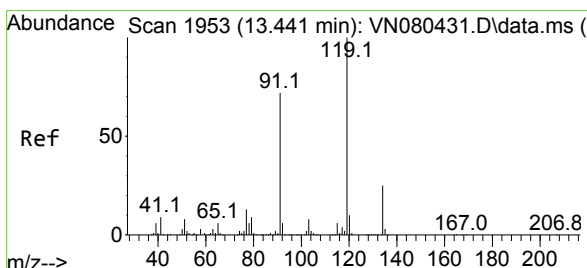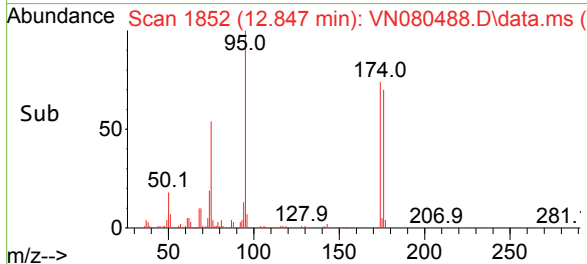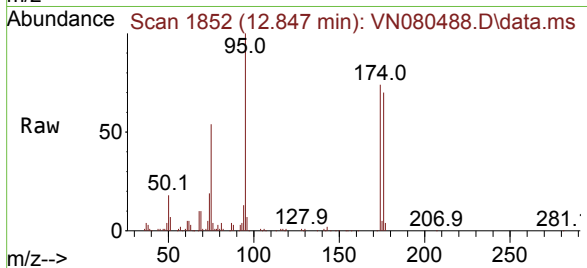

#83
 tert-Butylbenzene
 Concen: 0.428 ug/l
 RT: 13.482 min Scan# 1960
 Delta R.T. 0.041 min
 Lab File: VN080488.D
 Acq: 14 Dec 2023 17:26

Tgt Ion: 119 Resp: 4696
 Ion Ratio Lower Upper
 119 100
 91 92.5 33.9 101.7
 134 0.0 13.2 39.6#


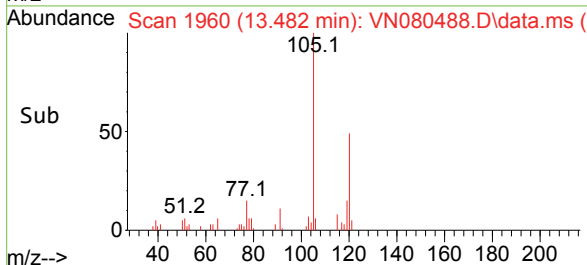

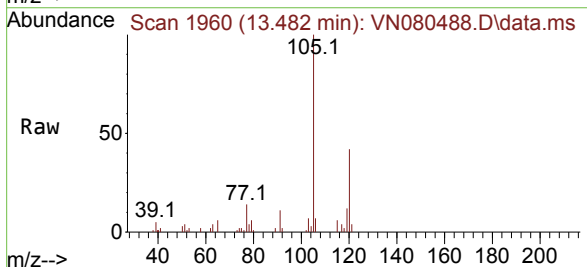




#84
1,2,4-Trimethylbenzene
Concen: 2.587 ug/l
RT: 13.482 min Scan# 1960
Delta R.T. 0.000 min
Lab File: VN080488.D
Acq: 14 Dec 2023 17:26




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:105 Resp: 34514
Ion Ratio Lower Upper
105 100
120 44.3 22.0 66.0

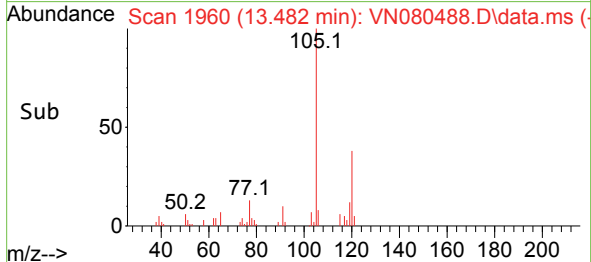

#85
sec-Butylbenzene
Concen: 0.260 ug/l
RT: 13.611 min Scan# 1982
Delta R.T. -0.006 min
Lab File: VN080488.D
Acq: 14 Dec 2023 17:26

Tgt Ion:105 Resp: 3659
Ion Ratio Lower Upper
105 100
134 21.0 9.8 29.3







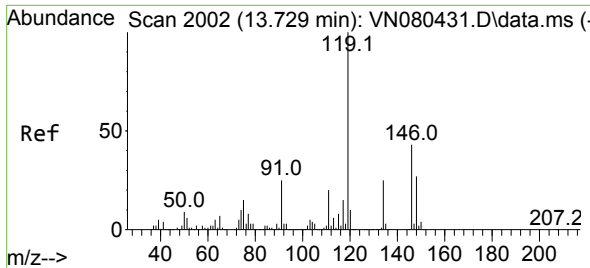

#86
 p-Isopropyltoluene
 Concen: 0.280 ug/l
 RT: 13.729 min Scan# 2002
 Delta R.T. 0.000 min
 Lab File: VN080488.D
 Acq: 14 Dec 2023 17:26




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion:119 Resp: 3552
 Ion Ratio Lower Upper
 119 100
 134 22.9 12.6 37.8
 91 29.0 12.4 37.2

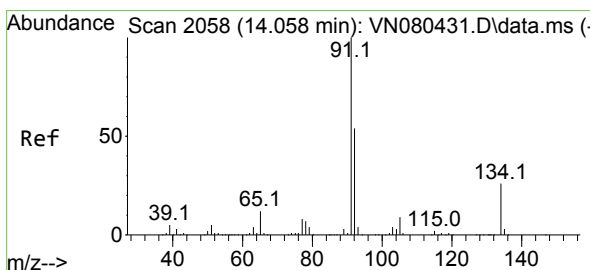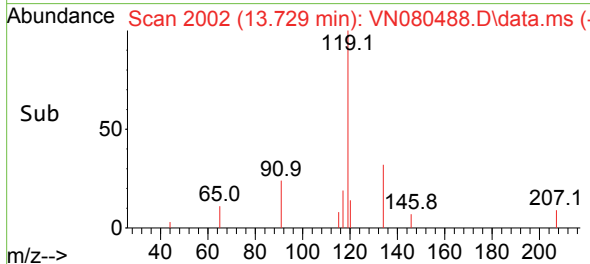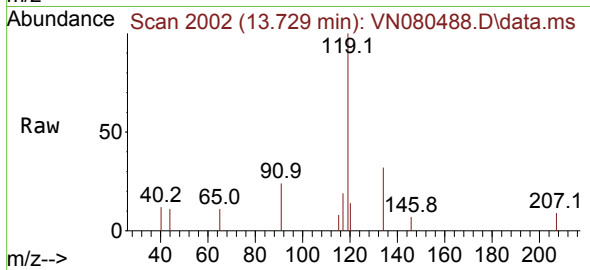

#89
 n-Butylbenzene
 Concen: 0.260 ug/l
 RT: 14.053 min Scan# 2057
 Delta R.T. -0.006 min
 Lab File: VN080488.D
 Acq: 14 Dec 2023 17:26

Tgt Ion: 91 Resp: 2757
 Ion Ratio Lower Upper
 91 100
 92 54.4 26.4 79.0
 134 0.0 12.6 37.6#


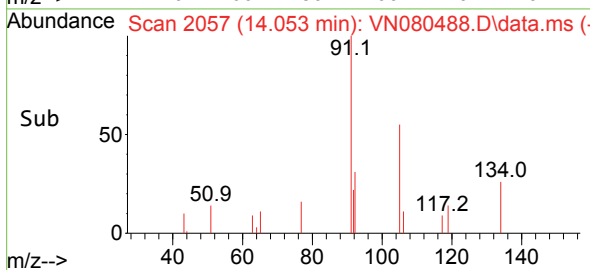

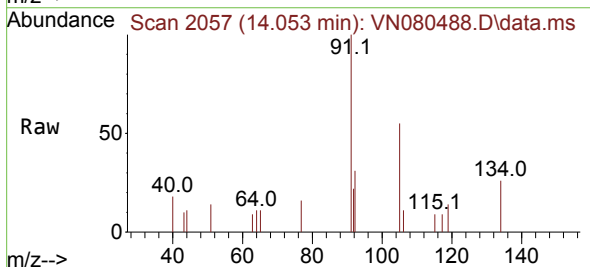


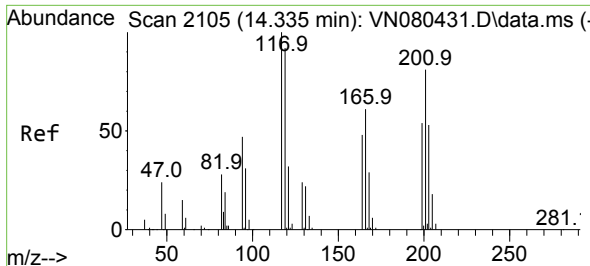

#90
Hexachloroethane
Concen: 0.677 ug/l
RT: 14.335 min Scan# 2105
Delta R.T. 0.000 min
Lab File: VN080488.D
Acq: 14 Dec 2023 17:26

Instrument :
MSVOA_N
ClientSampleId :

Tgt Ion:117 Resp: 1364
Ion Ratio Lower Upper
117 100
201 0.0 29.3 88.0#

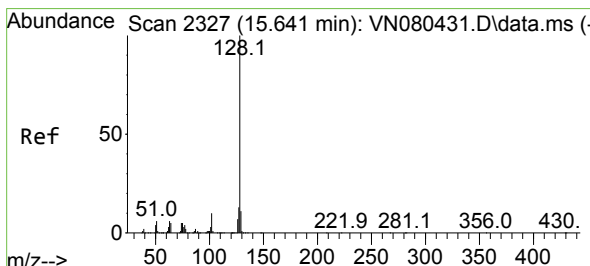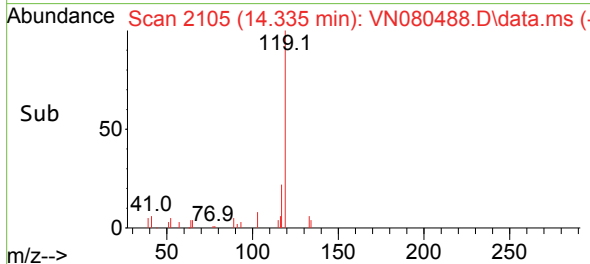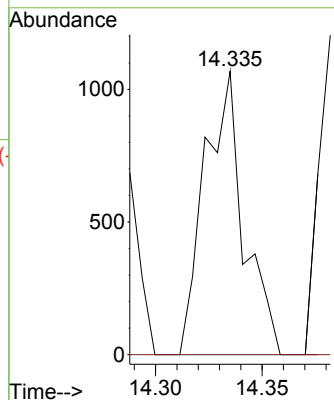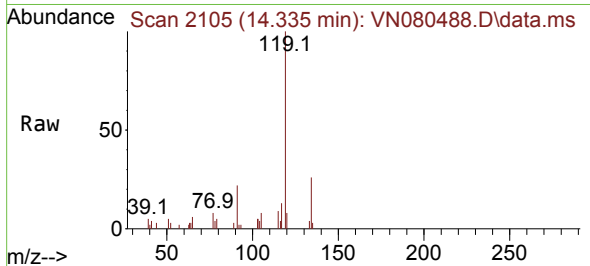

#95
Naphthalene
Concen: 0.232 ug/l
RT: 15.647 min Scan# 2328
Delta R.T. 0.006 min
Lab File: VN080488.D
Acq: 14 Dec 2023 17:26

Tgt Ion:128 Resp: 2502
Ion Ratio Lower Upper
128 100
127 6.0 10.0 15.0#
129 0.0 8.7 13.1#

