
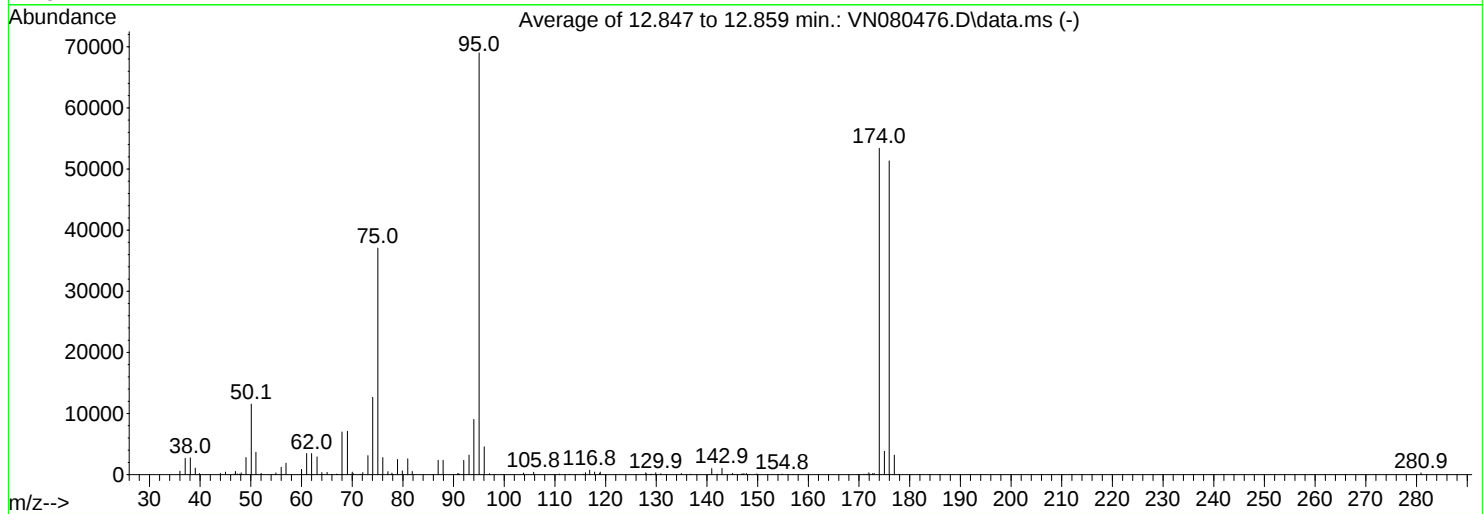


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121423\
Data File : VN080476.D
Acq On : 14 Dec 2023 09:49
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121223W.M
Title : SW846 8260
Last Update : Wed Dec 13 01:57:14 2023

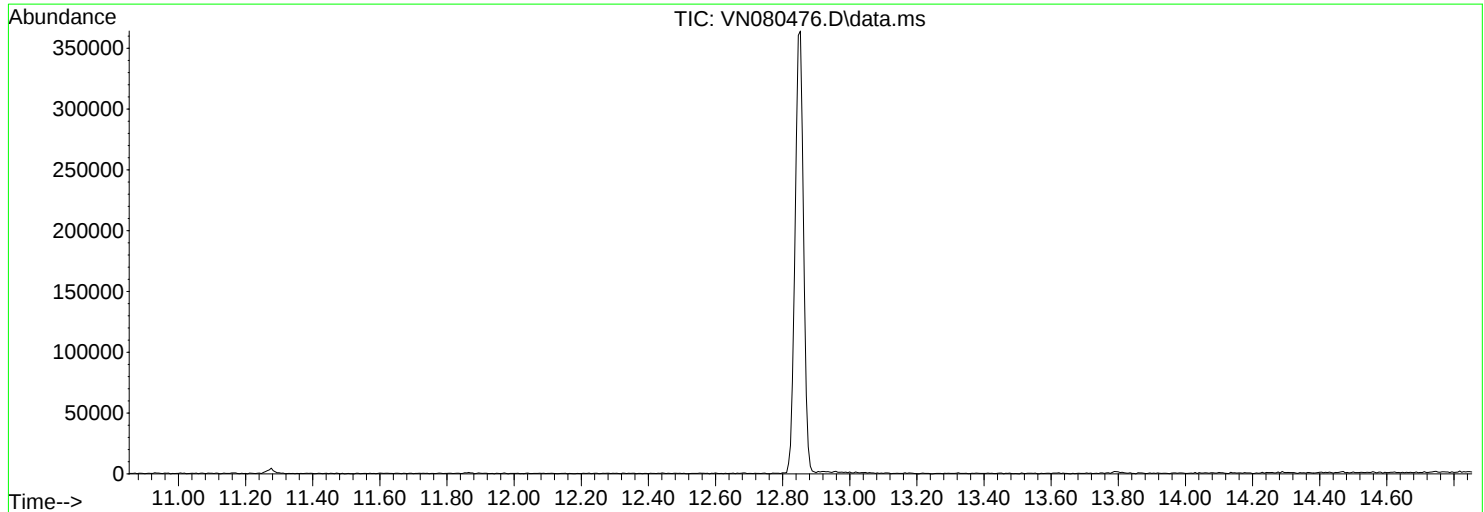

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	11558	PASS
75	95	30	60	53.7	37077	PASS
95	95	100	100	100.0	69008	PASS
96	95	5	9	6.6	4546	PASS
173	174	0.00	2	0.4	214	PASS
174	95	50	100	77.4	53403	PASS
175	174	5	9	7.2	3826	PASS
176	174	95	101	96.1	51323	PASS
177	176	5	9	6.2	3200	PASS

Average of 12.847 to 12.859 min.: VN080476.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	575	48.10	299	62.00	3468	72.10	351
37.05	2683	49.05	2810	63.05	2899	73.10	311
38.05	2749	50.10	11558	64.00	345	74.05	1265
39.05	1065	51.00	3673	65.05	380	75.05	3707
39.90	196	52.05	213	66.90	101	76.05	2795
44.00	208	54.95	291	67.20	55	77.05	493
45.00	432	56.00	1192	68.00	7002	77.85	260
46.70	87	56.95	1884	69.05	7092	78.95	2480
46.95	537	58.00	64	70.00	419	79.90	634
47.30	136	60.00	864	70.20	174	80.95	2587
47.80	106	61.00	3457	71.60	68	81.85	521

Average of 12.847 to 12.859 min.: VN080476.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
86.95	2360	104.00	62	128.10	120	146.80	80
87.95	2353	105.80	385	128.80	51	147.00	96
90.85	206	110.85	119	129.00	82	147.30	182
91.05	150	112.80	50	129.90	325	147.80	198
92.00	2343	115.70	91	130.90	152	149.85	123
93.05	3203	116.05	318	134.95	198	154.85	113
94.00	9031	116.85	734	136.80	76	157.00	52
95.05	69008	117.85	435	140.95	994	171.00	74
96.05	4546	118.80	212	142.10	69	171.60	92
97.10	167	118.95	410	142.95	1053	171.95	329
103.80	255	127.90	279	145.05	215	172.20	78

Average of 12.847 to 12.859 min.: VN080476.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
172.70	183						
173.00	214						
174.00	53403						
175.00	3826						
175.95	51323						
176.95	3200						
177.90	72						
280.90	289						

Instrument :

MSVOA_N

ClientSampleId :

BFB