


Abundance Scan 1682 (7.148 min): VN065141.D\data.ms (-1662) (-)

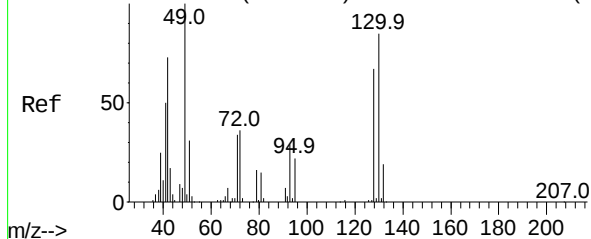




Bromochloromethane
Concen: 30.00 ug/l
RT: 7.152 min Scan# 1683
Delta R.T. 0.004 min
Lab File: VN065154.D
Acq: 15 Dec 2020 20:09

Tgt Ion:	128	Resp:	104277
Ion	Ratio	Lower	Upper
128	100		
49	145.6	0.0	475.5
130	127.1	0.0	315.3


Instrument :
MSVOA_N
ClientSampleId :
VSTDCCC020EC

Manual Integrations
APPROVED

MMDadoda
12/16/2020 1:47:38 PM

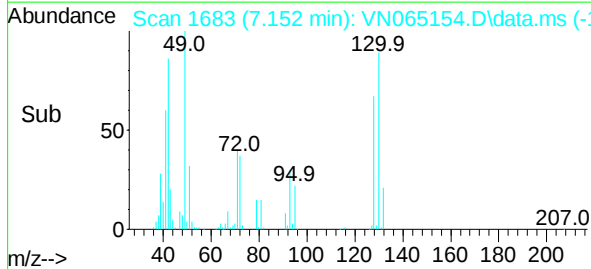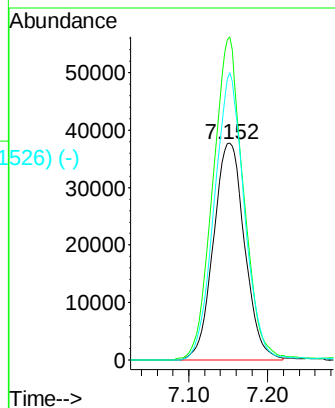
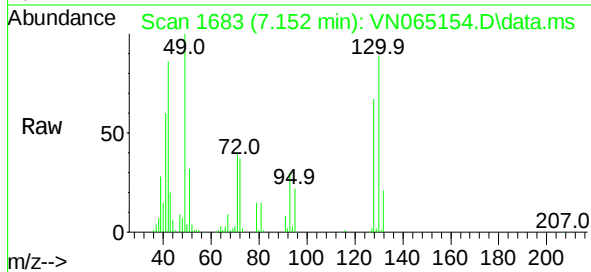


Abundance Scan 29 (1.833 min): VN065141.D\data.ms (-19) (-#2)

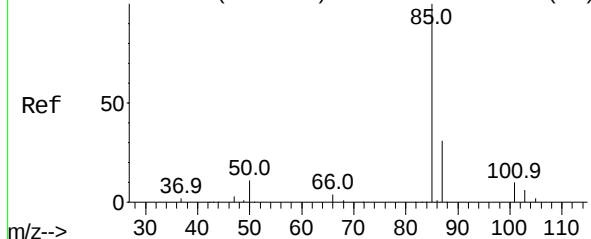



Dichlorodifluoromethane
Concen: 12.92 ug/l
RT: 1.830 min Scan# 28
Delta R.T. -0.003 min
Lab File: VN065154.D
Acq: 15 Dec 2020 20:09

Tgt Ion:	85	Resp:	76365
Ion	Ratio	Lower	Upper
85	100		
87	32.1	17.0	50.9

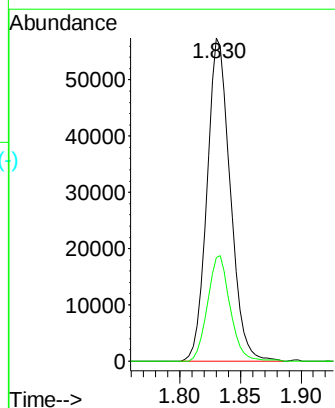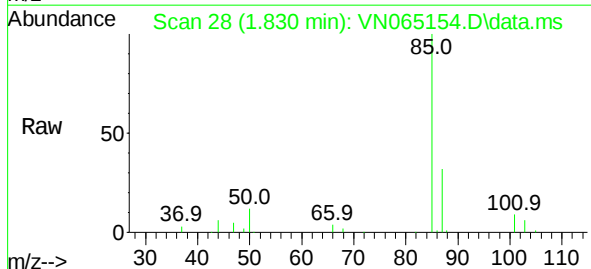

Abundance Scan 28 (1.830 min): VN065154.D\data.ms (-1) (-)

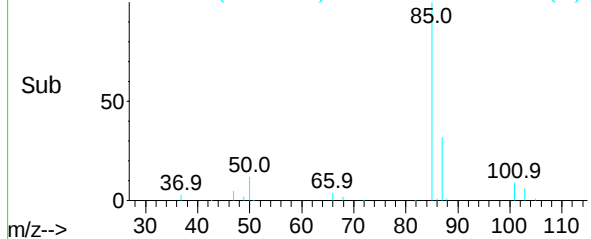

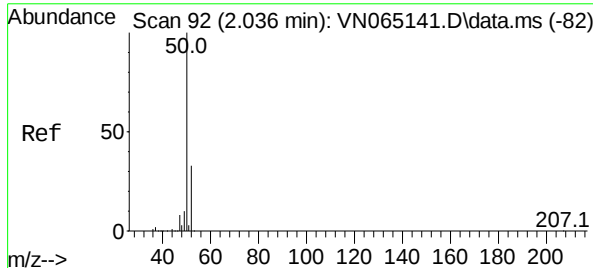





Chloromethane
Concen: 10.96 ug/l
RT: 2.036 min Scan# 92
Delta R.T. 0.000 min
Lab File: VN065154.D
Acq: 15 Dec 2020 20:09

Tgt Ion: 50 Resp: 74658
Ion Ratio Lower Upper
50 100
52 35.1 26.0 39.0

Instrument :
MSVOA_N
ClientSampleId :
VSTDCCC020EC




Manual Integrations
APPROVED


MMDadoda
12/16/2020 1:47:38 PM

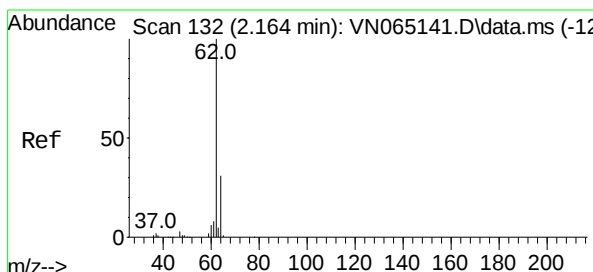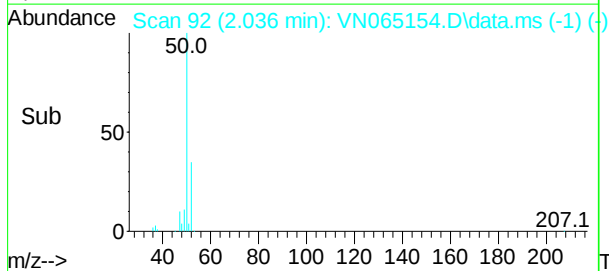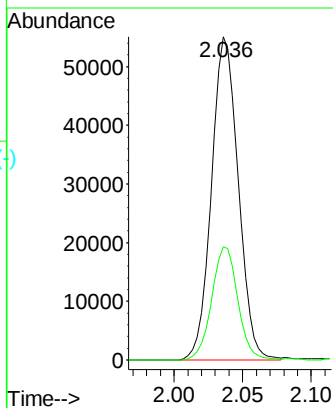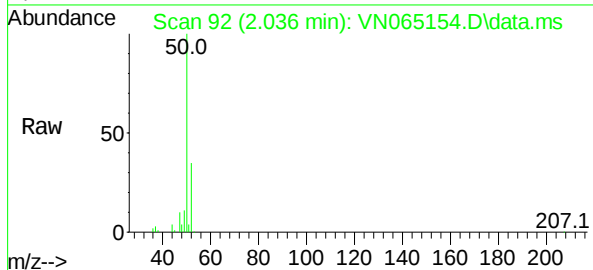

Vinyl Chloride
Concen: 15.19 ug/l
RT: 2.165 min Scan# 132
Delta R.T. 0.000 min
Lab File: VN065154.D
Acq: 15 Dec 2020 20:09

Tgt Ion: 62 Resp: 113936
Ion Ratio Lower Upper
62 100
64 32.2 25.8 38.8

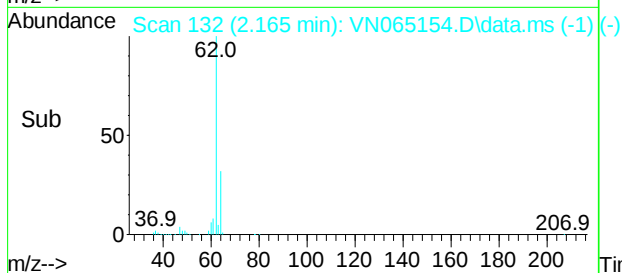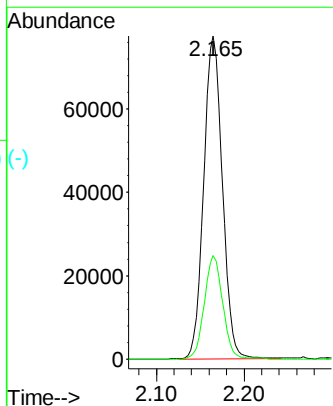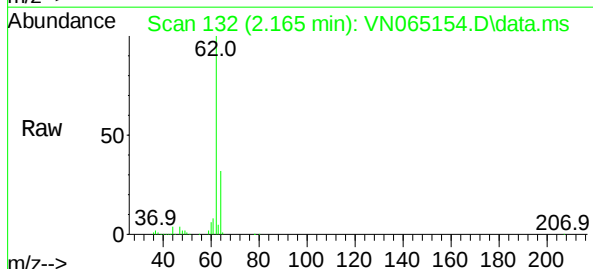

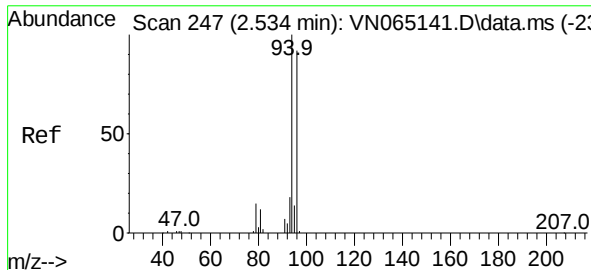





Bromomethane
 Concen: 16.78 ug/l
 RT: 2.534 min Scan# 247
 Delta R.T. 0.000 min
 Lab File: VN065154.D
 Acq: 15 Dec 2020 20:09

Instrument :
 MSVOA_N
 ClientSampleId :
 VSTDCCC020EC

Tgt Ion: 94 Resp: 88397
 Ion Ratio Lower Upper
 94 100
 96 91.4 79.3 118.9




Manual Integrations
 APPROVED


MMDadoda
 12/16/2020 1:47:38 PM

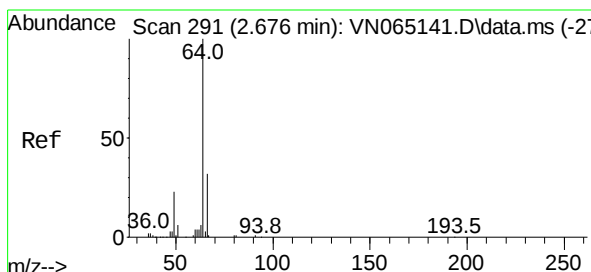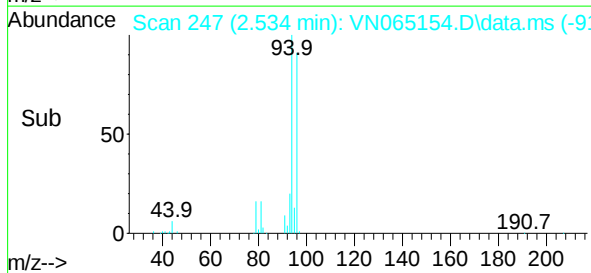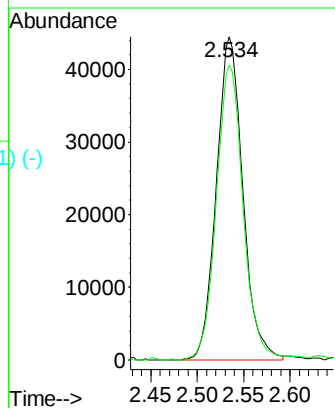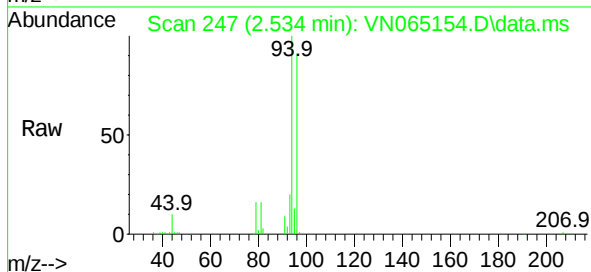

Chloroethane
 Concen: 18.17 ug/l
 RT: 2.676 min Scan# 291
 Delta R.T. 0.000 min
 Lab File: VN065154.D
 Acq: 15 Dec 2020 20:09

Tgt Ion: 64 Resp: 81243
 Ion Ratio Lower Upper
 64 100
 66 34.9 26.0 39.0

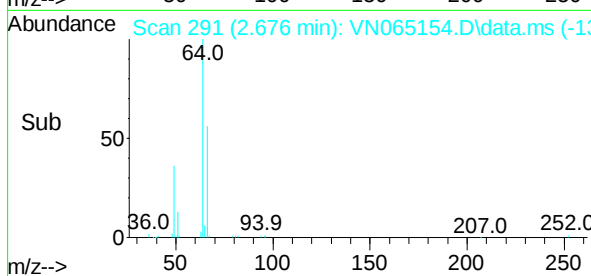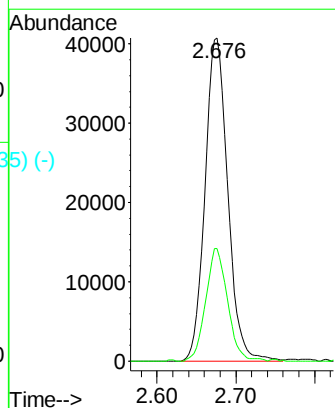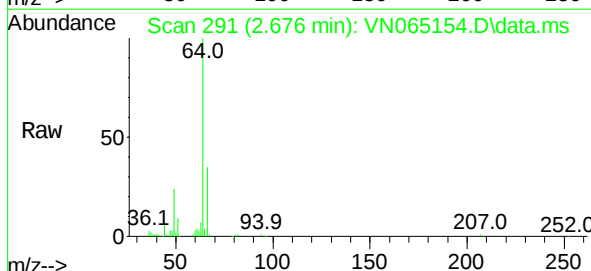

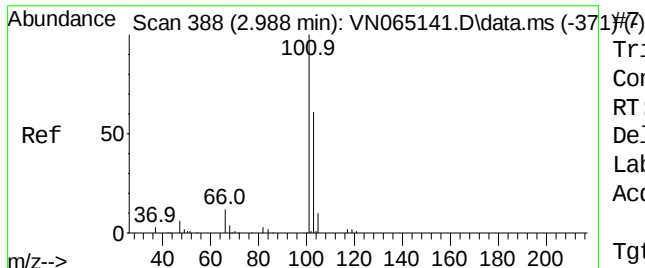





Trichlorofluoromethane
 Concen: 14.98 ug/l
 RT: 2.988 min Scan# 388
 Delta R.T. 0.000 min
 Lab File: VN065154.D
 Acq: 15 Dec 2020 20:09

Instrument :
 MSVOA_N
 ClientSampleId :
 VSTDCCC020EC

Tgt Ion:101 Resp: 166217
 Ion Ratio Lower Upper
 101 100
 103 64.1 49.3 73.9




Manual Integrations
 APPROVED

MMDadoda
 12/16/2020 1:47:38 PM

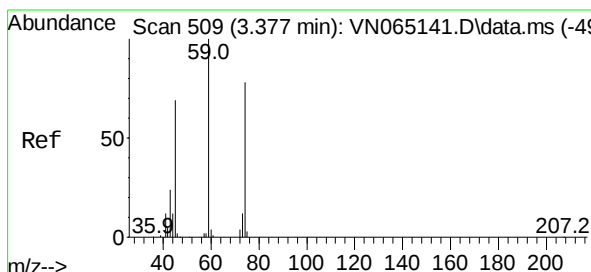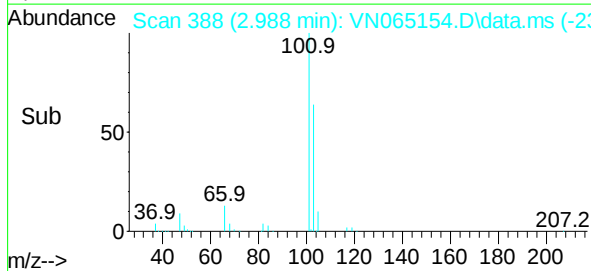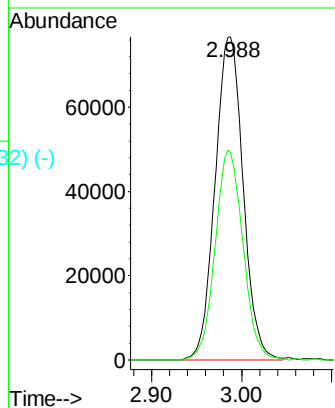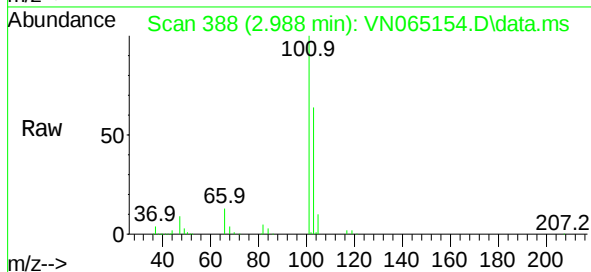




Diethyl Ether
 Concen: 10.44 ug/l
 RT: 3.374 min Scan# 508
 Delta R.T. -0.003 min
 Lab File: VN065154.D
 Acq: 15 Dec 2020 20:09

Tgt Ion: 74 Resp: 37014
 Ion Ratio Lower Upper
 74 100
 45 88.3 22.1 198.5

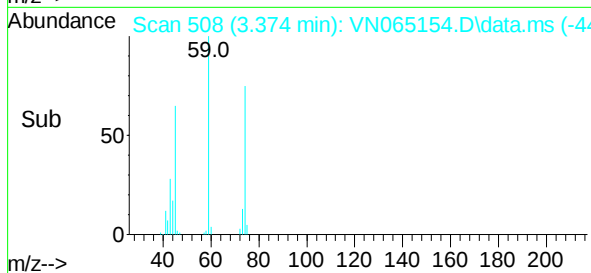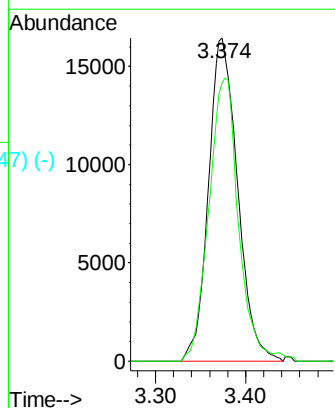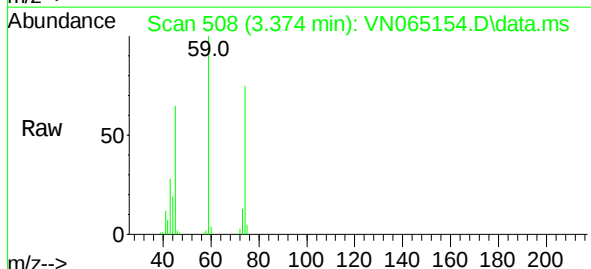


Abundance Scan 676 (3.914 min): VN065141.D\data.ms (-657) #11

Methyl Iodide
Concen: 10.54 ug/l
RT: 3.917 min Scan# 677
Delta R.T. 0.003 min
Lab File: VN065154.D
Acq: 15 Dec 2020 20:09

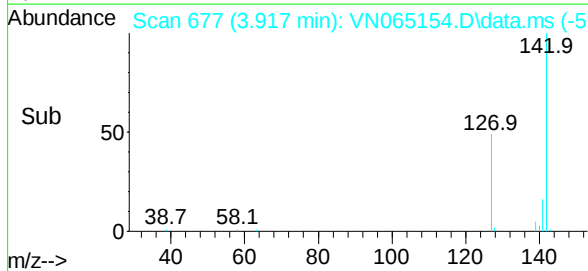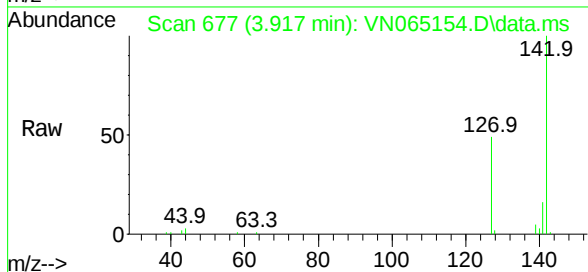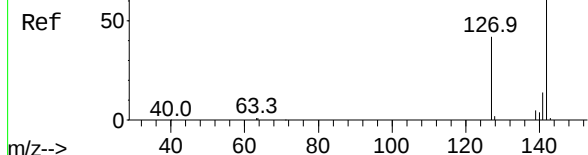

Tgt Ion	Ratio	Lower	Upper
142	100		
127	49.3	24.7	74.1
141	16.4	7.8	23.3

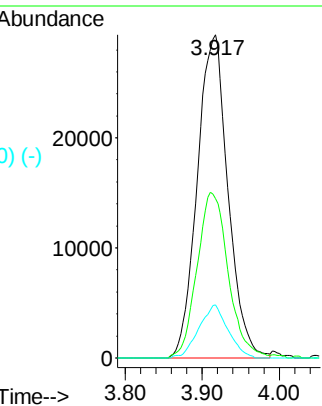




Instrument :
MSVOA_N
ClientSampleId :
VSTDCCC020EC

Manual Integrations
APPROVED

MMDadoda
12/16/2020 1:47:38 PM

Abundance Scan 790 (4.280 min): VN065141.D\data.ms (-770) #12

Methyl Acetate
Concen: 11.41 ug/l
RT: 4.277 min Scan# 789
Delta R.T. -0.003 min
Lab File: VN065154.D
Acq: 15 Dec 2020 20:09

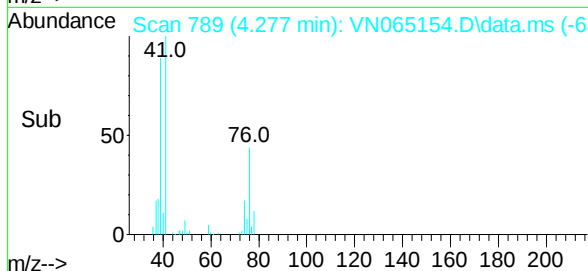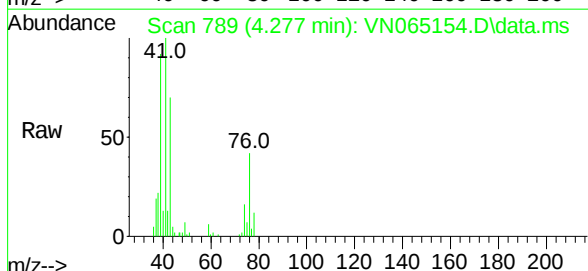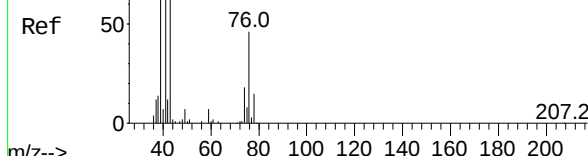

Tgt Ion	Ratio	Lower	Upper
43	100		
74	23.4	17.7	26.5

