

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN121521\  
 Data File : VN070116.D  
 Acq On : 15 Dec 2021 17:09  
 Operator : JC/MD  
 Sample : M4970-14  
 Misc : 5.00mL/MSVOA\_N/WATER  
 ALS Vial : 15 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 SW-3

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N120221W.M

Title : SW846 8260

Signal : TIC: VN070116.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 4.293       | 838           | 859         | 902          | rBV      | 77175          | 261915        | 3.09%           | 0.590%        |
| 2         | 4.591       | 942           | 970         | 995          | rBV      | 64982          | 215637        | 2.54%           | 0.486%        |
| 3         | 8.024       | 2227          | 2250        | 2261         | rBV2     | 871756         | 2113381       | 24.93%          | 4.764%        |
| 4         | 8.086       | 2262          | 2273        | 2303         | rVB      | 1538454        | 3489308       | 41.17%          | 7.866%        |
| 5         | 8.440       | 2382          | 2405        | 2431         | rBV2     | 1074141        | 2607178       | 30.76%          | 5.877%        |
| 6         | 8.968       | 2583          | 2602        | 2652         | rBV      | 2605258        | 5493575       | 64.81%          | 12.384%       |
| 7         | 10.443      | 3132          | 3152        | 3169         | rBV      | 4231468        | 8005024       | 94.44%          | 18.046%       |
| 8         | 11.189      | 3418          | 3430        | 3449         | rBV6     | 51763          | 103751        | 1.22%           | 0.234%        |
| 9         | 11.746      | 3619          | 3638        | 3670         | rBV      | 4638755        | 8476230       | 100.00%         | 19.108%       |
| 10        | 12.733      | 3988          | 4006        | 4037         | rBV      | 3683626        | 6518951       | 76.91%          | 14.696%       |
| 11        | 13.675      | 4342          | 4357        | 4385         | rVB      | 4055230        | 7074928       | 83.47%          | 15.949%       |


Sum of corrected areas: 44359878

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN121521\  
Data File : VN070116.D  
Acq On : 15 Dec 2021 17:09  
Operator : JC/MD  
Sample : M4970-14  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
SW-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N120221W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

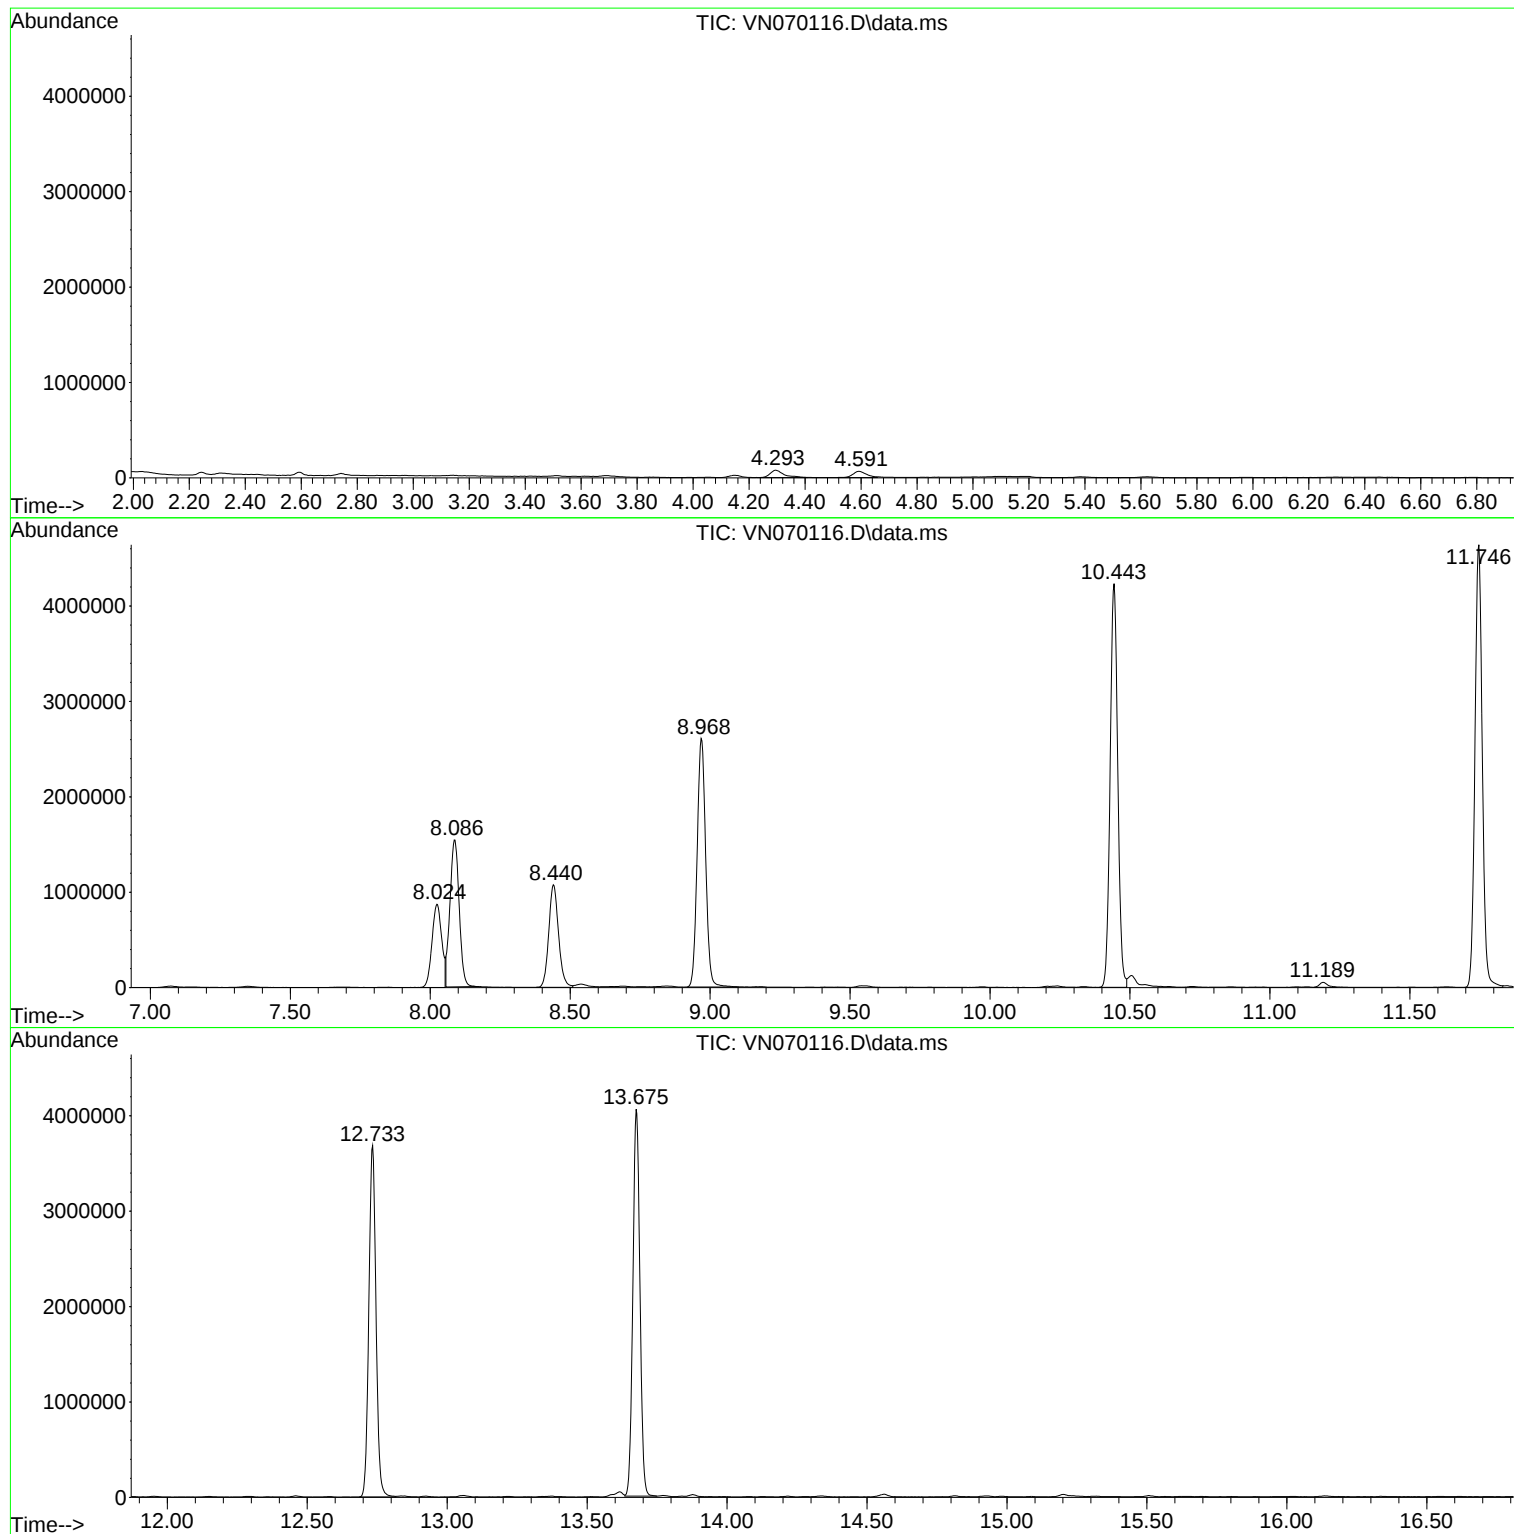

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN121521\  
Data File : VN070116.D  
Acq On : 15 Dec 2021 17:09  
Operator : JC/MD  
Sample : M4970-14  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
SW-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N120221W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN121521\  
Data File : VN070116.D  
Acq On : 15 Dec 2021 17:09  
Operator : JC/MD  
Sample : M4970-14  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
SW-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N120221W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |

-----