


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN121521\  
 Data File : VN070103.D  
 Acq On : 15 Dec 2021 9:42  
 Operator : JC/MD  
 Sample : BFB  
 Misc : 5.00mL/MSVOA\_N/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N120221W.M  
 Title : SW846 8260  
 Last Update : Fri Dec 03 08:46:47 2021

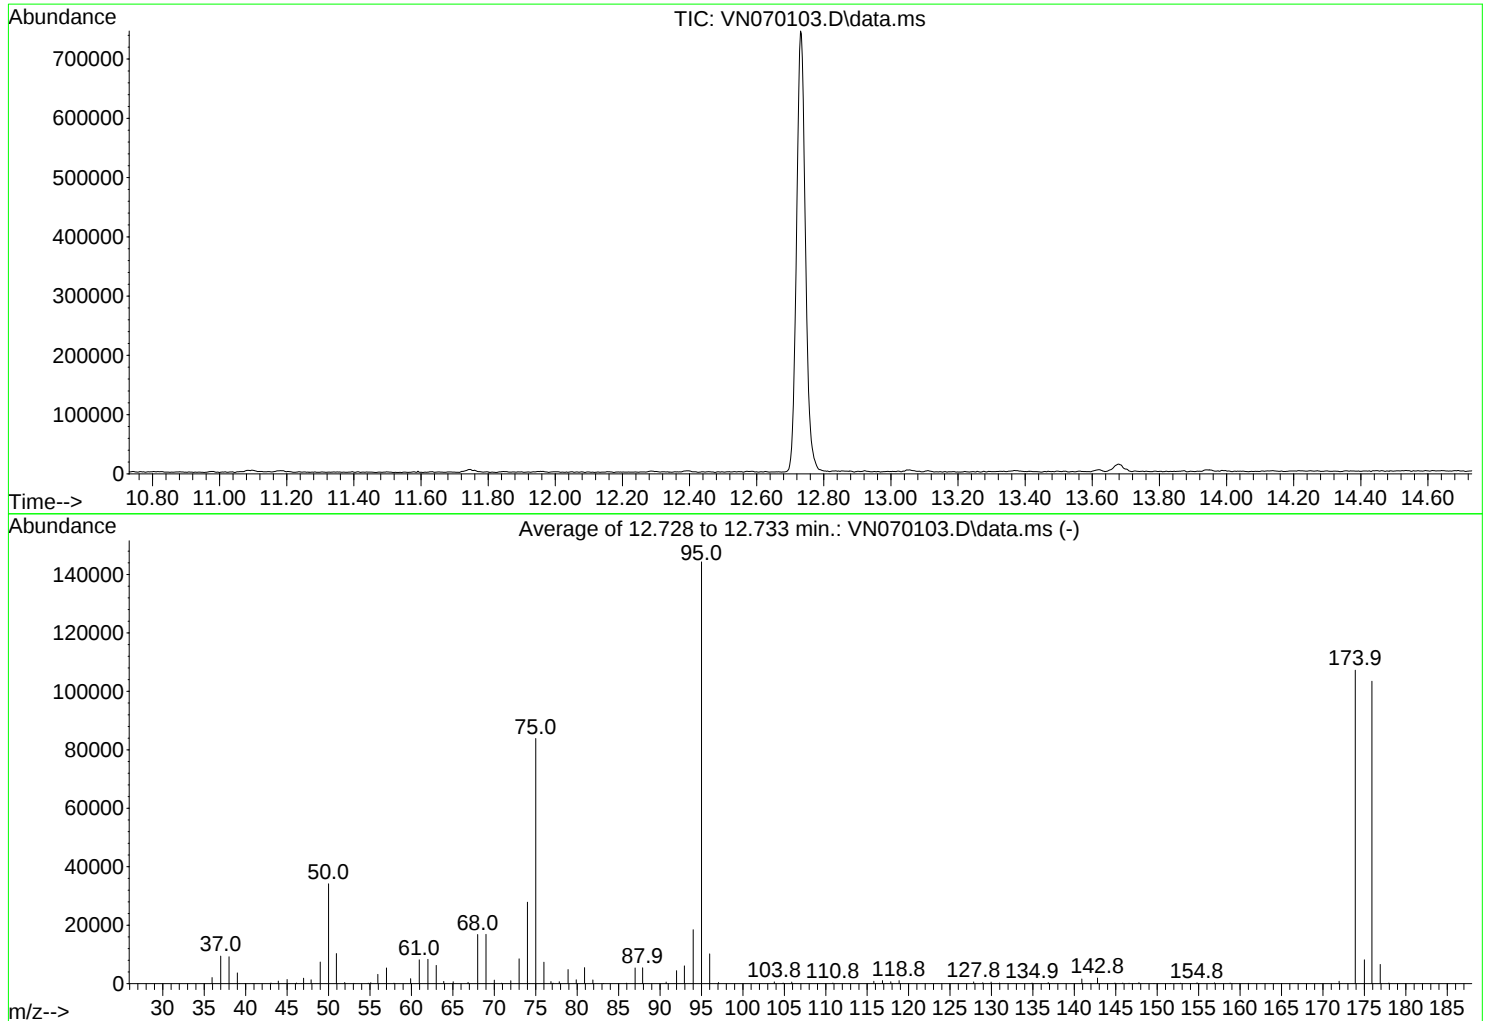

AutoFind: Scans 4004, 4005, 4006; Background Corrected with Scan 3987

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 23.7         | 34157      | PASS                |
| 75             | 95              | 30              | 60              | 58.1         | 83864      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 144320     | PASS                |
| 96             | 95              | 5               | 9               | 7.1          | 10211      | PASS                |
| 173            | 174             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 174            | 95              | 50              | 100             | 74.3         | 107235     | PASS                |
| 175            | 174             | 5               | 9               | 7.6          | 8161       | PASS                |
| 176            | 174             | 95              | 101             | 96.5         | 103491     | PASS                |
| 177            | 176             | 5               | 9               | 6.4          | 6593       | PASS                |