

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121522\
 Data File : VN075829.D
 Acq On : 15 Dec 2022 19:47
 Operator : JC\MD
 Sample : N5990-12DL 40X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 DUP120822DL

Quant Time: Dec 16 03:13:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
 Quant Title : SW846 8260
 QLast Update : Wed Dec 14 13:03:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.235	168	360507	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	558260	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	481814	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	216972	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.588	65	182477	46.527	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	93.060%		
35) Dibromofluoromethane	8.177	113	167031	48.314	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	96.620%		
50) Toluene-d8	10.570	98	648679	50.183	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	100.360%		
62) 4-Bromofluorobenzene	12.853	95	208415	48.680	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	97.360%		
Target Compounds					Qvalue	
16) Acetone	4.459	43	346	0.256	ug/l #	39
18) Methyl Acetate	5.294	43	2442	0.611	ug/l #	45
20) Methylene Chloride	5.294	84	1659	Below Cal	#	78
25) 2-Butanone	7.341	43	783	0.414	ug/l #	40
31) Cyclohexane	8.235	56	12931	2.302	ug/l #	41
36) 1,1-Dichloropropene	8.229	75	24609	5.358	ug/l #	51
37) Ethyl Acetate	7.341	43	783	0.212	ug/l #	73
38) Carbon Tetrachloride	8.229	117	35005	6.810	ug/l #	16
39) Methylcyclohexane	9.606	83	6648	1.200	ug/l	94
40) Benzene	8.612	78	19332	1.364	ug/l	97
48) Methyl methacrylate	9.606	41	1924	0.702	ug/l #	73
52) Toluene	10.641	92	3407	0.369	ug/l	99
67) Ethyl Benzene	11.964	91	847446	50.775	ug/l	99
68) m/p-Xylenes	12.076	106	302979	45.864	ug/l	97
69) o-Xylene	12.400	106	142625	21.817	ug/l	99
70) Styrene	12.400	104	7158	0.689	ug/l #	1
71) Bromoform	12.853	173	1502	0.564	ug/l #	1
73) Isopropylbenzene	12.700	105	46065	2.938	ug/l	98
76) 1,2,3-Trichloropropane	12.853	75	105717	24.171	ug/l #	1
78) n-propylbenzene	13.041	91	138679	8.019	ug/l	97
79) 2-Chlorotoluene	13.135	91	18358	1.701	ug/l #	40
80) 1,3,5-Trimethylbenzene	13.176	105	111567	8.502	ug/l	94
81) trans-1,4-Dichloro-2-b...	12.853	75	105717	87.005	ug/l #	12
82) 4-Chlorotoluene	13.135	91	18358	1.701	ug/l #	40
83) tert-Butylbenzene	13.482	119	73998	6.396	ug/l #	65
84) 1,2,4-Trimethylbenzene	13.488	105	609195	46.795	ug/l	100
85) sec-Butylbenzene	13.488	105	609195	38.147	ug/l #	56
86) p-Isopropyltoluene	13.735	119	2855	0.215	ug/l #	68
89) n-Butylbenzene	14.058	91	5573	0.518	ug/l #	72
90) Hexachloroethane	14.335	117	6660	2.802	ug/l #	11
95) Naphthalene	15.647	128	190301	17.591	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121522\
Data File : VN075829.D
Acq On : 15 Dec 2022 19:47
Operator : JC\MD
Sample : N5990-12DL 40X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
DUP120822DL

Quant Time: Dec 16 03:13:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
Quant Title : SW846 8260
QLast Update : Wed Dec 14 13:03:41 2022
Response via : Initial Calibration




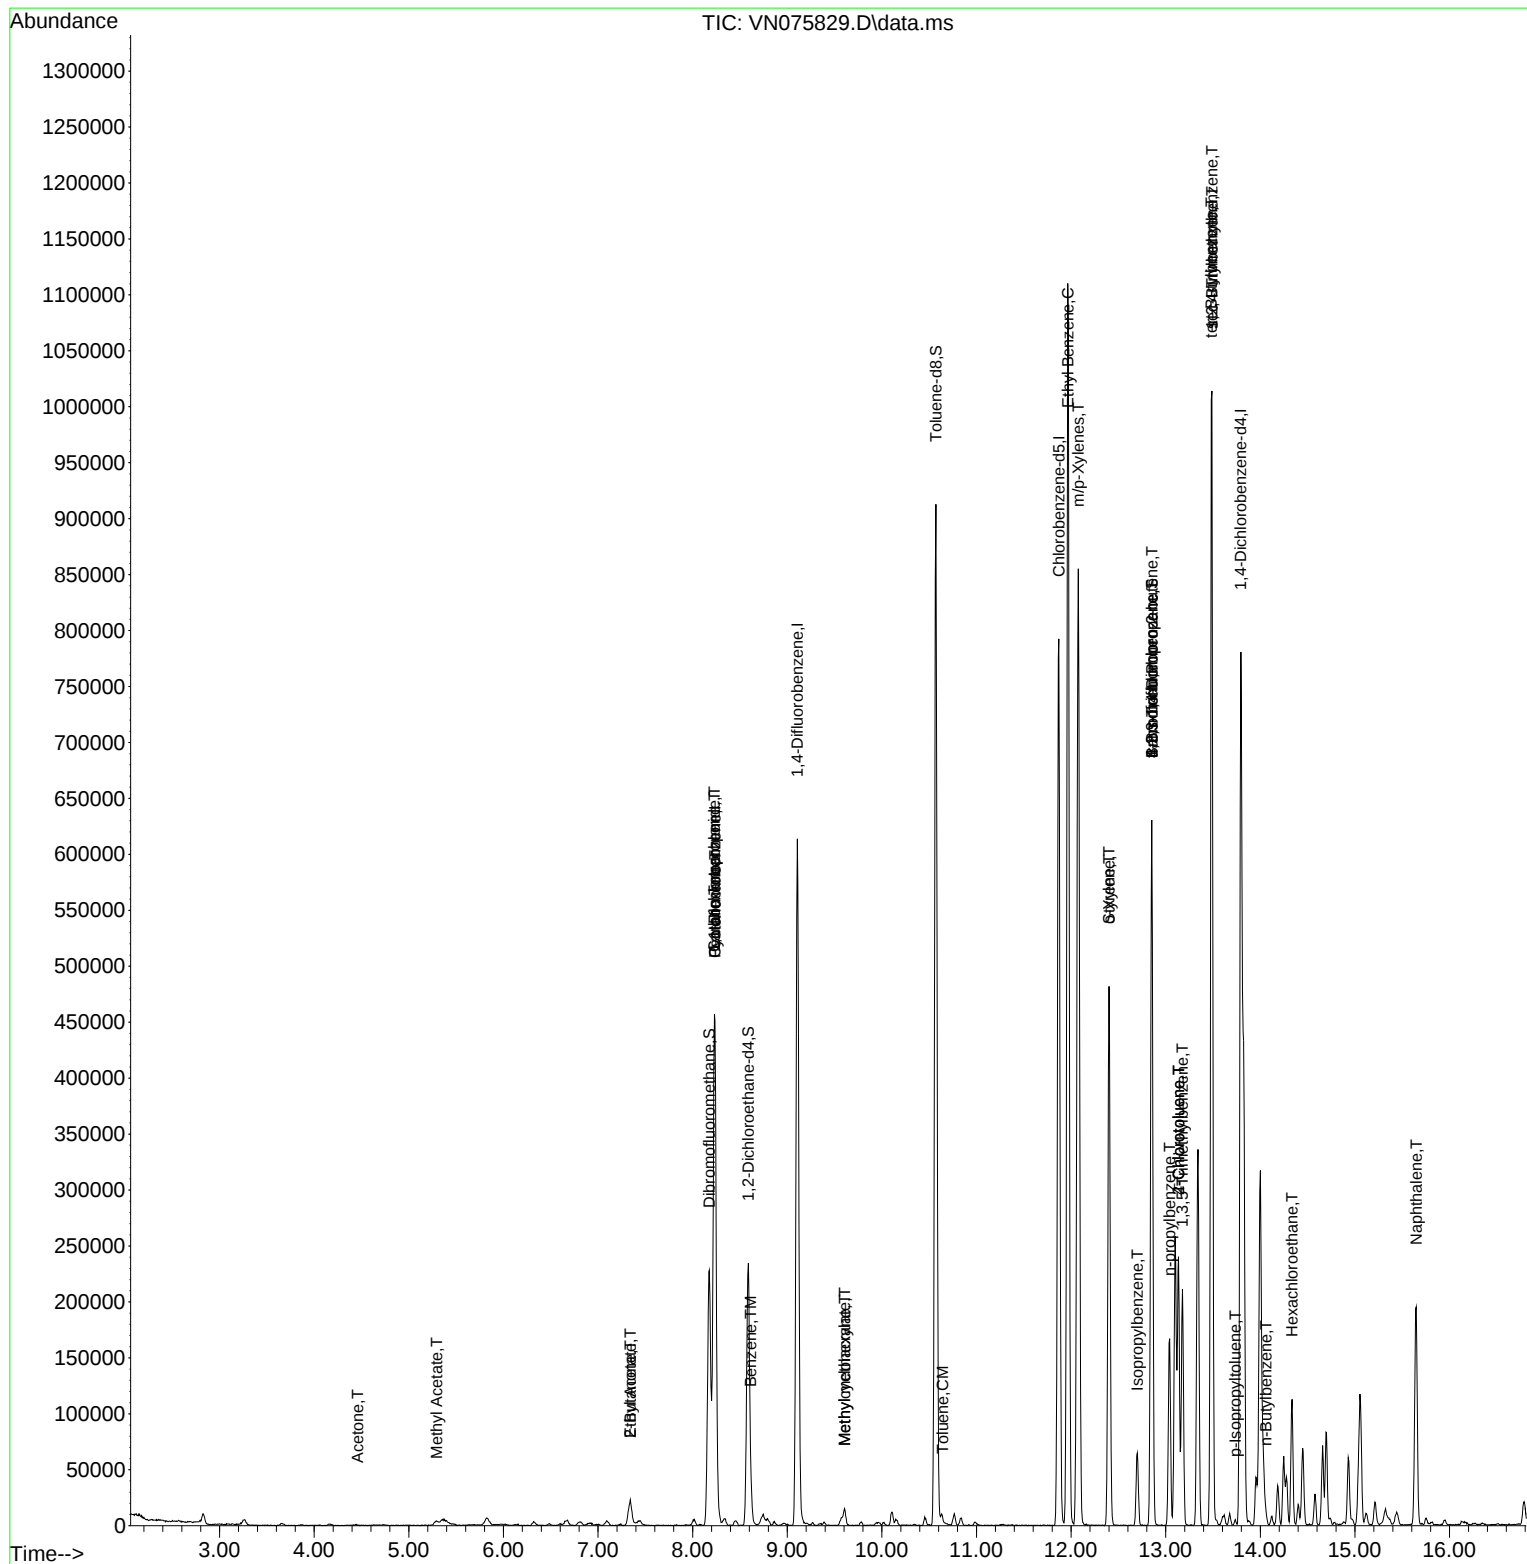




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.235 min Scan# 1050
Delta R.T. 0.005 min
Lab File: VN075829.D
Acq: 15 Dec 2022 19:47




Instrument :
MSVOA_N
ClientSampleId :
DUP120822DL


Tgt Ion:168 Resp: 360507
Ion Ratio Lower Upper
168 100
99 54.2 44.2 66.4

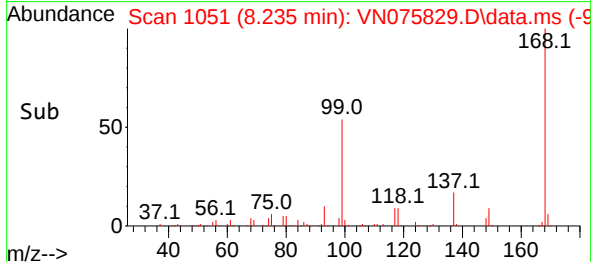

#16
Acetone
Concen: 0.256 ug/l
RT: 4.459 min Scan# 409
Delta R.T. 0.017 min
Lab File: VN075829.D
Acq: 15 Dec 2022 19:47

Tgt Ion: 43 Resp: 346
Ion Ratio Lower Upper
43 100
58 0.0 28.6 43.0#


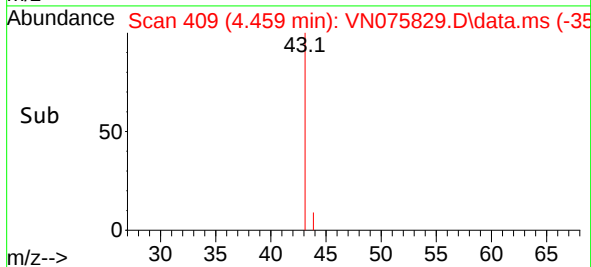

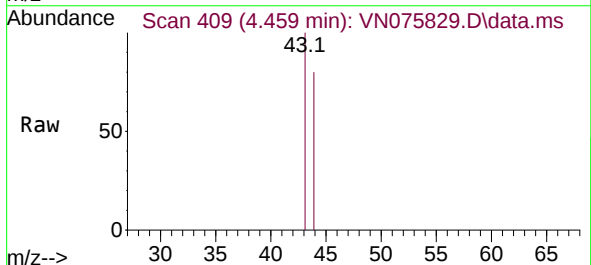


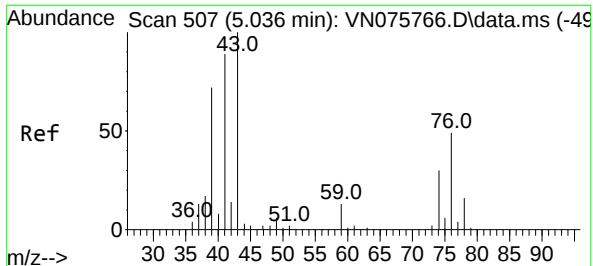

#18
Methyl Acetate
Concen: 0.611 ug/l
RT: 5.294 min Scan# 511
Delta R.T. 0.259 min
Lab File: VN075829.D
Acq: 15 Dec 2022 19:47




Instrument :
MSVOA_N
ClientSampleId :
DUP120822DL


Tgt Ion: 43 Resp: 2442
Ion Ratio Lower Upper
43 100
74 0.0 23.6 35.4#

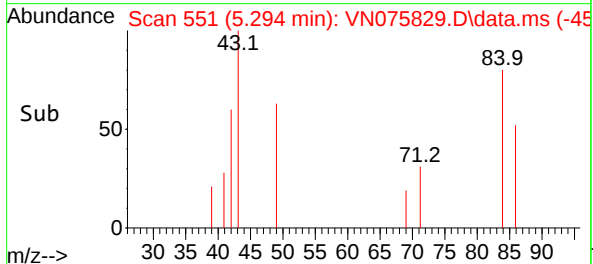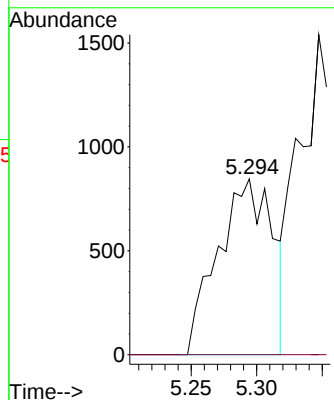

#25
2-Butanone
Concen: 0.414 ug/l
RT: 7.341 min Scan# 899
Delta R.T. -0.147 min
Lab File: VN075829.D
Acq: 15 Dec 2022 19:47


Tgt Ion: 43 Resp: 783
Ion Ratio Lower Upper
43 100
72 0.0 28.0 42.0#

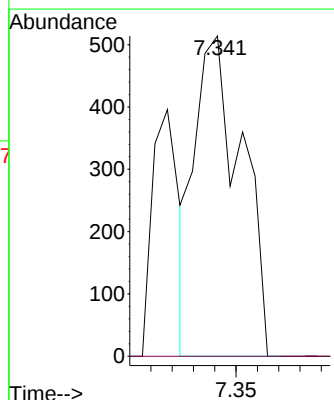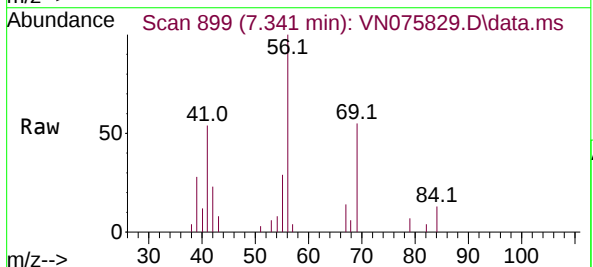



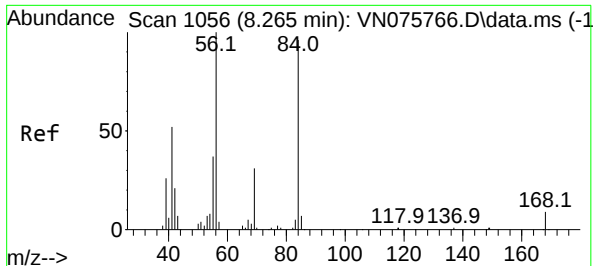


#31
Cyclohexane
Concen: 2.302 ug/l
RT: 8.235 min Scan# 1051
Delta R.T. -0.030 min
Lab File: VN075829.D
Acq: 15 Dec 2022 19:47

Instrument :
MSVOA_N
ClientSampleId :
DUP120822DL



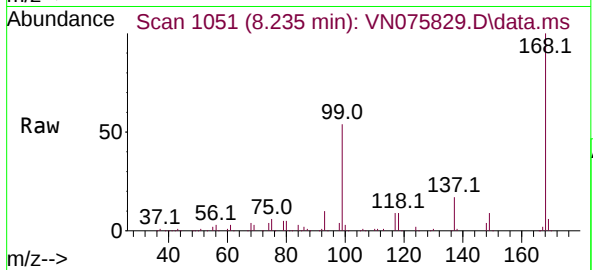



Tgt Ion: 56 Resp: 12931
Ion Ratio Lower Upper
56 100
69 113.4 24.7 37.1#
84 124.9 76.5 114.7#

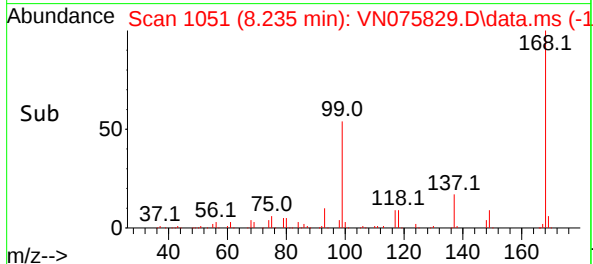

#33
1,2-Dichloroethane-d4
Concen: 46.527 ug/l
RT: 8.588 min Scan# 1111
Delta R.T. 0.006 min
Lab File: VN075829.D
Acq: 15 Dec 2022 19:47

Tgt Ion: 65 Resp: 182477
Ion Ratio Lower Upper
65 100
67 51.9 0.0 103.4

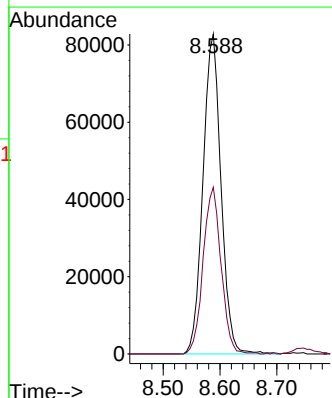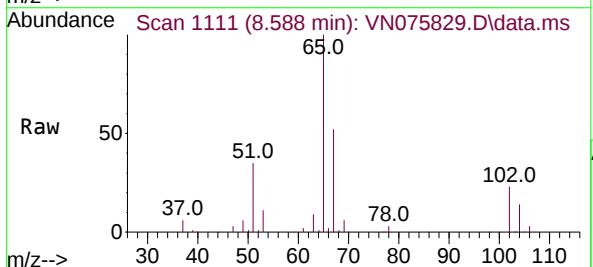

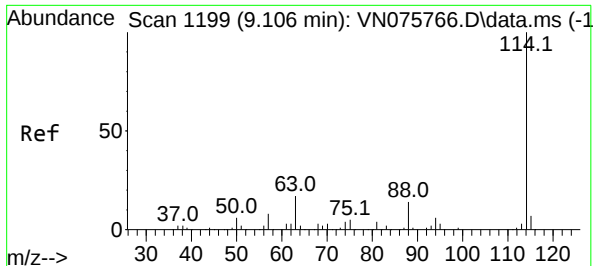

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1199

Delta R.T. -0.000 min

Lab File: VN075829.D

Acq: 15 Dec 2022 19:47

Instrument :

MSVOA_N

ClientSampleId :

DUP120822DL





Tgt Ion:114 Resp: 558260

Ion Ratio Lower Upper

114 100

63 17.4 0.0 34.4

88 15.1 0.0 28.8

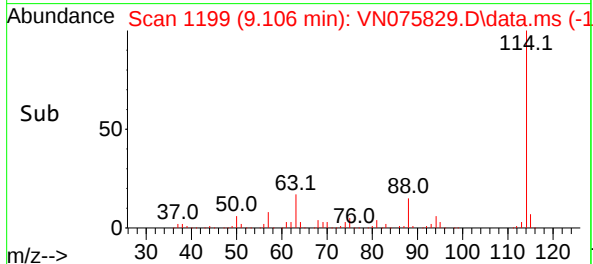

#35

Dibromofluoromethane

Concen: 48.314 ug/l

RT: 8.177 min Scan# 1041

Delta R.T. 0.006 min

Lab File: VN075829.D

Acq: 15 Dec 2022 19:47




Tgt Ion:113 Resp: 167031


Ion Ratio Lower Upper

113 100

111 101.9 83.4 125.2

192 19.7 16.1 24.1

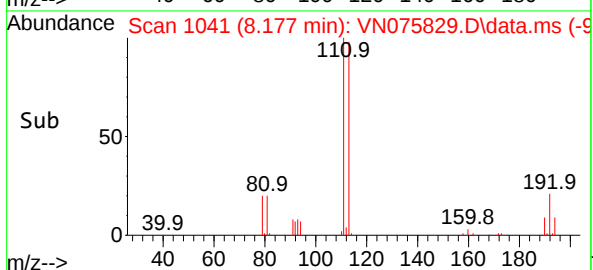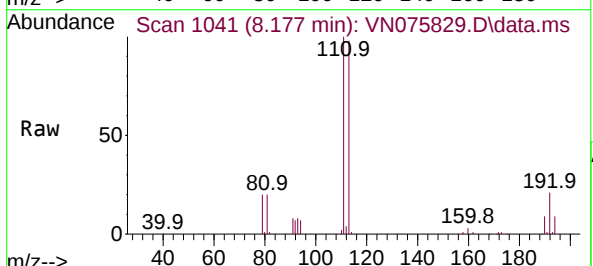

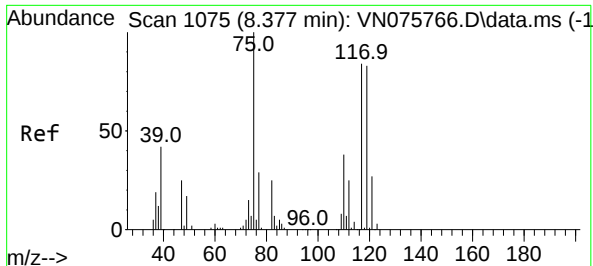

#36

1,1-Dichloropropene

Concen: 5.358 ug/l

RT: 8.229 min Scan# 1050

Delta R.T. -0.147 min

Lab File: VN075829.D

Acq: 15 Dec 2022 19:47

Instrument :

MSVOA_N

ClientSampleId :

DUP120822DL





Tgt Ion: 75 Resp: 24609

Ion Ratio Lower Upper

75 100

110 10.8 18.8 56.4#

77 0.0 24.1 36.1#

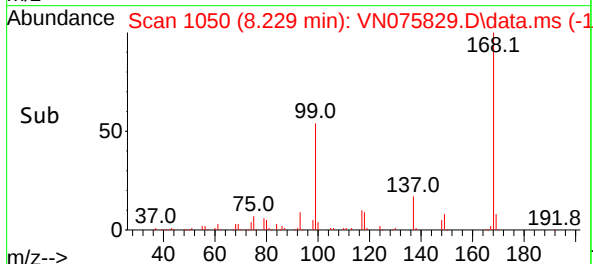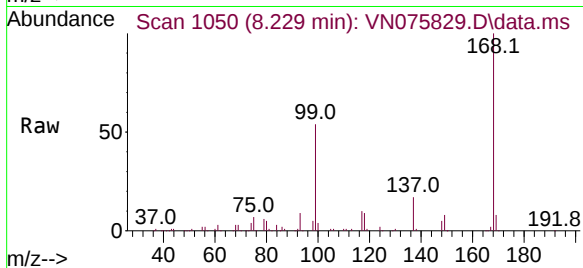

#37

Ethyl Acetate

Concen: 0.212 ug/l

RT: 7.341 min Scan# 899

Delta R.T. -0.224 min

Lab File: VN075829.D

Acq: 15 Dec 2022 19:47




Tgt Ion: 43 Resp: 783


Ion Ratio Lower Upper

43 100

61 0.0 13.0 19.4#

70 7.5 9.4 14.0#


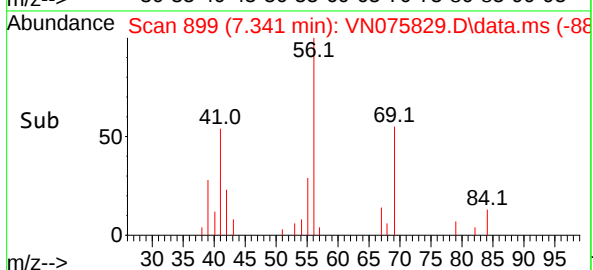

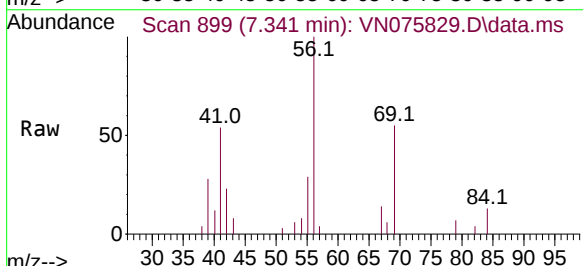




#38
Carbon Tetrachloride
Concen: 6.810 ug/l
RT: 8.229 min Scan# 1050
Delta R.T. -0.135 min
Lab File: VN075829.D
Acq: 15 Dec 2022 19:47




Instrument :
MSVOA_N
ClientSampleId :
DUP120822DL


Tgt Ion:117 Resp: 35005
Ion Ratio Lower Upper
117 100
119 4.9 76.1 114.1#
121 0.0 24.5 36.7#

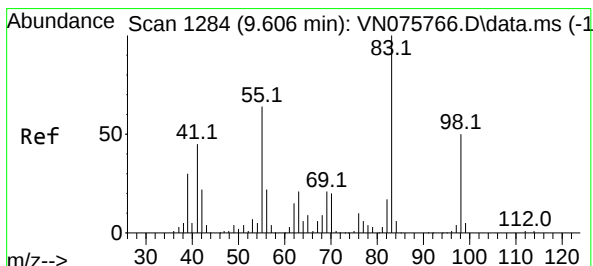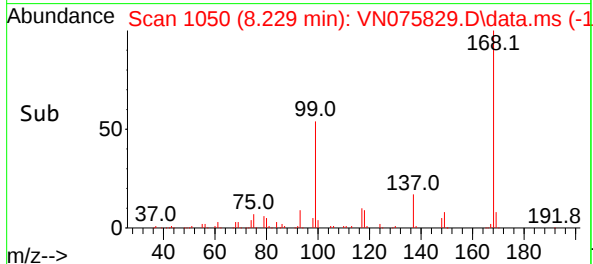

#39
Methylcyclohexane
Concen: 1.200 ug/l
RT: 9.606 min Scan# 1284
Delta R.T. -0.000 min
Lab File: VN075829.D
Acq: 15 Dec 2022 19:47

Tgt Ion: 83 Resp: 6648
Ion Ratio Lower Upper
83 100
55 72.5 51.4 77.0
98 49.7 39.8 59.8


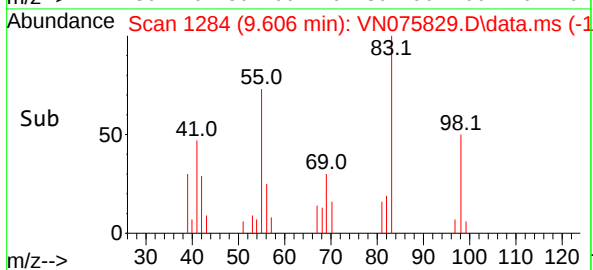

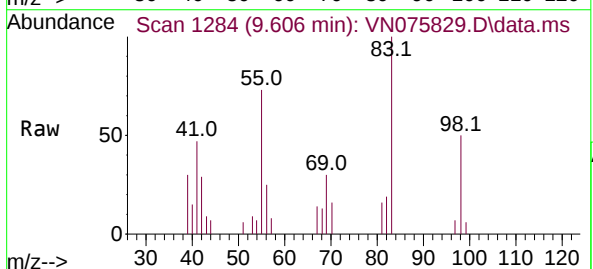


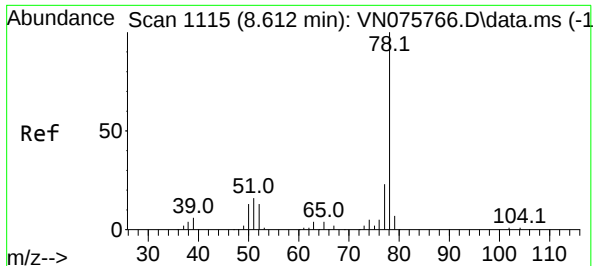

#40
Benzene
Concen: 1.364 ug/l
RT: 8.612 min Scan# 1115
Delta R.T. -0.000 min
Lab File: VN075829.D
Acq: 15 Dec 2022 19:47




Instrument :
MSVOA_N
ClientSampleId :
DUP120822DL


Tgt Ion: 78 Resp: 19332
Ion Ratio Lower Upper
78 100
77 24.6 18.5 27.7

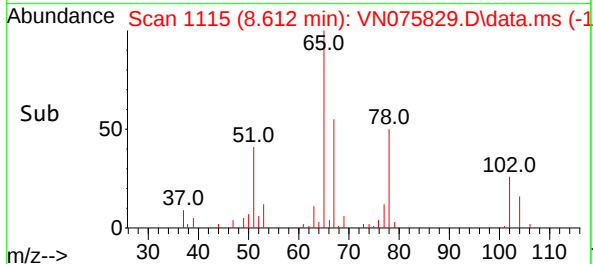

#48
Methyl methacrylate
Concen: 0.702 ug/l
RT: 9.606 min Scan# 1284
Delta R.T. -0.077 min
Lab File: VN075829.D
Acq: 15 Dec 2022 19:47

Tgt Ion: 41 Resp: 1924
Ion Ratio Lower Upper
41 100
69 119.6 81.9 122.9
39 97.8 51.6 77.4#


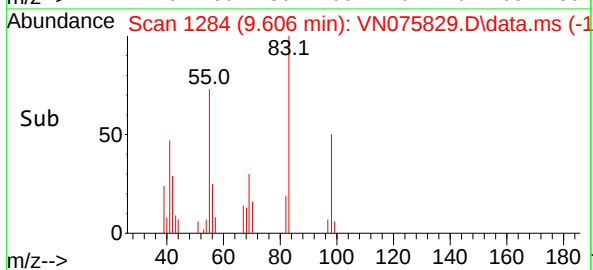

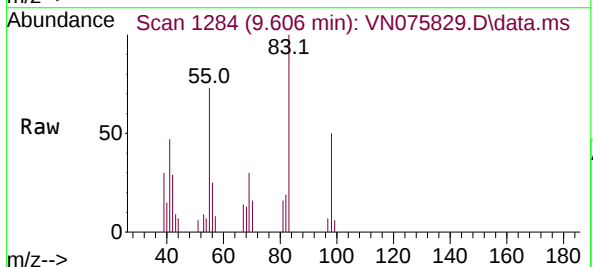




#50
Toluene-d8
Concen: 50.183 ug/l
RT: 10.570 min Scan# 1448
Delta R.T. -0.000 min
Lab File: VN075829.D
Acq: 15 Dec 2022 19:47




Instrument :
MSVOA_N
ClientSampleId :
DUP120822DL


Tgt Ion: 98 Resp: 648679
Ion Ratio Lower Upper
98 100
100 65.2 52.1 78.1

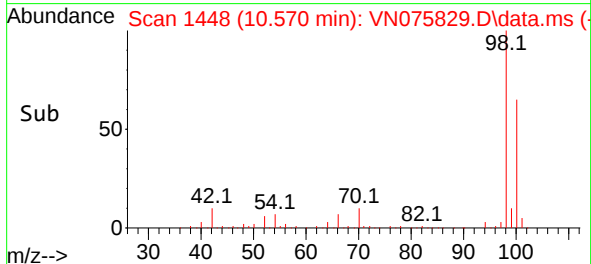

#52
Toluene
Concen: 0.369 ug/l
RT: 10.641 min Scan# 1460
Delta R.T. 0.006 min
Lab File: VN075829.D
Acq: 15 Dec 2022 19:47

Tgt Ion: 92 Resp: 3407
Ion Ratio Lower Upper
92 100
91 172.7 137.3 205.9

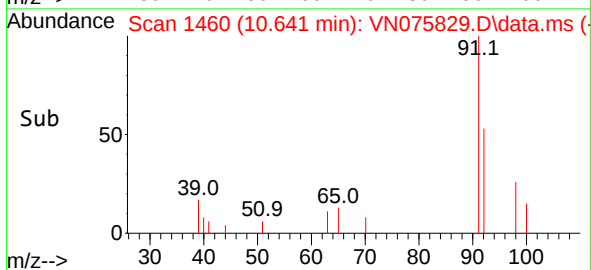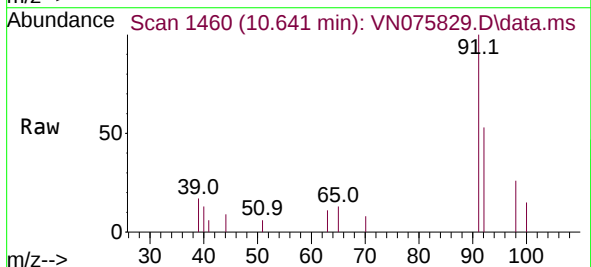



#62

4-Bromofluorobenzene

Concen: 48.680 ug/l

RT: 12.853 min Scan# 1836

Delta R.T. -0.000 min

Lab File: VN075829.D

Acq: 15 Dec 2022 19:47

Instrument :

MSVOA_N

ClientSampleId :

DUP120822DL





Tgt Ion: 95 Resp: 208415

Ion Ratio Lower Upper

95 100

174 87.0 0.0 171.6

176 83.8 0.0 169.2

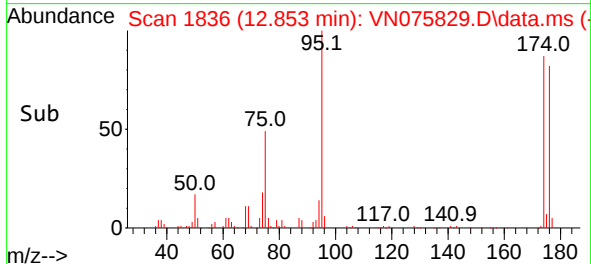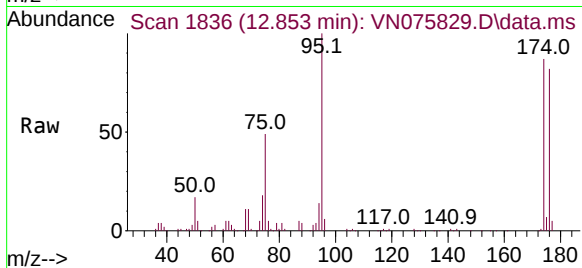

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.870 min Scan# 1669

Delta R.T. 0.006 min

Lab File: VN075829.D

Acq: 15 Dec 2022 19:47




Tgt Ion: 117 Resp: 481814


Ion Ratio Lower Upper

117 100

82 53.6 41.3 61.9

119 32.6 24.6 37.0


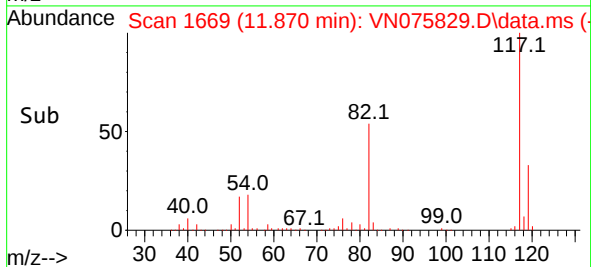

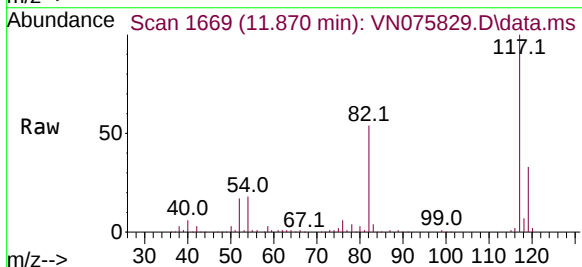


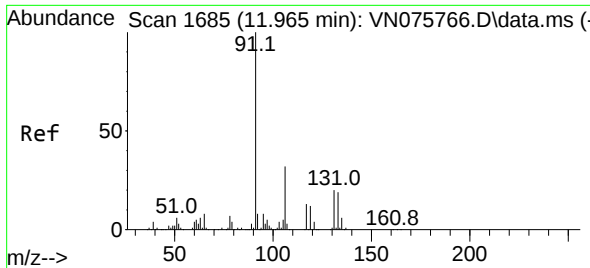

#67
Ethyl Benzene
Concen: 50.775 ug/l
RT: 11.964 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN075829.D
Acq: 15 Dec 2022 19:47




Instrument :
MSVOA_N
ClientSampleId :
DUP120822DL


Tgt Ion: 91 Resp: 847446
Ion Ratio Lower Upper
91 100
106 31.7 25.7 38.5

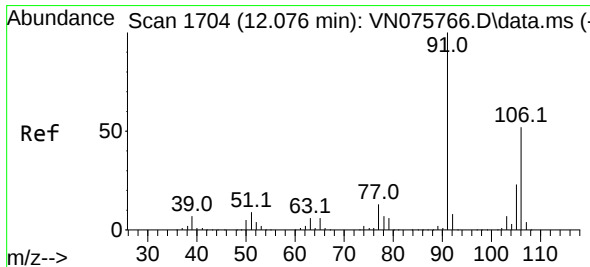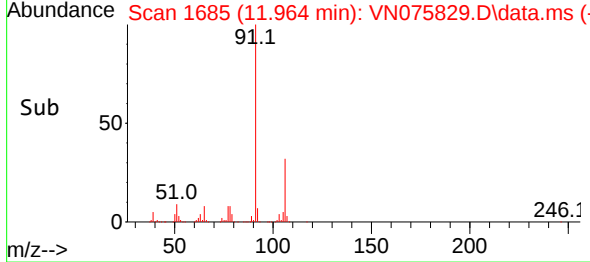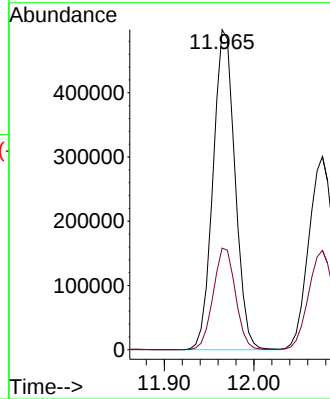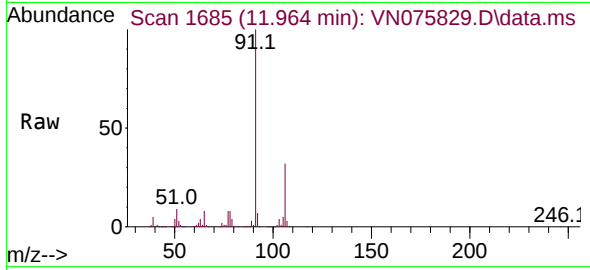

#68
m/p-Xylenes
Concen: 45.864 ug/l
RT: 12.076 min Scan# 1704
Delta R.T. -0.000 min
Lab File: VN075829.D
Acq: 15 Dec 2022 19:47

Tgt Ion: 106 Resp: 302979
Ion Ratio Lower Upper
106 100
91 192.0 156.6 235.0


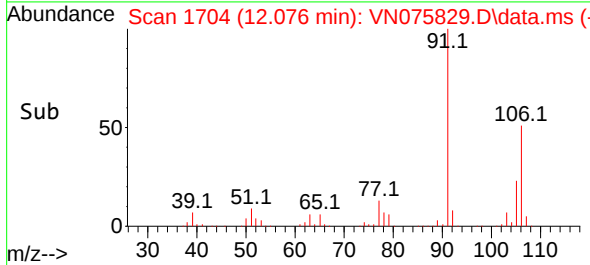

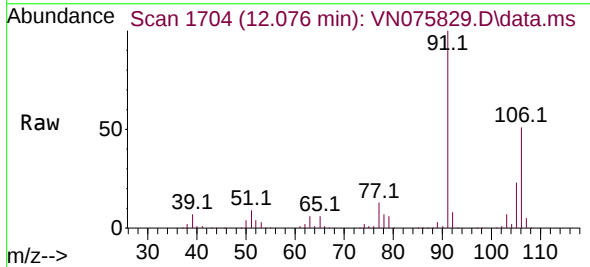




#69
o-Xylene
Concen: 21.817 ug/l
RT: 12.400 min Scan# 1759
Delta R.T. -0.000 min
Lab File: VN075829.D
Acq: 15 Dec 2022 19:47




Instrument :
MSVOA_N
ClientSampleId :
DUP120822DL


Tgt Ion:106 Resp: 142625
Ion Ratio Lower Upper
106 100
91 209.3 103.8 311.6

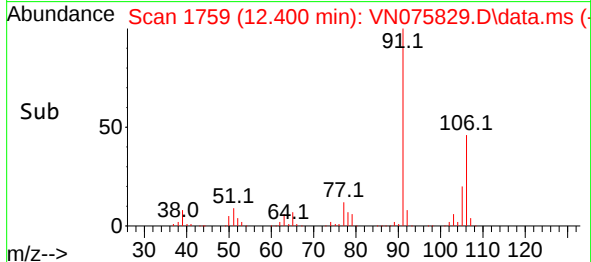

#70
Styrene
Concen: 0.689 ug/l
RT: 12.400 min Scan# 1759
Delta R.T. -0.012 min
Lab File: VN075829.D
Acq: 15 Dec 2022 19:47

Tgt Ion:104 Resp: 7158
Ion Ratio Lower Upper
104 100
78 295.9 37.5 56.3#
103 273.7 43.5 65.3#

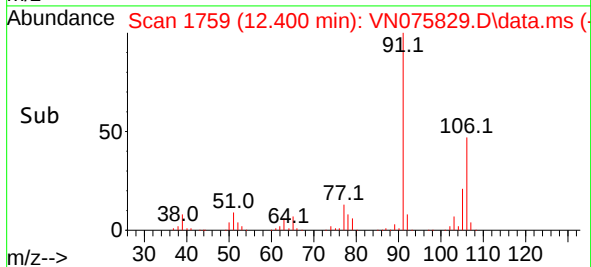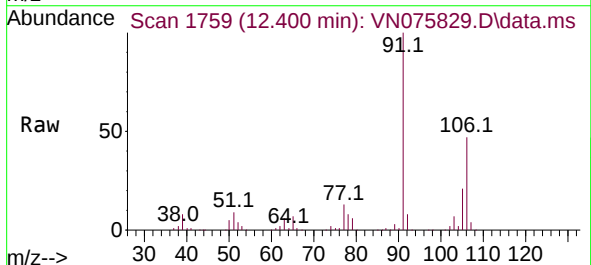



#71

Bromoform

Concen: 0.564 ug/l

RT: 12.853 min Scan# 1836

Delta R.T. 0.270 min

Lab File: VN075829.D

Acq: 15 Dec 2022 19:47

Instrument :

MSVOA_N

ClientSampleId :

DUP120822DL





Tgt Ion:173 Resp: 1502

Ion Ratio Lower Upper

173 100

175 718.7 24.3 72.8#

254 0.0 0.0 0.0

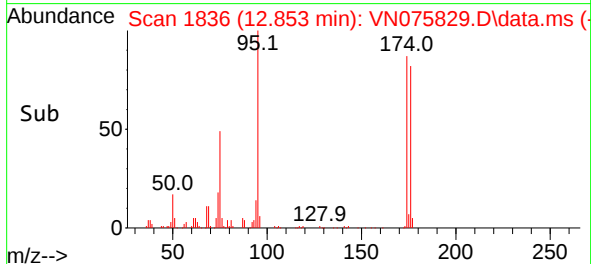

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.794 min Scan# 1996

Delta R.T. -0.000 min

Lab File: VN075829.D

Acq: 15 Dec 2022 19:47




Tgt Ion:152 Resp: 216972


Ion Ratio Lower Upper

152 100

115 62.6 29.1 87.4

150 156.8 0.0 347.0

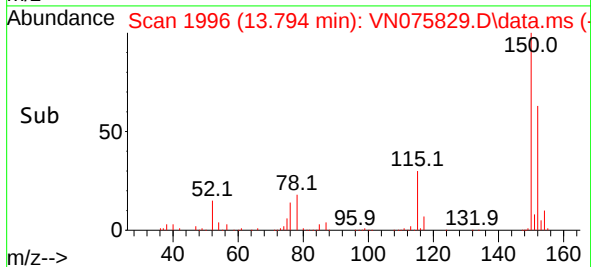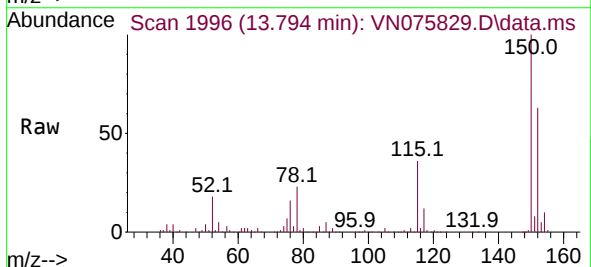



#73

Isopropylbenzene

Concen: 2.938 ug/l

RT: 12.700 min Scan# 11

Delta R.T. -0.000 min

Lab File: VN075829.D

Acq: 15 Dec 2022 19:47

Instrument :

MSVOA_N

ClientSampleId :





DUP120822DL

Tgt Ion:105 Resp: 46065

Ion Ratio Lower Upper

105 100

120 25.7 13.4 40.2

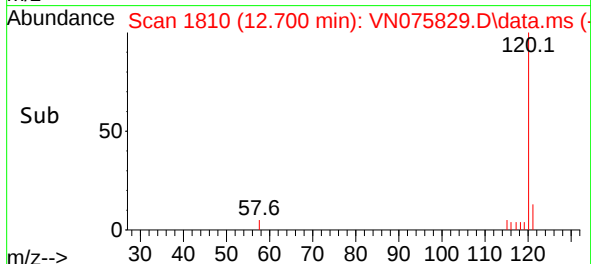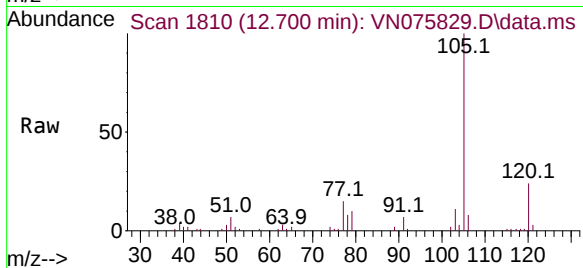

#76

1,2,3-Trichloropropane

Concen: 24.171 ug/l

RT: 12.853 min Scan# 1836

Delta R.T. -0.141 min

Lab File: VN075829.D




Acq: 15 Dec 2022 19:47


Tgt Ion: 75 Resp: 105717

Ion Ratio Lower Upper

75 100

77 1.4 82.6 247.8#


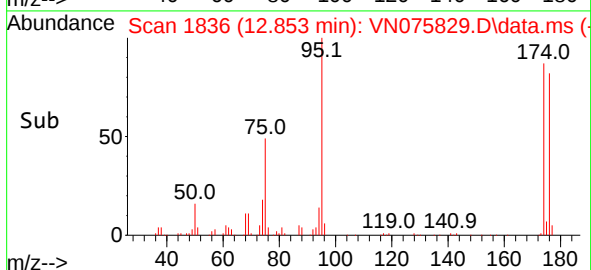

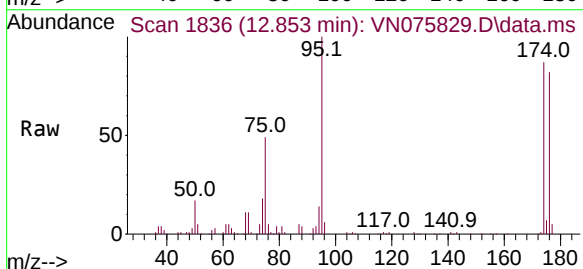




#78
n-propylbenzene
Concen: 8.019 ug/l
RT: 13.041 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VN075829.D
Acq: 15 Dec 2022 19:47




Instrument :
MSVOA_N
ClientSampleId :
DUP120822DL


Tgt Ion: 91 Resp: 138679
Ion Ratio Lower Upper
91 100
120 22.9 12.0 36.1

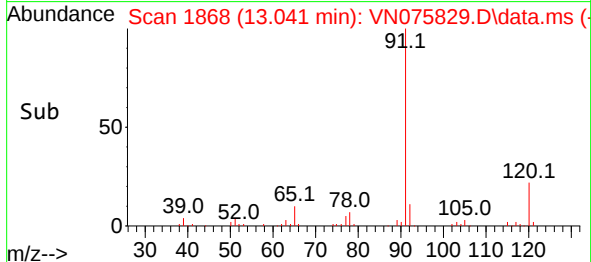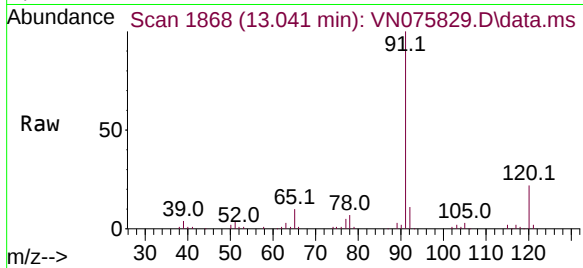

#79
2-Chlorotoluene
Concen: 1.701 ug/l
RT: 13.135 min Scan# 1884
Delta R.T. 0.006 min
Lab File: VN075829.D
Acq: 15 Dec 2022 19:47

Tgt Ion: 91 Resp: 18358
Ion Ratio Lower Upper
91 100
126 0.0 17.5 52.5#

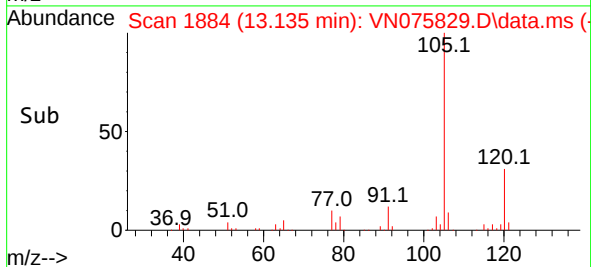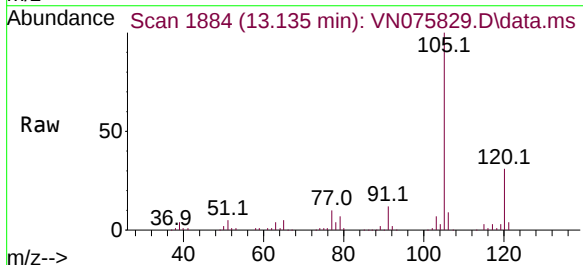



#80

1,3,5-Trimethylbenzene

Concen: 8.502 ug/l

RT: 13.176 min Scan# 1891

Delta R.T. -0.000 min

Lab File: VN075829.D

Acq: 15 Dec 2022 19:47

Instrument :

MSVOA_N

ClientSampleId :





DUP120822DL

Tgt Ion:105 Resp: 111567

Ion Ratio Lower Upper

105 100

120 53.6 24.7 74.1



#81

trans-1,4-Dichloro-2-butene

Concen: 87.005 ug/l

RT: 12.853 min Scan# 1836

Delta R.T. 0.112 min

Lab File: VN075829.D

Acq: 15 Dec 2022 19:47




Tgt Ion: 75 Resp: 105717


Ion Ratio Lower Upper

75 100

53 0.0 73.8 110.6#

89 0.1 39.5 59.3#


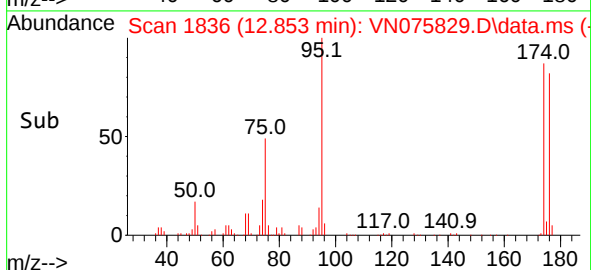






#82
4-Chlorotoluene
Concen: 1.701 ug/l
RT: 13.135 min Scan# 1884
Delta R.T. 0.006 min
Lab File: VN075829.D
Acq: 15 Dec 2022 19:47




Instrument :
MSVOA_N
ClientSampleId :
DUP120822DL


Tgt Ion: 91 Resp: 18358
Ion Ratio Lower Upper
91 100
126 0.0 17.5 52.5#

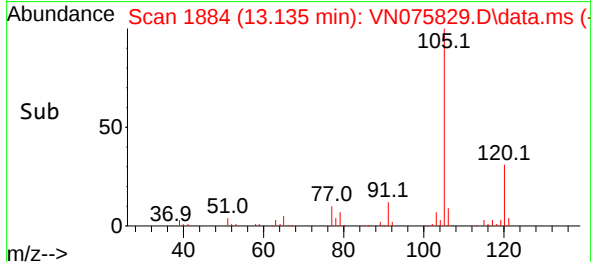

#83
tert-Butylbenzene
Concen: 6.396 ug/l
RT: 13.482 min Scan# 1943
Delta R.T. 0.041 min
Lab File: VN075829.D
Acq: 15 Dec 2022 19:47

Tgt Ion: 119 Resp: 73998
Ion Ratio Lower Upper
119 100
91 85.0 31.9 95.5
134 0.0 13.8 41.4#


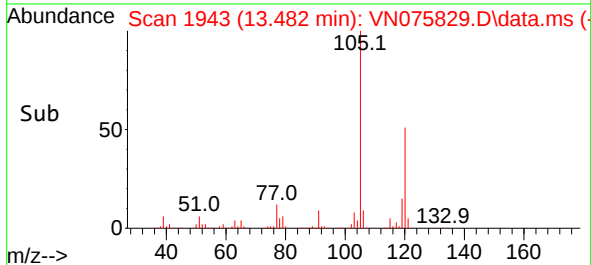

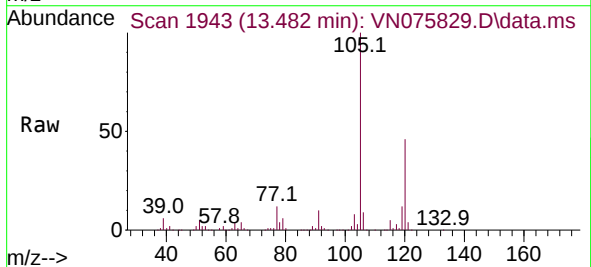




#84
1,2,4-Trimethylbenzene
Concen: 46.795 ug/l
RT: 13.488 min Scan# 1944
Delta R.T. 0.006 min
Lab File: VN075829.D
Acq: 15 Dec 2022 19:47




Instrument :
MSVOA_N
ClientSampleId :
DUP120822DL


Tgt Ion:105 Resp: 609195
Ion Ratio Lower Upper
105 100
120 46.6 23.3 69.8

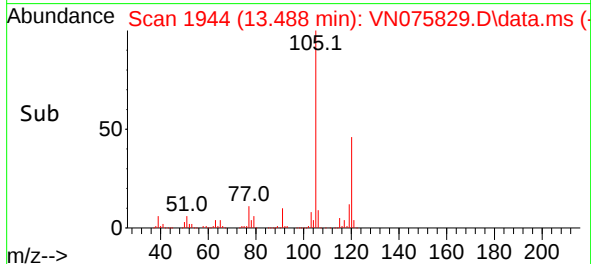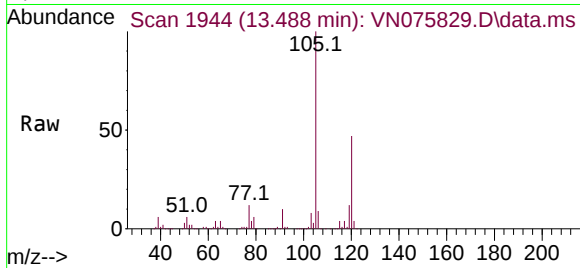

#85
sec-Butylbenzene
Concen: 38.147 ug/l
RT: 13.488 min Scan# 1944
Delta R.T. -0.130 min
Lab File: VN075829.D
Acq: 15 Dec 2022 19:47

Tgt Ion:105 Resp: 609195
Ion Ratio Lower Upper
105 100
134 0.0 10.1 30.1#



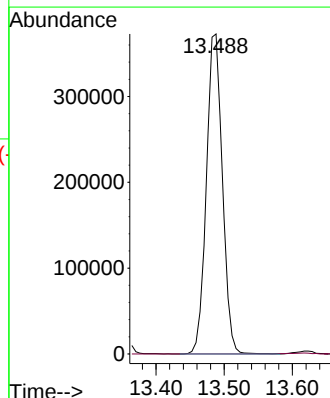
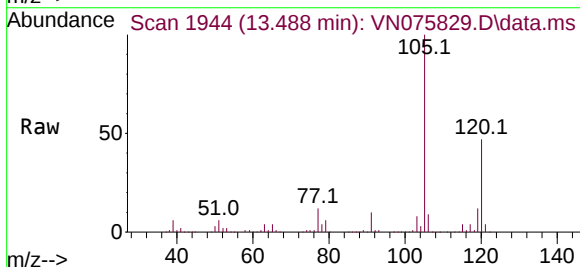




#86
p-Isopropyltoluene
Concen: 0.215 ug/l
RT: 13.735 min Scan# 1985
Delta R.T. 0.006 min
Lab File: VN075829.D
Acq: 15 Dec 2022 19:47




Instrument :
MSVOA_N
ClientSampleId :
DUP120822DL


Tgt Ion: 119 Resp: 2855
Ion Ratio Lower Upper
119 100
134 16.2 13.0 39.0
91 0.0 11.2 33.6#

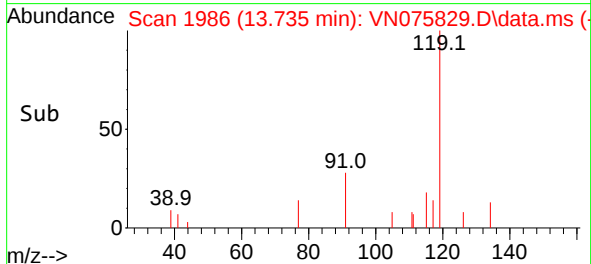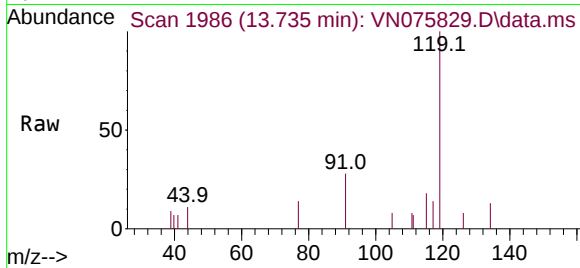

#89
n-Butylbenzene
Concen: 0.518 ug/l
RT: 14.058 min Scan# 2041
Delta R.T. -0.000 min
Lab File: VN075829.D
Acq: 15 Dec 2022 19:47

Tgt Ion: 91 Resp: 5573
Ion Ratio Lower Upper
91 100
92 64.4 26.4 79.2
134 0.0 13.4 40.2#


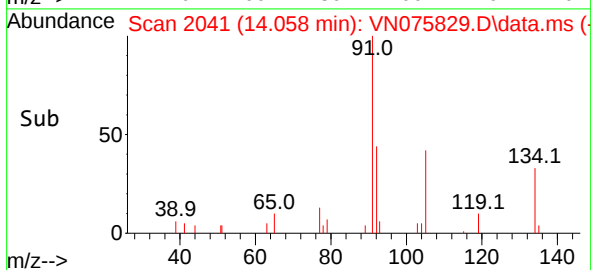

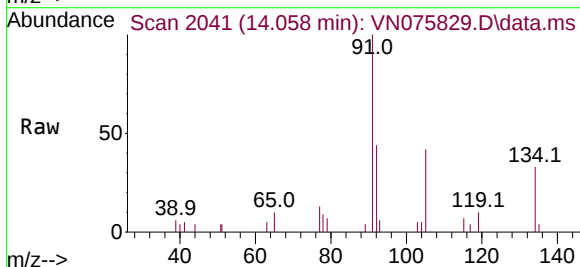


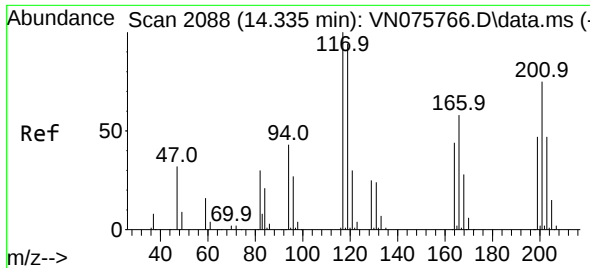

#90
Hexachloroethane
Concen: 2.802 ug/l
RT: 14.335 min Scan# 2088
Delta R.T. -0.000 min
Lab File: VN075829.D
Acq: 15 Dec 2022 19:47

Instrument :
MSVOA_N
ClientSampleId :
DUP120822DL

Tgt Ion:117 Resp: 6660
Ion Ratio Lower Upper
117 100
201 0.0 38.0 114.1#

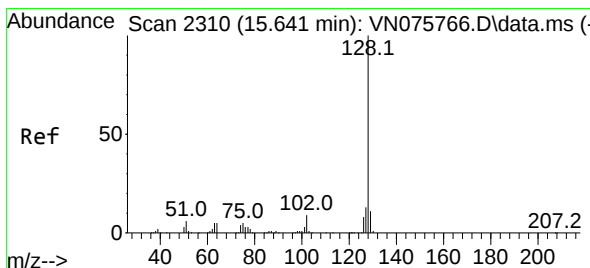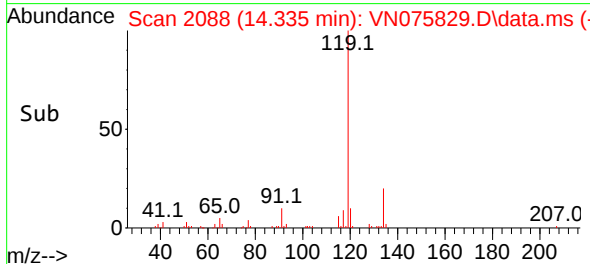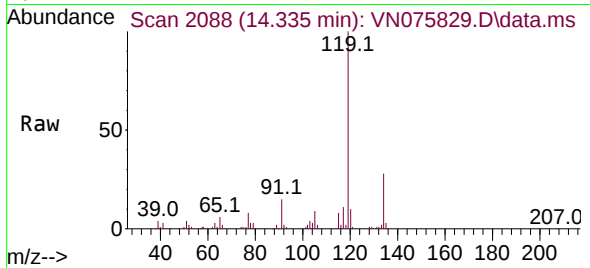

#95
Naphthalene
Concen: 17.591 ug/l
RT: 15.647 min Scan# 2311
Delta R.T. 0.006 min
Lab File: VN075829.D
Acq: 15 Dec 2022 19:47

Tgt Ion:128 Resp: 190301
Ion Ratio Lower Upper
128 100
127 12.5 10.4 15.6
129 10.6 8.7 13.1

