

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121522\
 Data File : VN075816.D
 Acq On : 15 Dec 2022 14:35
 Operator : JC\MD
 Sample : N5990-10
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 DUP120722-1

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
 Title : SW846 8260

Signal : TIC: VN075816.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.301	33	42	44	rBV	39312	77021	4.45%	0.712%
2	2.524	75	80	84	rBV4	9854	18358	1.06%	0.170%
3	2.830	127	132	142	rVB3	20237	49485	2.86%	0.458%
4	3.259	198	205	215	rVB3	18565	50436	2.91%	0.466%
5	5.530	578	591	611	rBV2	71698	261122	15.09%	2.415%
6	5.806	622	638	656	rBV	265982	933250	53.93%	8.631%
7	6.677	776	786	800	rBV3	23993	76694	4.43%	0.709%
8	7.336	890	898	904	rBV4	6870	18420	1.06%	0.170%
9	8.171	1031	1040	1045	rBV	242812	588946	34.03%	5.447%
10	8.230	1045	1050	1065	rVB	478546	1077526	62.27%	9.965%
11	8.588	1101	1111	1121	rBV2	251491	664978	38.43%	6.150%
12	8.677	1121	1126	1133	rVB	24513	56770	3.28%	0.525%
13	9.106	1190	1199	1213	rBV	644086	1300871	75.18%	12.030%
14	10.571	1439	1448	1458	rBV	935076	1730413	100.00%	16.003%
15	11.871	1659	1669	1679	rBV	815797	1472141	85.07%	13.614%
16	11.965	1679	1685	1693	rVB	11456	20658	1.19%	0.191%
17	12.853	1826	1836	1846	rBV	629182	1069678	61.82%	9.892%
18	13.488	1938	1944	1951	rVB2	12516	20215	1.17%	0.187%
19	13.794	1988	1996	2006	rBV	772864	1276776	73.78%	11.808%
20	15.647	2299	2311	2319	rBV	24332	49408	2.86%	0.457%




Sum of corrected areas: 10813166

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121522\
Data File : VN075816.D
Acq On : 15 Dec 2022 14:35
Operator : JC\MD
Sample : N5990-10
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
DUP120722-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

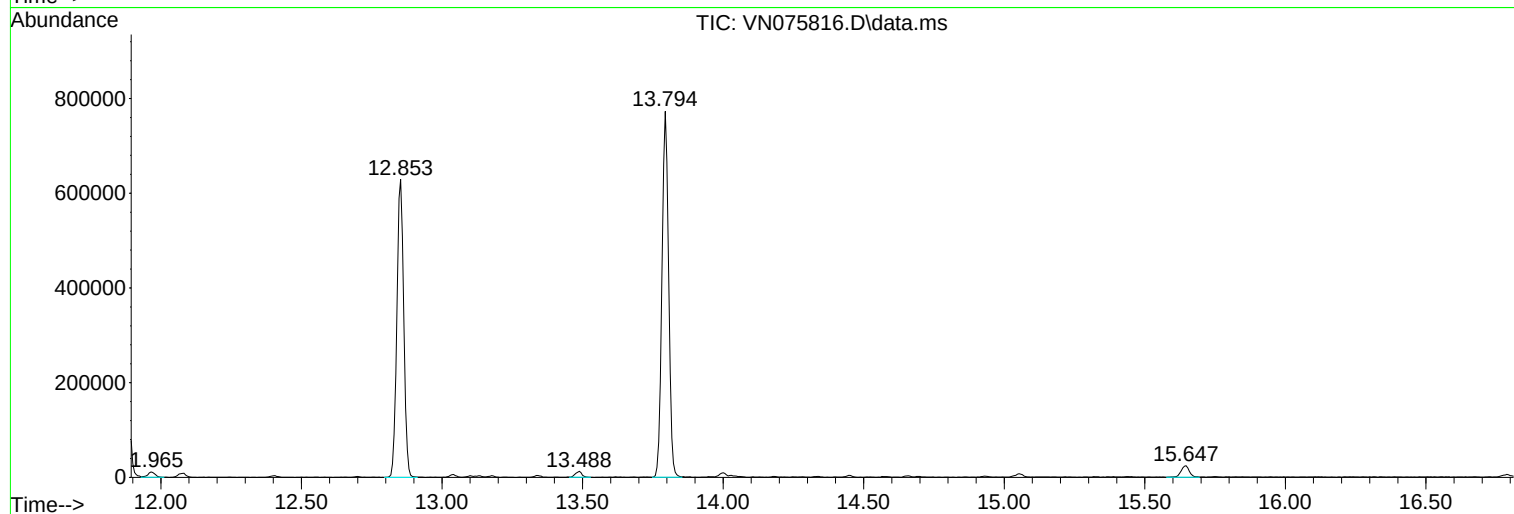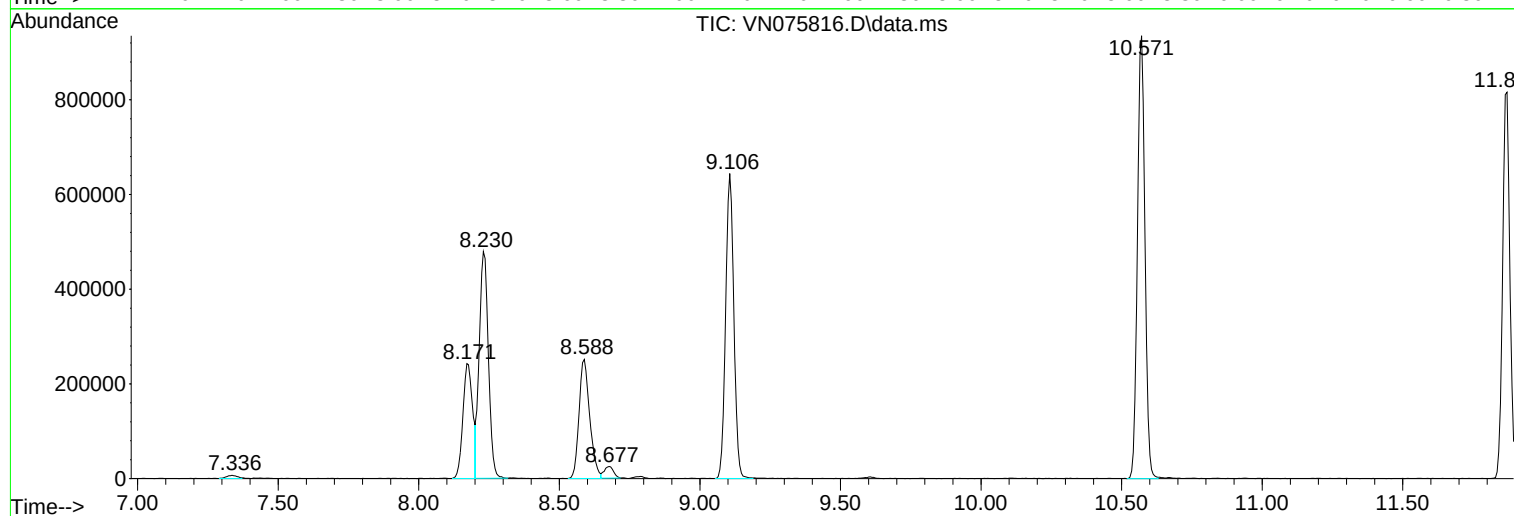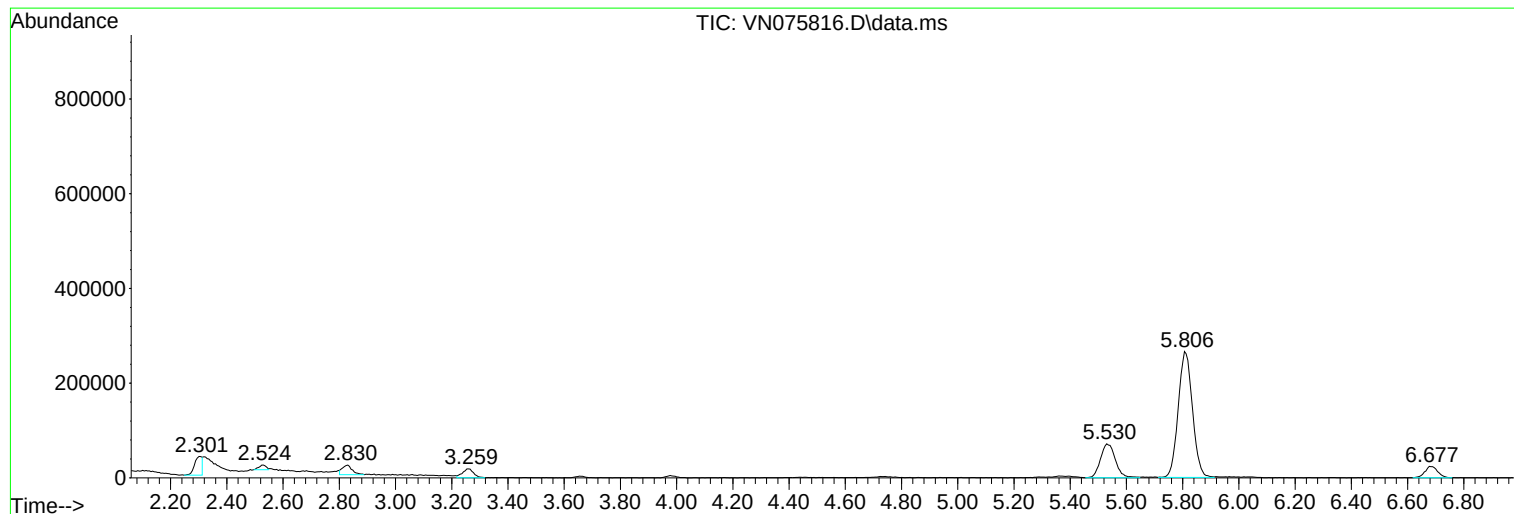

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121522\
Data File : VN075816.D
Acq On : 15 Dec 2022 14:35
Operator : JC\MD
Sample : N5990-10
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
DUP120722-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121522\
Data File : VN075816.D
Acq On : 15 Dec 2022 14:35
Operator : JC\MD
Sample : N5990-10
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
DUP120722-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
