
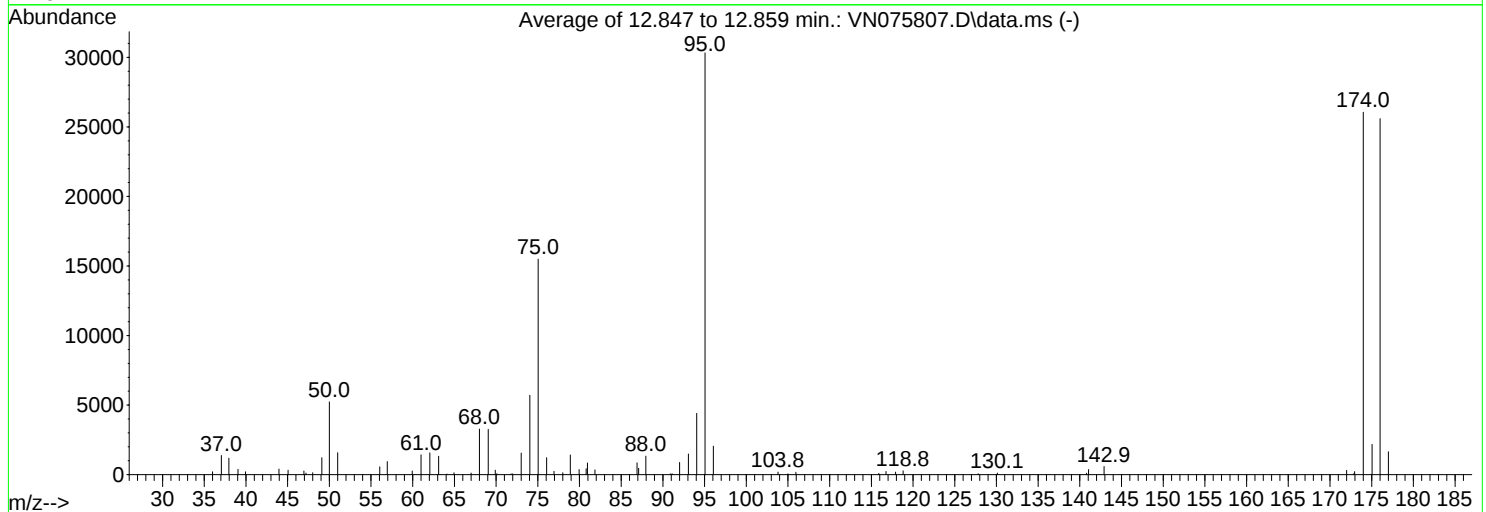


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121522\
Data File : VN075807.D
Acq On : 15 Dec 2022 09:47
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
Title : SW846 8260
Last Update : Wed Dec 14 13:03:41 2022

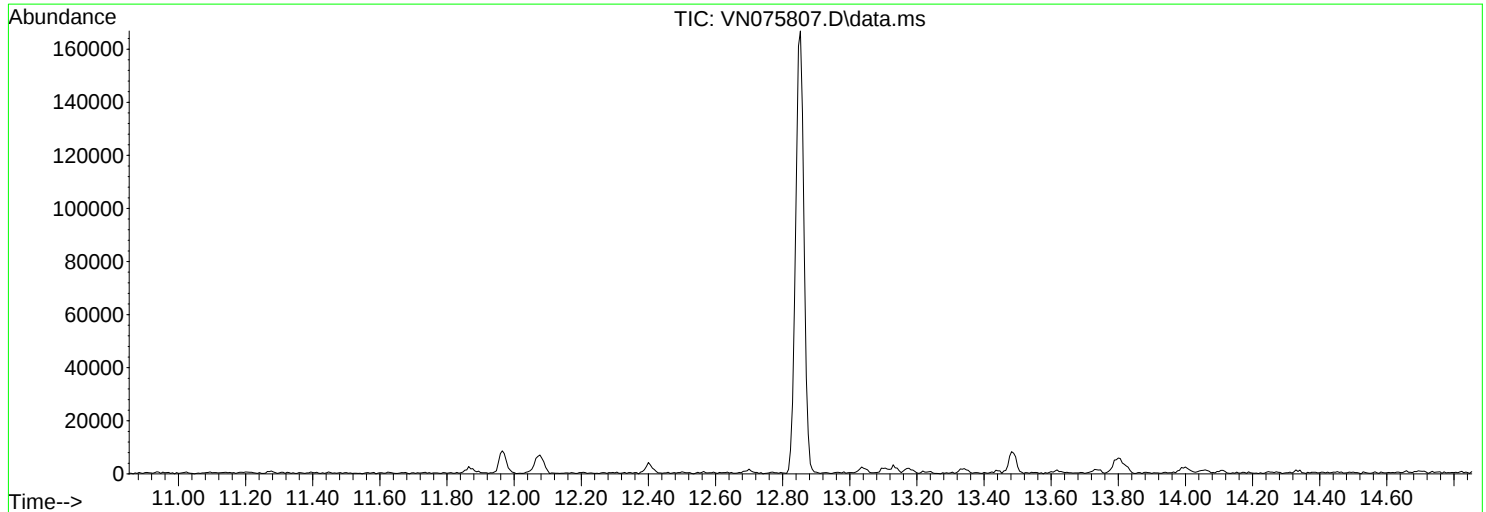

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	5235	PASS
75	95	30	60	51.1	15499	PASS
95	95	100	100	100.0	30325	PASS
96	95	5	9	6.8	2051	PASS
173	174	0.00	2	0.8	215	PASS
174	95	50	100	85.9	26053	PASS
175	174	5	9	8.3	2175	PASS
176	174	95	101	98.3	25600	PASS
177	176	5	9	6.4	1644	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	210	50.00	5235	68.00	3275	78.00	141
37.05	1378	51.00	1578	69.05	3254	78.90	141
37.95	1181	56.05	563	69.90	320	79.95	36
39.05	384	56.95	939	70.10	74	80.80	42
39.95	202	59.95	265	71.80	53	80.95	835
43.95	401	61.00	1430	72.00	62	81.85	340
45.05	325	62.05	1561	73.00	1550	86.90	848
46.95	268	63.10	1328	74.05	5703	87.10	463
47.20	121	64.10	52	75.05	15499	87.95	1337
48.00	133	64.95	142	76.05	1225	90.90	56
49.10	1219	67.00	116	76.95	244	91.10	75

Average of 12.847 to 12.859 min.: VN075807.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.00	871	118.80	282	176.00	25600		
93.05	1479	127.80	71	177.00	1644		
94.05	4408	130.10	115				
95.05	30325	140.80	107				
96.05	2051	141.05	370				
103.80	186	142.90	588				
105.00	57	172.00	312				
105.95	171	172.80	57				
115.90	98	172.95	215				
116.75	228	174.00	26053				
117.90	181	175.05	2175				

Instrument :

MSVOA_N

ClientSampleId :

BFB